


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF081219\
 Data File : BF116195.D
 Acq On : 12 Aug 2019 17:41
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF073019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 07 11:13:18 2019

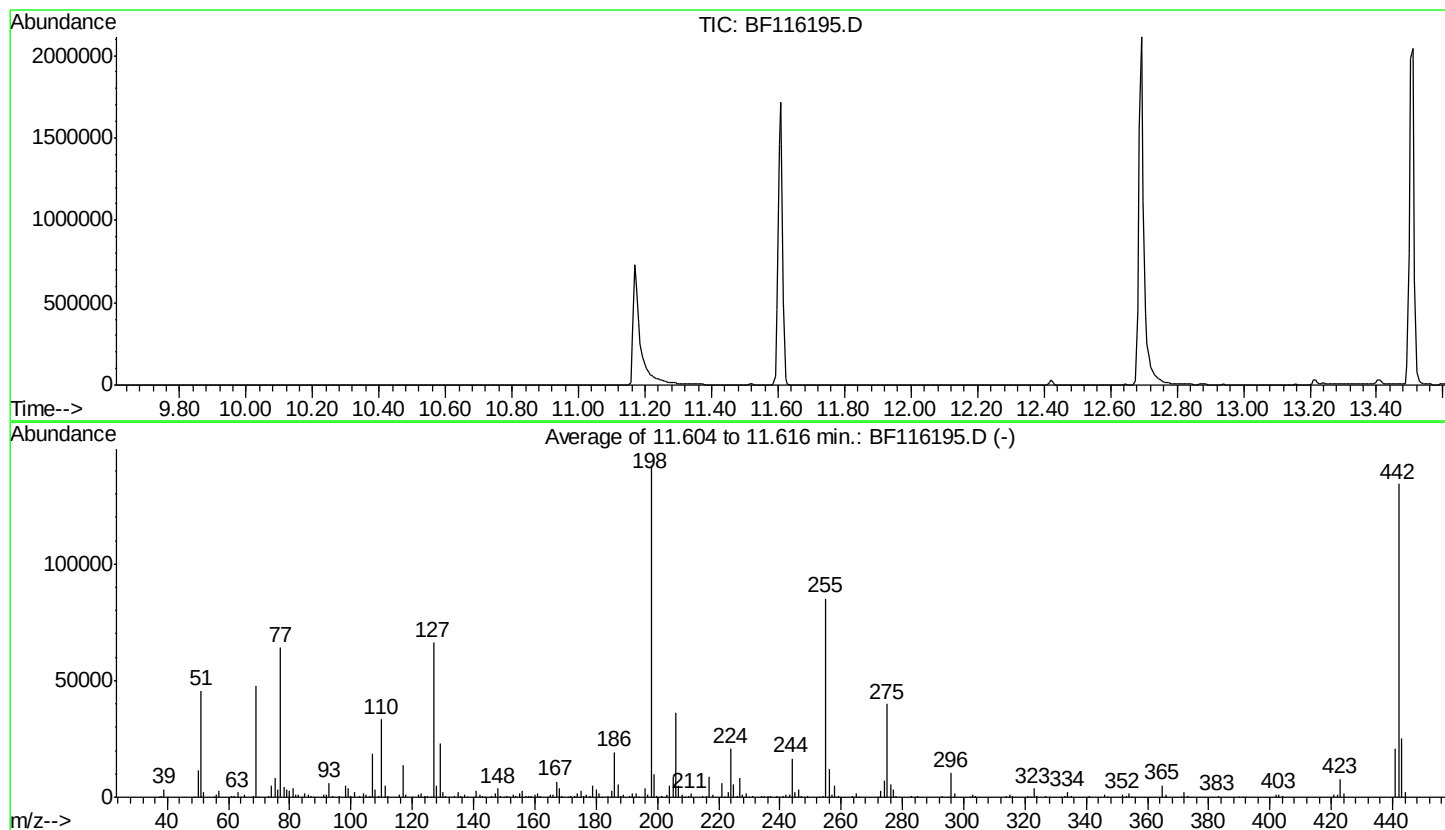

AutoFind: Scans 1618, 1619, 1620; Background Corrected with Scan 1612

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.2	45817	PASS
68	69	0.00	2	1.5	741	PASS
69	198	0.00	100	33.7	47904	PASS
70	69	0.00	2	0.6	279	PASS
127	198	10	80	46.7	66346	PASS
197	198	0.00	2	0.6	852	PASS
198	198	100	100	100.0	142138	PASS
199	198	5	9	6.9	9796	PASS
275	198	10	60	28.1	39989	PASS
365	198	1	100	3.6	5110	PASS
441	198	0.01	100	14.8	21107	PASS
442	198	50	100	94.5	134328	PASS
443	442	15	24	18.7	25109	PASS