

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF081319\
 Data File : BF116240.D
 Acq On : 13 Aug 2019 19:54
 Operator : HP/JU
 Sample : K4230-12
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 2S-J(0-1)-COMP

Quant Time: Aug 13 23:19:58 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF073019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 07 11:13:18 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.83	152	149189	20.00	ng	-0.01
21) Naphthalene-d8	8.12	136	590439	20.00	ng	-0.01
39) Acenaphthene-d10	9.87	164	320589	20.00	ng	-0.02
64) Phenanthrene-d10	11.36	188	611612	20.00	ng	-0.01
76) Chrysene-d12	14.00	240	484574	20.00	ng	0.00
87) Perylene-d12	15.47	264	422068	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.47	112	1047136	117.50	ng	0.00
7) Phenol-d6	6.47	99	1275185	113.41	ng	-0.01
23) Nitrobenzene-d5	7.40	82	993812	97.16	ng	-0.02
42) 2,4,6-Tribromophenol	10.66	330	455529	146.56	ng	-0.01
45) 2-Fluorobiphenyl	9.19	172	1638072	95.71	ng	-0.01
79) Terphenyl-d14	12.94	244	1985015	86.32	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.40	70	130943	18.793	ng	# 79
25) Isophorone	7.40	82	981153	50.164	ng	# 65
51) 2,6-Dinitrotoluene	9.87	165	41454	8.739	ng	# 29
57) 2,4-Dinitrotoluene	9.87	165	41455	6.564	ng	# 20
67) 4-Bromophenyl-phenylether	10.66	248	27304	4.170	ng	# 1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF081319\
Data File : BF116240.D
Acq On : 13 Aug 2019 19:54
Operator : HP/JU
Sample : K4230-12
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
2S-J-(0-1)-COMP

Quant Time: Aug 13 23:19:58 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF073019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 07 11:13:18 2019
Response via : Initial Calibration




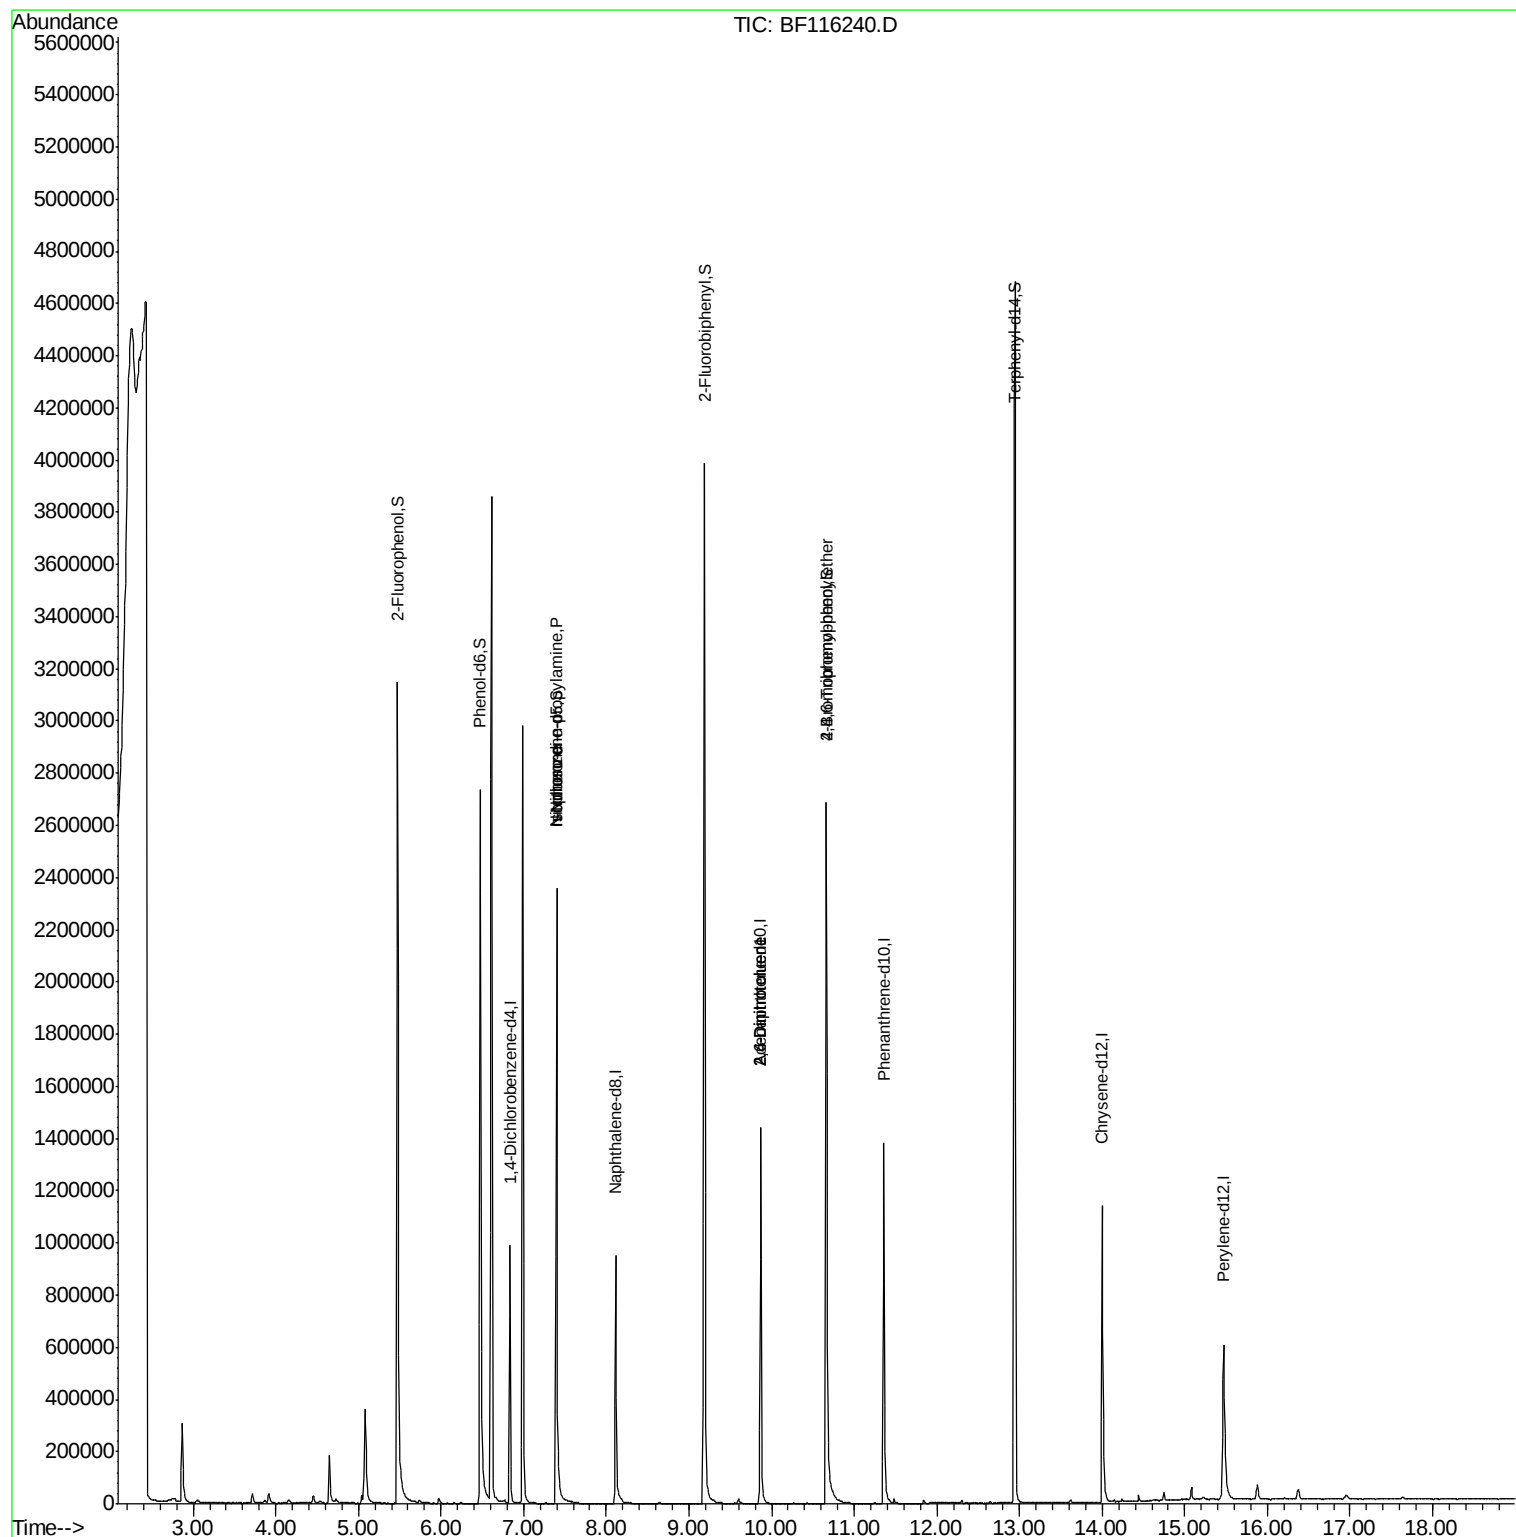




#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.83 min Scan# 807
 Delta R.T. -0.01 min
 Lab File: BF116240.D
 Acq: 13 Aug 2019 19:54




Instrument :
 BNA_F
 ClientSampleId :
 2S-J-(0-1)-COMP

Tgt Ion:152 Resp: 149189
 Ion Ratio Lower Upper
 152 100
 150 157.5 126.2 189.2
 115 60.8 49.9 74.9

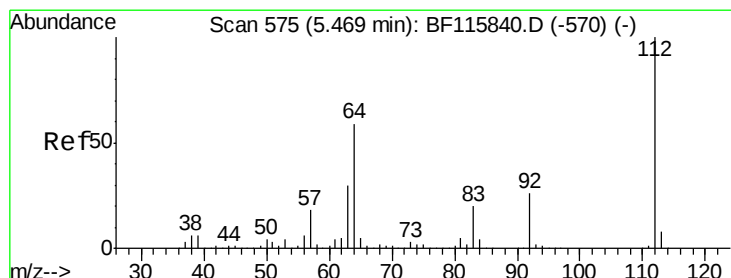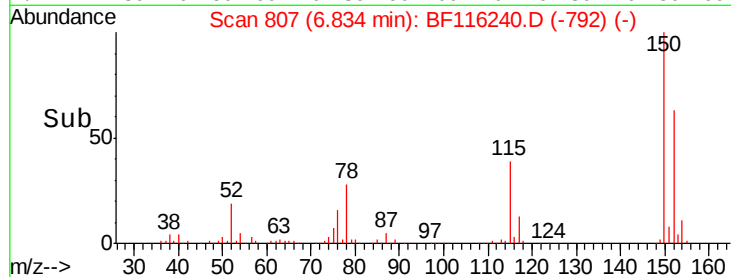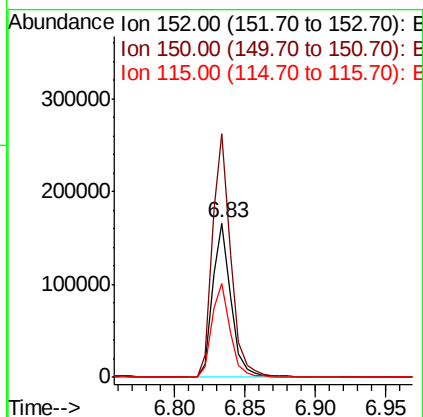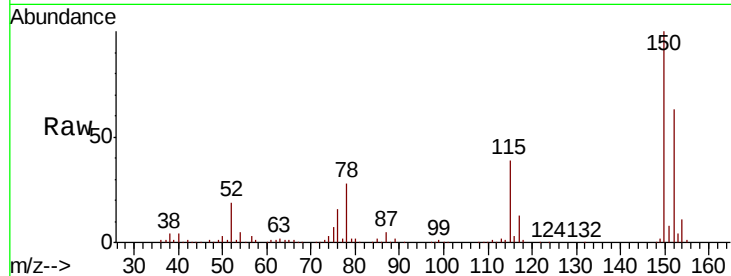

#5
 2-Fluorophenol
 Concen: 117.500 ng
 RT: 5.47 min Scan# 576
 Delta R.T. 0.01 min
 Lab File: BF116240.D
 Acq: 13 Aug 2019 19:54

Tgt Ion:112 Resp: 1047136
 Ion Ratio Lower Upper
 112 100
 64 59.0 45.4 68.2
 63 30.5 23.7 35.5

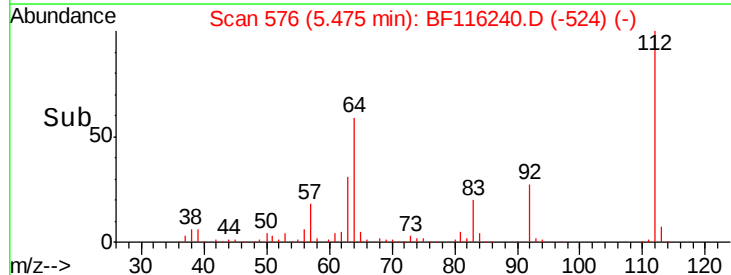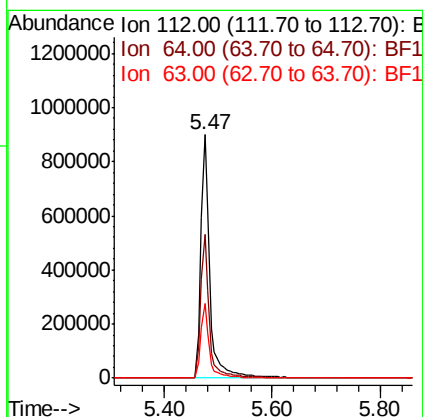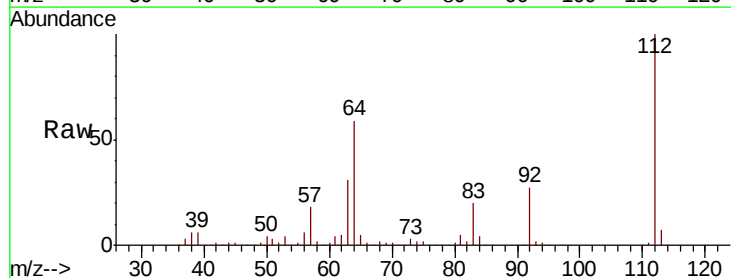



#7

Phenol-d6

Concen: 113.412 ng

RT: 6.47 min Scan# 746

Delta R.T. -0.01 min

Lab File: BF116240.D

Acq: 13 Aug 2019 19:54

Instrument :

BNA_F

ClientSampleId :

2S-J(0-1)-COMP


Tgt Ion: 99 Resp: 1275185

Ion Ratio Lower Upper

99 100

42 17.3 13.8 20.8



71 34.9 27.3 40.9

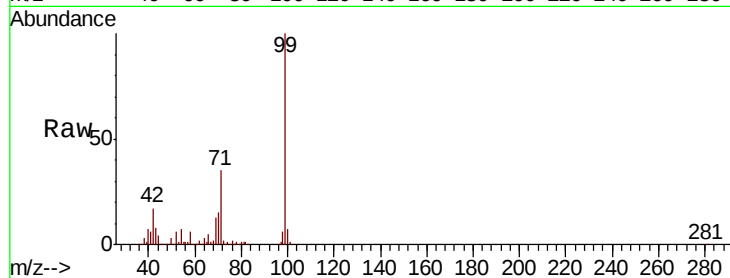

Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

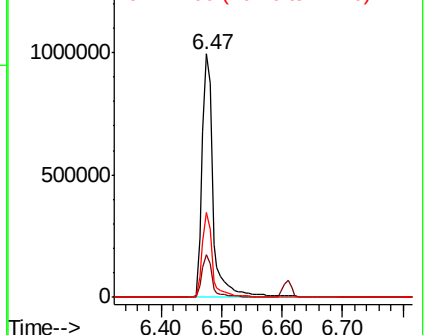

#19

n-Nitroso-di-n-propylamine

Concen: 18.793 ng

RT: 7.40 min Scan# 903

Delta R.T. 0.13 min

Lab File: BF116240.D

Acq: 13 Aug 2019 19:54

Tgt Ion: 70 Resp: 130943


Ion Ratio Lower Upper

70 100

42 42.2 40.9 61.3

101 0.0 7.9 11.9#

130 2.3 16.9 25.3#


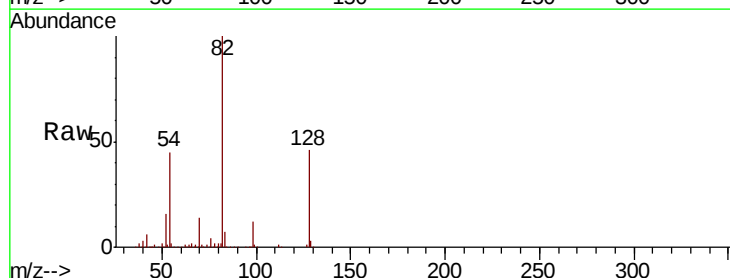


Abundance Ion 70.00 (69.70 to 70.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 101.00 (100.70 to 101.70): BF1

Ion 130.00 (129.70 to 130.70): BF1

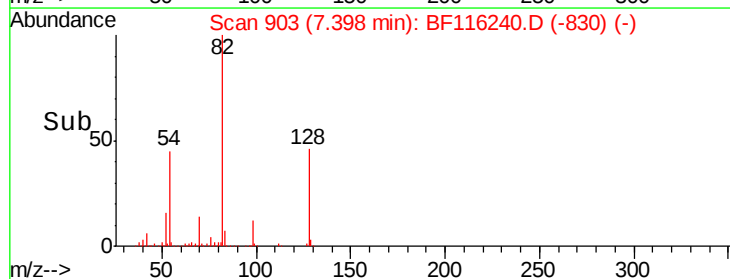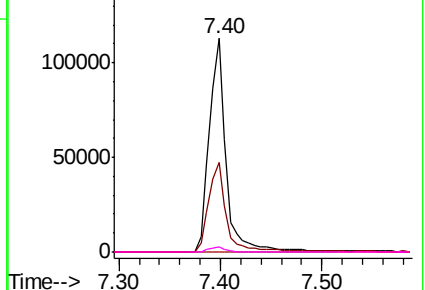






#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.12 min Scan# 1025
Delta R.T. -0.01 min
Lab File: BF116240.D
Acq: 13 Aug 2019 19:54

Instrument :
BNA_F
ClientSampleId :
2S-J-(0-1)-COMP

Tgt Ion:	136	Resp:	590439
Ion	Ratio	Lower	Upper
136	100		
137	10.6	9.0	13.4
54	6.7	5.8	8.6
68	6.0	5.2	7.8

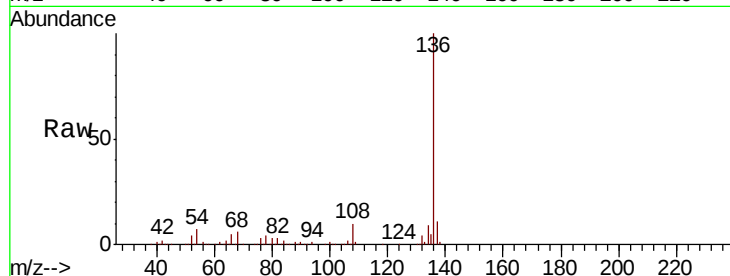


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

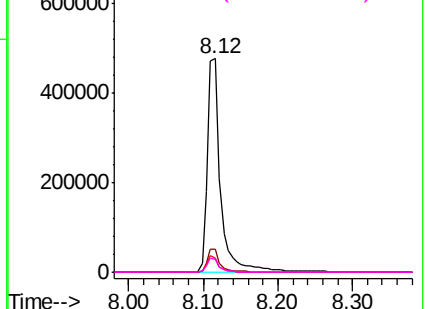




#23
Nitrobenzene-d5
Concen: 97.158 ng
RT: 7.40 min Scan# 903
Delta R.T. -0.02 min
Lab File: BF116240.D
Acq: 13 Aug 2019 19:54

Tgt Ion:	82	Resp:	993812
Ion	Ratio	Lower	Upper
82	100		
128	46.0	36.5	54.7
54	45.2	36.0	54.0

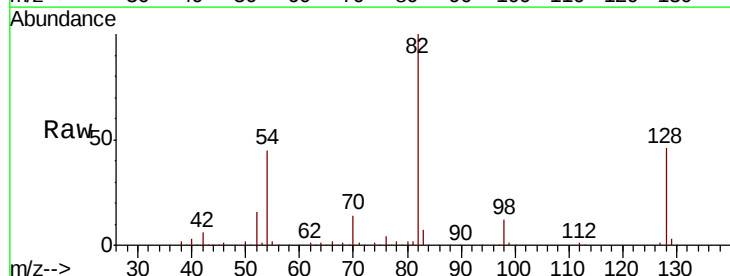

Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF1

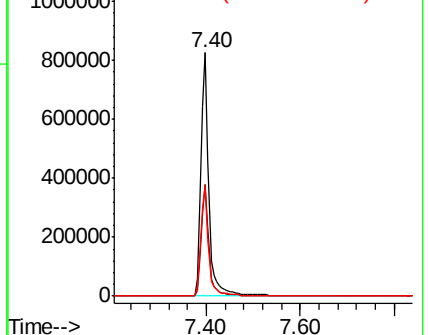

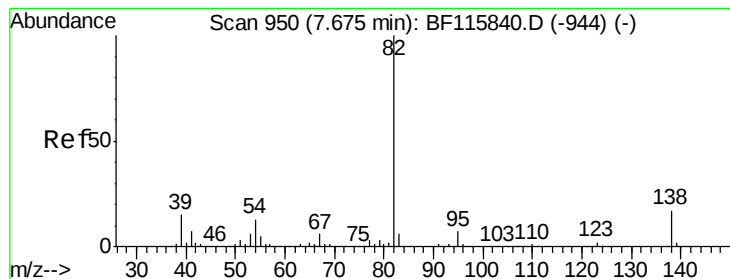

#25

Isophorone

Concen: 50.164 ng

RT: 7.40 min Scan# 903

Delta R.T. -0.28 min

Lab File: BF116240.D

Acq: 13 Aug 2019 19:54

Instrument :

BNA_F

ClientSampleId :

2S-J-(0-1)-COMP


Tgt Ion: 82 Resp: 981153

Ion Ratio Lower Upper

82 100

95 0.0 5.4 8.0#




138 0.0 14.5 21.7#

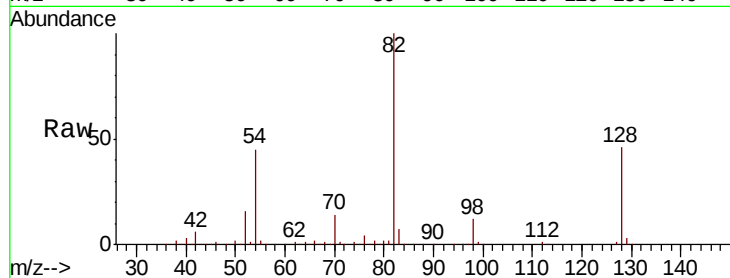

Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 95.00 (94.70 to 95.70): BF1

Ion 138.00 (137.70 to 138.70): BF1

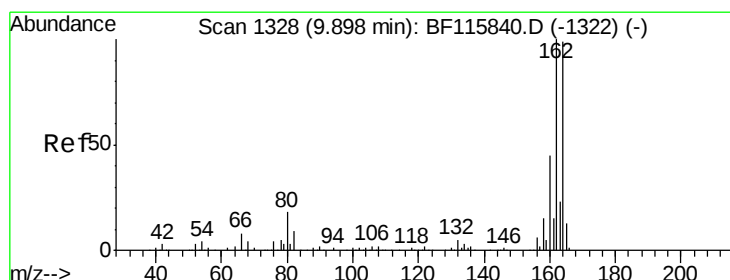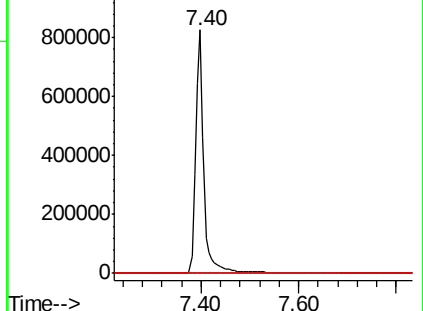

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.87 min Scan# 1323

Delta R.T. -0.02 min

Lab File: BF116240.D

Acq: 13 Aug 2019 19:54


Tgt Ion: 164 Resp: 320589

Ion Ratio Lower Upper

164 100

162 102.3 82.6 124.0



160 46.4 37.6 56.4

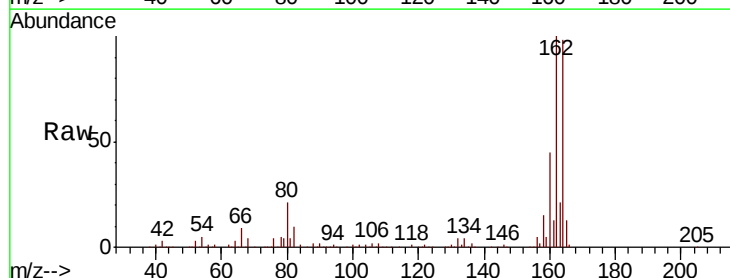

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

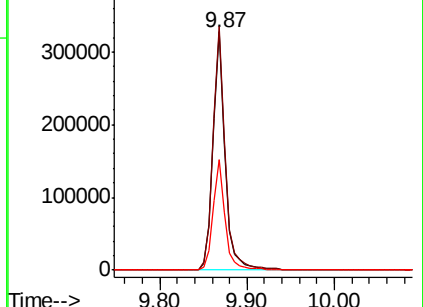






#42
 2,4,6-Tribromophenol
 Concen: 146.557 ng
 RT: 10.66 min Scan# 1458
 Delta R.T. -0.01 min
 Lab File: BF116240.D
 Acq: 13 Aug 2019 19:54

Instrument :
 BNA_F
 ClientSampleId :
 2S-J-(0-1)-COMP

Tgt Ion:330 Resp: 455529
 Ion Ratio Lower Upper
 330 100
 332 95.8 76.8 115.2
 141 32.9 26.3 39.5

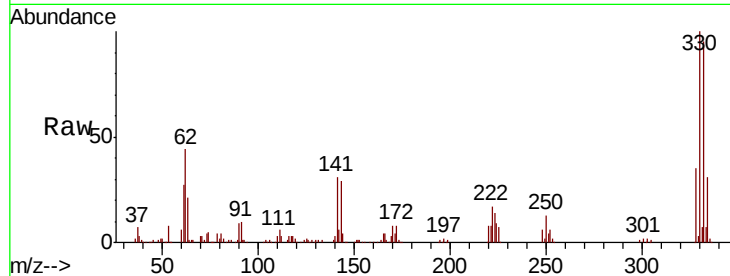


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E


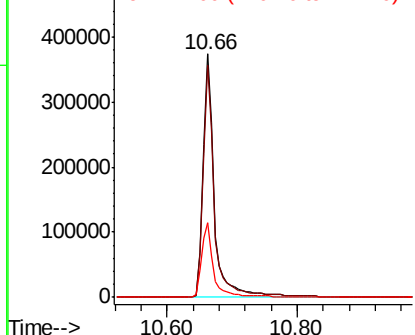



#45
 2-Fluorobiphenyl
 Concen: 95.706 ng
 RT: 9.19 min Scan# 1208
 Delta R.T. -0.01 min
 Lab File: BF116240.D
 Acq: 13 Aug 2019 19:54

Tgt Ion:172 Resp: 1638072
 Ion Ratio Lower Upper
 172 100
 171 36.6 29.6 44.4
 170 25.0 20.1 30.1

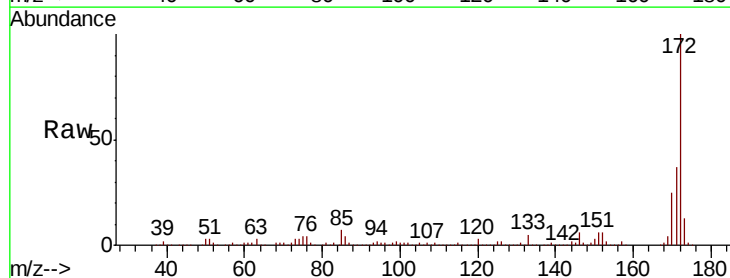

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

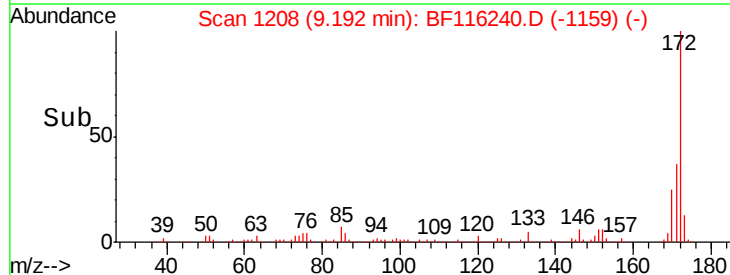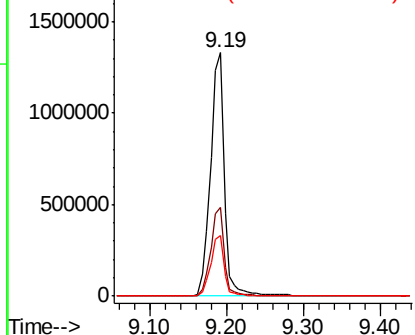







#51
 2,6-Dinitrotoluene
 Concen: 8.739 ng
 RT: 9.87 min Scan# 1323
 Delta R.T. 0.19 min
 Lab File: BF116240.D
 Acq: 13 Aug 2019 19:54

Instrument :
 BNA_F
 ClientSampleId :
 2S-J-(0-1)-COMP

Tgt Ion	Ratio	Lower	Upper
165	100		
63	1.1	38.2	57.2#
89	1.4	42.9	64.3#

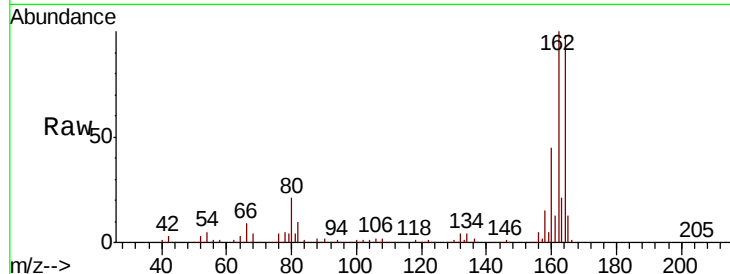




Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BF1
 Ion 89.00 (88.70 to 89.70): BF1

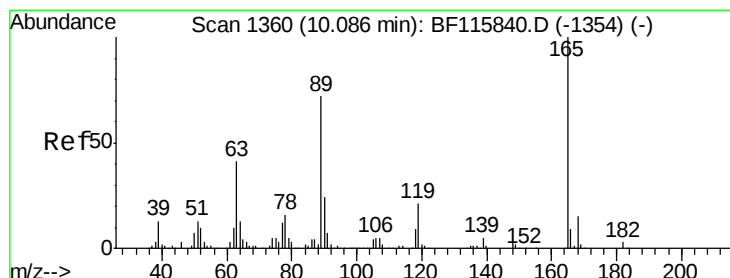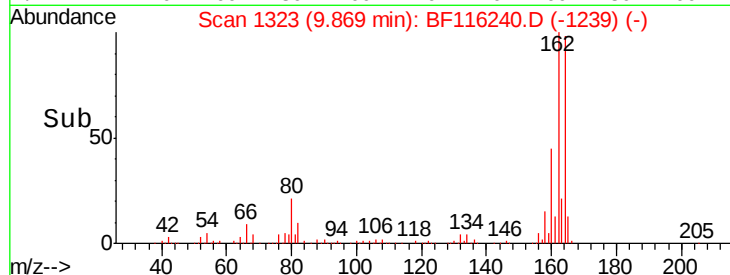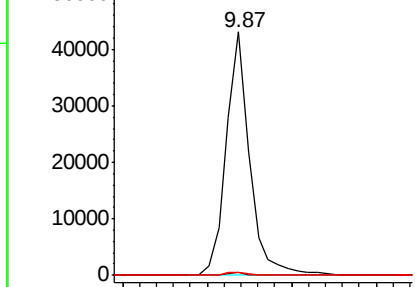


#57
 2,4-Dinitrotoluene
 Concen: 6.564 ng
 RT: 9.87 min Scan# 1323
 Delta R.T. -0.21 min
 Lab File: BF116240.D
 Acq: 13 Aug 2019 19:54

Tgt Ion	Ratio	Lower	Upper
165	100		
63	1.1	39.6	59.4#
89	1.4	62.2	93.2#
182	0.0	2.1	3.1#

Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BF1
 Ion 89.00 (88.70 to 89.70): BF1
 Ion 182.00 (181.70 to 182.70): E

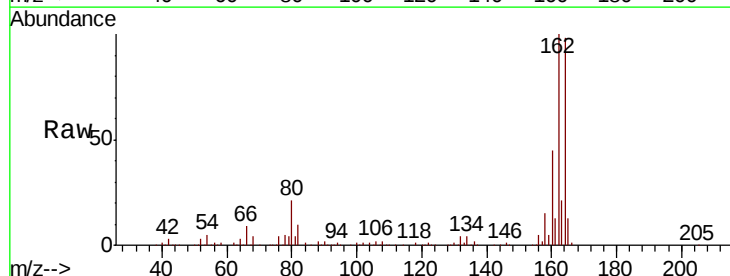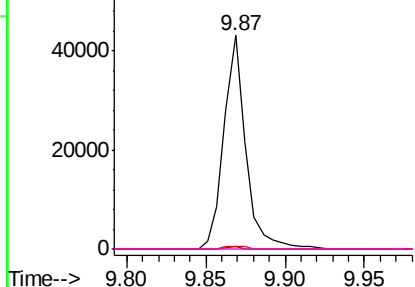


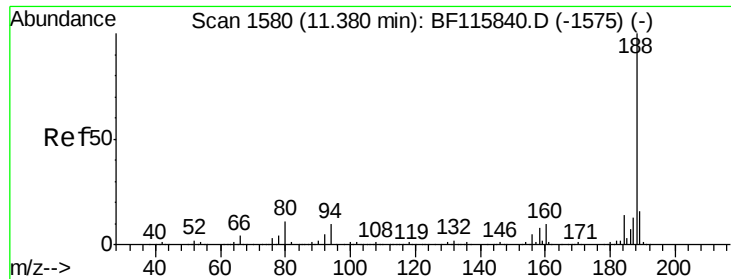




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.36 min Scan# 1576
Delta R.T. -0.01 min
Lab File: BF116240.D
Acq: 13 Aug 2019 19:54

Instrument :
BNA_F
ClientSampleId :
2S-J-(0-1)-COMP

Tgt Ion:188 Resp: 611612
Ion Ratio Lower Upper
188 100
94 9.8 8.1 12.1
80 10.6 8.7 13.1

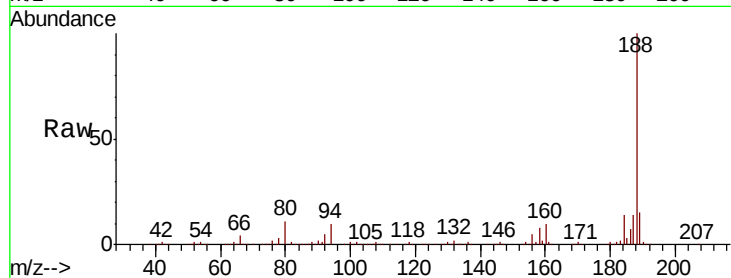


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1

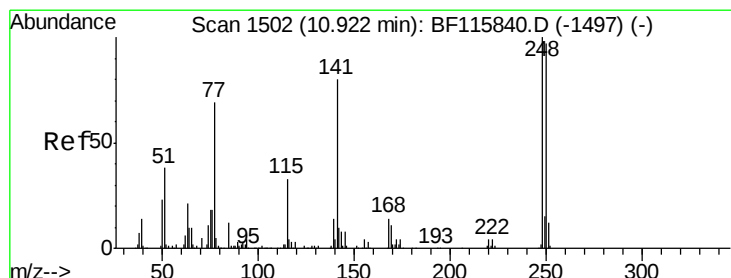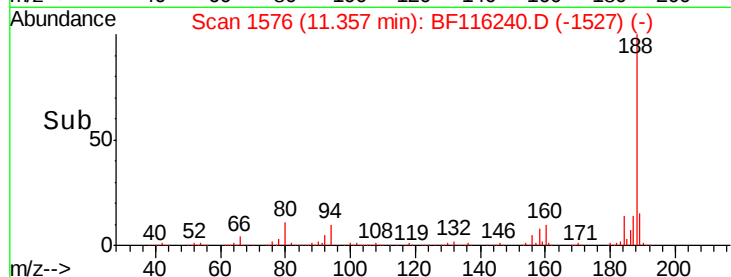
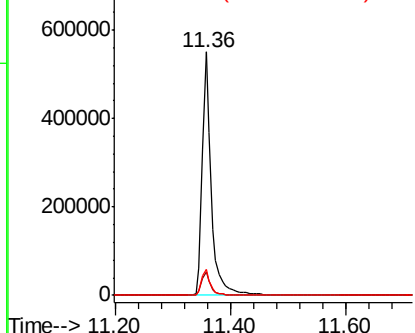


#67
4-Bromophenyl-phenylether
Concen: 4.170 ng
RT: 10.66 min Scan# 1458
Delta R.T. -0.25 min
Lab File: BF116240.D
Acq: 13 Aug 2019 19:54

Tgt Ion:248 Resp: 27304
Ion Ratio Lower Upper
248 100
250 210.5 77.4 116.2#
141 516.5 56.8 85.2#

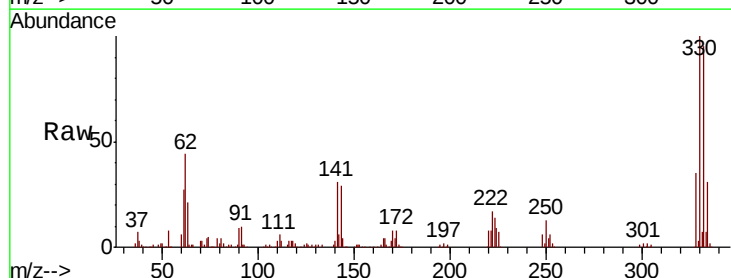

Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E

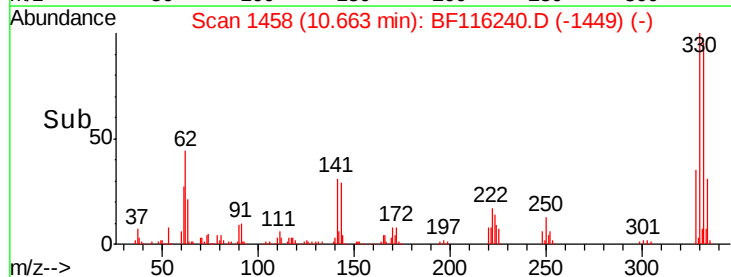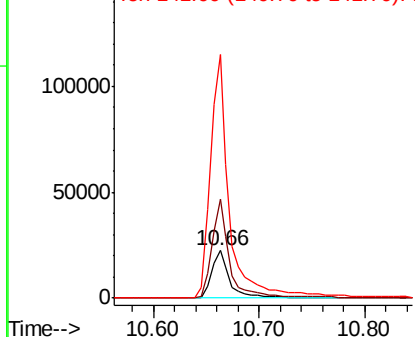







#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.00 min Scan# 2026
Delta R.T. -0.01 min
Lab File: BF116240.D
Acq: 13 Aug 2019 19:54

Instrument :
BNA_F
ClientSampleId :
2S-J-(0-1)-COMP

Tgt Ion:240 Resp: 484574
Ion Ratio Lower Upper
240 100
120 11.6 10.7 16.1
236 27.6 22.2 33.2

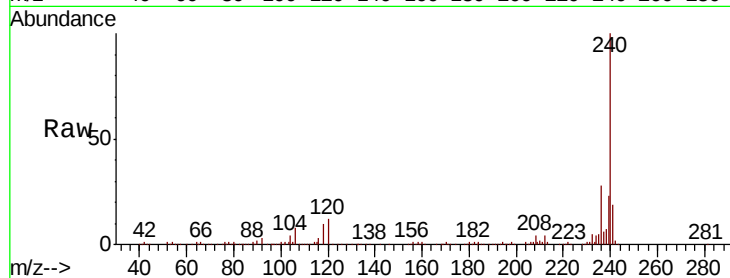


Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

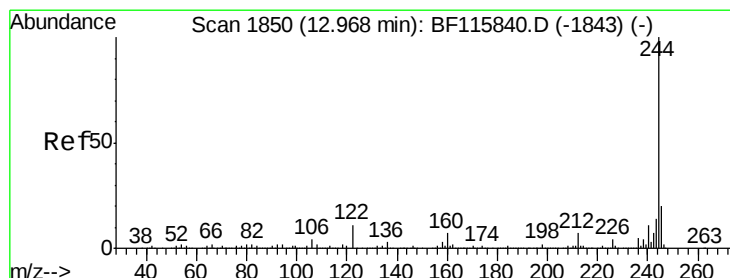
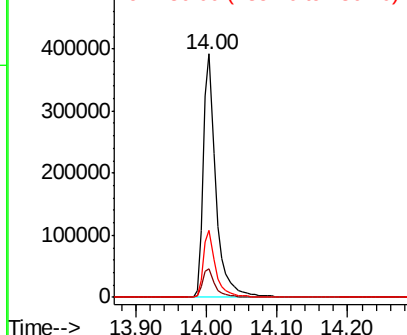



#79
Terphenyl-d14
Concen: 86.318 ng
RT: 12.94 min Scan# 1846
Delta R.T. -0.01 min
Lab File: BF116240.D
Acq: 13 Aug 2019 19:54

Tgt Ion:244 Resp: 1985015
Ion Ratio Lower Upper
244 100
212 7.2 5.8 8.8
122 10.3 9.0 13.4

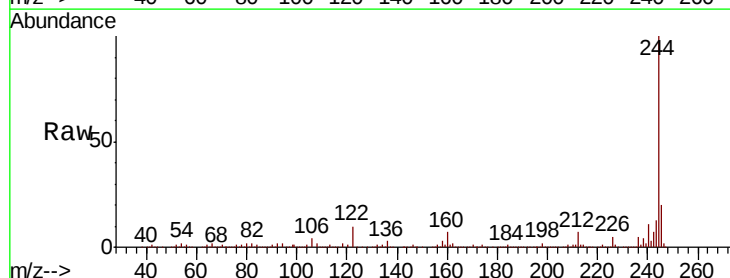

Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

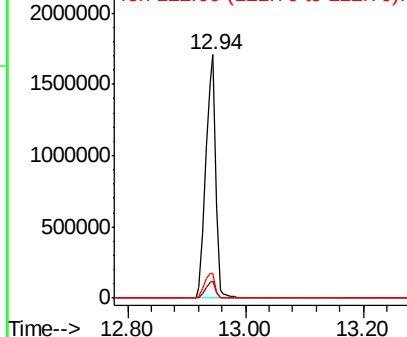

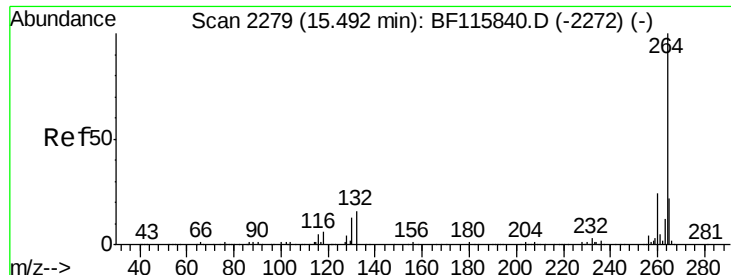

#87
Perylene-d12
Concen: 20.000 ng
RT: 15.47 min Scan# 2275
Delta R.T. -0.01 min
Lab File: BF116240.D
Acq: 13 Aug 2019 19:54

Instrument :
BNA_F
ClientSampleId :
2S-J-(0-1)-COMP

Tgt Ion	Ratio	Lower	Upper
264	100		
260	24.8	19.7	29.5
265	22.2	17.4	26.0

