

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF081319\
 Data File : BF116246.D
 Acq On : 13 Aug 2019 22:35
 Operator : HP/JU
 Sample : K4227-07
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 1S-K-(0-1)-COMP

Quant Time: Aug 13 23:20:48 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF073019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 07 11:13:18 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.83	152	145792	20.00	ng	-0.01
21) Naphthalene-d8	8.12	136	571891	20.00	ng	-0.01
39) Acenaphthene-d10	9.87	164	315697	20.00	ng	-0.02
64) Phenanthrene-d10	11.36	188	594698	20.00	ng	-0.01
76) Chrysene-d12	14.00	240	459322	20.00	ng	-0.01
87) Perylene-d12	15.47	264	392546	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.47	112	1017453	116.83	ng	0.00
7) Phenol-d6	6.47	99	1218124	110.86	ng	-0.01
23) Nitrobenzene-d5	7.40	82	966175	97.52	ng	-0.02
42) 2,4,6-Tribromophenol	10.66	330	445040	145.40	ng	-0.01
45) 2-Fluorobiphenyl	9.19	172	1605651	95.27	ng	-0.01
79) Terphenyl-d14	12.95	244	1945522	89.25	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.40	70	127897	18.784	ng	# 79
25) Isophorone	7.40	82	966170	51.000	ng	# 65
51) 2,6-Dinitrotoluene	9.87	165	39801	8.520	ng	# 29
57) 2,4-Dinitrotoluene	9.87	165	39803	6.400	ng	# 20
67) 4-Bromophenyl-phenylether	10.66	248	26663	4.188	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF081319\
Data File : BF116246.D
Acq On : 13 Aug 2019 22:35
Operator : HP/JU
Sample : K4227-07
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
1S-K-(0-1)-COMP

Quant Time: Aug 13 23:20:48 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF073019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 07 11:13:18 2019
Response via : Initial Calibration

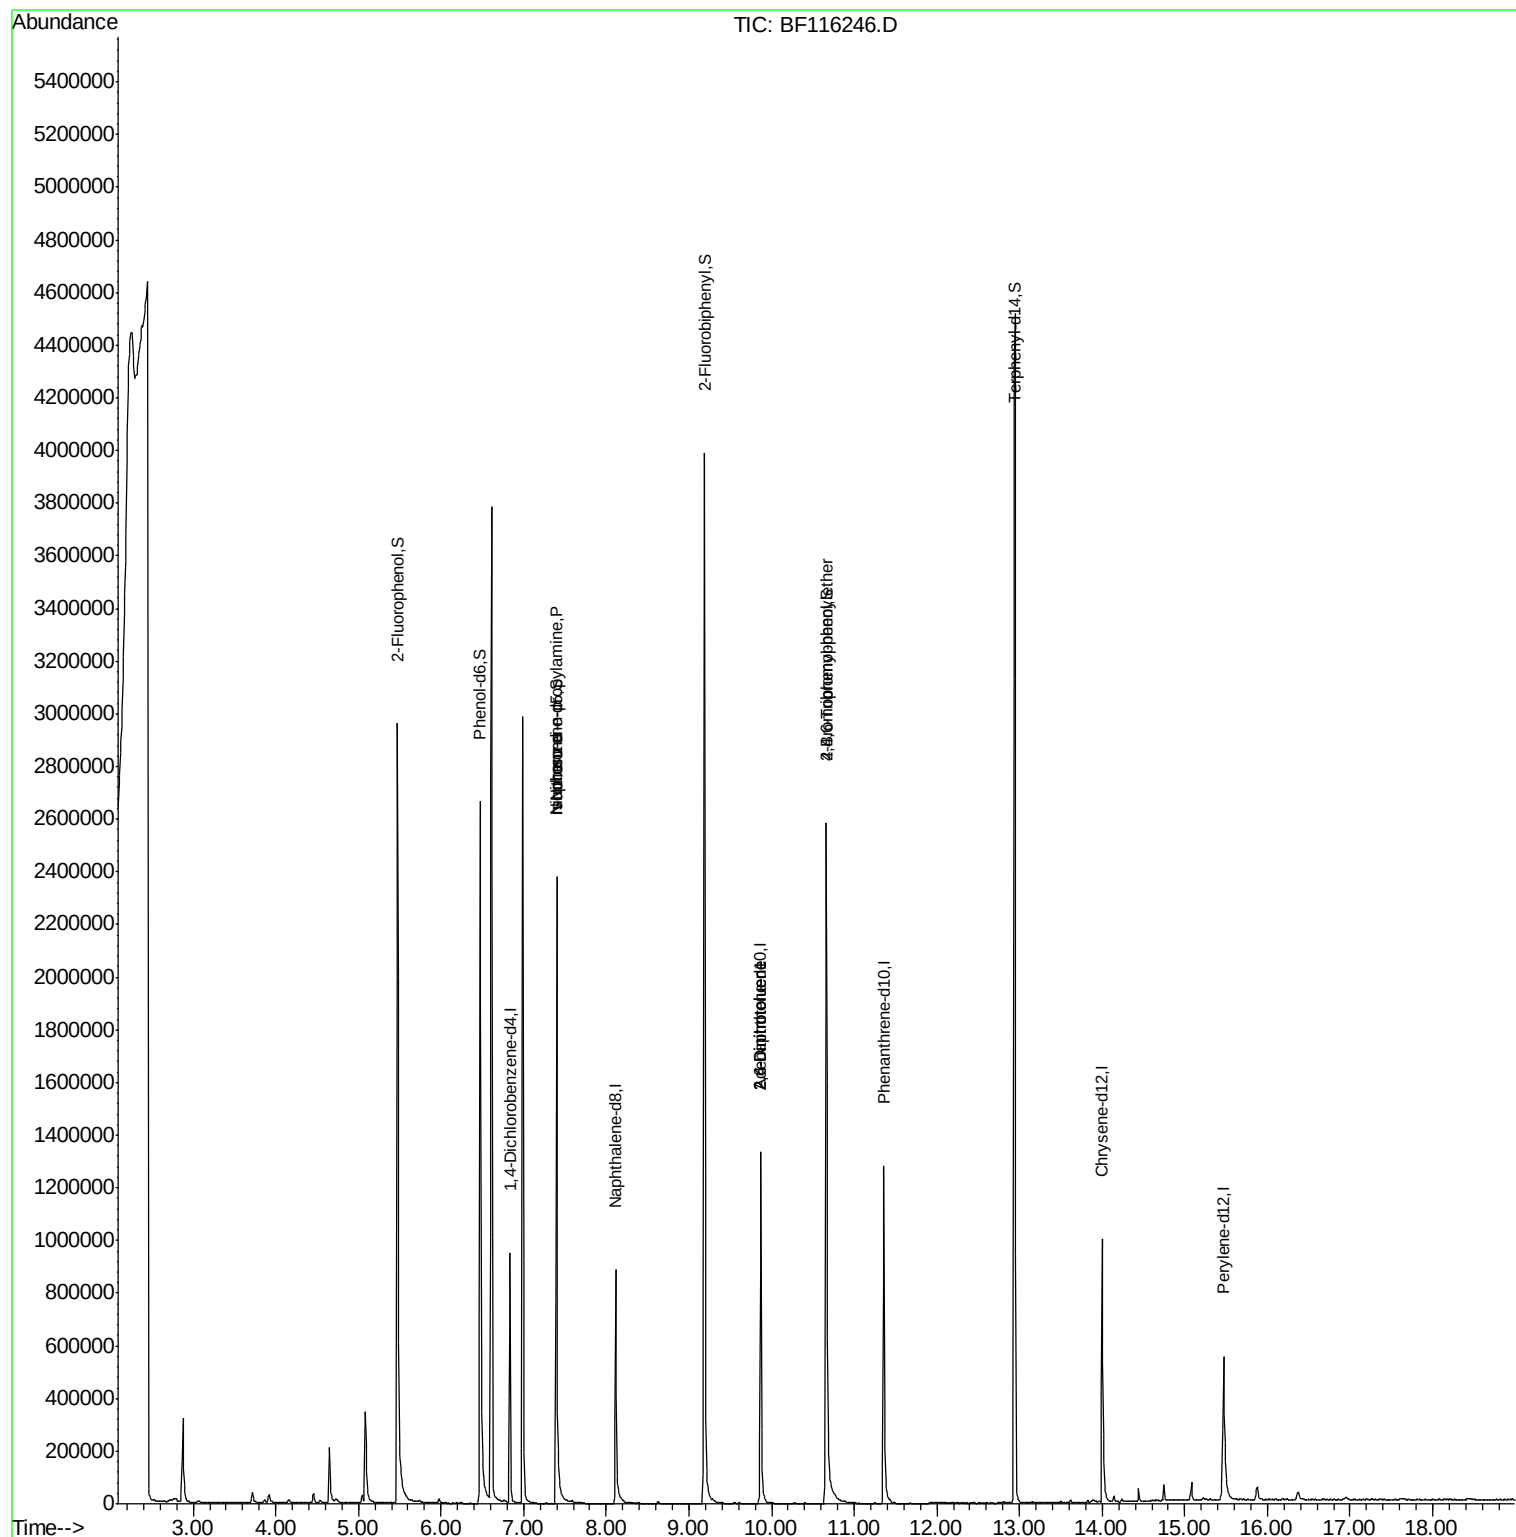

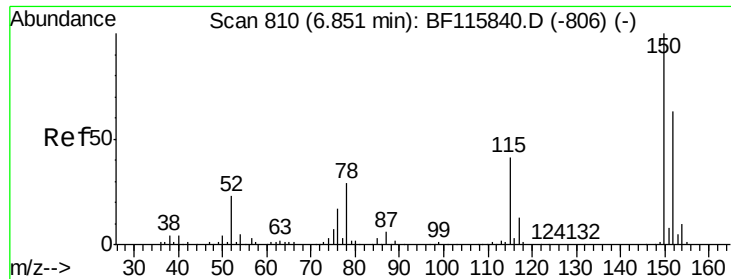


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.83 min Scan# 807
Delta R.T. -0.01 min
Lab File: BF116246.D
Acq: 13 Aug 2019 22:35

Instrument :
BNA_F
ClientSampleId :
1S-K-(0-1)-COMP

Tgt Ion:152 Resp: 145792
Ion Ratio Lower Upper
152 100
150 155.0 126.2 189.2
115 61.5 49.9 74.9

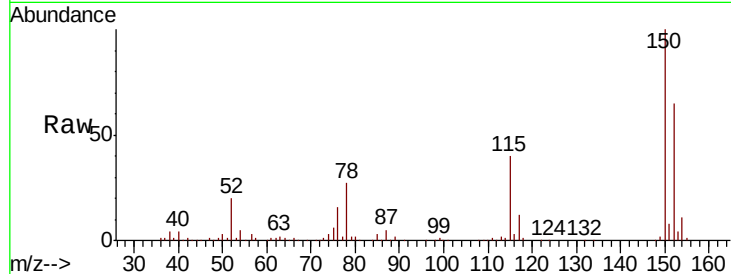


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

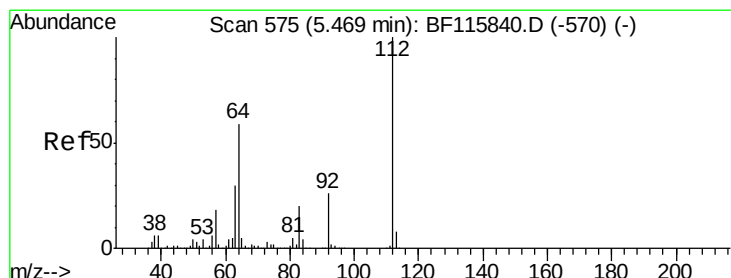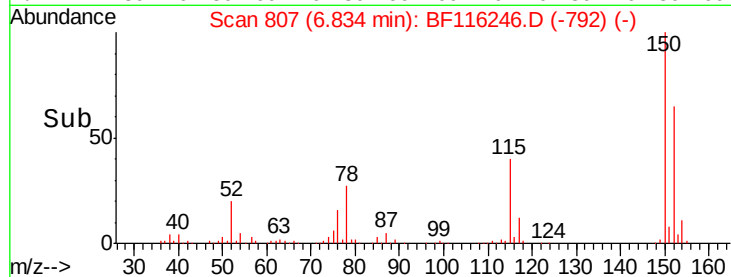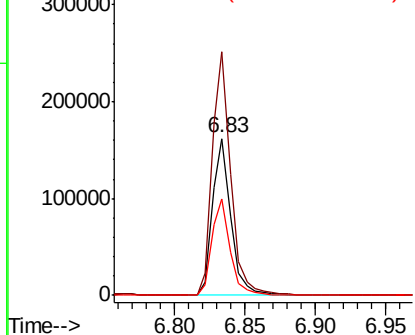



#5


2-Fluorophenol
Concen: 116.829 ng
RT: 5.47 min Scan# 576
Delta R.T. 0.01 min
Lab File: BF116246.D
Acq: 13 Aug 2019 22:35

Tgt Ion:112 Resp: 1017453
Ion Ratio Lower Upper
112 100
64 58.9 45.4 68.2
63 30.6 23.7 35.5

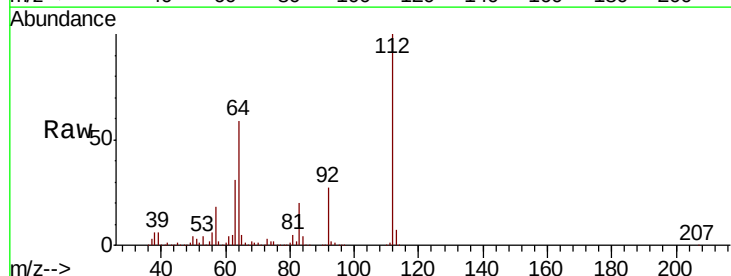

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

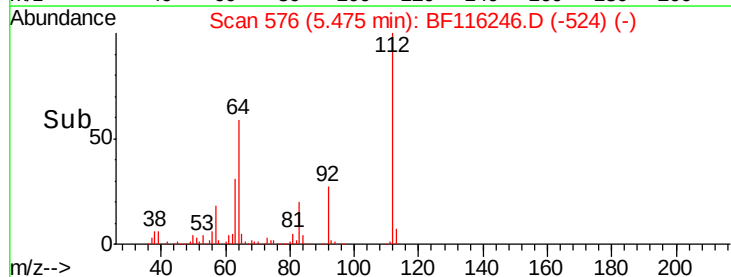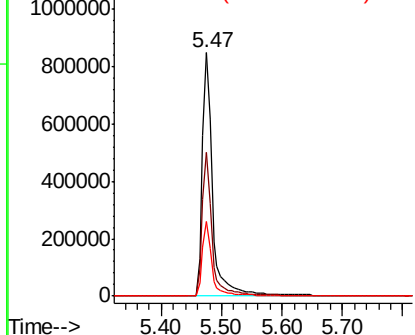



#7

Phenol-d6

Concen: 110.862 ng

RT: 6.47 min Scan# 746

Delta R.T. -0.01 min

Lab File: BF116246.D

Acq: 13 Aug 2019 22:35

Instrument :

BNA_F

ClientSampleId :

1S-K-(0-1)-COMP


Tgt Ion: 99 Resp: 1218124

Ion Ratio Lower Upper

99 100

42 17.3 13.8 20.8




71 34.7 27.3 40.9

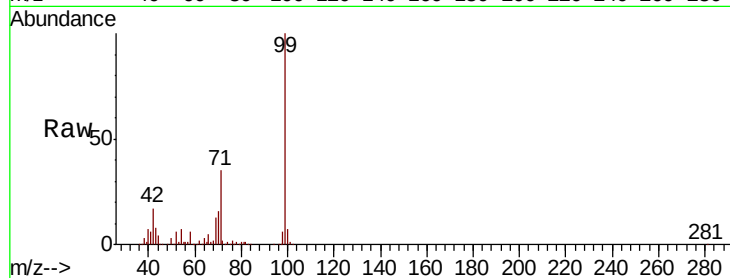

Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

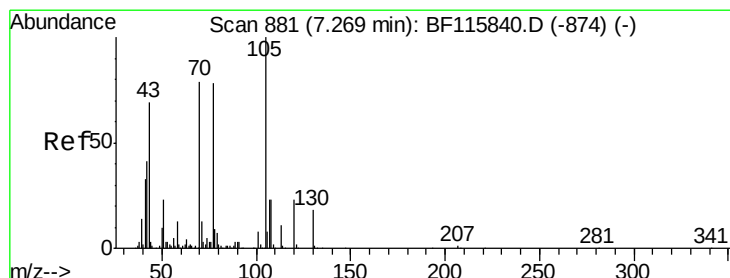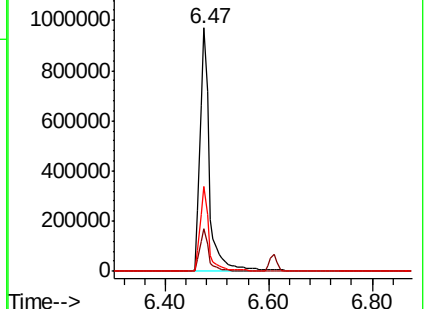

#19

n-Nitroso-di-n-propylamine

Concen: 18.784 ng

RT: 7.40 min Scan# 903

Delta R.T. 0.13 min

Lab File: BF116246.D

Acq: 13 Aug 2019 22:35

Tgt Ion: 70 Resp: 127897


Ion Ratio Lower Upper

70 100

42 42.5 40.9 61.3

101 0.0 7.9 11.9#

130 2.1 16.9 25.3#


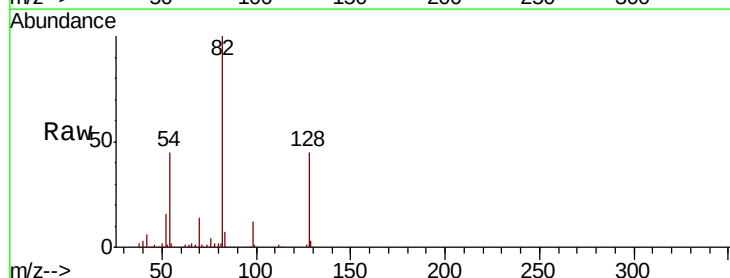



Abundance Ion 70.00 (69.70 to 70.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 101.00 (100.70 to 101.70): BF1

Ion 130.00 (129.70 to 130.70): BF1

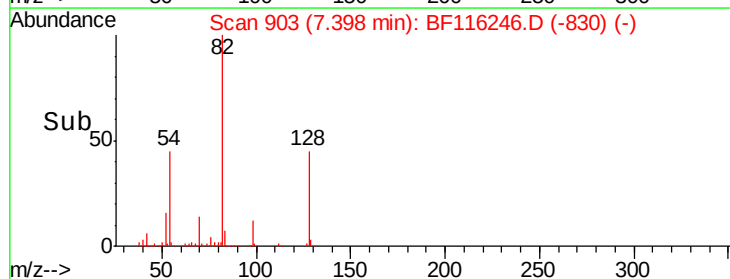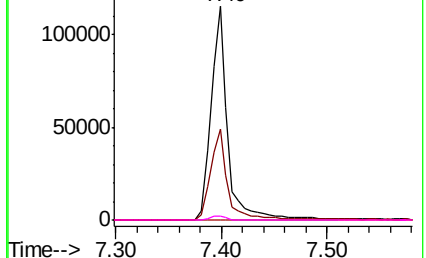







#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.12 min Scan# 1025
Delta R.T. -0.01 min
Lab File: BF116246.D
Acq: 13 Aug 2019 22:35

Instrument :
BNA_F
ClientSampleId :
1S-K-(0-1)-COMP

Tgt Ion:	136	Resp:	571891
Ion	Ratio	Lower	Upper
136	100		
137	10.8	9.0	13.4
54	6.7	5.8	8.6
68	5.7	5.2	7.8

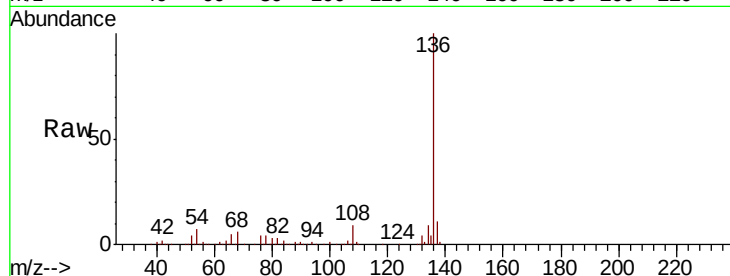


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

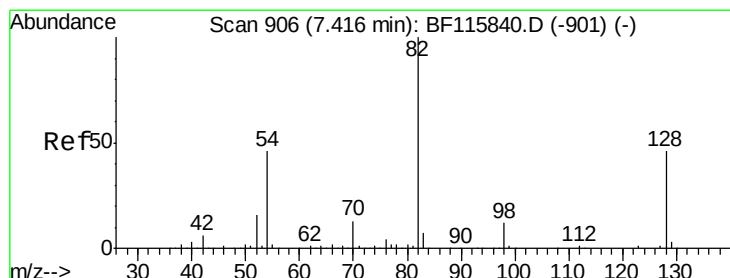
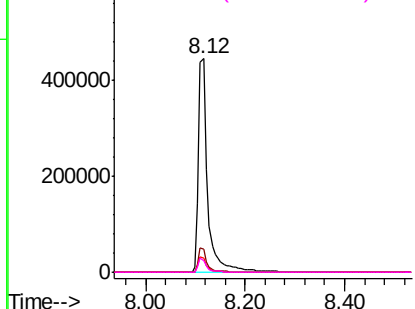



#23
Nitrobenzene-d5
Concen: 97.520 ng
RT: 7.40 min Scan# 903
Delta R.T. -0.02 min
Lab File: BF116246.D
Acq: 13 Aug 2019 22:35

Tgt Ion:	82	Resp:	966175
Ion	Ratio	Lower	Upper
82	100		
128	44.8	36.5	54.7
54	45.4	36.0	54.0

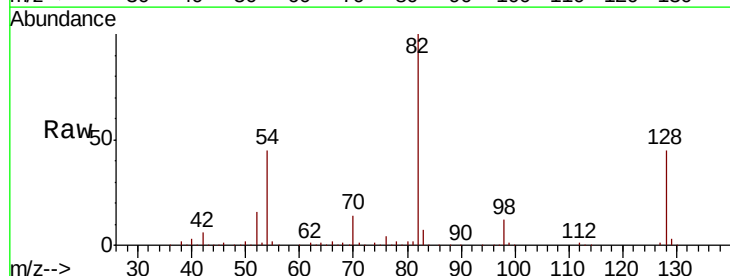

Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF1

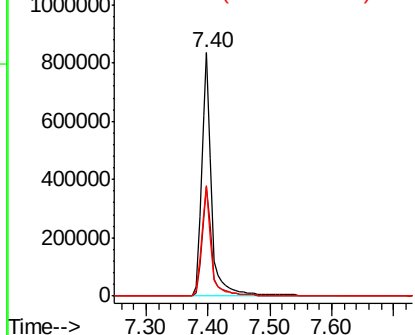



#25

Isophorone

Concen: 51.000 ng

RT: 7.40 min Scan# 903

Delta R.T. -0.28 min

Lab File: BF116246.D

Acq: 13 Aug 2019 22:35

Instrument :

BNA_F

ClientSampleId :

1S-K-(0-1)-COMP


Tgt Ion: 82 Resp: 966170

Ion Ratio Lower Upper

82 100

95 0.0 5.4 8.0#




138 0.0 14.5 21.7#

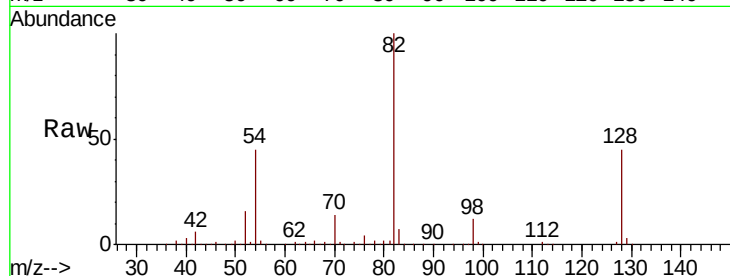

Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 95.00 (94.70 to 95.70): BF1

Ion 138.00 (137.70 to 138.70): BF1

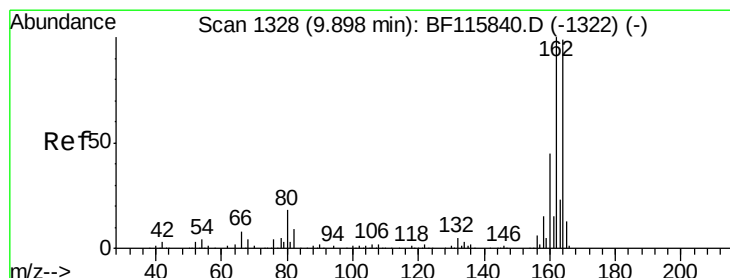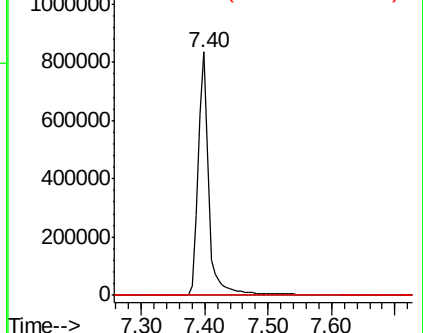

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.87 min Scan# 1323

Delta R.T. -0.02 min

Lab File: BF116246.D

Acq: 13 Aug 2019 22:35


Tgt Ion: 164 Resp: 315697

Ion Ratio Lower Upper

164 100

162 101.6 82.6 124.0



160 45.4 37.6 56.4

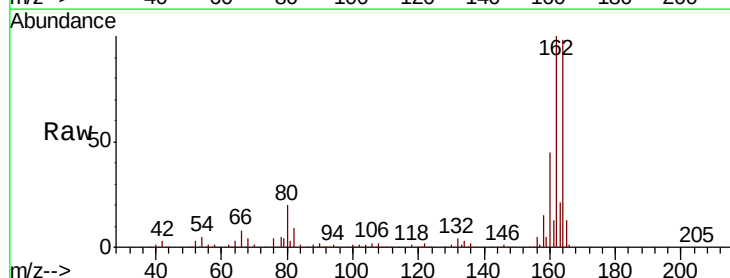


Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

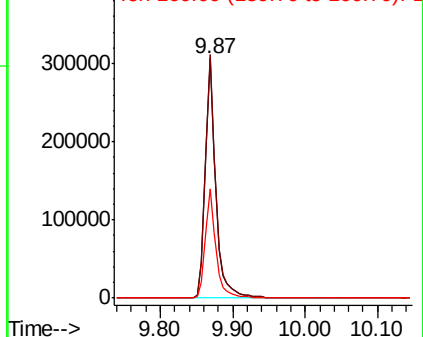


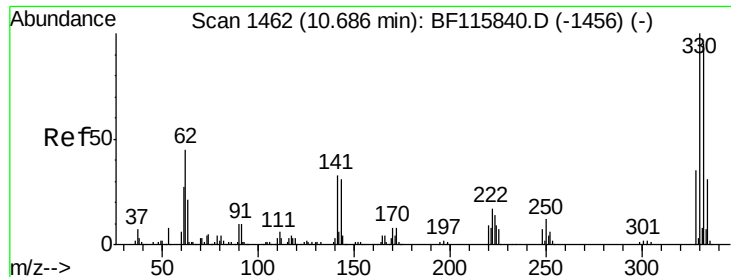




#42
 2,4,6-Tribromophenol
 Concen: 145.401 ng
 RT: 10.66 min Scan# 1458
 Delta R.T. -0.01 min
 Lab File: BF116246.D
 Acq: 13 Aug 2019 22:35

Instrument :
 BNA_F
 ClientSampleId :
 1S-K-(0-1)-COMP

Tgt Ion:330 Resp: 445040
 Ion Ratio Lower Upper
 330 100
 332 95.2 76.8 115.2
 141 33.3 26.3 39.5

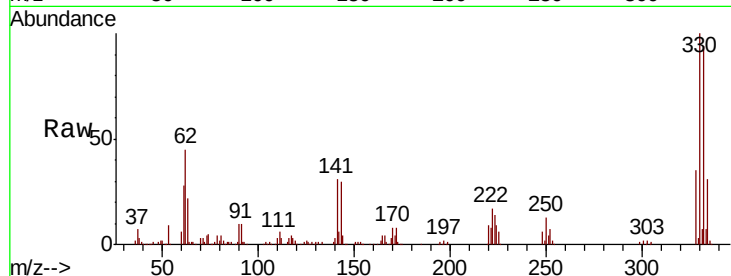


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

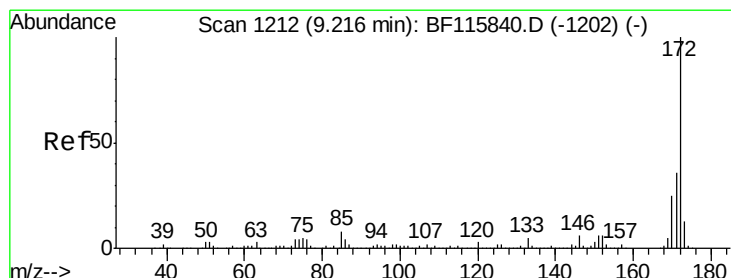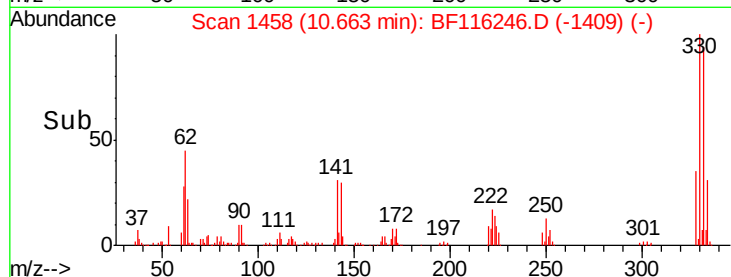
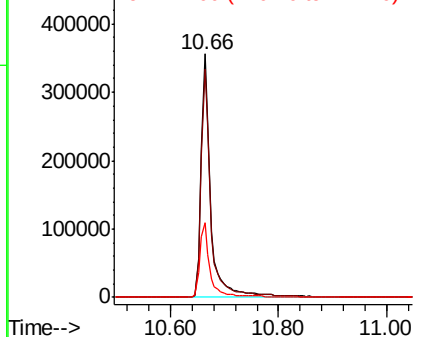



#45
 2-Fluorobiphenyl
 Concen: 95.265 ng
 RT: 9.19 min Scan# 1208
 Delta R.T. -0.01 min
 Lab File: BF116246.D
 Acq: 13 Aug 2019 22:35

Tgt Ion:172 Resp: 1605651
 Ion Ratio Lower Upper
 172 100
 171 35.9 29.6 44.4
 170 24.9 20.1 30.1

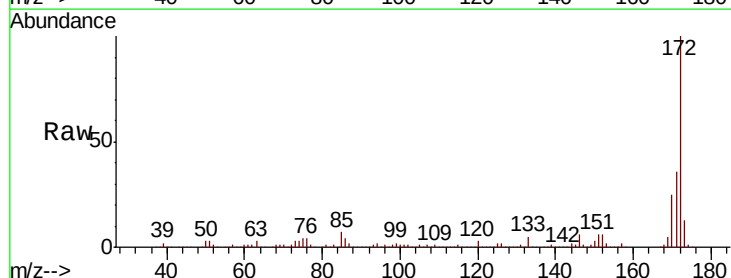

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



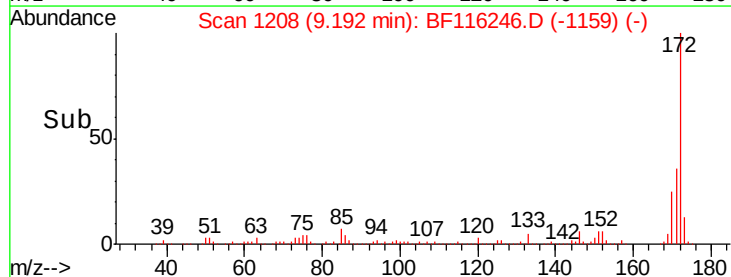
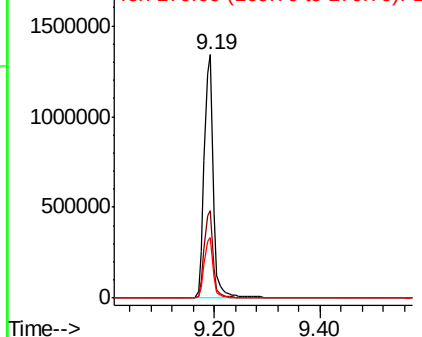


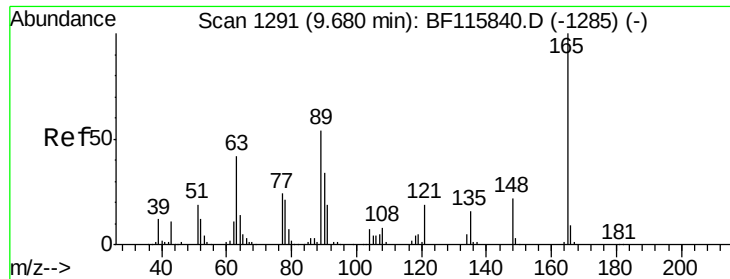

#51
 2,6-Dinitrotoluene
 Concen: 8.520 ng
 RT: 9.87 min Scan# 1323
 Delta R.T. 0.19 min
 Lab File: BF116246.D
 Acq: 13 Aug 2019 22:35




Instrument :
 BNA_F
 ClientSampleId :
 1S-K-(0-1)-COMP


Tgt Ion	Ratio	Lower	Upper
165	100		
63	1.0	38.2	57.2#
89	1.2	42.9	64.3#

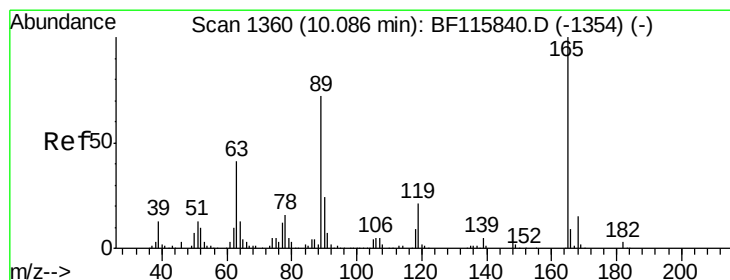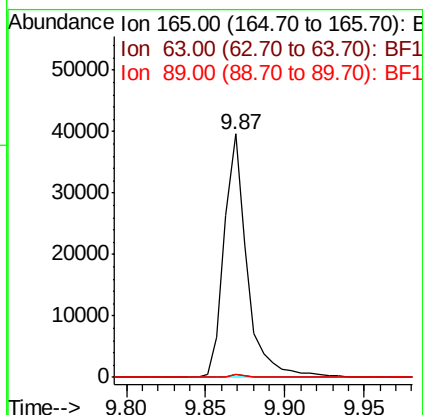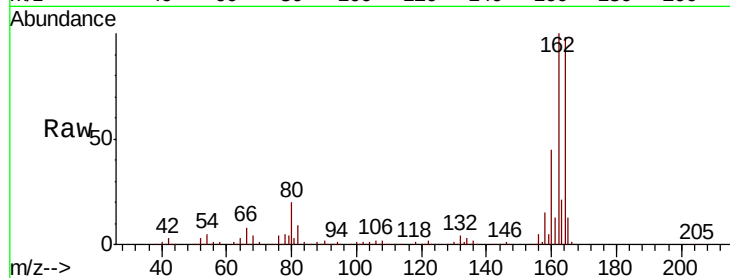

#57
 2,4-Dinitrotoluene
 Concen: 6.400 ng
 RT: 9.87 min Scan# 1323
 Delta R.T. -0.21 min
 Lab File: BF116246.D
 Acq: 13 Aug 2019 22:35

Tgt Ion	Ratio	Lower	Upper
165	100		
63	1.0	39.6	59.4#
89	1.2	62.2	93.2#
182	0.0	2.1	3.1#

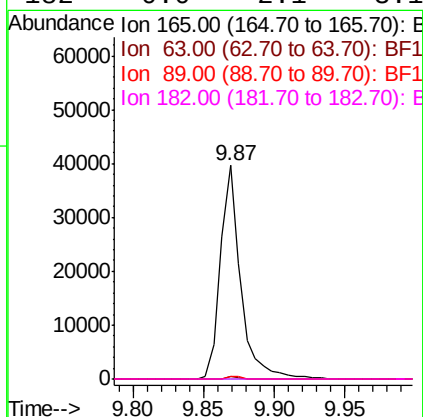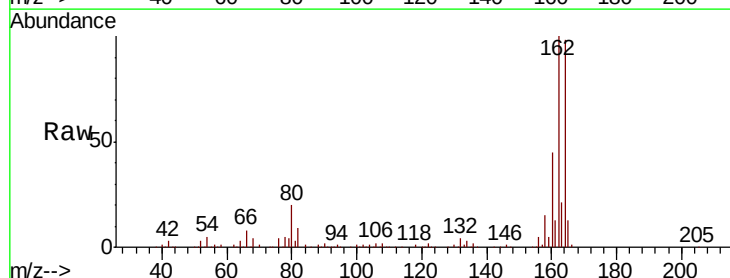

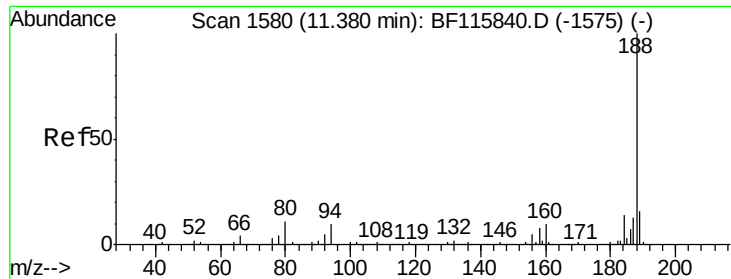

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.36 min Scan# 1576

Delta R.T. -0.01 min

Lab File: BF116246.D

Acq: 13 Aug 2019 22:35

Instrument :

BNA_F

ClientSampleId :

1S-K-(0-1)-COMP


Tgt Ion:188 Resp: 594698

Ion Ratio Lower Upper

188 100

94 9.6 8.1 12.1




80 10.4 8.7 13.1

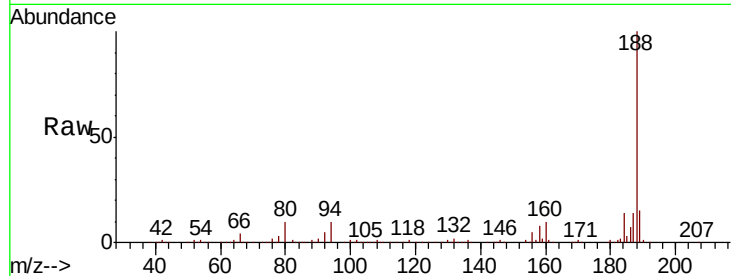

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

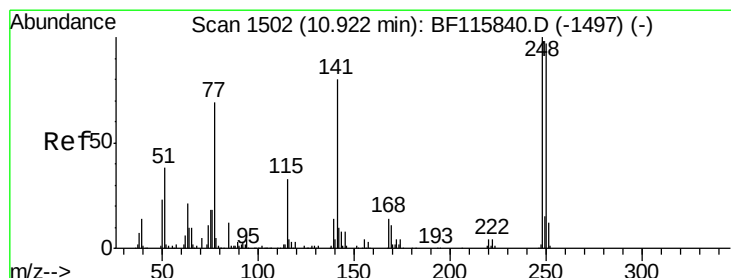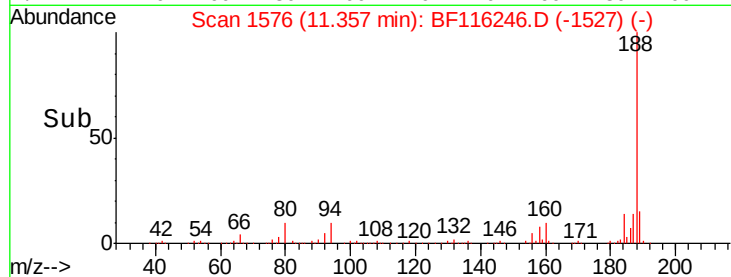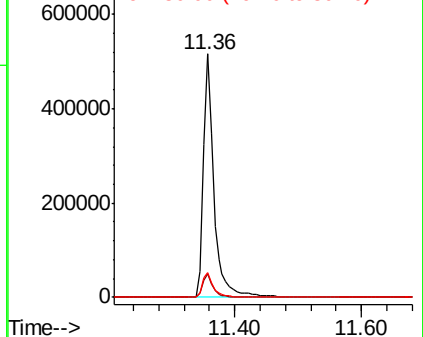

#67

4-Bromophenyl-phenylether

Concen: 4.188 ng

RT: 10.66 min Scan# 1458

Delta R.T. -0.25 min

Lab File: BF116246.D

Acq: 13 Aug 2019 22:35


Tgt Ion:248 Resp: 26663

Ion Ratio Lower Upper

248 100

250 205.4 77.4 116.2#



141 507.2 56.8 85.2#

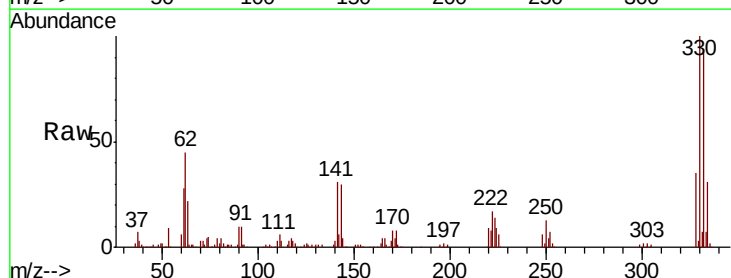


Abundance Ion 248.00 (247.70 to 248.70): E

Ion 250.00 (249.70 to 250.70): E

Ion 141.00 (140.70 to 141.70): E



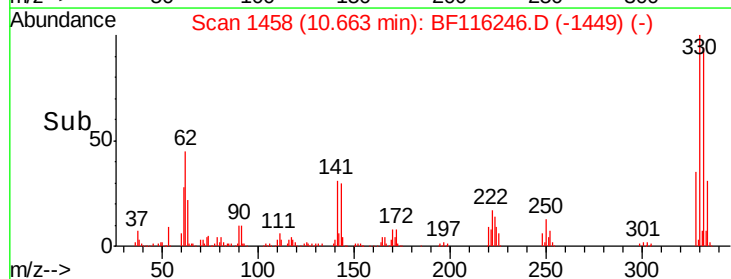
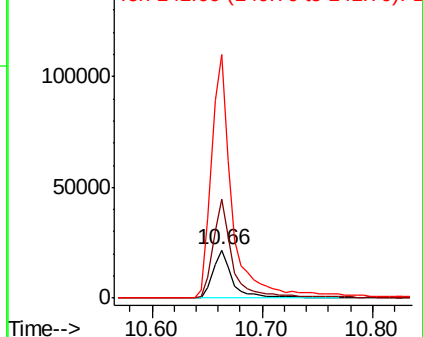




#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.00 min Scan# 2025
Delta R.T. -0.01 min
Lab File: BF116246.D
Acq: 13 Aug 2019 22:35




Instrument :
BNA_F
ClientSampleId :
1S-K-(0-1)-COMP




Tgt Ion:240 Resp: 459322
Ion Ratio Lower Upper
240 100
120 12.7 10.7 16.1
236 26.9 22.2 33.2

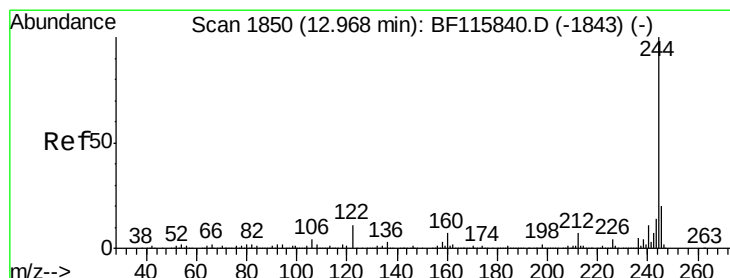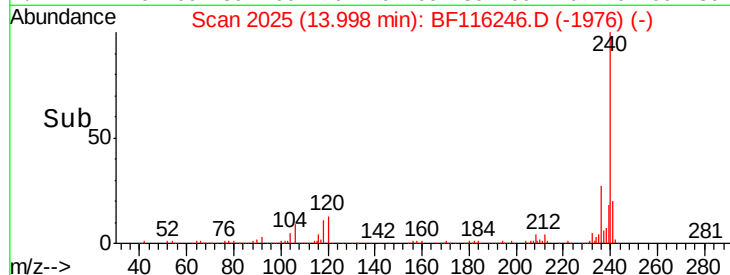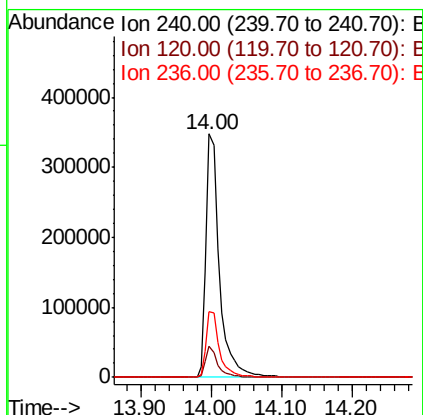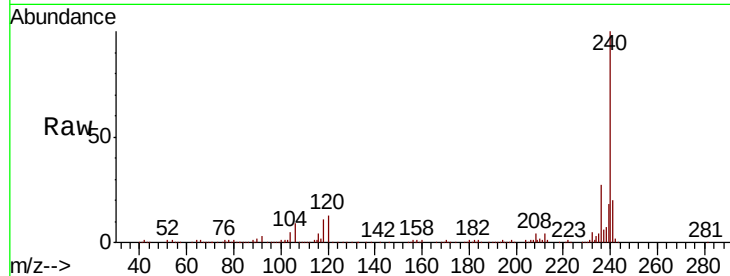

#79
Terphenyl-d14
Concen: 89.252 ng
RT: 12.95 min Scan# 1846
Delta R.T. -0.01 min
Lab File: BF116246.D
Acq: 13 Aug 2019 22:35

Tgt Ion:244 Resp: 1945522
Ion Ratio Lower Upper
244 100
212 7.0 5.8 8.8
122 10.3 9.0 13.4

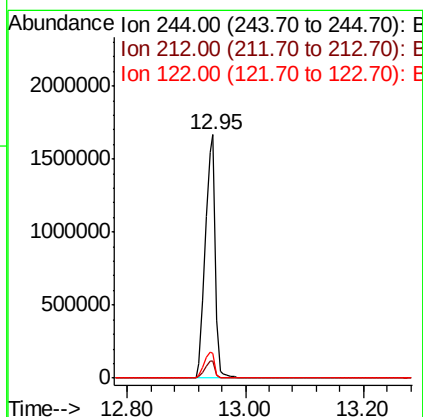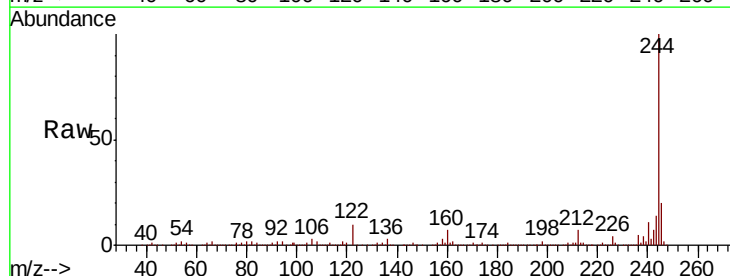

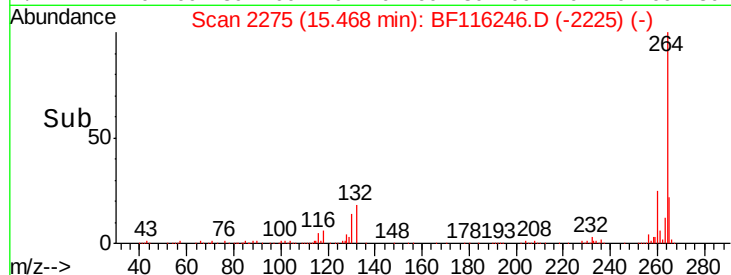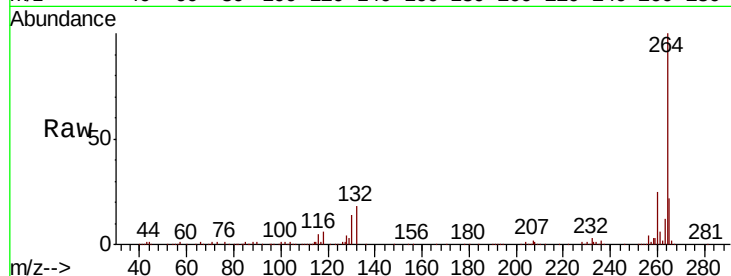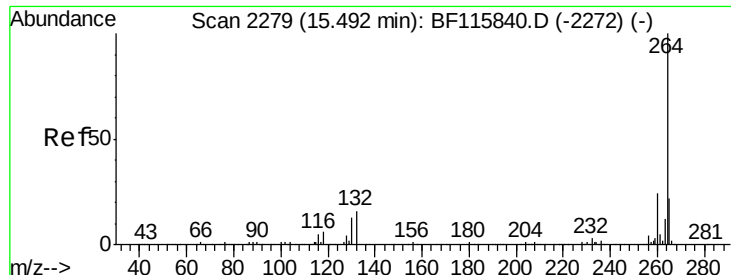

#87
Perylene-d12
Concen: 20.000 ng
RT: 15.47 min Scan# 2275
Delta R.T. -0.01 min
Lab File: BF116246.D
Acq: 13 Aug 2019 22:35

Instrument :
BNA_F
ClientSampleId :
1S-K-(0-1)-COMP

Tgt Ion:	264	Resp:	392546
Ion	Ratio	Lower	Upper
264	100		
260	24.9	19.7	29.5
265	22.4	17.4	26.0

