

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF081319\
 Data File : BF116258.D
 Acq On : 14 Aug 2019 3:58
 Operator : HP/JU
 Sample : K4088-01 5X
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CL-01-081219

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF073019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.893	302	307	314	rBV	13153	27115	2.08%	0.211%
2	5.469	572	575	610	rBV	208691	533537	40.86%	4.145%
3	6.481	744	747	766	rBV	254271	544557	41.71%	4.231%
4	6.610	766	769	777	rVV	558111	603821	46.25%	4.691%
5	6.834	803	807	817	rBV	900740	854196	65.42%	6.636%
6	6.986	830	833	846	rBV	455899	520272	39.85%	4.042%
7	7.404	901	904	926	rBV	180530	363941	27.87%	2.827%
8	8.116	1021	1025	1050	rBV	910225	1146664	87.82%	8.908%
9	9.186	1204	1207	1219	rBV	672452	770034	58.98%	5.982%
10	9.304	1225	1227	1238	rVB4	9010	17190	1.32%	0.134%
11	9.592	1270	1276	1284	rBV	39184	56766	4.35%	0.441%
12	9.739	1297	1301	1306	rBV	10119	13930	1.07%	0.108%
13	9.869	1319	1323	1341	rBV	1377658	1291167	98.89%	10.031%
14	10.669	1455	1459	1469	rBV	234916	354779	27.17%	2.756%
15	10.780	1473	1478	1484	rVB6	12083	21366	1.64%	0.166%
16	11.357	1572	1576	1587	rBV2	1084758	1305689	100.00%	10.144%
17	11.439	1587	1590	1599	rVB	28889	54690	4.19%	0.425%
18	11.863	1660	1662	1665	rBV	25010	30101	2.31%	0.234%
19	11.898	1665	1668	1673	rVB2	35027	43149	3.30%	0.335%
20	11.974	1678	1681	1684	rBV	37570	42530	3.26%	0.330%
21	12.157	1708	1712	1717	rBV2	17018	27064	2.07%	0.210%
22	12.421	1752	1757	1758	rBV2	38044	54346	4.16%	0.422%
23	12.445	1758	1761	1764	rVV3	55566	61595	4.72%	0.479%
24	12.510	1767	1772	1774	rBV3	16048	21714	1.66%	0.169%
25	12.574	1780	1783	1788	rBV	373291	359394	27.53%	2.792%
26	12.727	1806	1809	1811	rBV	21760	22631	1.73%	0.176%
27	12.804	1816	1822	1828	rVV	297482	378235	28.97%	2.938%
28	12.857	1828	1831	1835	rVB	20305	23358	1.79%	0.181%
29	12.933	1840	1844	1855	rVV	712150	687704	52.67%	5.343%
30	13.027	1855	1860	1865	rVB3	21508	40228	3.08%	0.313%
31	13.110	1871	1874	1876	rBV3	21887	28074	2.15%	0.218%
32	13.133	1876	1878	1881	rVB	22528	24628	1.89%	0.191%
33	13.239	1893	1896	1900	rBV2	26557	28957	2.22%	0.225%
34	13.333	1909	1912	1914	rBV	19036	17660	1.35%	0.137%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF081319\
Data File : BF116258.D
Acq On : 14 Aug 2019 3:58
Operator : HP/JU
Sample : K4088-01 5X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-01-081219

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF073019.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	13.363	1915	1917	1927	rVB3	21267	37883	2.90%	0.294%
36	13.657	1965	1967	1973	rVB	23711	30931	2.37%	0.240%
37	13.762	1982	1985	1986	rBV2	27522	32171	2.46%	0.250%
38	13.810	1990	1993	1994	rBV	23448	20349	1.56%	0.158%
39	13.998	2020	2025	2029	rBV2	876022	1091250	83.58%	8.478%
40	14.392	2090	2092	2096	rBV	25306	28979	2.22%	0.225%
41	15.045	2200	2203	2206	rBV	112473	153889	11.79%	1.196%
42	15.351	2252	2255	2259	rVV	57520	68349	5.23%	0.531%
43	15.409	2262	2265	2269	rVV	93924	124254	9.52%	0.965%
44	15.468	2270	2275	2289	rVB	585820	912996	69.92%	7.093%


Sum of corrected areas: 12872133

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF081319\
Data File : BF116258.D
Acq On : 14 Aug 2019 3:58
Operator : HP/JU
Sample : K4088-01 5X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-01-081219

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF073019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

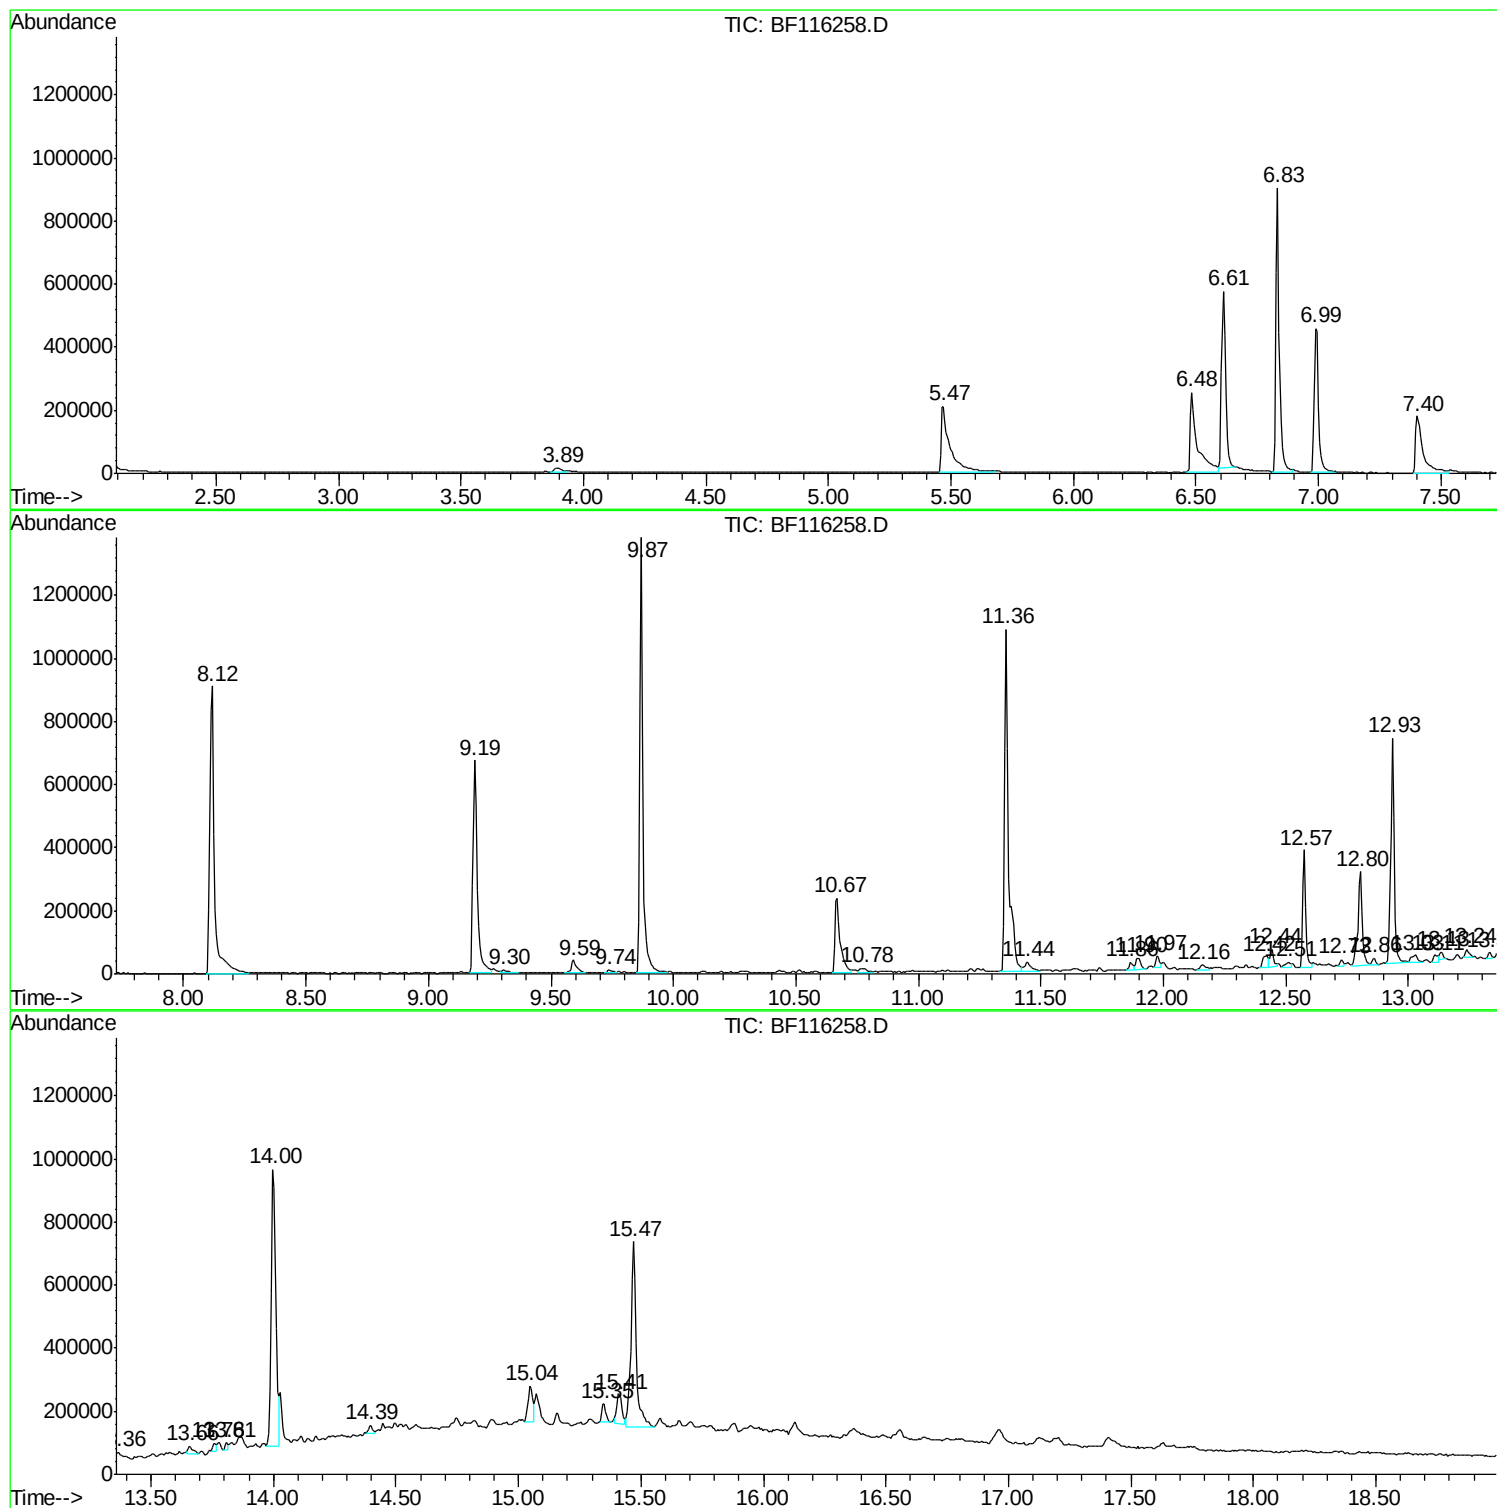

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF081319\
Data File : BF116258.D
Acq On : 14 Aug 2019 3:58
Operator : HP/JU
Sample : K4088-01 5X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-01-081219










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF073019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.61 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.61	14.14 ng	603821	1,4-Dichlorobenzene-d4	6.83

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
2		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
3		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
4		Xenon	132	Xe	007440-63-3	9
5		Imidazole, 4,5-dicyano-1-methyl-	132	C6H4N4	019485-35-9	9

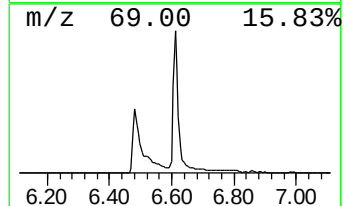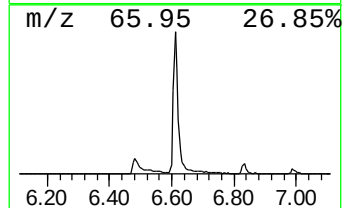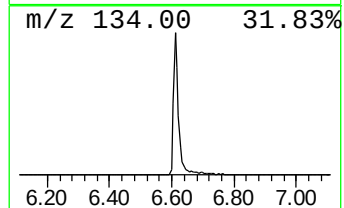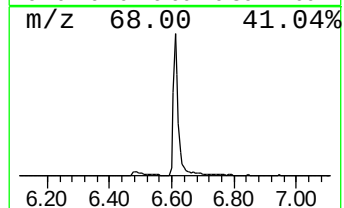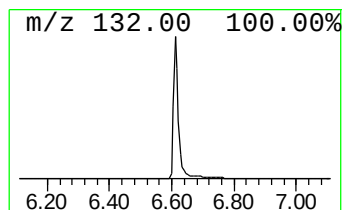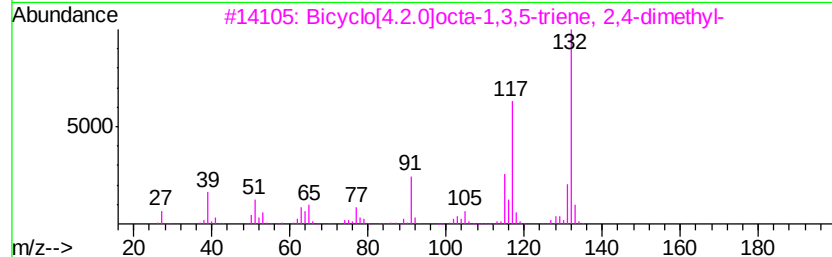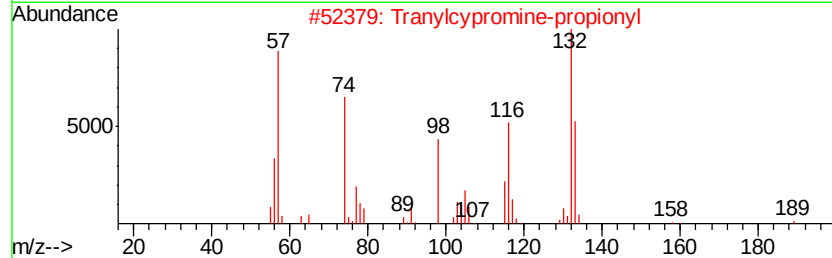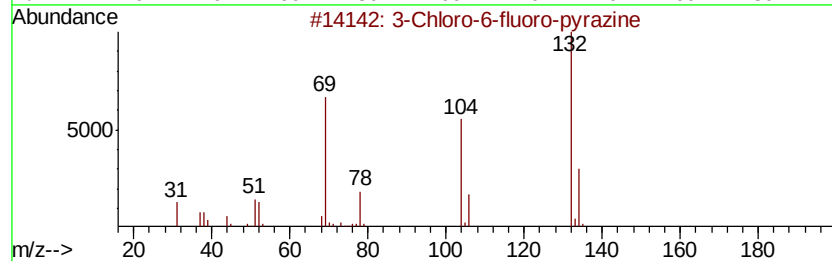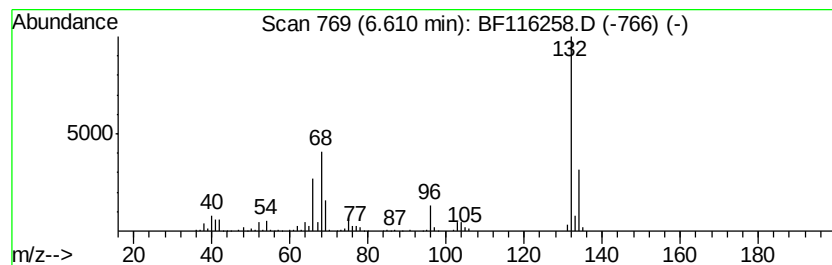

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF081319\
Data File : BF116258.D
Acq On : 14 Aug 2019 3:58
Operator : HP/JU
Sample : K4088-01 5X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-01-081219

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF073019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.61	6.61	14.1	ng	603821	1	6.83	854196	20.0