


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081319\
 Data File : BF116219.D
 Acq On : 13 Aug 2019 9:29
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF073019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 07 11:13:18 2019

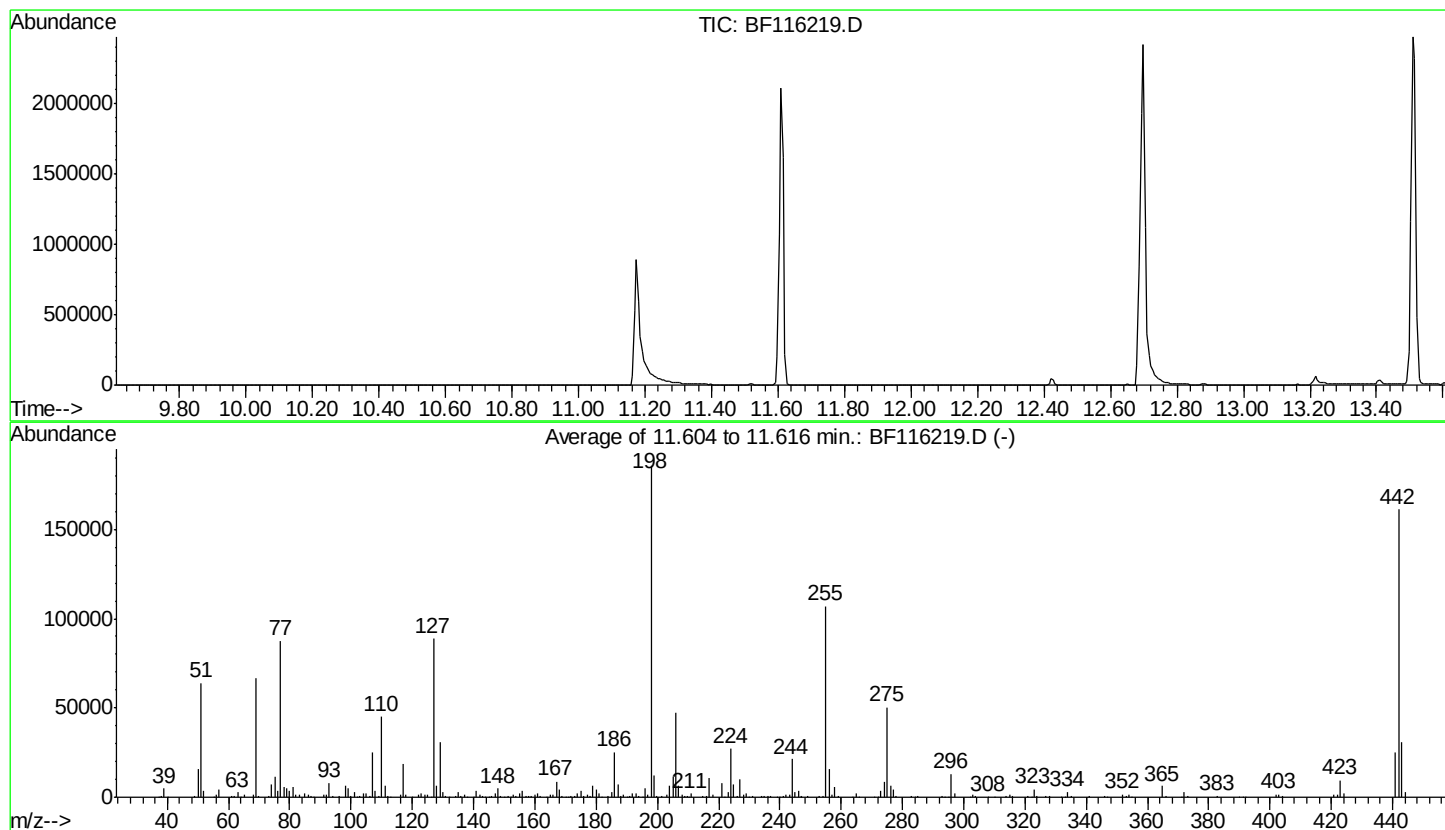

AutoFind: Scans 1618, 1619, 1620; Background Corrected with Scan 1613

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.4	63920	PASS
68	69	0.00	2	1.8	1183	PASS
69	198	0.00	100	35.9	66666	PASS
70	69	0.00	2	0.6	387	PASS
127	198	10	80	47.8	88858	PASS
197	198	0.00	2	0.6	1150	PASS
198	198	100	100	100.0	185720	PASS
199	198	5	9	6.6	12260	PASS
275	198	10	60	27.2	50525	PASS
365	198	1	100	3.5	6426	PASS
441	198	0.01	100	13.7	25395	PASS
442	198	50	100	86.8	161189	PASS
443	442	15	24	19.1	30725	PASS