


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081319\
 Data File : BF116234.D
 Acq On : 13 Aug 2019 16:49
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF073019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 07 11:13:18 2019

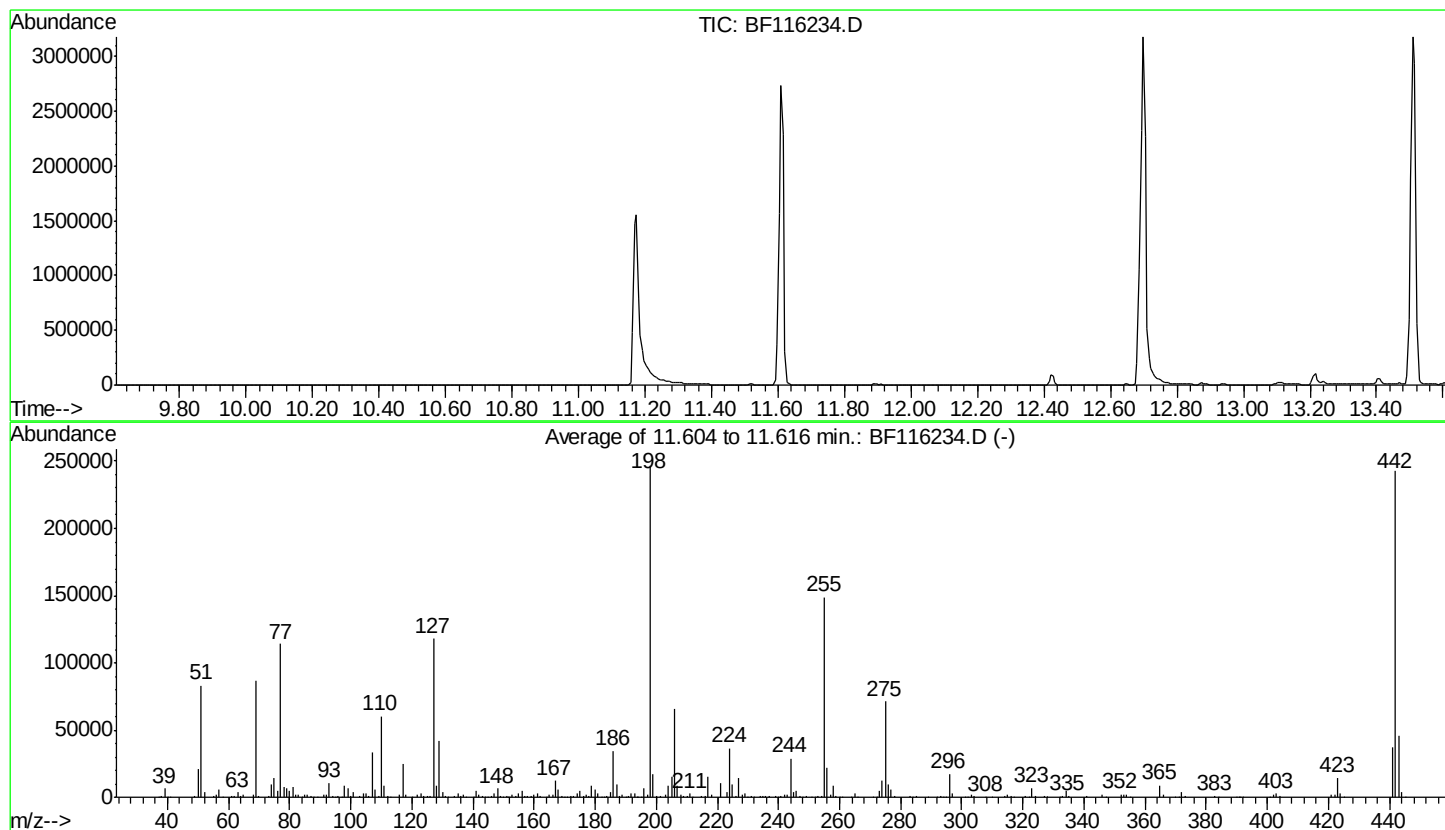

AutoFind: Scans 1618, 1619, 1620; Background Corrected with Scan 1612

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.8	83317	PASS
68	69	0.00	2	1.7	1511	PASS
69	198	0.00	100	35.1	86616	PASS
70	69	0.00	2	0.6	543	PASS
127	198	10	80	47.7	117738	PASS
197	198	0.00	2	0.7	1714	PASS
198	198	100	100	100.0	246677	PASS
199	198	5	9	6.8	16736	PASS
275	198	10	60	28.9	71189	PASS
365	198	1	100	3.6	8898	PASS
441	198	0.01	100	15.2	37409	PASS
442	198	50	100	98.4	242706	PASS
443	442	15	24	19.0	46024	PASS