


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081419\
 Data File : BF116259.D
 Acq On : 14 Aug 2019 10:47
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF073019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 07 11:13:18 2019

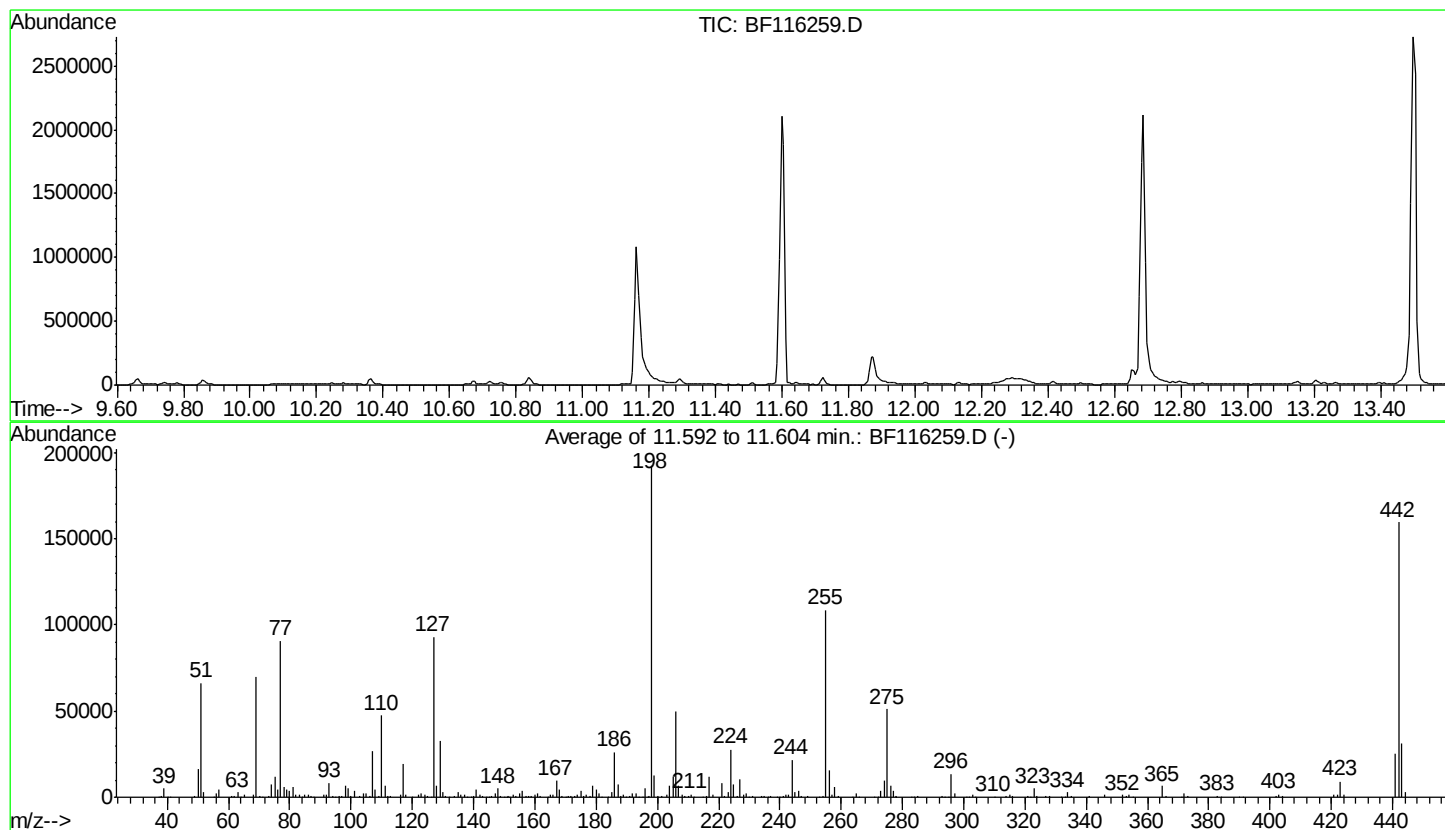

AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1611

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.4	66229	PASS
68	69	0.00	2	1.9	1310	PASS
69	198	0.00	100	36.2	69744	PASS
70	69	0.00	2	1.0	669	PASS
127	198	10	80	48.4	93069	PASS
197	198	0.00	2	0.4	866	PASS
198	198	100	100	100.0	192448	PASS
199	198	5	9	6.7	12828	PASS
275	198	10	60	26.5	51002	PASS
365	198	1	100	3.4	6589	PASS
441	198	0.01	100	13.1	25177	PASS
442	198	50	100	82.8	159402	PASS
443	442	15	24	19.4	30895	PASS