
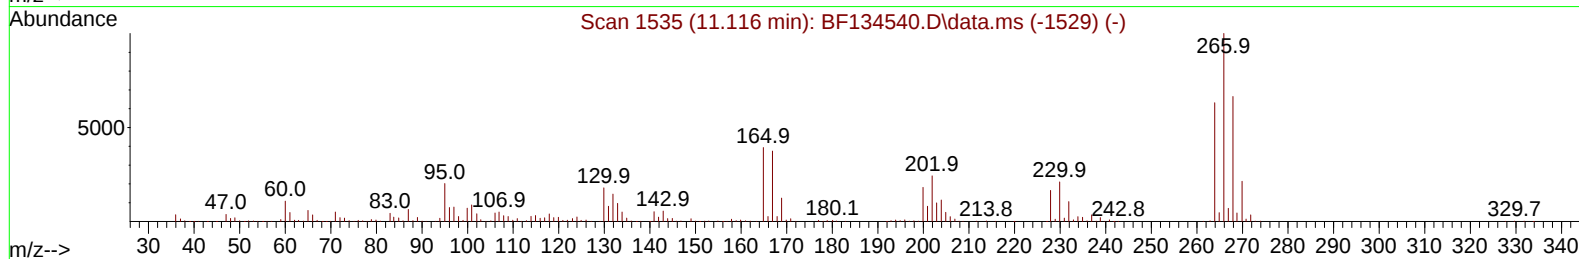
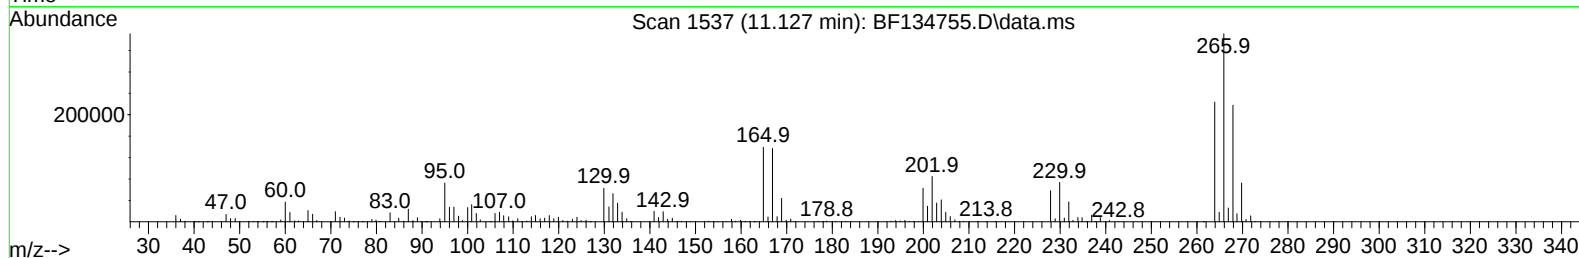


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081423\
Data File : BF134755.D
Acq On : 14 Aug 2023 12:43
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 14 13:03:15 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 04 09:29:15 2023
Response via : Initial Calibration

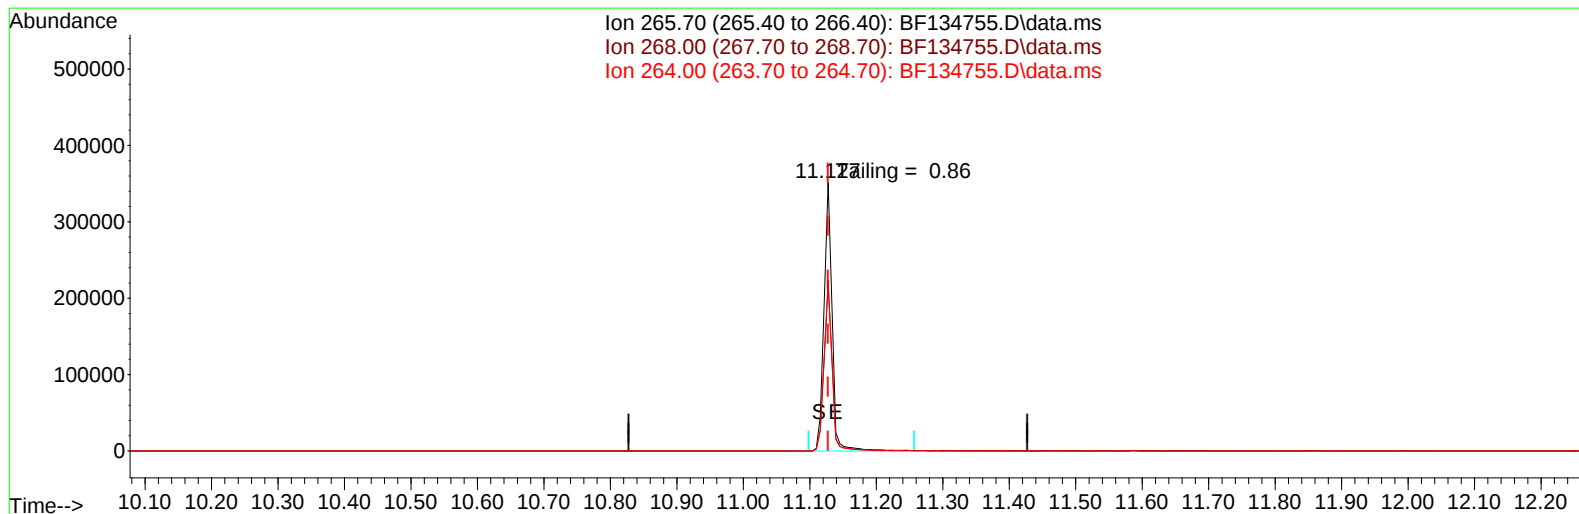

TIC: BF134755.D\data.ms

(70) Pentachlorophenol (C)




11.127min (+ 0.000) 765206.78 ng

response 301227

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.10	62.00
264.00	59.70	63.67
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081423\
Data File : BF134755.D
Acq On : 14 Aug 2023 12:43
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 14 13:03:15 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 04 09:29:15 2023
Response via : Initial Calibration

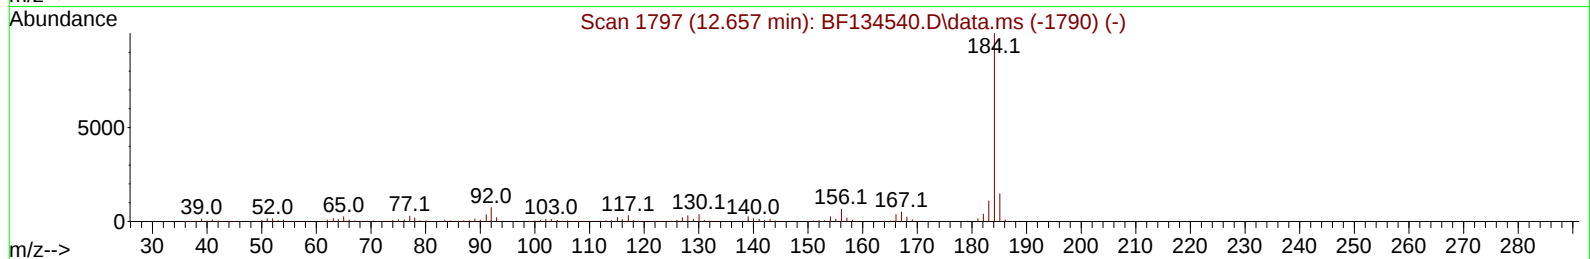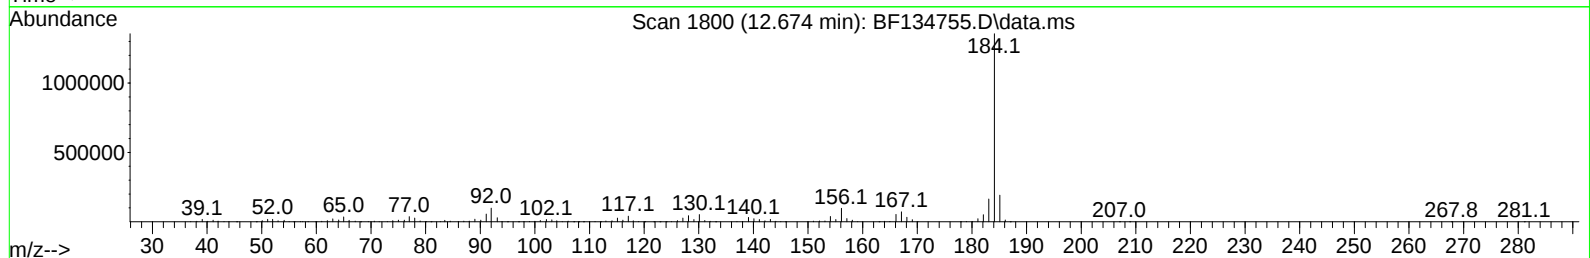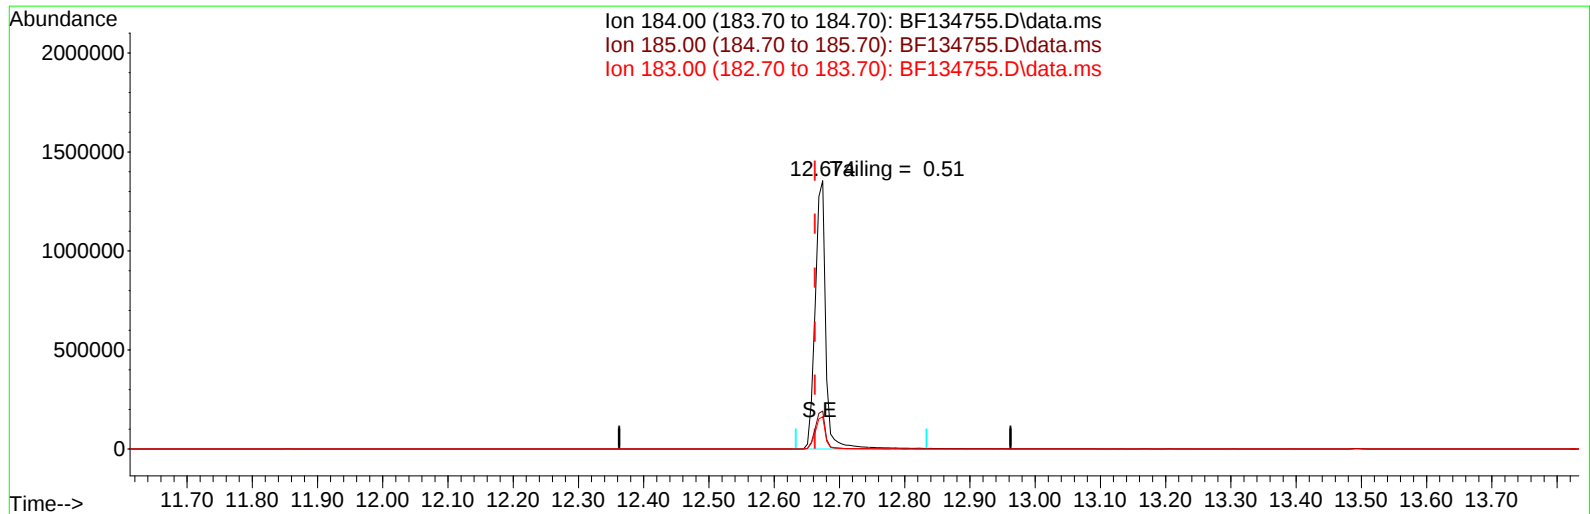

TIC: BF134755.D\data.ms

(77) Benzidine**12.674min (+ 0.012) 459522.28 ng****response 1526214**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.17
183.00	10.80	12.08
0.00	0.00	0.00