
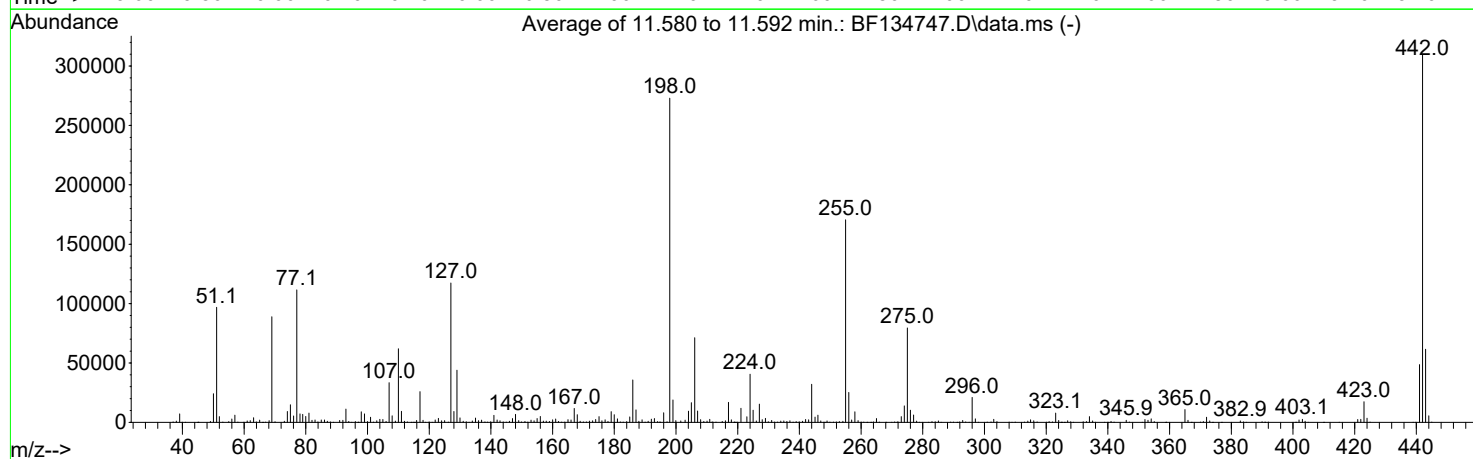


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081423\
 Data File : BF134747.D
 Acq On : 14 Aug 2023 08:14
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 04 09:29:15 2023

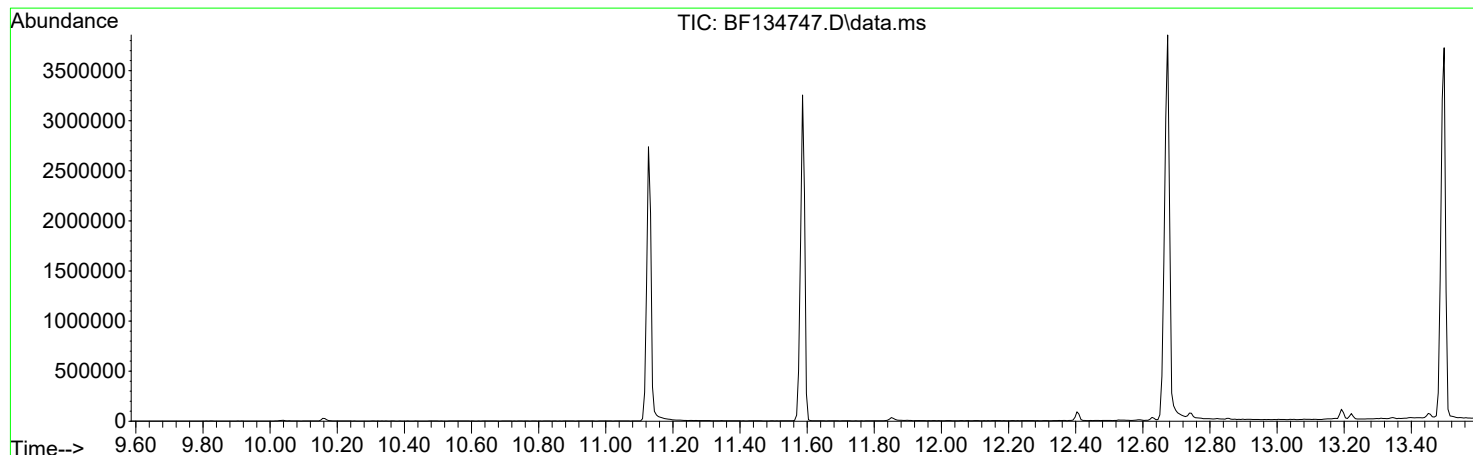




AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.5	96877	PASS
68	69	0.00	2	1.7	1527	PASS
69	198	0.00	100	32.6	88912	PASS
70	69	0.00	2	0.6	551	PASS
127	198	10	80	43.0	117392	PASS
197	198	0.00	2	0.2	554	PASS
198	198	100	100	100.0	272896	PASS
199	198	5	9	6.9	18835	PASS
275	198	10	60	29.1	79453	PASS
365	198	1	100	3.9	10729	PASS
441	198	0.01	100	17.8	48680	PASS
442	442	50	100	100.0	309739	PASS
443	442	15	24	19.9	61640	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081423\
Data File : BF134747.D
Acq On : 14 Aug 2023 08:14
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 14 11:36:36 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 04 09:29:15 2023
Response via : Initial Calibration

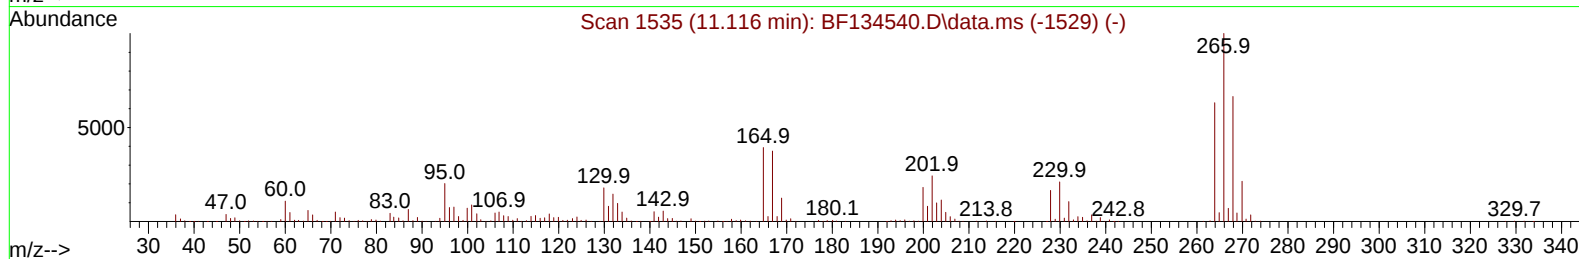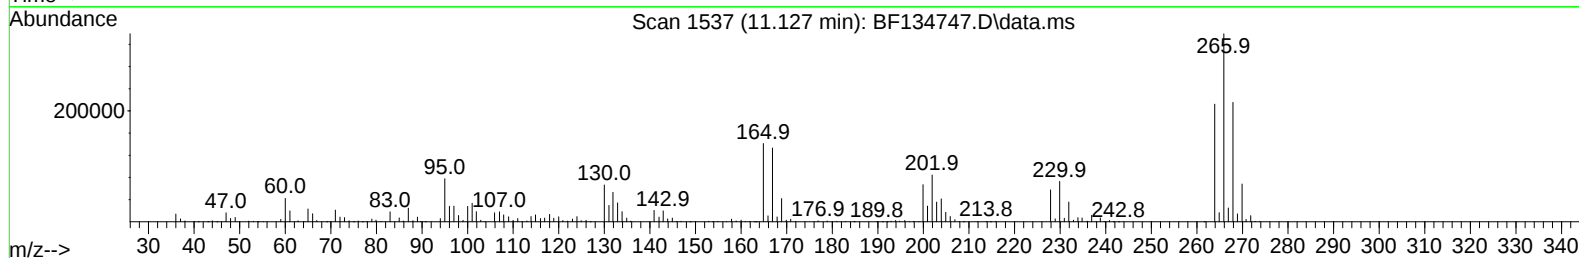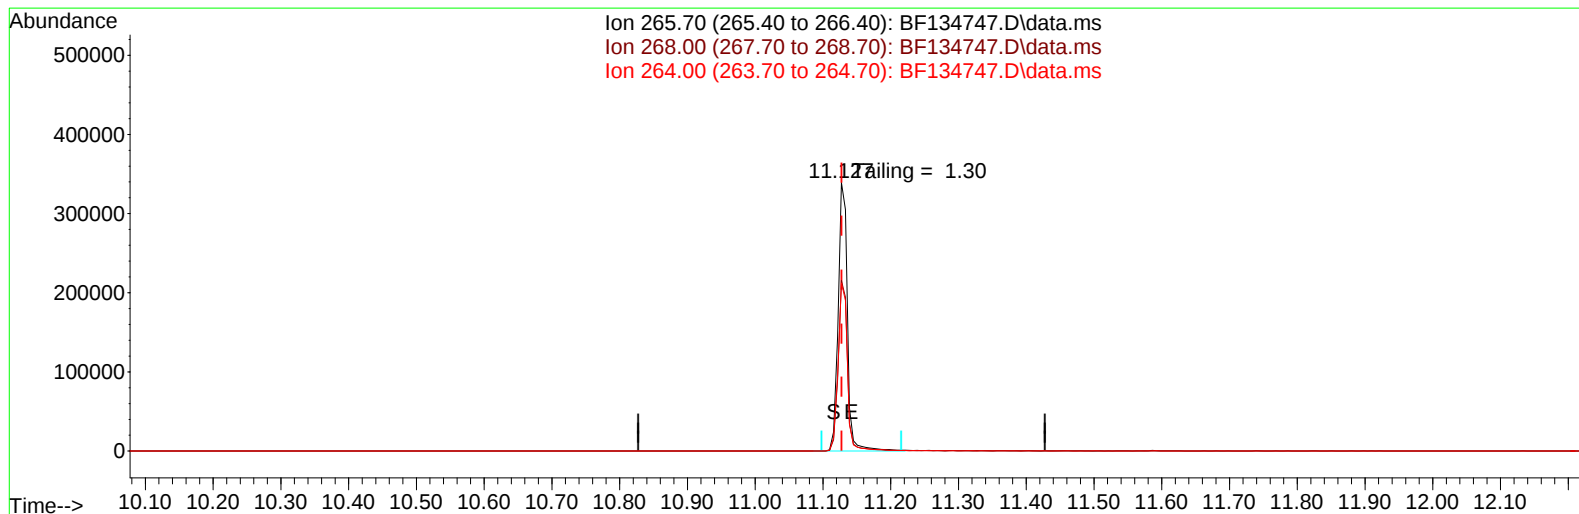

TIC: BF134747.D\data.ms

(70) Pentachlorophenol (C)

11.127min (-0.000) 708172.57 ng




response 324393

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.10	63.48
264.00	59.70	62.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081423\
Data File : BF134747.D
Acq On : 14 Aug 2023 08:14
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 14 11:36:36 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 04 09:29:15 2023
Response via : Initial Calibration

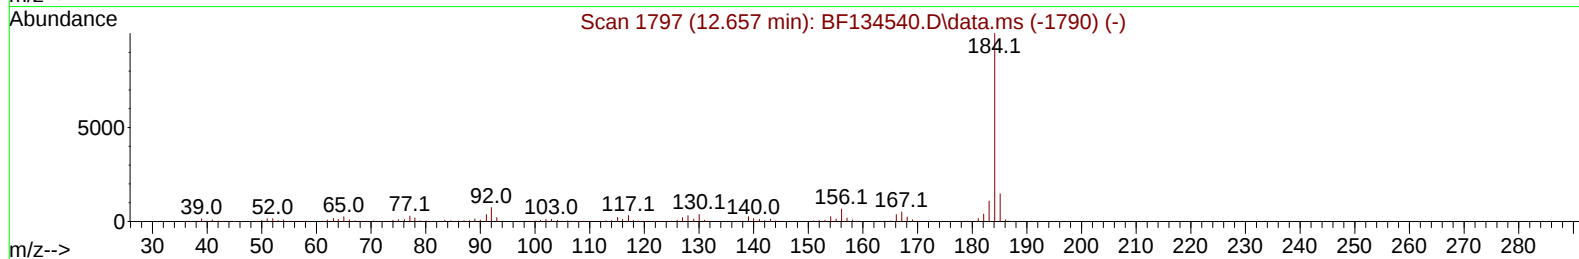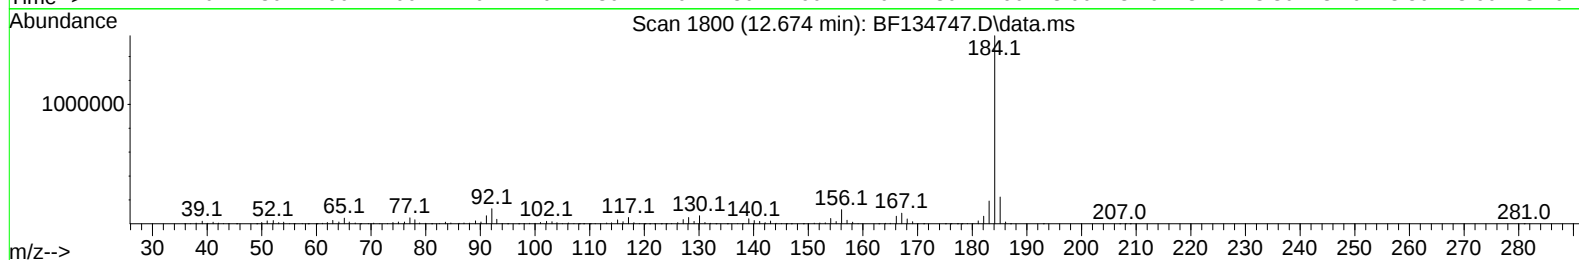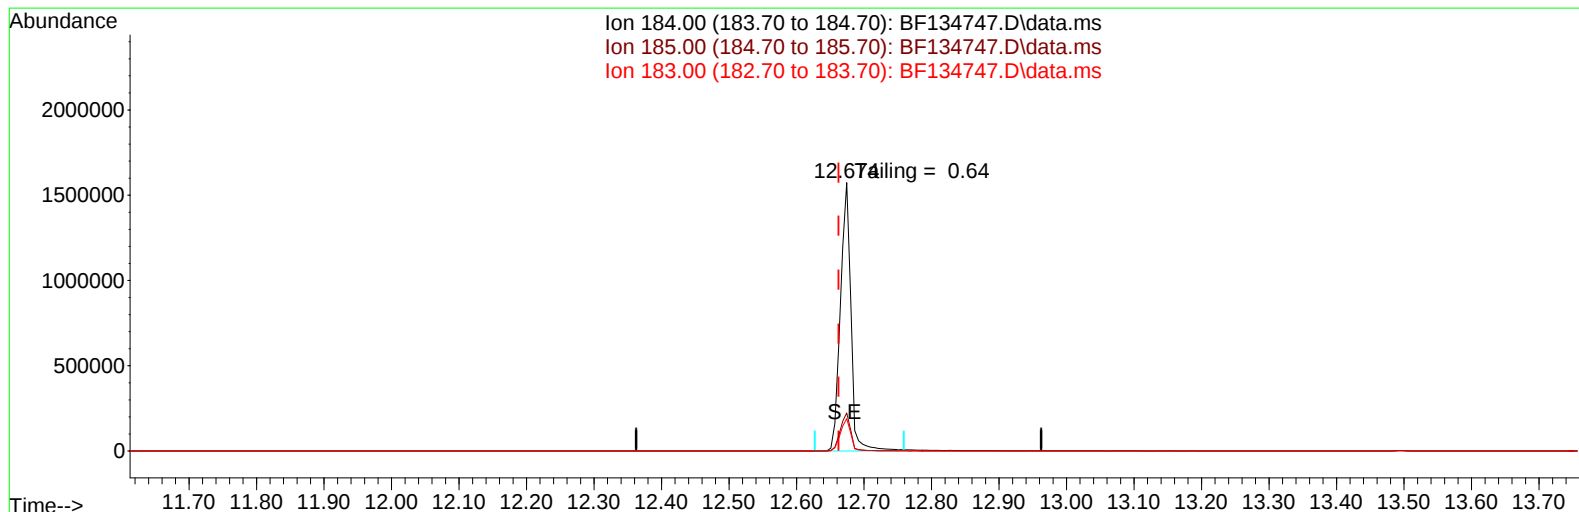

TIC: BF134747.D\data.ms

(77) Benzidine

12.674min (+ 0.012) 7451.77 ng m

response 1704165

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.18
183.00	10.80	12.09
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/14/2023	BNA_F	<u>BF134747.D</u>
Compound Name	Response	Retention Time
DDT	706850	13.498
DDD	23673	13.192
DDE	1497	12.851
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
25170	732020	3.44

Instrument :
BNA_F
ClientSampleId :
DFTPP