
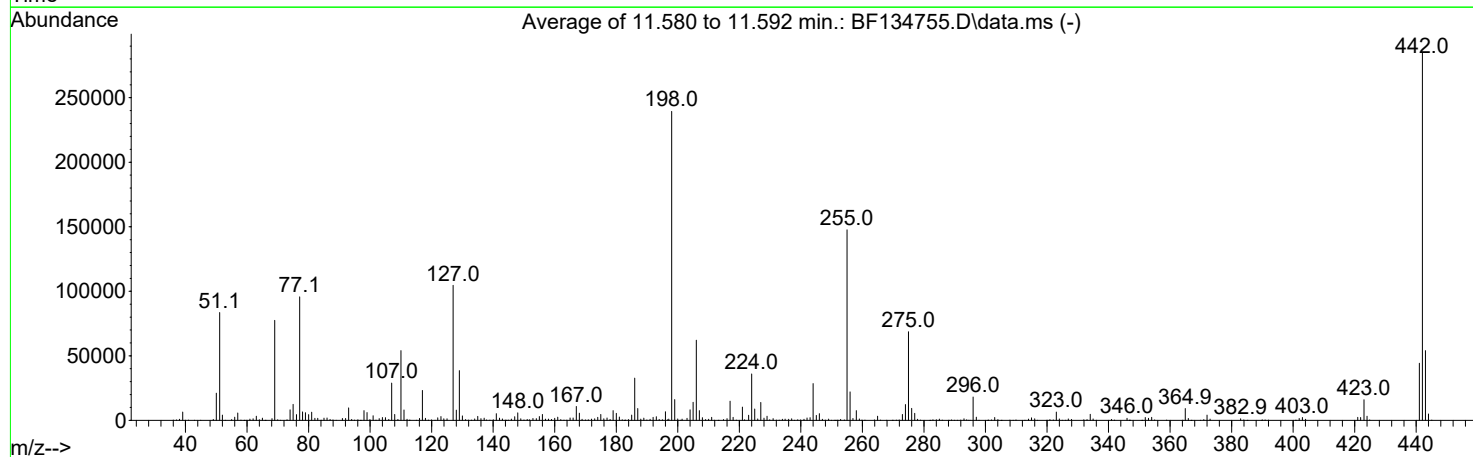


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081423\
Data File : BF134755.D
Acq On : 14 Aug 2023 12:43
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Aug 04 09:29:15 2023

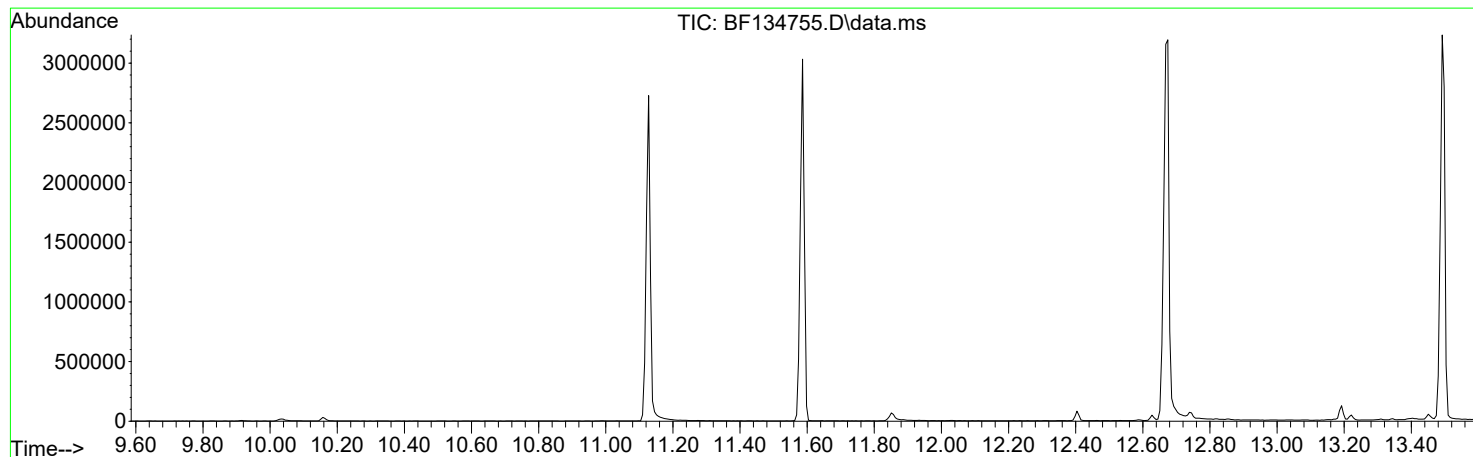




AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.9	83552	PASS
68	69	0.00	2	1.8	1420	PASS
69	198	0.00	100	32.4	77496	PASS
70	69	0.00	2	0.6	494	PASS
127	198	10	80	43.7	104608	PASS
197	198	0.00	2	0.4	1034	PASS
198	198	100	100	100.0	239403	PASS
199	198	5	9	6.7	16089	PASS
275	198	10	60	28.7	68741	PASS
365	198	1	100	3.9	9220	PASS
441	198	0.01	100	18.5	44240	PASS
442	442	50	100	100.0	284992	PASS
443	442	15	24	19.0	54109	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081423\
 Data File : BF134755.D
 Acq On : 14 Aug 2023 12:43
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Aug 14 13:03:15 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 04 09:29:15 2023
 Response via : Initial Calibration

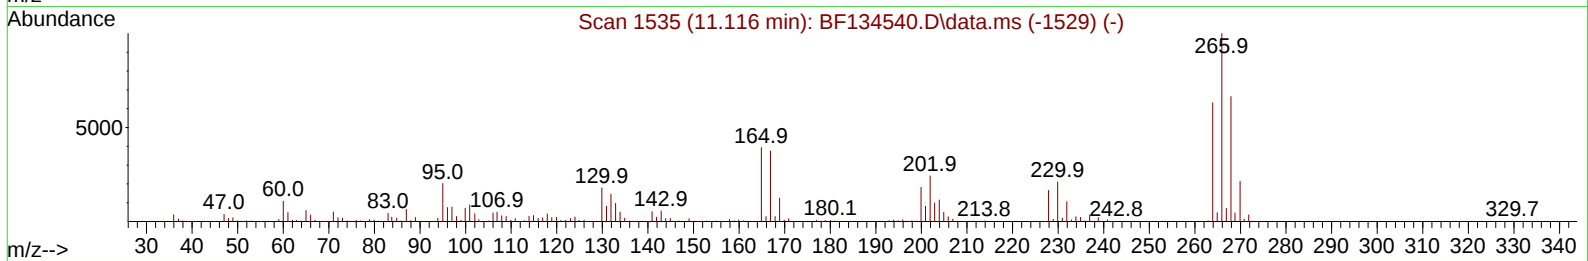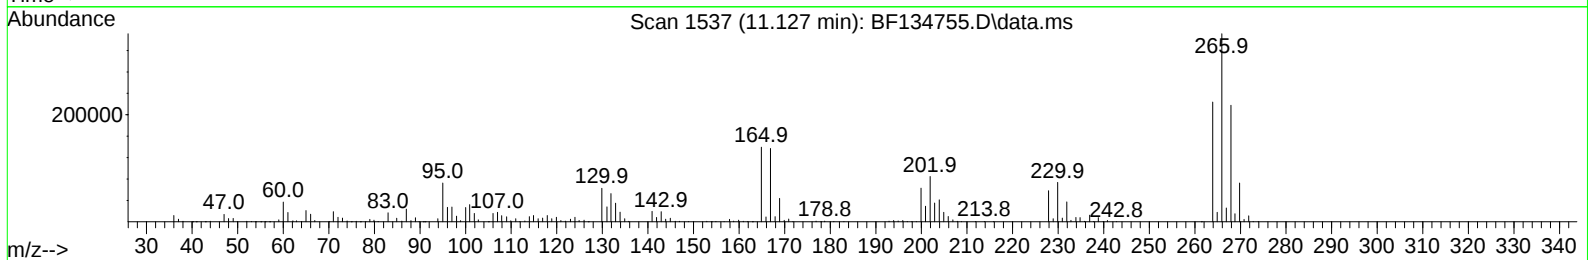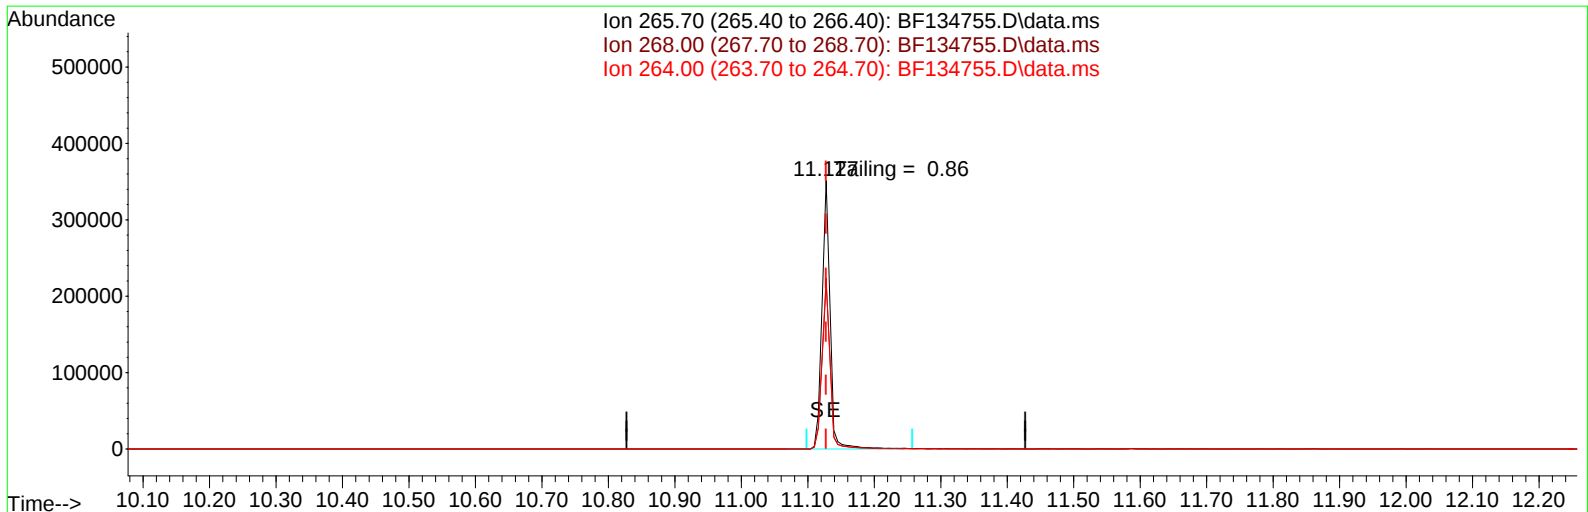

TIC: BF134755.D\data.ms

(70) Pentachlorophenol (C)

11.127min (+ 0.000) 765206.78 ng




response 301227

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.10	62.00
264.00	59.70	63.67
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081423\
Data File : BF134755.D
Acq On : 14 Aug 2023 12:43
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 14 13:03:15 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 04 09:29:15 2023
Response via : Initial Calibration

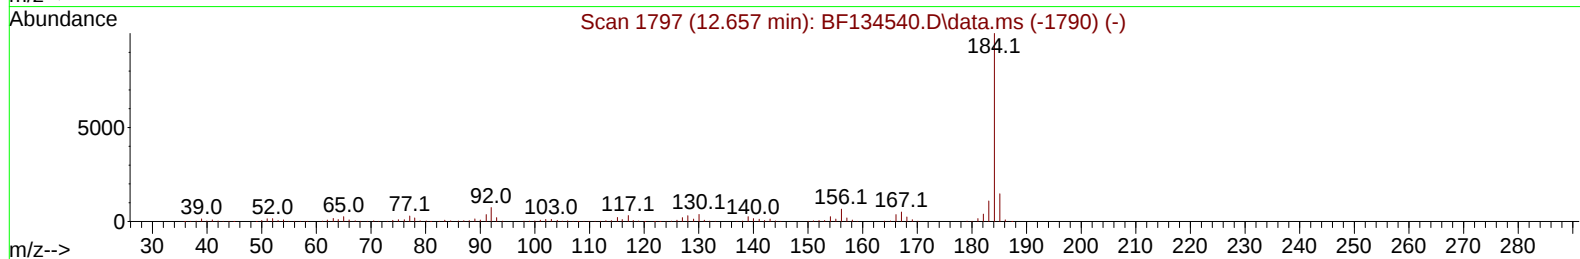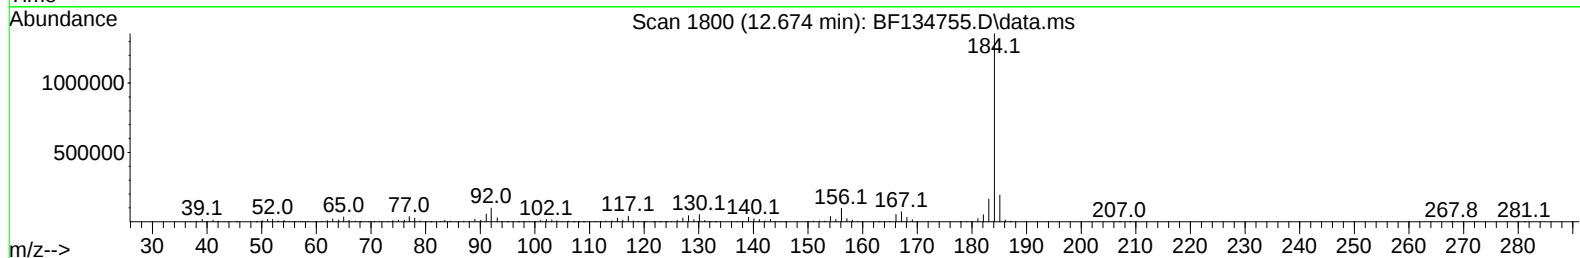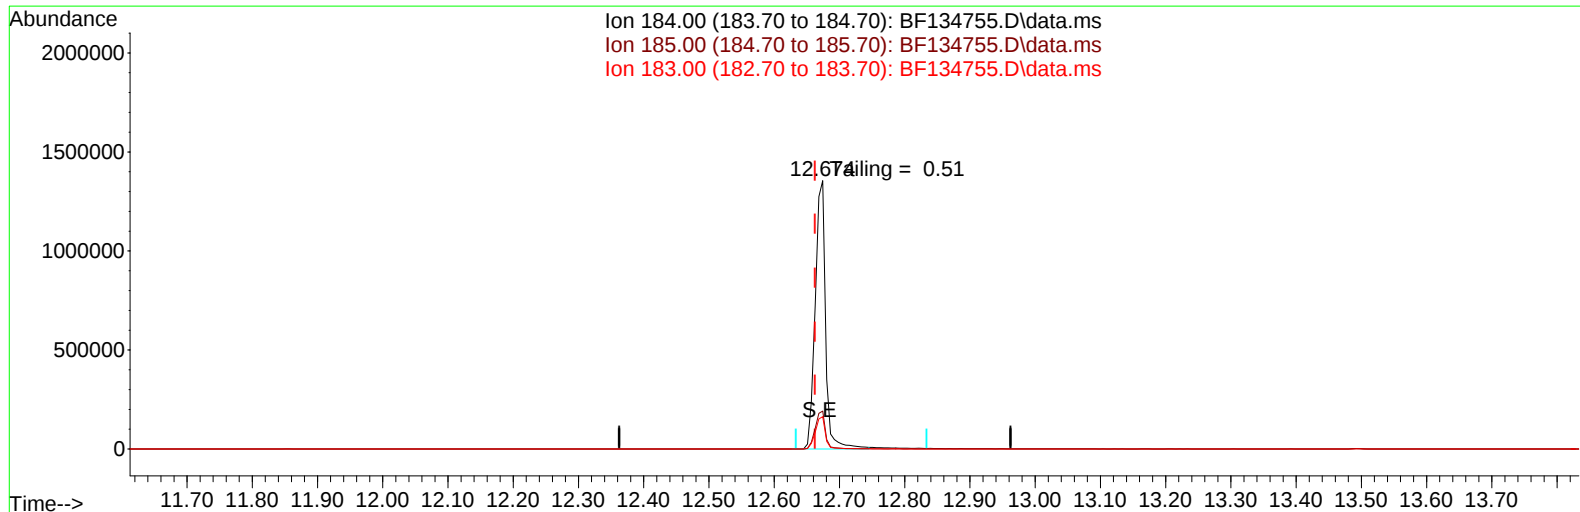

TIC: BF134755.D\data.ms

(77) Benzidine

12.674min (+ 0.012) 459522.28 ng

response 1526214

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.17
183.00	10.80	12.08
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/14/2023	BNA_F	<u>BF134755.D</u>
Compound Name	Response	Retention Time
DDT	621722	13.492
DDD	26389	13.192
DDE	1339	12.851
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
27728	649450	4.27

Instrument :
BNA_F
ClientSampleId :
DFTPP