
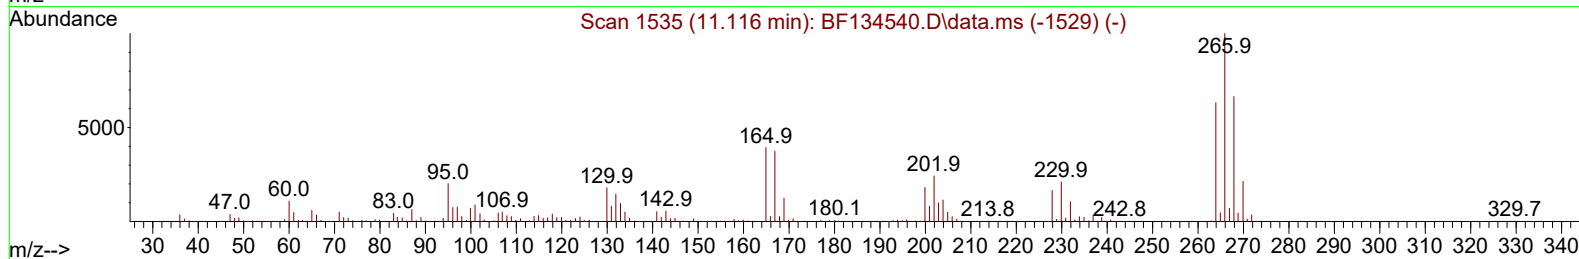
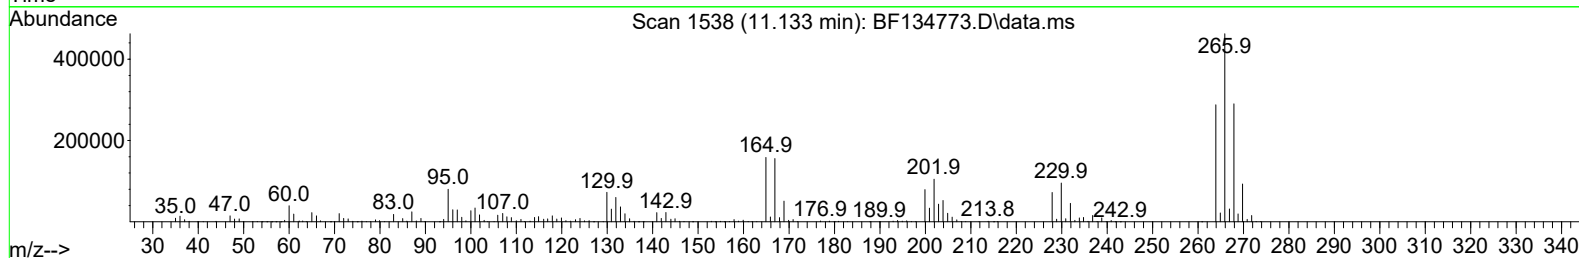


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081523\
Data File : BF134773.D
Acq On : 15 Aug 2023 08:02
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 15 11:03:52 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 04 09:29:15 2023
Response via : Initial Calibration

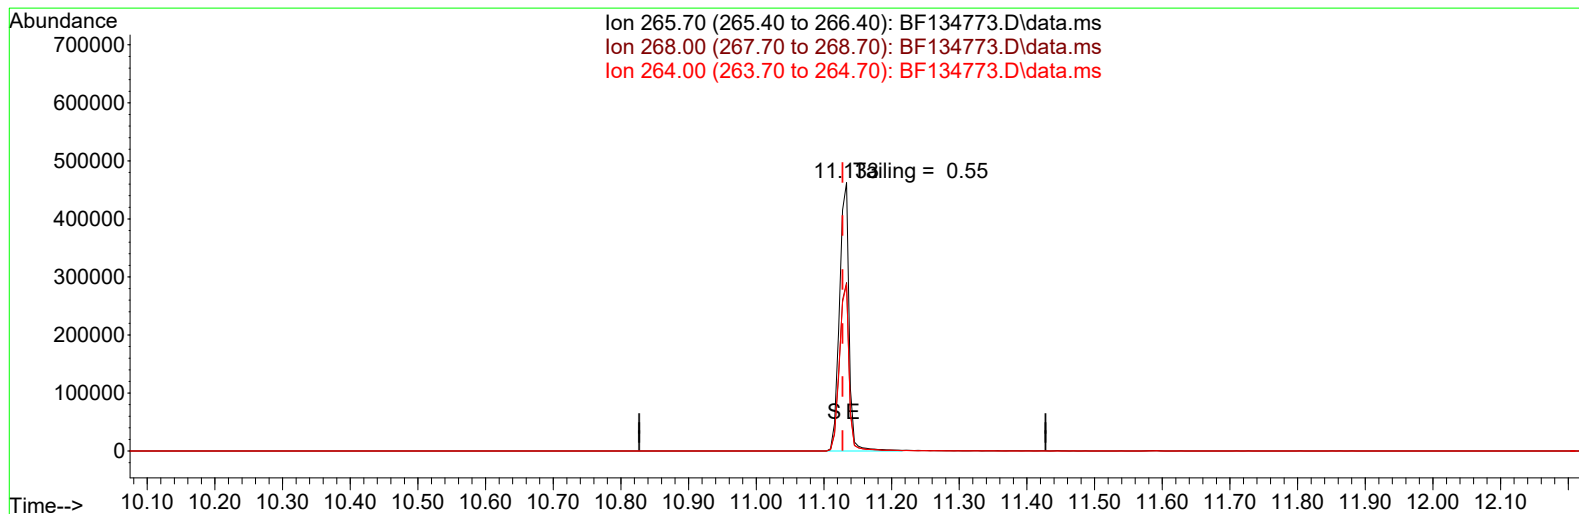

TIC: BF134773.D\data.ms

(70) Pentachlorophenol (C)




11.133min (+ 0.006) 632607.12 ng

response 457307

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.10	62.71
264.00	59.70	62.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081523\
Data File : BF134773.D
Acq On : 15 Aug 2023 08:02
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 15 11:03:52 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 04 09:29:15 2023
Response via : Initial Calibration

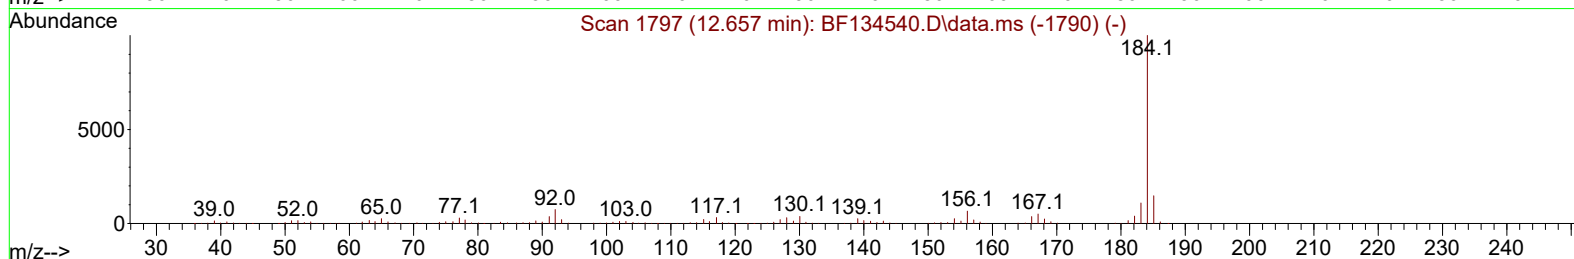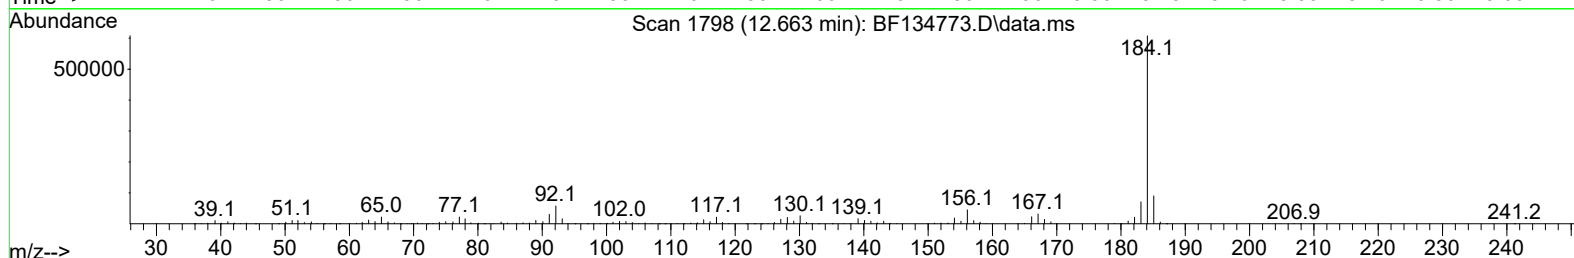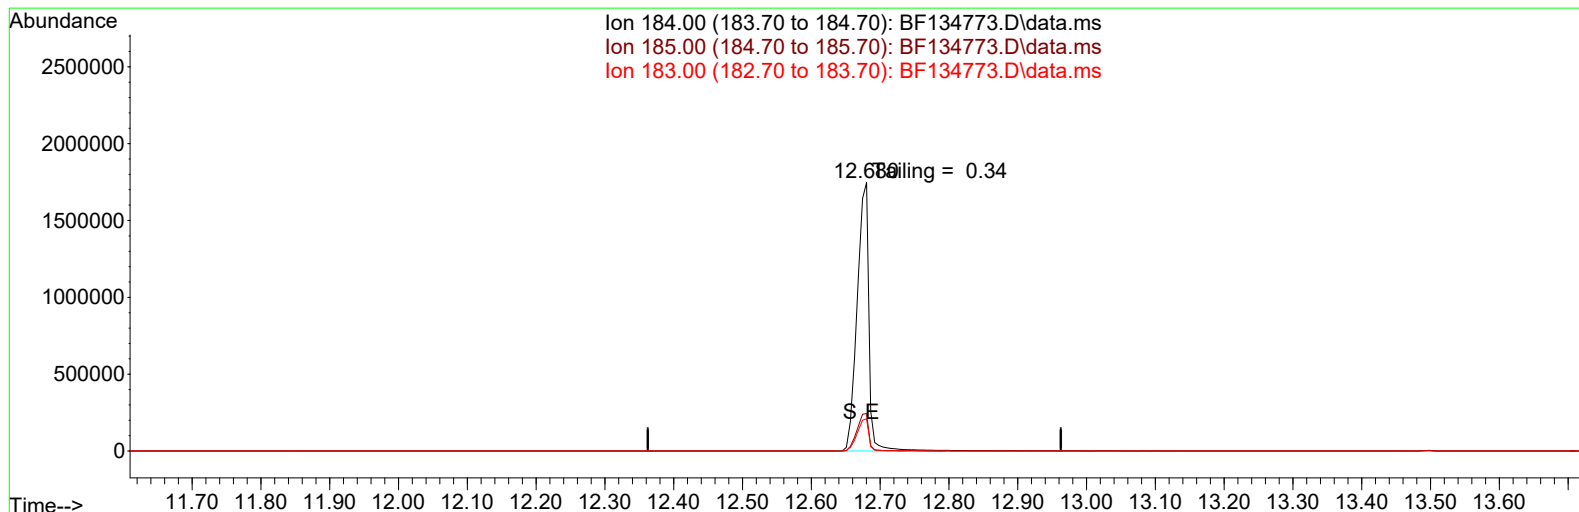

TIC: BF134773.D\data.ms

(77) Benzidine

12.663min (-12.663) 0.00 ng

response 0

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	14.00	0.00#
183.00	10.80	0.00#
0.00	0.00	0.00