

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081523\
 Data File : BF134791.D
 Acq On : 15 Aug 2023 18:51
 Operator : CG\JU
 Sample : 04017-01 10X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 JC-03-081423-A

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF134791.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.416	562	566	576	rBV	211383	195893	15.07%	2.584%
2	6.422	734	737	755	rBV	213007	192562	14.82%	2.540%
3	6.798	797	801	804	rBV	1189442	935641	71.99%	12.344%
4	7.351	892	895	904	rBV	124702	116133	8.94%	1.532%
5	8.075	1014	1018	1022	rBV	1486758	1190246	91.58%	15.703%
6	9.151	1198	1201	1213	rBV	264332	252143	19.40%	3.326%
7	9.833	1313	1317	1333	rBV	1395695	1299650	100.00%	17.146%
8	10.622	1447	1451	1456	rBV	111954	120384	9.26%	1.588%
9	10.757	1469	1474	1476	rBV3	14762	19435	1.50%	0.256%
10	11.222	1551	1553	1557	rVB3	19775	19378	1.49%	0.256%
11	11.322	1566	1570	1573	rBV	1232069	1091342	83.97%	14.398%
12	11.345	1573	1574	1580	rVB	73496	46044	3.54%	0.607%
13	11.851	1657	1660	1665	rVB2	28640	32962	2.54%	0.435%
14	11.933	1671	1674	1677	rBV4	16267	19426	1.49%	0.256%
15	12.410	1752	1755	1757	rBV3	16313	18383	1.41%	0.243%
16	12.533	1773	1776	1780	rBV	73506	72965	5.61%	0.963%
17	12.763	1812	1815	1819	rVB	69890	67479	5.19%	0.890%
18	12.910	1837	1840	1847	rVB	247908	222549	17.12%	2.936%
19	13.092	1869	1871	1875	rVB4	17078	14891	1.15%	0.196%
20	13.969	2016	2020	2023	rBV	1035573	963375	74.13%	12.710%
21	15.439	2266	2270	2278	rVB	530981	688983	53.01%	9.090%




Sum of corrected areas: 7579864

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081523\
Data File : BF134791.D
Acq On : 15 Aug 2023 18:51
Operator : CG\JU
Sample : 04017-01 10X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
JC-03-081423-A

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

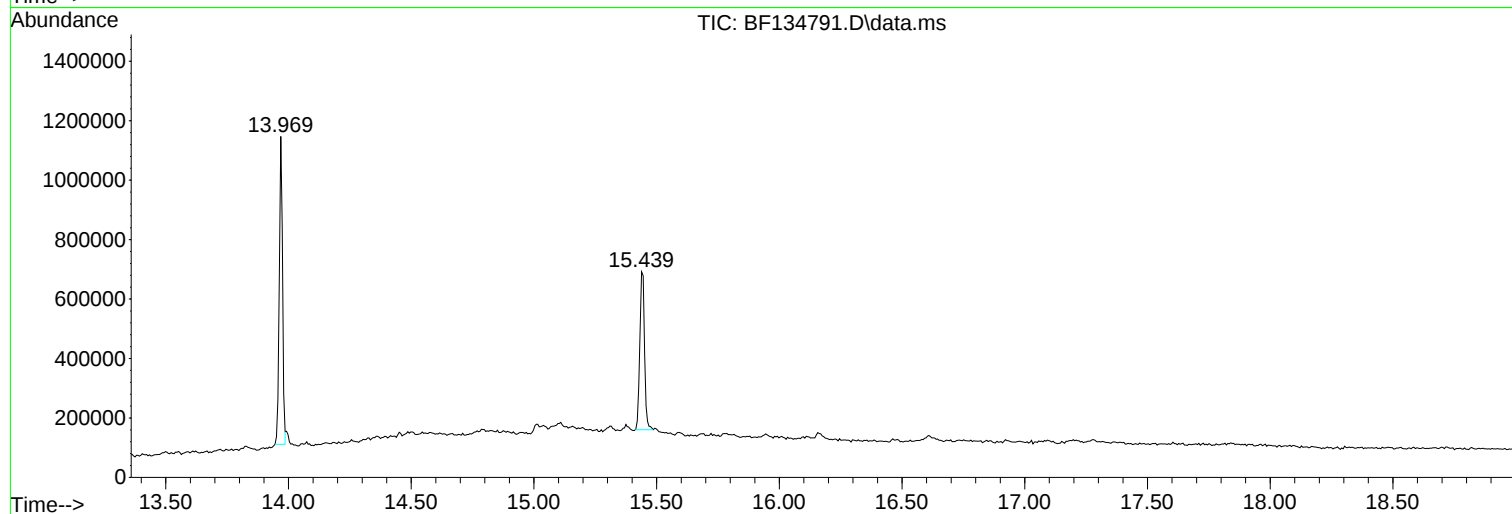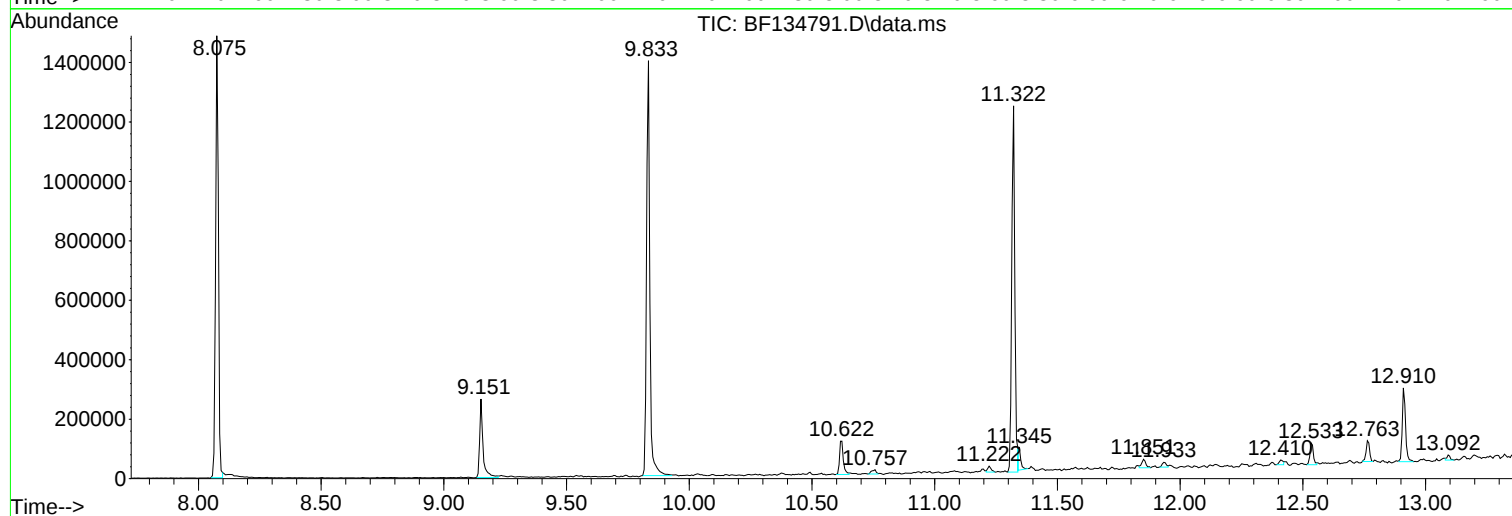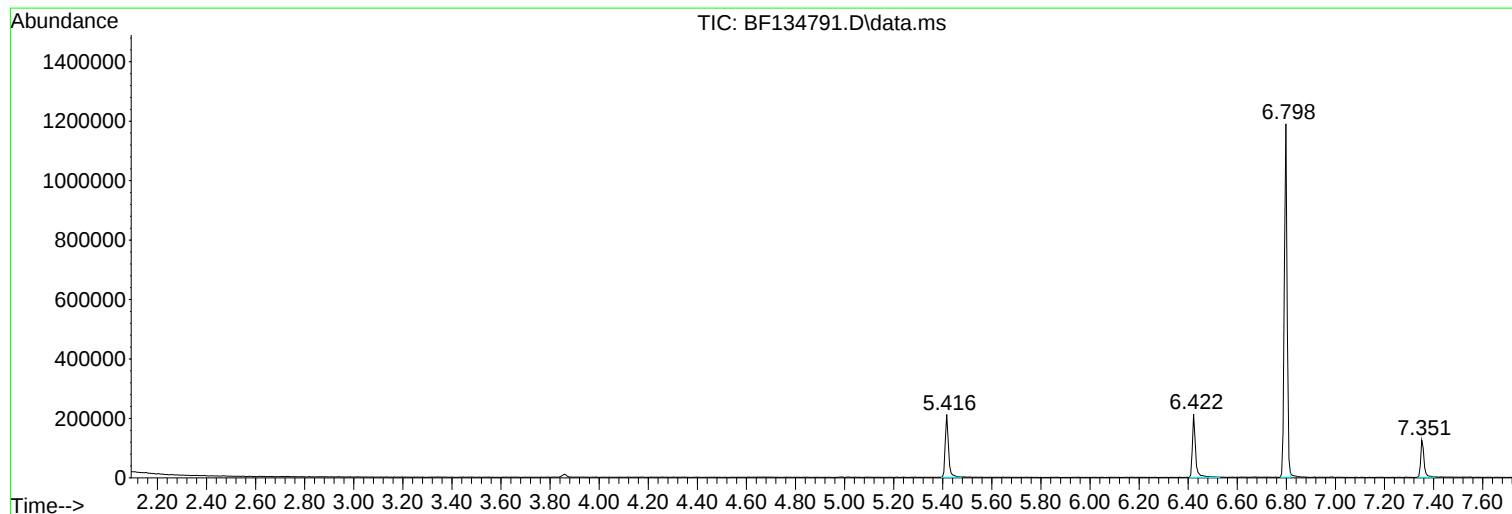

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081523\
Data File : BF134791.D
Acq On : 15 Aug 2023 18:51
Operator : CG\JU
Sample : 04017-01 10X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
JC-03-081423-A

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081523\
Data File : BF134791.D
Acq On : 15 Aug 2023 18:51
Operator : CG\JU
Sample : 04017-01 10X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
JC-03-081423-A

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------