


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081523\
 Data File : BF134773.D
 Acq On : 15 Aug 2023 08:02
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 04 09:29:15 2023

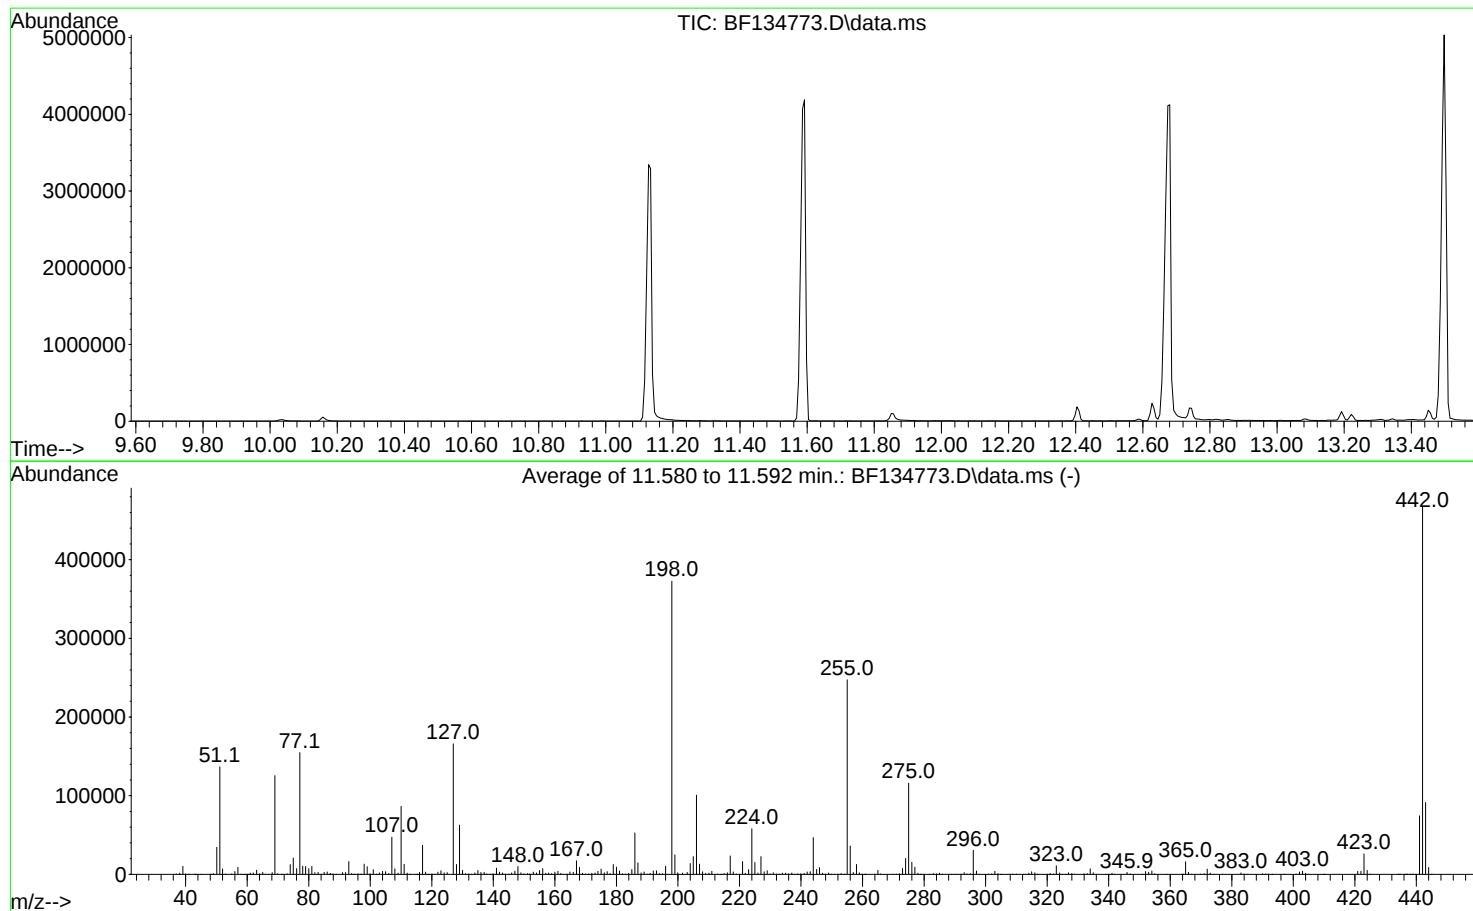




AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.7	136589	PASS
68	69	0.00	2	1.8	2223	PASS
69	198	0.00	100	33.7	125435	PASS
70	69	0.00	2	0.6	738	PASS
127	198	10	80	44.5	165939	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	372544	PASS
199	198	5	9	6.7	24843	PASS
275	198	10	60	31.1	115968	PASS
365	198	1	100	4.3	16021	PASS
441	198	0.01	100	20.0	74400	PASS
442	442	50	100	100.0	467541	PASS
443	442	15	24	19.5	91341	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081523\
 Data File : BF134773.D
 Acq On : 15 Aug 2023 08:02
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Aug 15 11:03:52 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 04 09:29:15 2023
 Response via : Initial Calibration

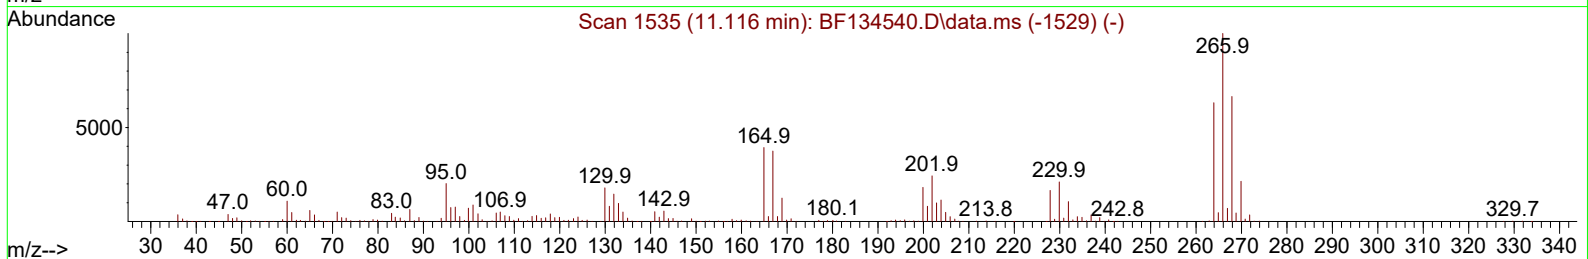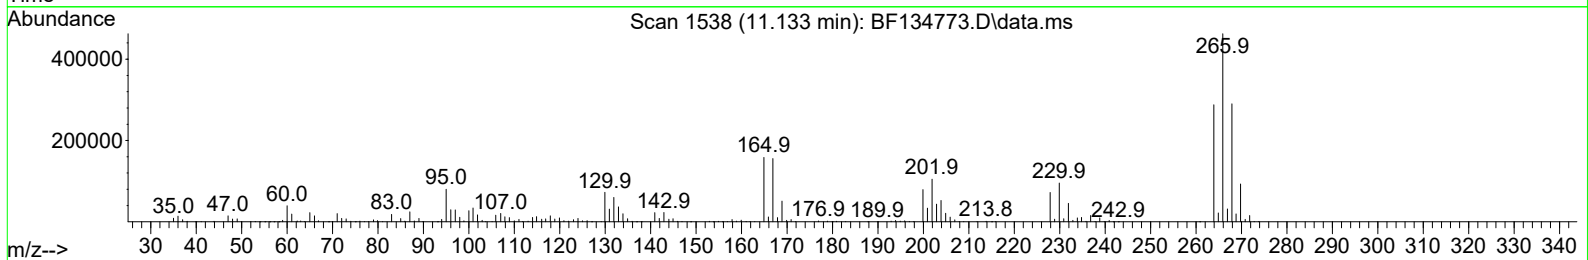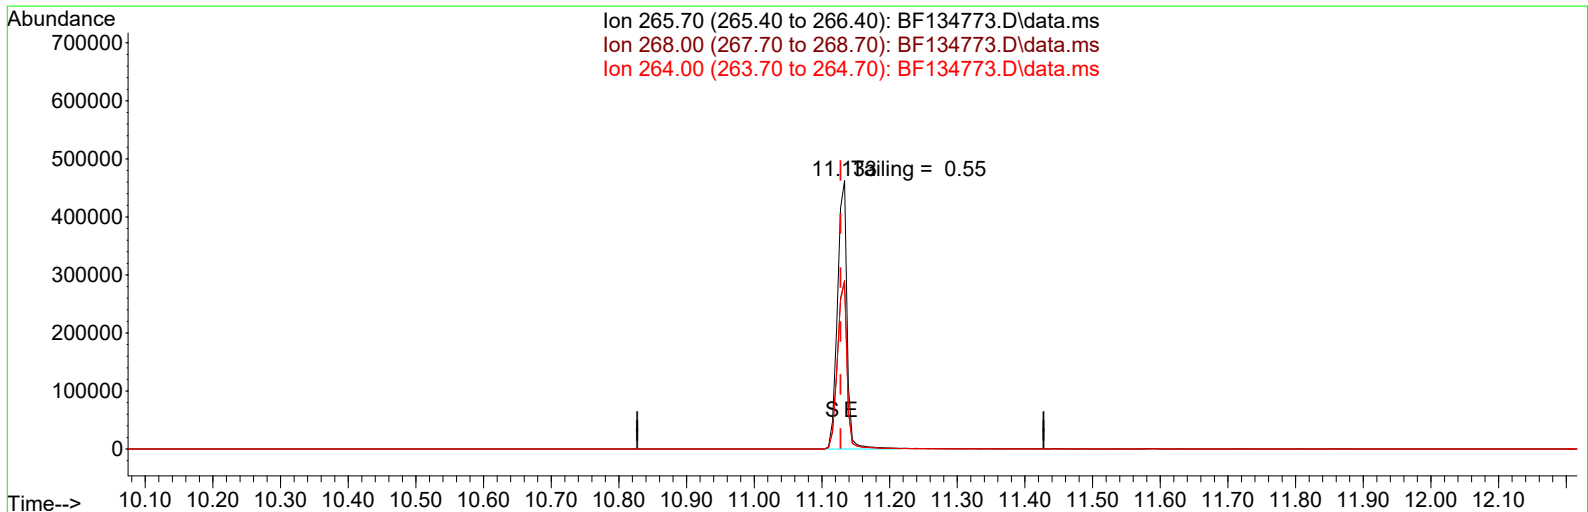

TIC: BF134773.D\data.ms

(70) Pentachlorophenol (C)

11.133min (+ 0.006) 632607.12 ng




response 457307

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.10	62.71
264.00	59.70	62.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081523\
Data File : BF134773.D
Acq On : 15 Aug 2023 08:02
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 15 11:03:52 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 04 09:29:15 2023
Response via : Initial Calibration

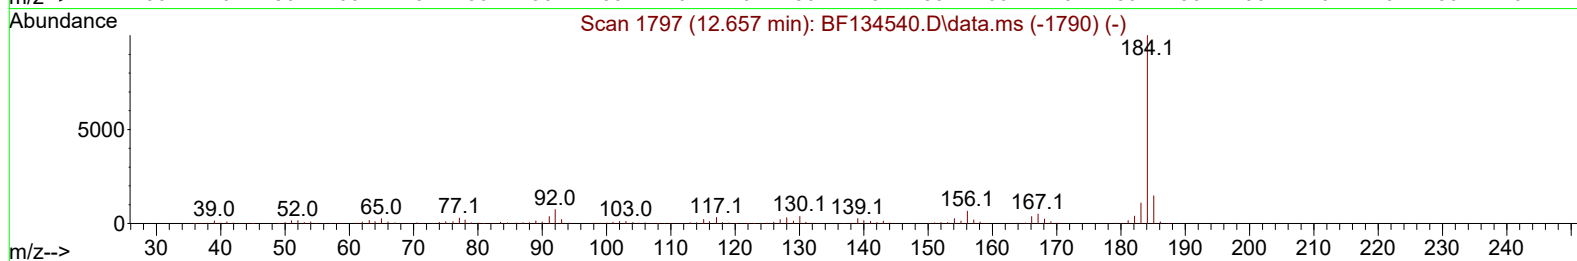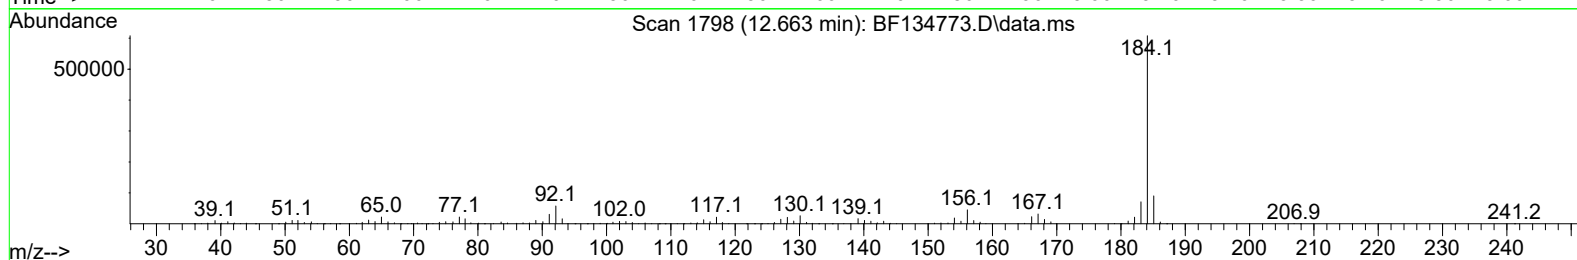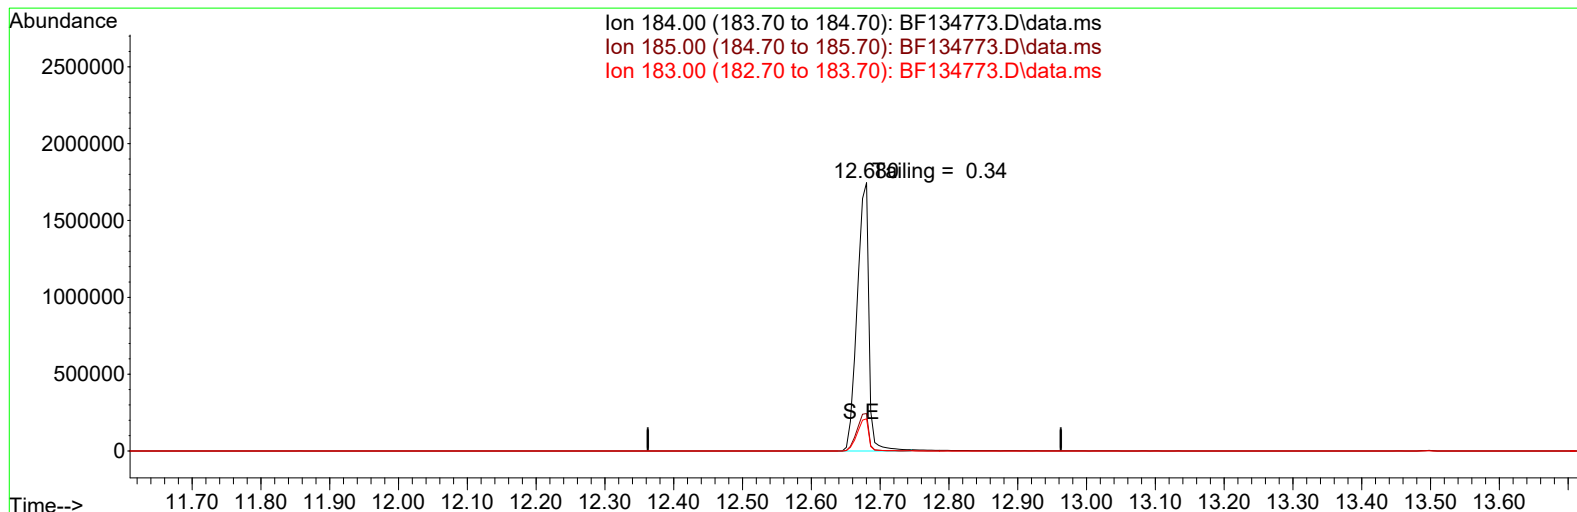

TIC: BF134773.D\data.ms

(77) Benzidine

12.663min (-12.663) 0.00 ng

response 0

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	14.00	0.00#
183.00	10.80	0.00#
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/15/2023	BNA_F	<u>BF134773.D</u>
Compound Name	Response	Retention Time
DDT	994362	13.498
DDD	31518	13.192
DDE	1369	12.851
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
32887	1027249	3.20

Instrument :
BNA_F
ClientSampleId :
DFTPP