


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081523\
 Data File : BF134782.D
 Acq On : 15 Aug 2023 13:45
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 04 09:29:15 2023

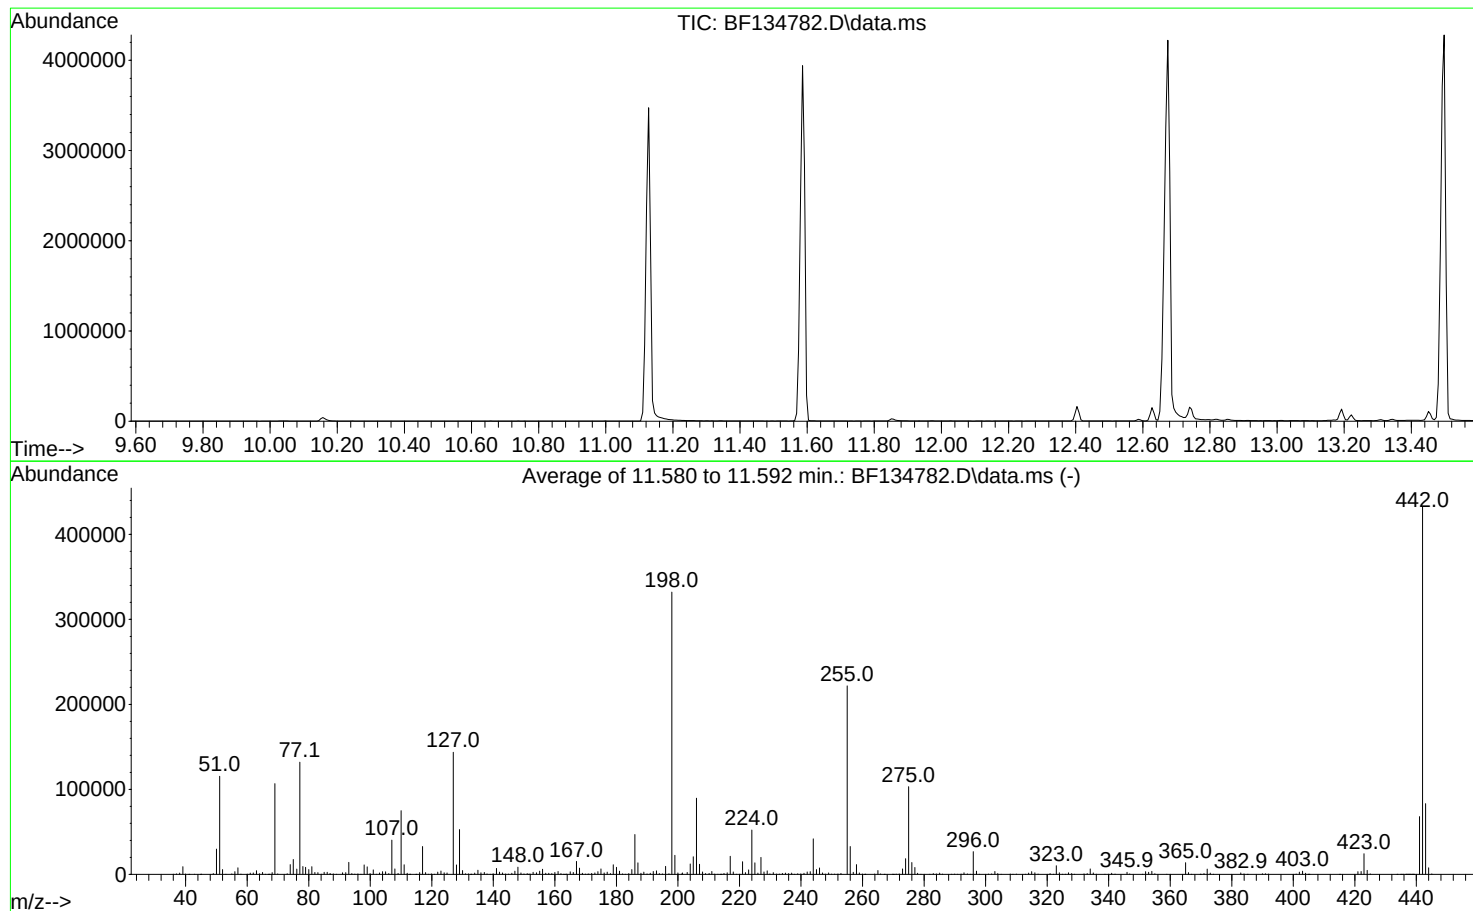


AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.8	115483	PASS
68	69	0.00	2	1.9	2017	PASS
69	198	0.00	100	32.2	106829	PASS
70	69	0.00	2	0.6	608	PASS
127	198	10	80	43.2	143557	PASS
197	198	0.00	2	0.2	699	PASS
198	198	100	100	100.0	332011	PASS
199	198	5	9	6.8	22491	PASS
275	198	10	60	31.1	103197	PASS
365	198	1	100	4.2	13808	PASS
441	198	0.01	100	20.5	68000	PASS
442	442	50	100	100.0	432811	PASS
443	442	15	24	19.2	83192	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081523\
Data File : BF134782.D
Acq On : 15 Aug 2023 13:45
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 15 14:13:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 04 09:29:15 2023
Response via : Initial Calibration

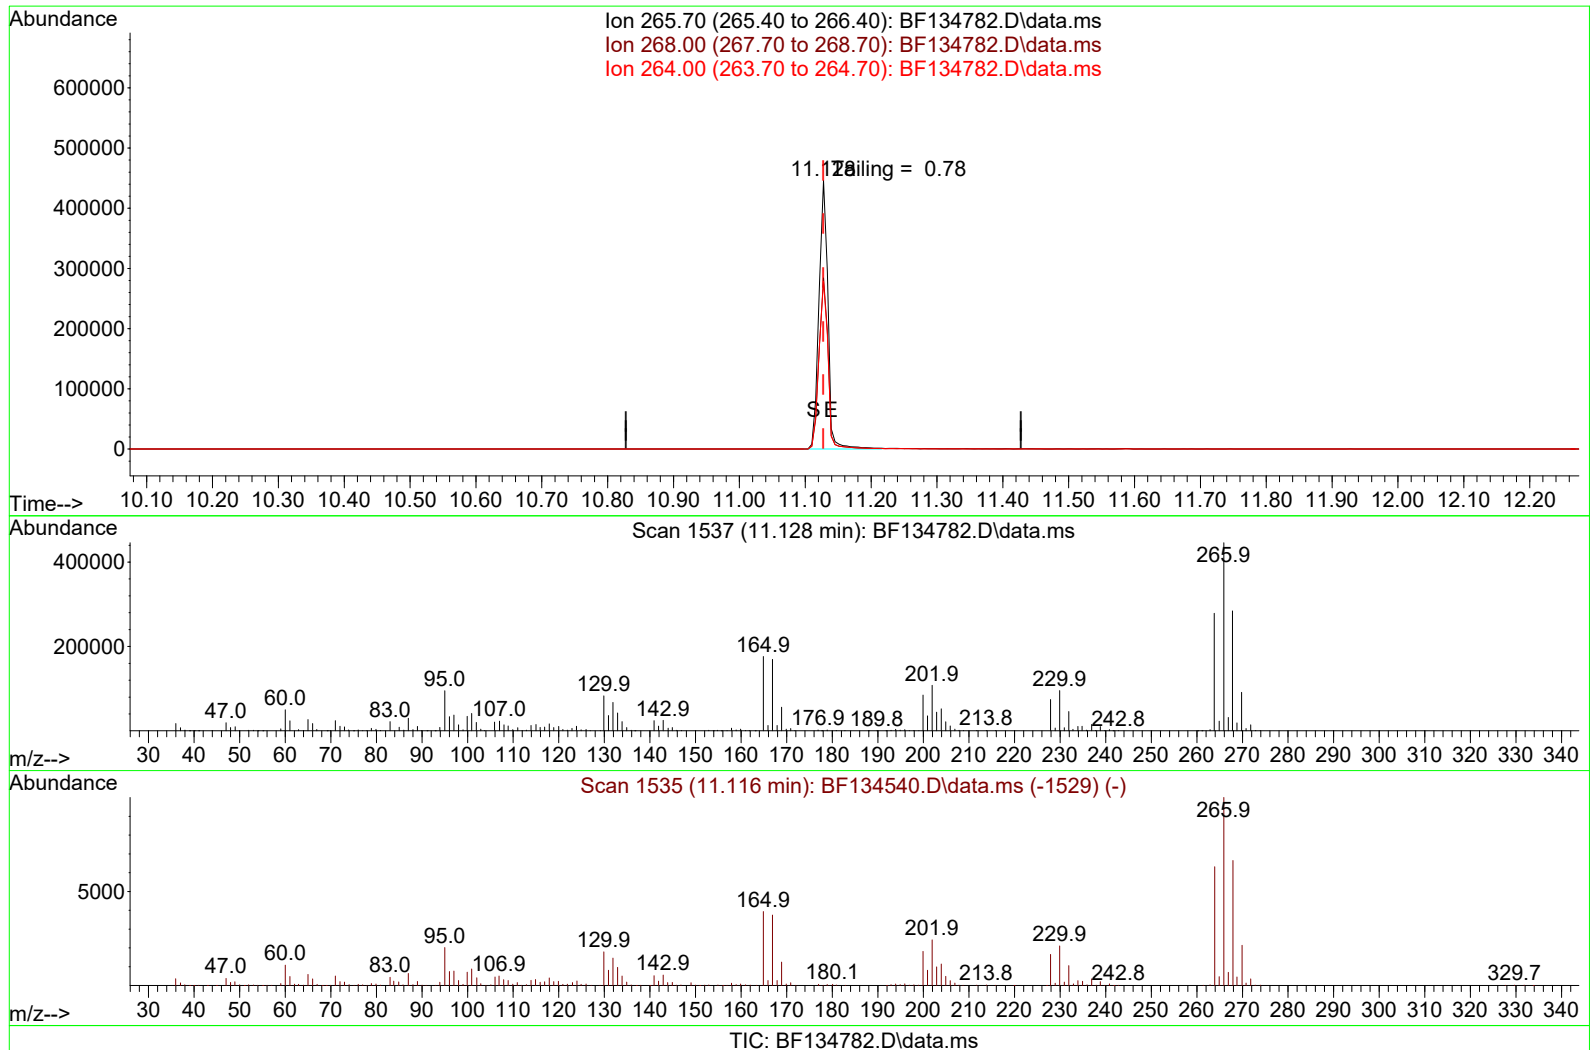

TIC: BF134782.D\data.ms

(70) Pentachlorophenol (C)

11.128min (+ 0.000) 515079.95 ng




response 423960

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.10	63.74
264.00	59.70	62.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081523\
Data File : BF134782.D
Acq On : 15 Aug 2023 13:45
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 15 14:13:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 04 09:29:15 2023
Response via : Initial Calibration

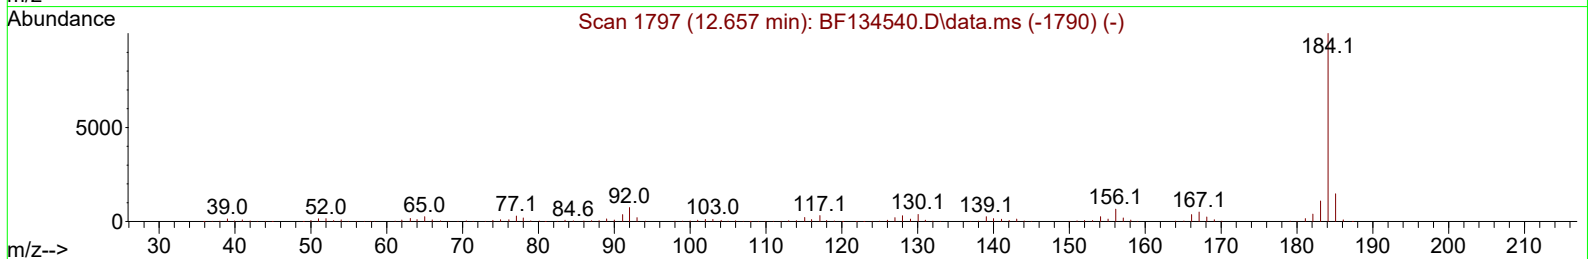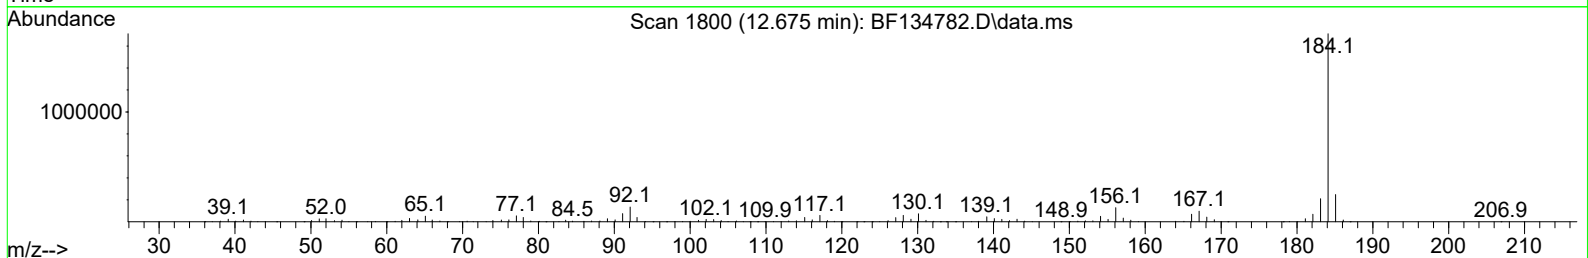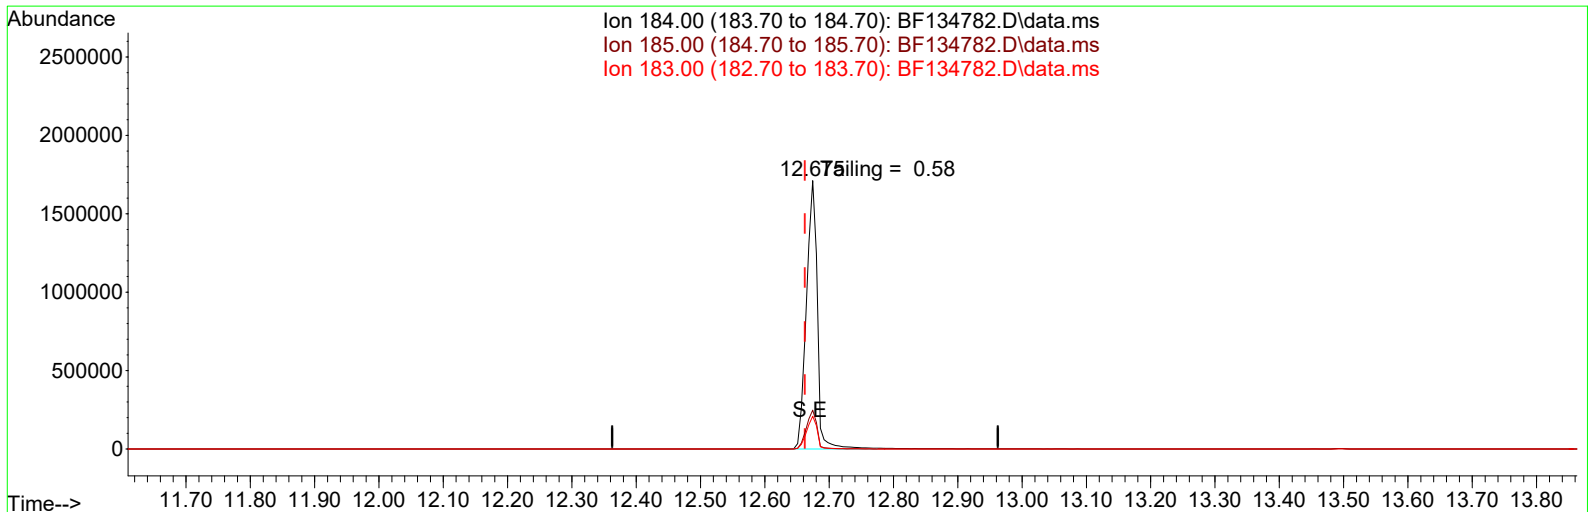

TIC: BF134782.D\data.ms

(77) Benzidine

12.675min (+ 0.012) 240732.35 ng

response 2032832

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.48
183.00	10.80	12.25
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/15/2023	BNA_F	<u>BF134782.D</u>
Compound Name	Response	Retention Time
DDT	867302	13.498
DDD	31833	13.192
DDE	1773	12.857
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
33606	900908	3.73

Instrument :
BNA_F
ClientSampleId :
DFTPP