

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF081618\
 Data File : BF108218.D
 Acq On : 17 Aug 2018 1:53
 Operator : JU/SJ
 Sample : J4501-02
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 RA-081318-FL-017

Manual Integrations
 APPROVED

Sohil
 8/17/2018 3:31:11 PM

Quant Time: Aug 17 05:24:46 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 12:24:24 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.02	152	152109	20.00	ng	0.00
21) Naphthalene-d8	8.30	136	523021	20.00	ng	0.00
38) Acenaphthene-d10	10.06	164	223783	20.00	ng	0.00
63) Phenanthrene-d10	11.55	188	401636	20.00	ng	0.00
75) Chrysene-d12	14.21	240	414988	20.00	ng	0.00
86) Perylene-d12	15.77	264	280524	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.64	112	925963	110.21	ng	0.01
7) Phenol-d6	6.64	99	1174782	105.22	ng	0.00
23) Nitrobenzene-d5	7.58	82	771355	82.30	ng	0.00
41) 2,4,6-Tribromophenol	10.85	330	250908	112.40	ng	0.00
44) 2-Fluorobiphenyl	9.37	172	1198080	85.95	ng	0.00
78) Terphenyl-d14	13.14	244	1180526	72.33	ng	0.00
Target Compounds						
49) Dimethylphthalate	9.76	163	77709	4.985	ng	Qvalue # 99
70) Phenanthrene	11.58	178	325679	17.192	ng	99
71) Anthracene	11.63	178	75147	3.870	ng	99
74) Fluoranthene	12.78	202	431197	20.856	ng	95
77) Pyrene	13.01	202	382977	14.577	ng	99
80) Benzo(a)anthracene	14.20	228	184871	7.762	ng	99
82) Chrysene	14.24	228	168673	7.725	ng	99
85) Indeno(1,2,3-cd)pyrene	17.38	276	53639m	2.835	ng	
87) Benzo(b)fluoranthene	15.30	252	158743m	9.470	ng	
88) Benzo(k)fluoranthene	15.33	252	54246m	3.520	ng	
89) Benzo(a)pyrene	15.70	252	104526	6.964	ng	97
91) Benzo(a,h,i)perylene	17.88	276	50190	4.104	ng	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF081618\
Data File : BF108218.D
Acq On : 17 Aug 2018 1:53
Operator : JU/SJ
Sample : J4501-02
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RA-081318-FL-017

Manual Integrations
APPROVED

Sohil
8/17/2018 3:31:11 PM

Quant Time: Aug 17 05:24:46 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 08 12:24:24 2018
Response via : Initial Calibration

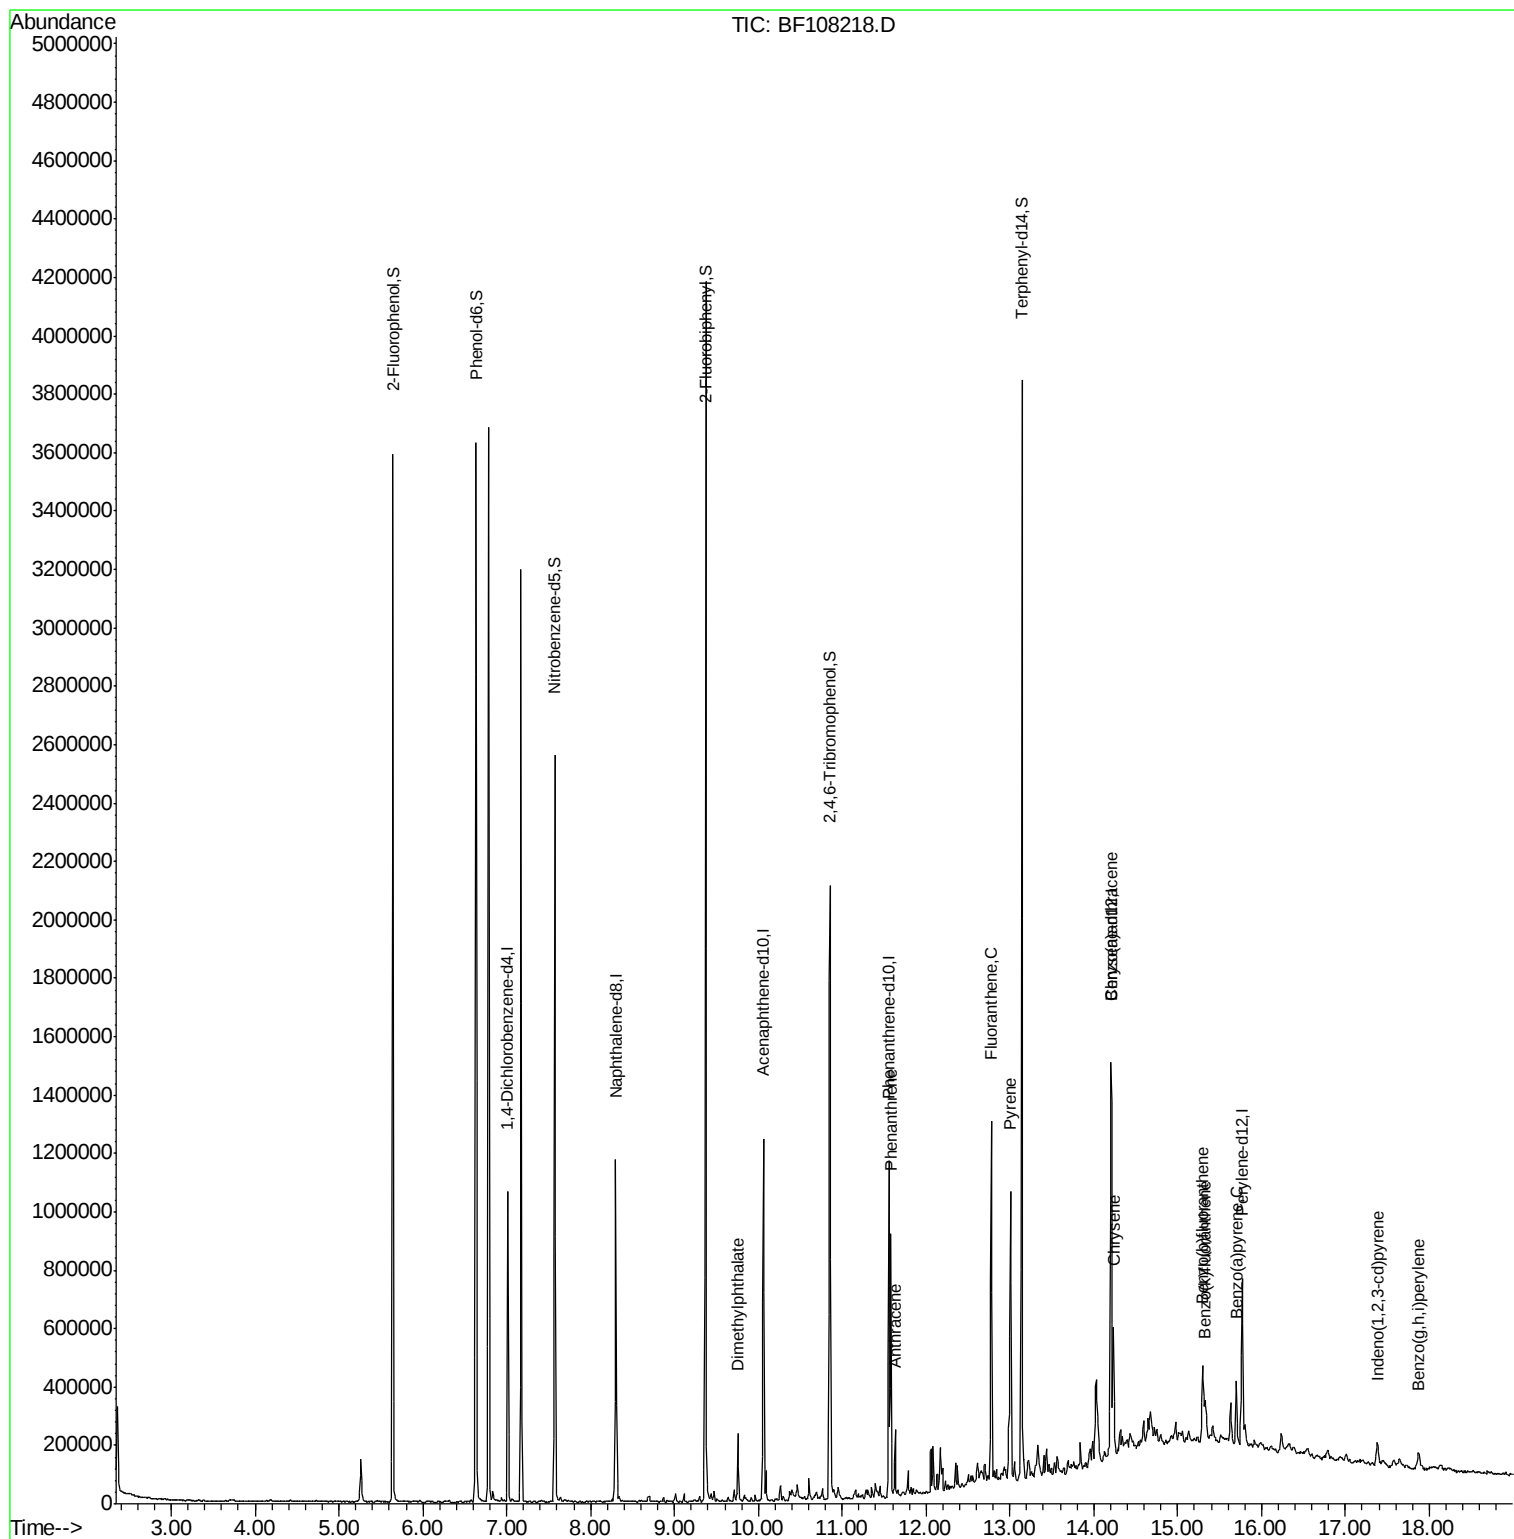







#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 7.02 min Scan# 796
 Delta R.T. 0.01 min
 Lab File: BF108218.D
 Acq: 17 Aug 2018 1:53

Instrument :
 BNA_F
 ClientSampleId :
 RA-081318-FL-017

Tot Ion	Ratio	Lower	Upper
152	100		
150	155.2	124.6	186.8
115	54.3	50.1	75.1




Manual Integrations
 APPROVED

Sohil
 8/17/2018 3:31:11 PM

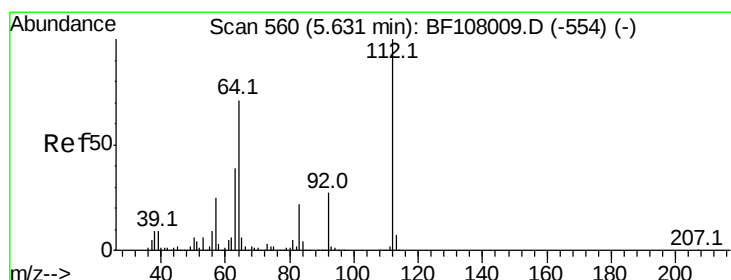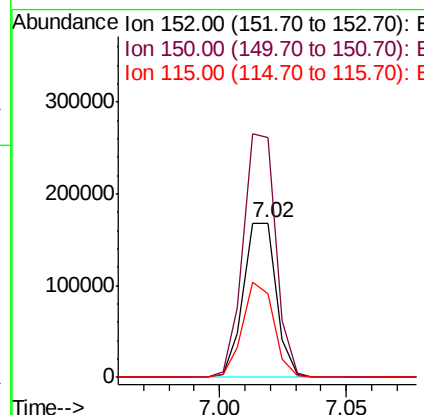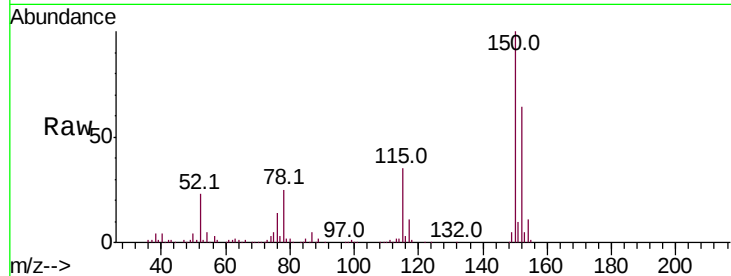

#5
 2-Fluorophenol
 Concen: 110.211 ng
 RT: 5.64 min Scan# 562
 Delta R.T. 0.01 min
 Lab File: BF108218.D
 Acq: 17 Aug 2018 1:53

Tgt Ion	Ratio	Lower	Upper
112	100		
64	71.0	47.9	71.9
63	37.6	23.7	35.5#

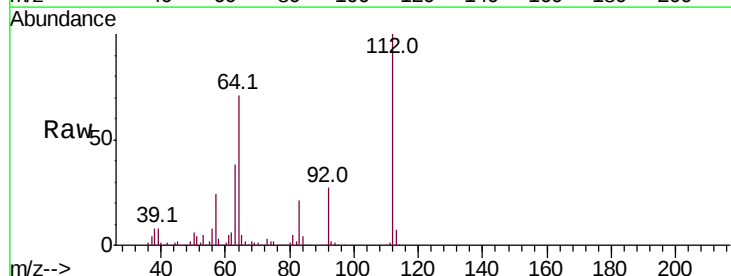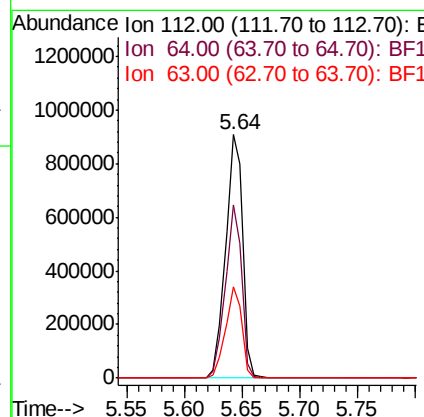



#7

Phenol-d6

Concen: 105.223 ng

RT: 6.64 min Scan# 731

Delta R.T. 0.01 min

Lab File: BF108218.D

Acq: 17 Aug 2018 1:53

Instrument :

BNA_F

ClientSampleId :

RA-081318-FL-017

Tot Ion: 99 Resp: 1174782

Ion Ratio Lower Upper

99 100

42 23.2 14.5 21.7#


71 37.3 25.4 38.0

Manual Integrations




APPROVED

Sohil

8/17/2018 3:31:11 PM

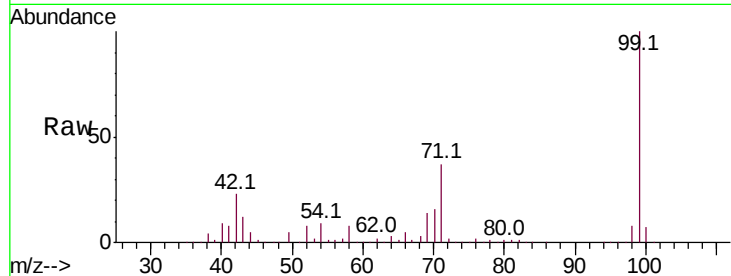

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

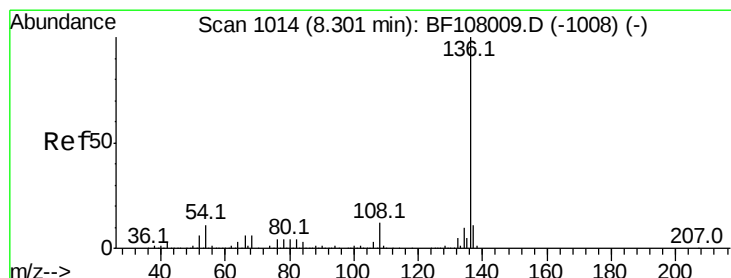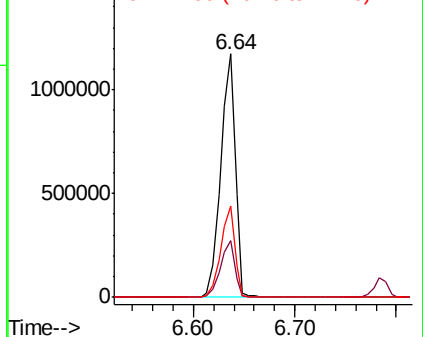

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.30 min Scan# 1014

Delta R.T. 0.00 min

Lab File: BF108218.D

Acq: 17 Aug 2018 1:53

Tgt Ion: 136 Resp: 523021

Ion Ratio Lower Upper




136 100

137 10.2 8.9 13.3

54 9.2 6.6 9.8

68 5.8 5.0 7.4

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

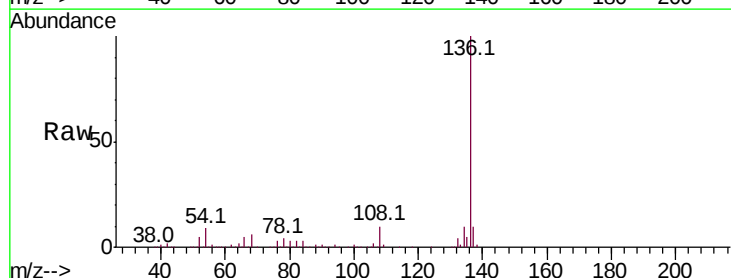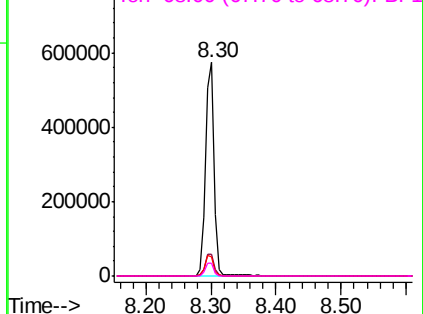







#23
Nitrobenzene-d5
Concen: 82.296 ng
RT: 7.58 min Scan# 891
Delta R.T. 0.00 min
Lab File: BF108218.D
Acq: 17 Aug 2018 1:53

Instrument :
BNA_F
ClientSampleId :
RA-081318-FL-017

Tot Ion	Ratio	Lower	Upper
82	100		
128	42.8	36.1	54.1
54	58.4	41.4	62.2




Manual Integrations
APPROVED

Sohil
8/17/2018 3:31:11 PM

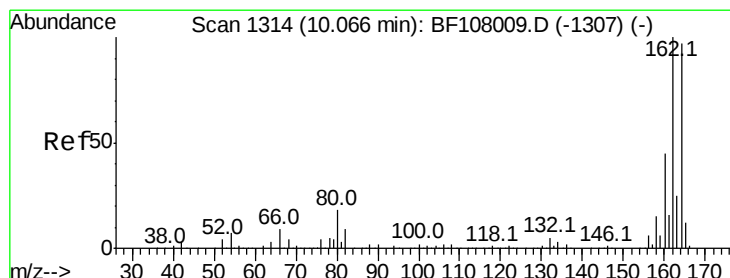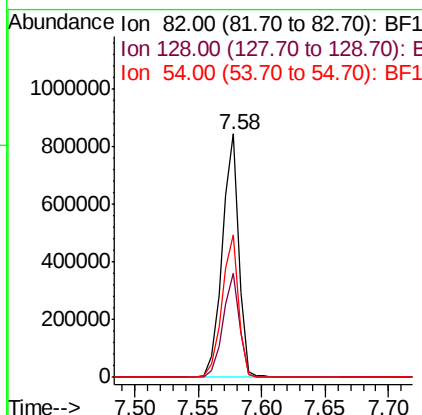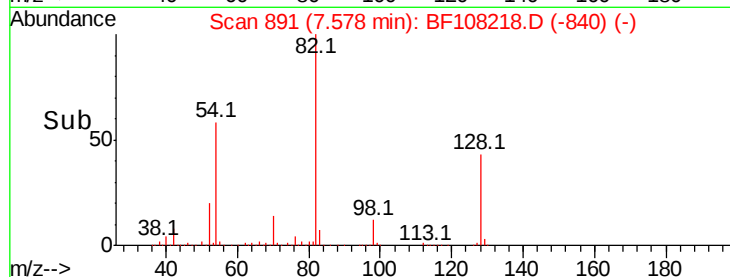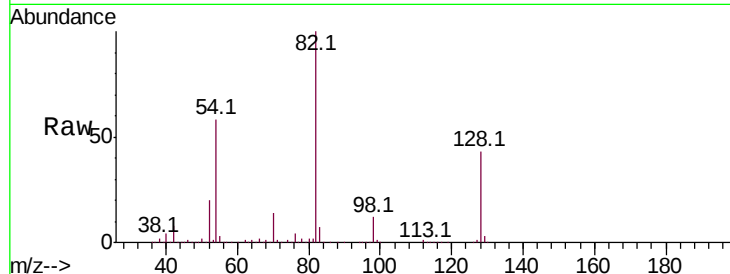

#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 10.06 min Scan# 1313
Delta R.T. -0.01 min
Lab File: BF108218.D
Acq: 17 Aug 2018 1:53

Tgt Ion	Ratio	Lower	Upper
164	100		
162	103.3	86.1	129.1
160	45.8	38.3	57.5

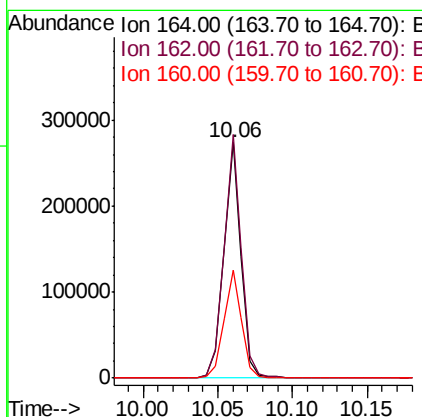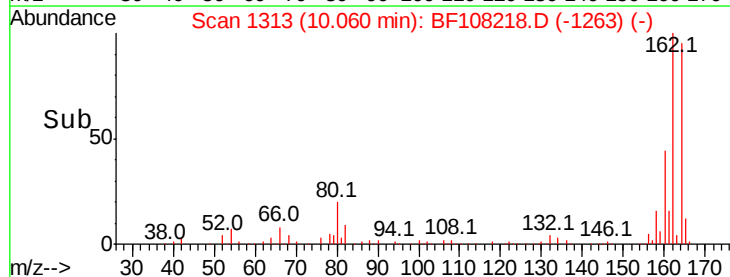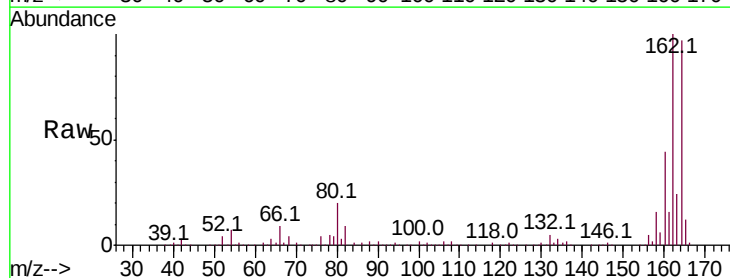




#41
 2,4,6-Tribromophenol
 Concen: 112.405 ng
 RT: 10.85 min Scan# 1448
 Delta R.T. -0.01 min
 Lab File: BF108218.D
 Acq: 17 Aug 2018 1:53

Instrument :
 BNA_F
 ClientSampleId :
 RA-081318-FL-017

Tot Ion	Ratio	Resp	Lower	Upper
330	100	250908		
332	96.6	77.0	115.6	
141	33.0	29.9	44.9	

Manual Integrations
 APPROVED

Sohil
 8/17/2018 3:31:11 PM



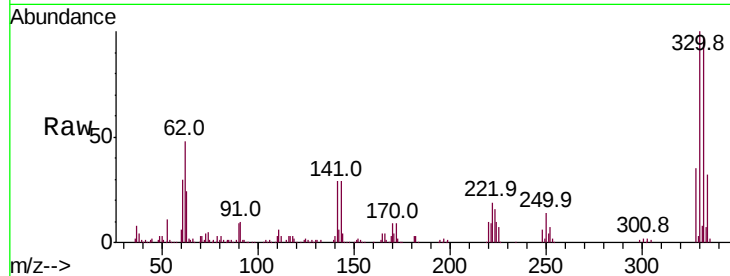


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

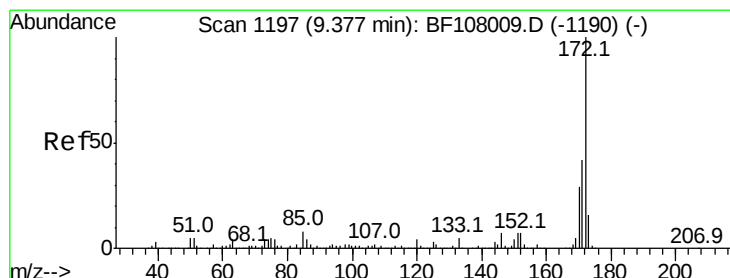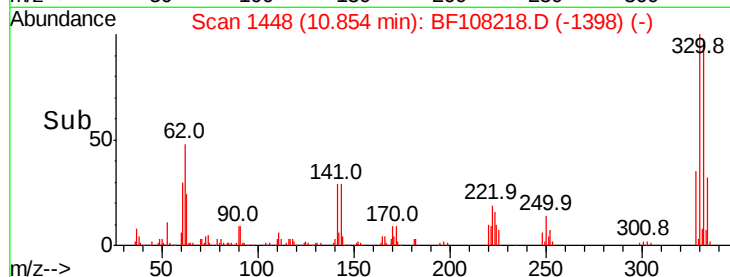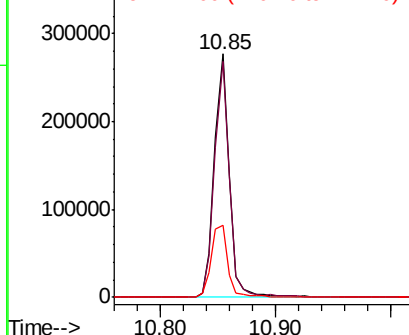

#44
 2-Fluorobiphenyl
 Concen: 85.953 ng
 RT: 9.37 min Scan# 1196
 Delta R.T. -0.01 min
 Lab File: BF108218.D
 Acq: 17 Aug 2018 1:53

Tgt Ion	Ratio	Resp	Lower	Upper
172	100	1198080		
171	36.8	29.7	44.5	
170	24.8	19.6	29.4	


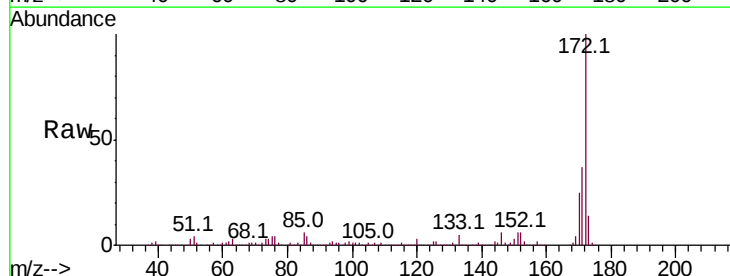


Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

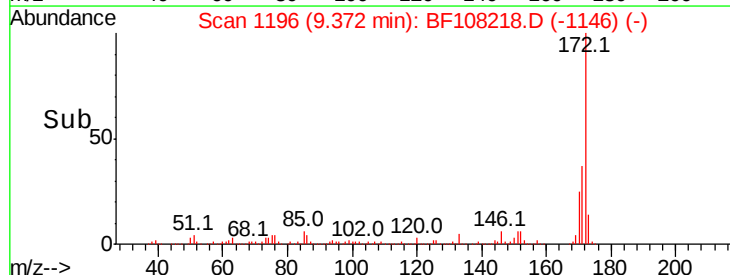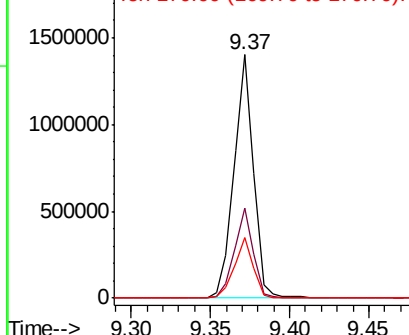




#49
 Dimethylphthalate
 Concen: 4.985 ng
 RT: 9.76 min Scan# 1262
 Delta R.T. -0.02 min
 Lab File: BF108218.D
 Acq: 17 Aug 2018 1:53

Instrument :
 BNA_F
 ClientSampleId :
 RA-081318-FL-017




Tot Ion:	163	Resp:	77709
Ion Ratio	Lower	Upper	
163	100		
194	4.1	2.7	4.1#
164	9.8	8.2	12.2

Manual Integrations
 APPROVED

Sohil
 8/17/2018 3:31:11 PM

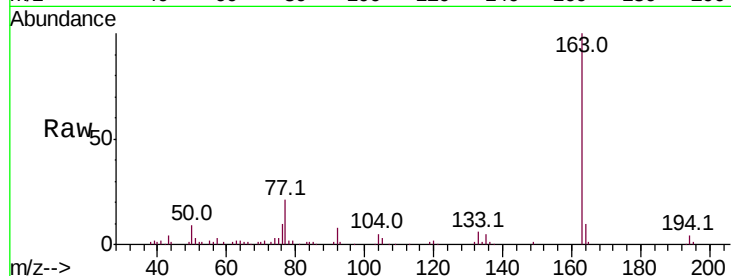


Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

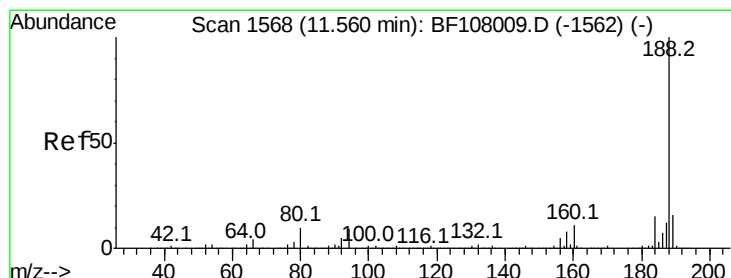
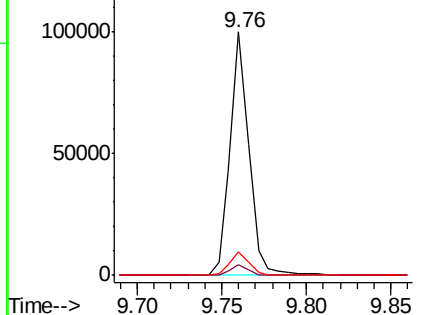



#63
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 11.55 min Scan# 1567
 Delta R.T. -0.01 min
 Lab File: BF108218.D
 Acq: 17 Aug 2018 1:53

Tgt Ion:	188	Resp:	401636
Ion Ratio	Lower	Upper	
188	100		
94	9.2	8.5	12.7
80	10.5	9.2	13.8

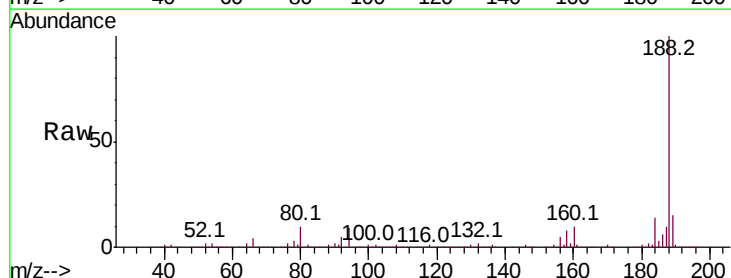

Abundance Ion 188.00 (187.70 to 188.70): E
 Ion 94.00 (93.70 to 94.70): BF1
 Ion 80.00 (79.70 to 80.70): BF1

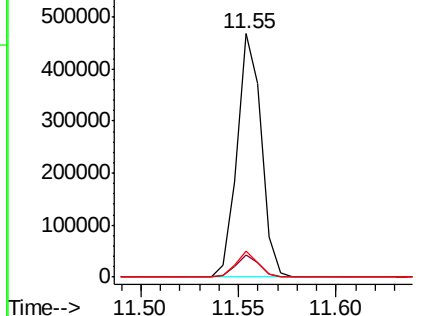

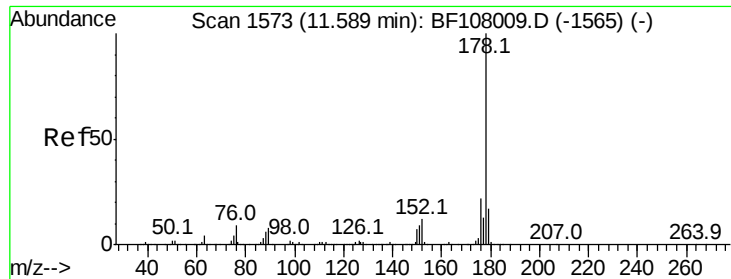


#70
Phenanthrene
Concen: 17.192 ng
RT: 11.58 min Scan# 1571
Delta R.T. -0.01 min
Lab File: BF108218.D
Acq: 17 Aug 2018 1:53

Instrument :
BNA_F
ClientSampleId :
RA-081318-FL-017




Tot Ion	Ratio	Lower	Upper
178	100		
176	19.5	15.8	23.8
179	15.5	13.0	19.6

Manual Integrations
APPROVED

Sohil
8/17/2018 3:31:11 PM

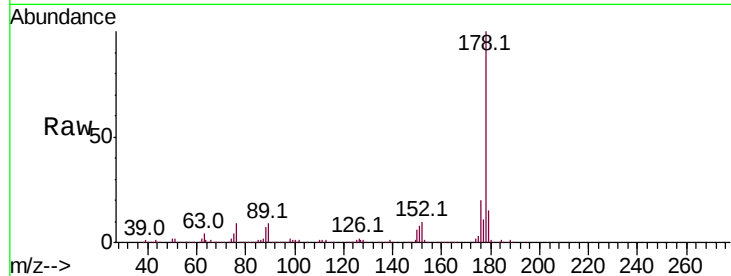




Abundance Ion 178.00 (177.70 to 178.70): E
Ion 176.00 (175.70 to 176.70): E
Ion 179.00 (178.70 to 179.70): E

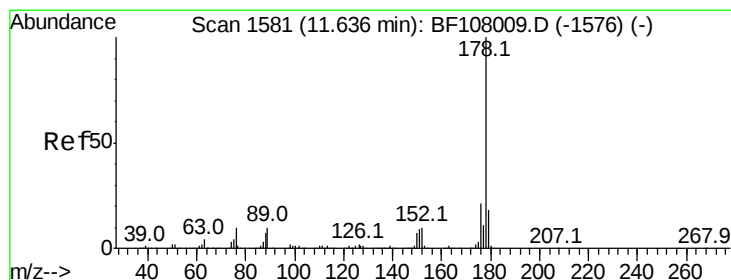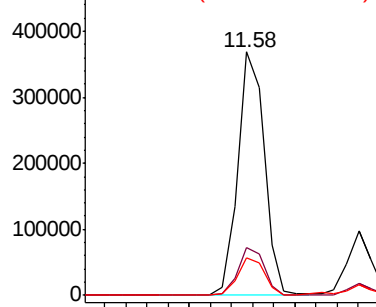


#71
Anthracene
Concen: 3.870 ng
RT: 11.63 min Scan# 1580
Delta R.T. -0.01 min
Lab File: BF108218.D
Acq: 17 Aug 2018 1:53

Tgt Ion	Ratio	Lower	Upper
178	100		
176	18.9	15.4	23.2
179	16.5	12.6	19.0

Abundance Ion 178.00 (177.70 to 178.70): E
Ion 176.00 (175.70 to 176.70): E
Ion 179.00 (178.70 to 179.70): E

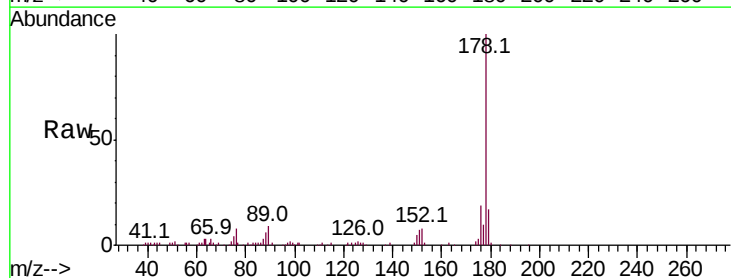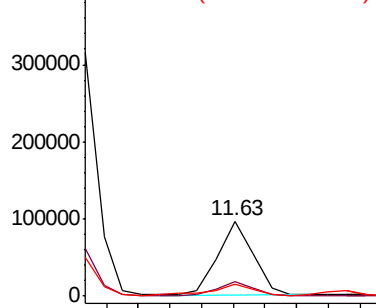

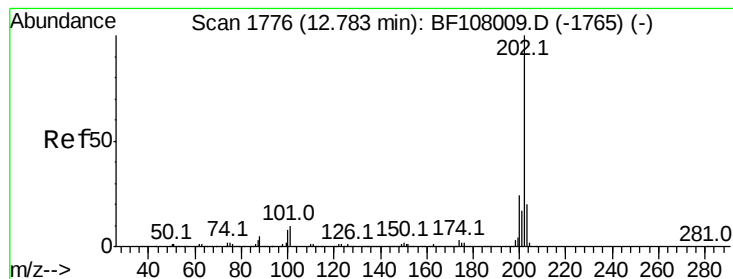

#74

Fluoranthene

Concen: 20.856 ng

RT: 12.78 min Scan# 1775

Delta R.T. -0.01 min

Lab File: BF108218.D

Acq: 17 Aug 2018 1:53

Instrument :

BNA_F





ClientSampleId :

RA-081318-FL-017

Tot Ion	Ratio	Resp Lower	Upper
202	100		
101	10.4	0.0	34.1
203	17.5	0.0	38.1

Manual Integrations
APPROVED

Sohil
8/17/2018 3:31:11 PM

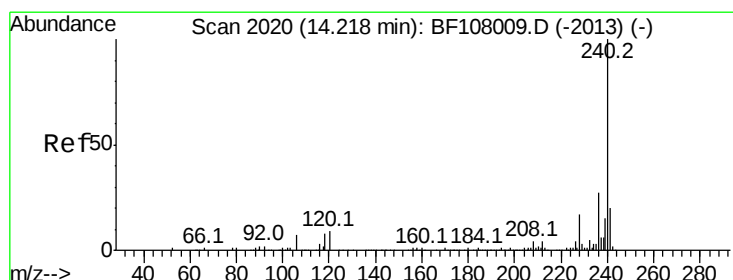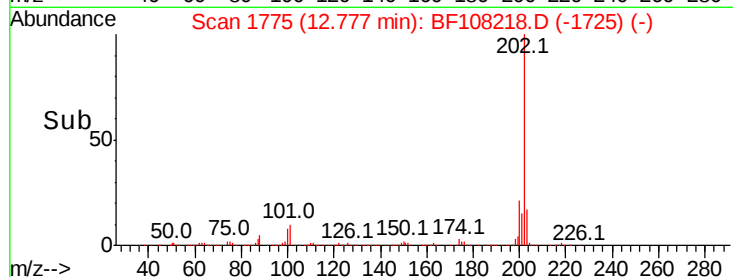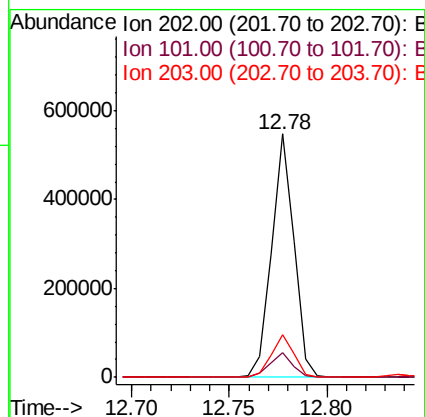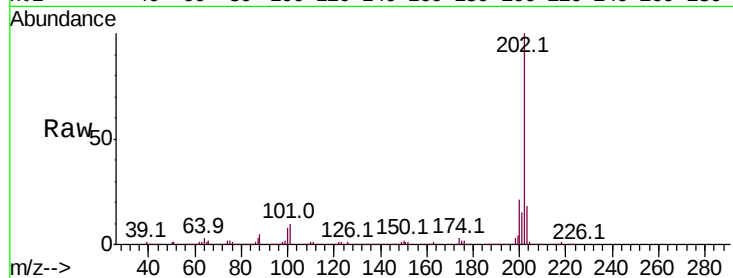

#75

Chrysene-d12

Concen: 20.000 ng




RT: 14.21 min Scan# 2019


Delta R.T. -0.01 min

Lab File: BF108218.D

Acq: 17 Aug 2018 1:53

Tgt Ion	Ratio	Resp Lower	Upper
240	100		
120	9.0	9.5	14.3#
236	26.0	20.7	31.1

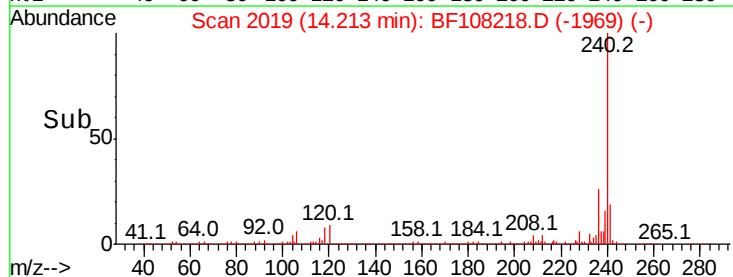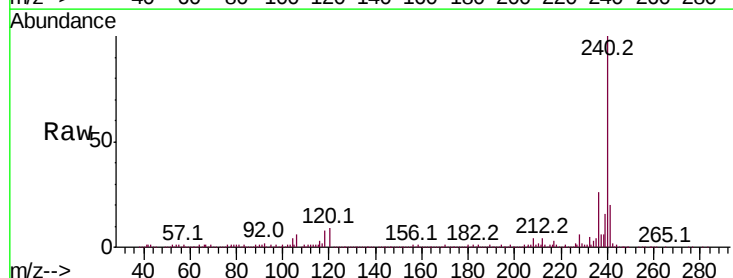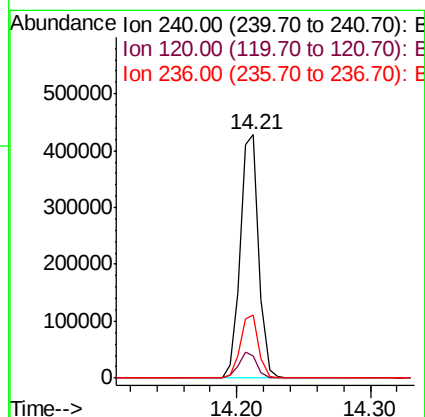

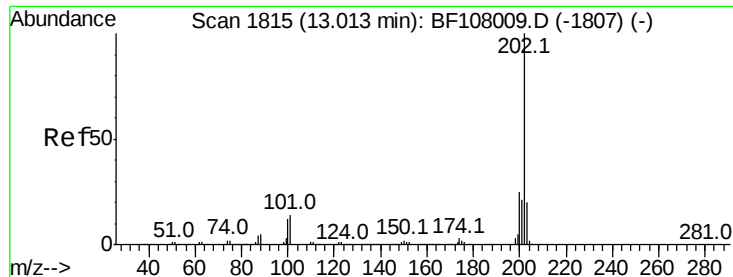

#77

Pvrene

Concen: 14.577 ng

RT: 13.01 min Scan# 1814

Delta R.T. -0.01 min

Lab File: BF108218.D

Acq: 17 Aug 2018 1:53

Instrument :

BNA_F





ClientSampleId :

RA-081318-FL-017

Tot Ion:	202	Resp:	382977
Ion Ratio	Lower	Upper	
202	100		
200	21.0	17.4	26.2
203	17.7	14.3	21.5

Manual Integrations
APPROVED

Sohil
8/17/2018 3:31:11 PM

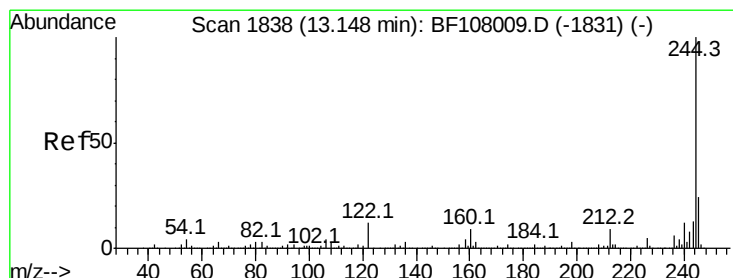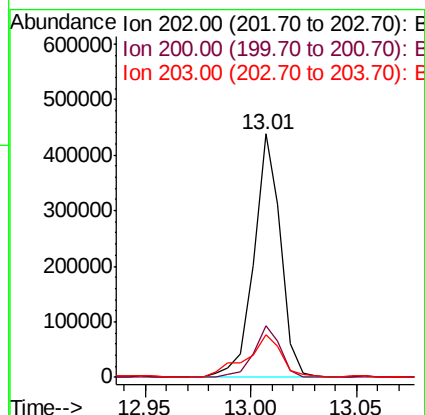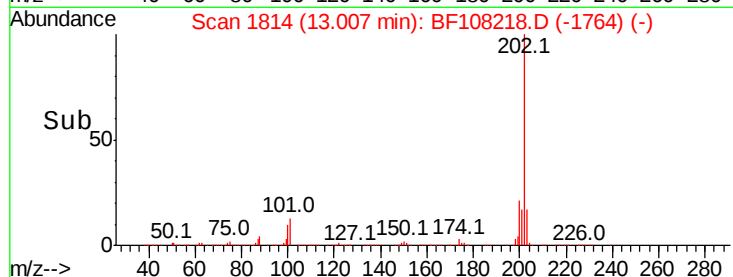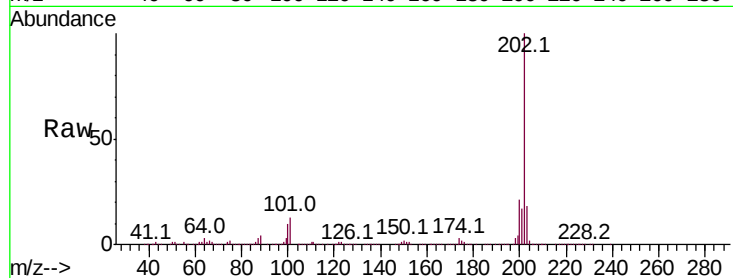

#78

Terphenyl-d14

Concen: 72.329 ng




RT: 13.14 min Scan# 1837


Delta R.T. -0.01 min

Lab File: BF108218.D

Acq: 17 Aug 2018 1:53

Tgt Ion:	244	Resp:	1180526
Ion Ratio	Lower	Upper	
244	100		
212	7.5	5.4	8.0
122	10.3	11.0	16.4#

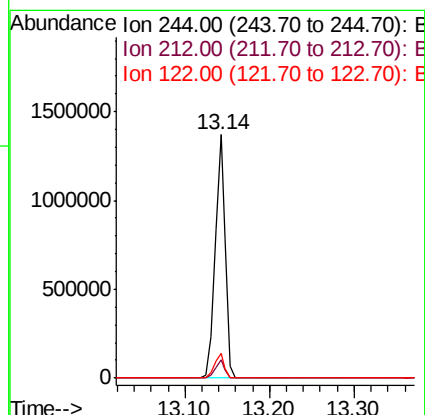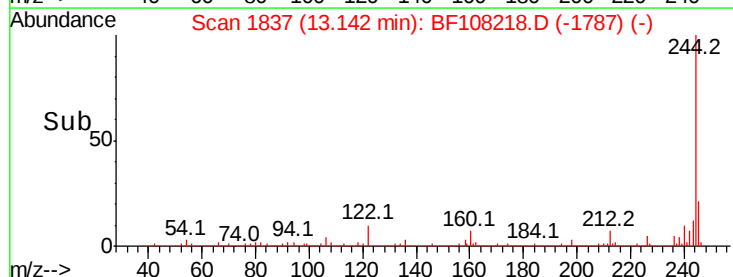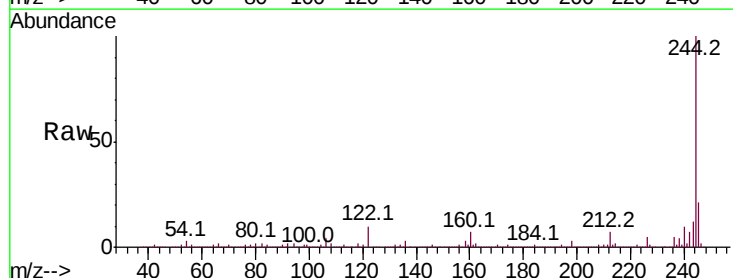

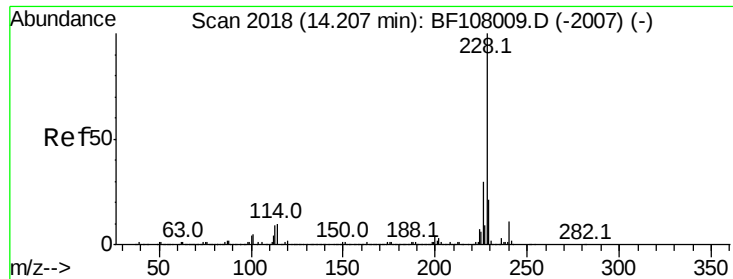





#80
Benzo(a)anthracene
Concen: 7.762 ng
RT: 14.20 min Scan# 2017
Delta R.T. -0.01 min
Lab File: BF108218.D
Acq: 17 Aug 2018 1:53

Instrument :
BNA_F
ClientSampleId :
RA-081318-FL-017

Tot Ion	Ratio	Lower	Upper
228	100		
226	27.6	22.6	33.8
229	19.7	15.8	23.6




Manual Integrations
APPROVED


Sohil
8/17/2018 3:31:11 PM

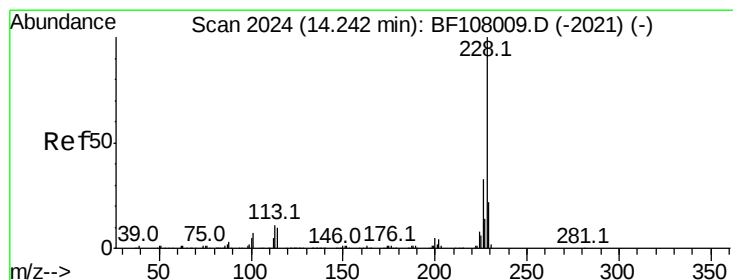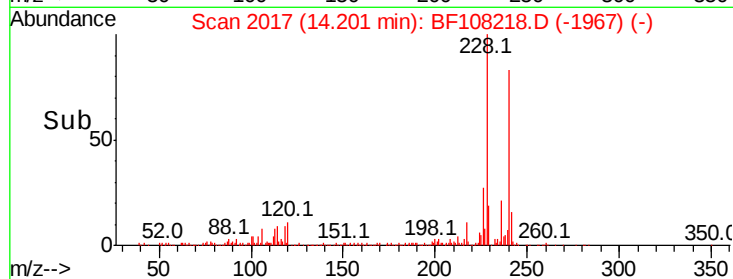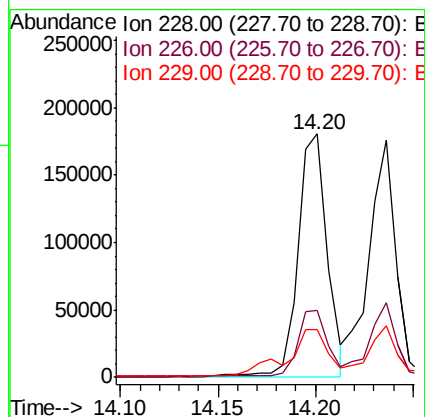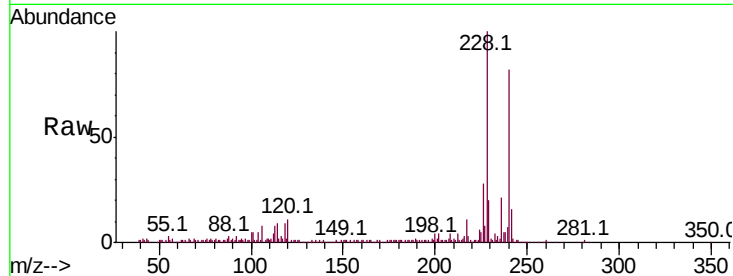

#82
Chrysene
Concen: 7.725 ng
RT: 14.24 min Scan# 2023
Delta R.T. -0.01 min
Lab File: BF108218.D
Acq: 17 Aug 2018 1:53

Tgt Ion	Ratio	Lower	Upper
228	100		
226	31.3	25.0	37.6
229	21.9	16.2	24.4

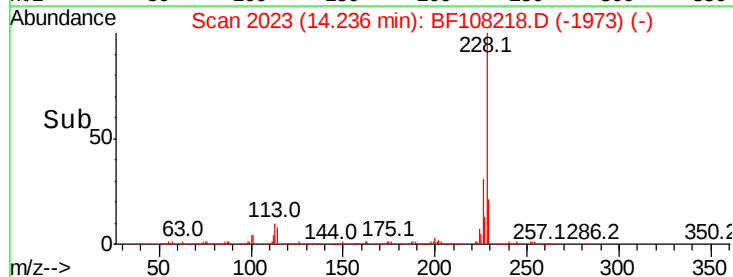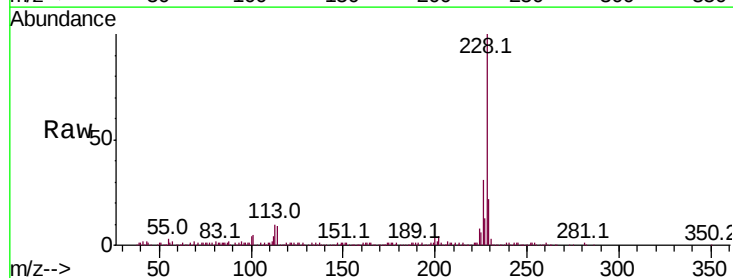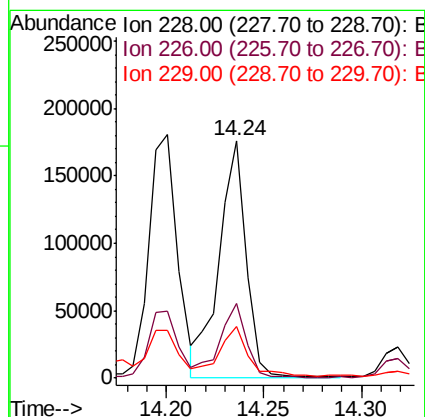

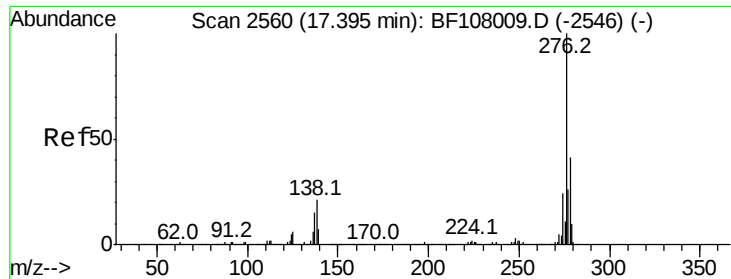


#85
 Indeno(1,2,3-cd)pyrene
 Concen: 2.835 ng/ml
 RT: 17.38 min Scan# 2558
 Delta R.T. -0.01 min
 Lab File: BF108218.D
 Acq: 17 Aug 2018 1:53

Instrument :
 BNA_F
 ClientSampleId :
 RA-081318-FL-017




Tot Ion	Ratio	Lower	Upper
276	100		
138	7.7	25.0	37.6#
277	4.5	20.1	30.1#

Manual Integrations
 APPROVED

Sohil
 8/17/2018 3:31:11 PM

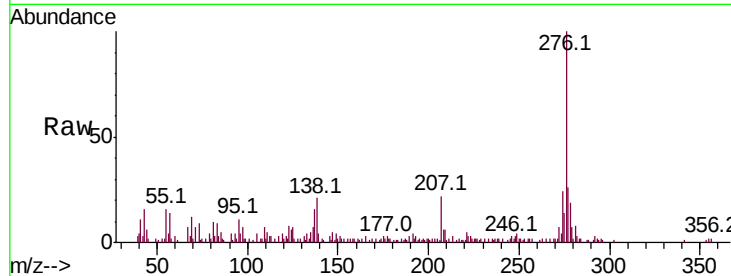


Abundance Ion 276.00 (275.70 to 276.70): E
 Ion 138.00 (137.70 to 138.70): E
 Ion 277.00 (276.70 to 277.70): E

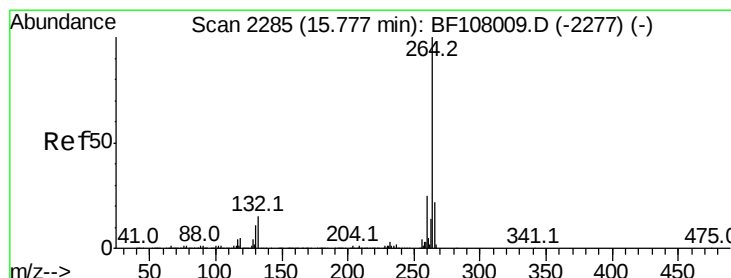
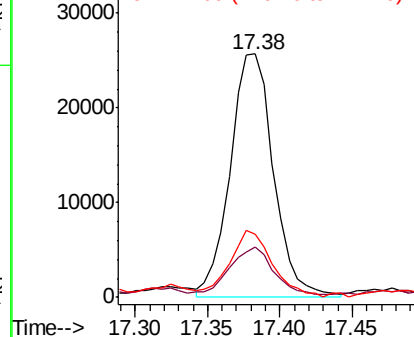



#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.77 min Scan# 2284
 Delta R.T. -0.01 min
 Lab File: BF108218.D
 Acq: 17 Aug 2018 1:53

Tgt Ion	Ratio	Lower	Upper
264	100		
260	24.1	19.2	28.8
265	21.5	17.5	26.3

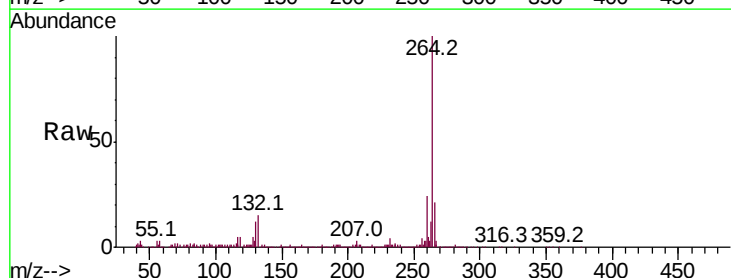

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

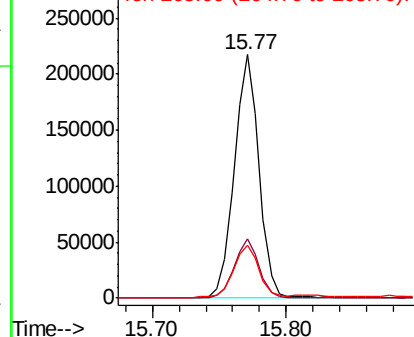

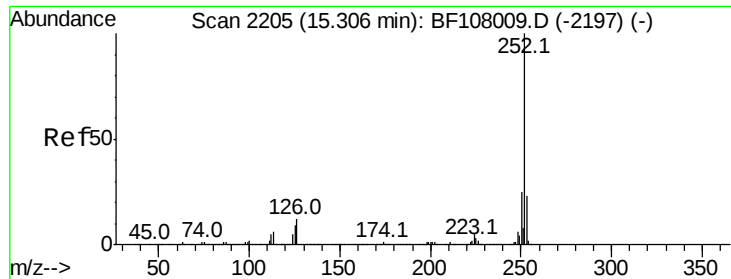





#87
Benzo(b)fluoranthene
Concen: 9.470 ng m
RT: 15.30 min Scan# 2204
Delta R.T. -0.01 min
Lab File: BF108218.D
Acq: 17 Aug 2018 1:53

Instrument :
BNA_F
ClientSampleId :
RA-081318-FL-017

Tot Ion	Ratio	Lower	Upper
252	100		
253	22.7	17.0	25.6
125	10.8	9.0	13.6




Manual Integrations
APPROVED


Sohil
8/17/2018 3:31:11 PM

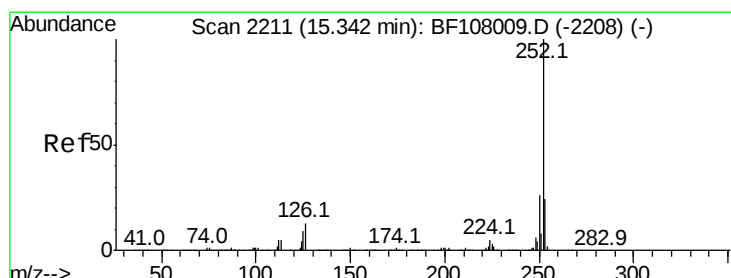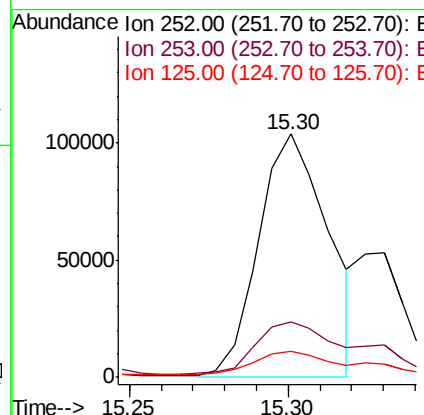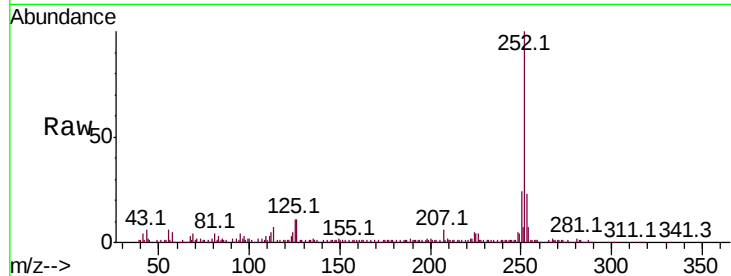

#88
Benzo(k)fluoranthene
Concen: 3.520 ng m
RT: 15.33 min Scan# 2209
Delta R.T. -0.01 min
Lab File: BF108218.D
Acq: 17 Aug 2018 1:53

Tgt Ion	Ratio	Lower	Upper
252	100		
253	26.5	17.9	26.9
125	10.5	10.2	15.2

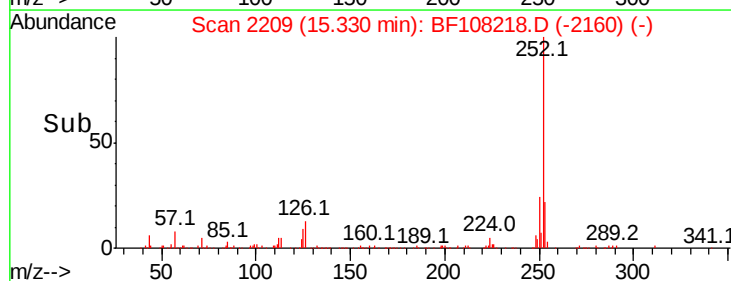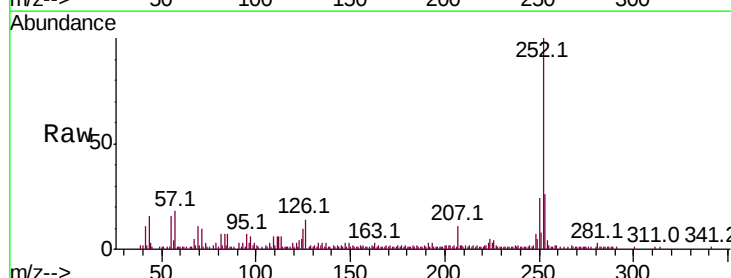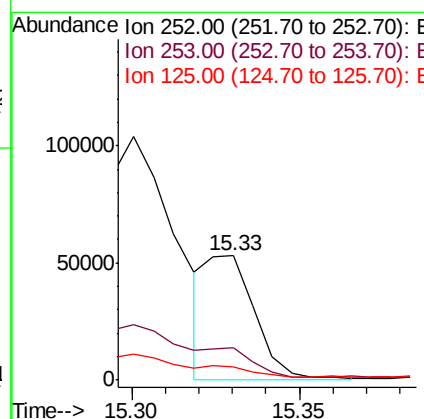

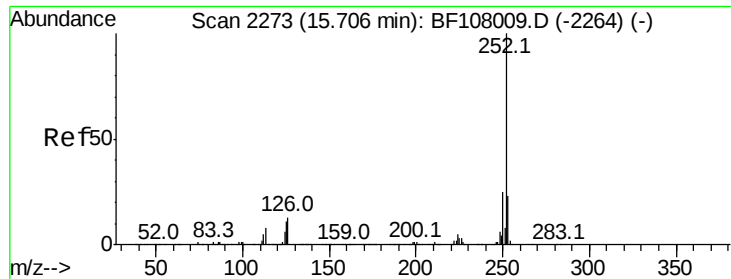





#89
Benzo(a)pyrene
Concen: 6.964 ng
RT: 15.70 min Scan# 2272
Delta R.T. -0.01 min
Lab File: BF108218.D
Acq: 17 Aug 2018 1:53

Instrument :
BNA_F
ClientSampleId :
RA-081318-FL-017

Tot Ion	Ratio	Lower	Upper
252	100		
253	22.7	17.1	25.7
125	11.0	9.8	14.6

Manual Integrations
APPROVED

Sohil
8/17/2018 3:31:11 PM

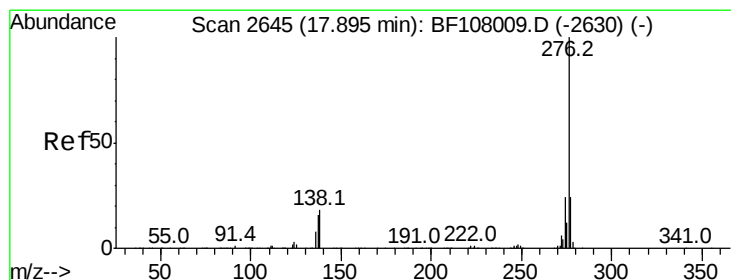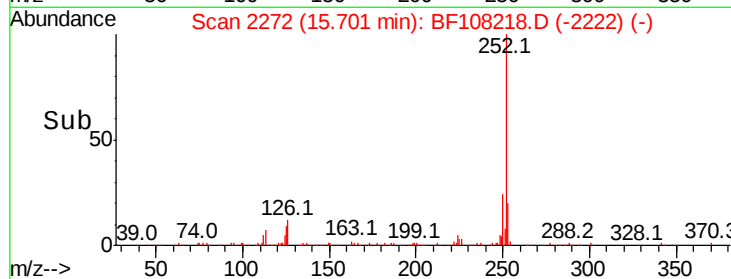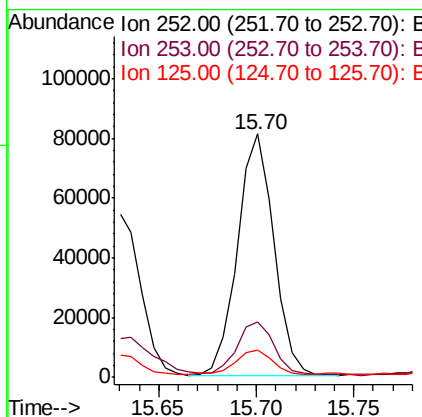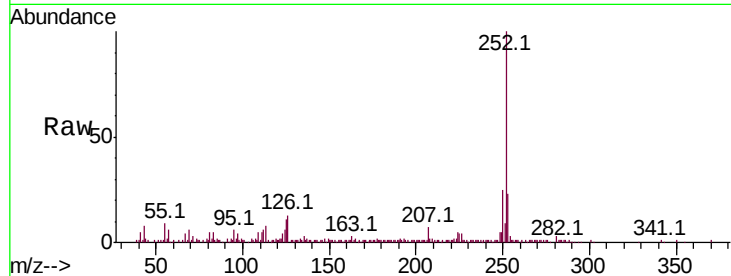

#91
Benzo(g,h,i)perylene
Concen: 4.104 ng
RT: 17.88 min Scan# 2642
Delta R.T. -0.02 min
Lab File: BF108218.D
Acq: 17 Aug 2018 1:53

Tgt Ion	Ratio	Lower	Upper
276	100		
277	25.6	17.9	26.9
138	24.5	21.8	32.8

