

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF081618\
 Data File : BF108226.D
 Acq On : 17 Aug 2018 5:32
 Operator : JU/SJ
 Sample : J4504-04
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 081418-DBRI-F-U-S

Quant Time: Aug 17 07:37:10 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 12:24:24 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.01	152	174804	20.00	ng	0.00
21) Naphthalene-d8	8.30	136	631031	20.00	ng	0.00
38) Acenaphthene-d10	10.06	164	301089	20.00	ng	0.00
63) Phenanthrene-d10	11.55	188	557117	20.00	ng	0.00
75) Chrysene-d12	14.21	240	477576	20.00	ng	-0.01
86) Perylene-d12	15.77	264	356248	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.64	112	410689	42.54	ng	0.00
7) Phenol-d6	6.62	99	335156	26.12	ng	0.00
23) Nitrobenzene-d5	7.58	82	1162693	102.82	ng	0.00
41) 2,4,6-Tribromophenol	10.85	330	293917	97.87	ng	0.00
44) 2-Fluorobiphenyl	9.37	172	2044340	109.01	ng	0.00
78) Terphenyl-d14	13.14	244	1952569	103.95	ng	0.00
Target Compounds						Qvalue
49) Dimethylphthalate	9.76	163	95810	4.568	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF081618\
Data File : BF108226.D
Acq On : 17 Aug 2018 5:32
Operator : JU/SJ
Sample : J4504-04
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
081418-DBRI-F-U-S

Quant Time: Aug 17 07:37:10 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 08 12:24:24 2018
Response via : Initial Calibration

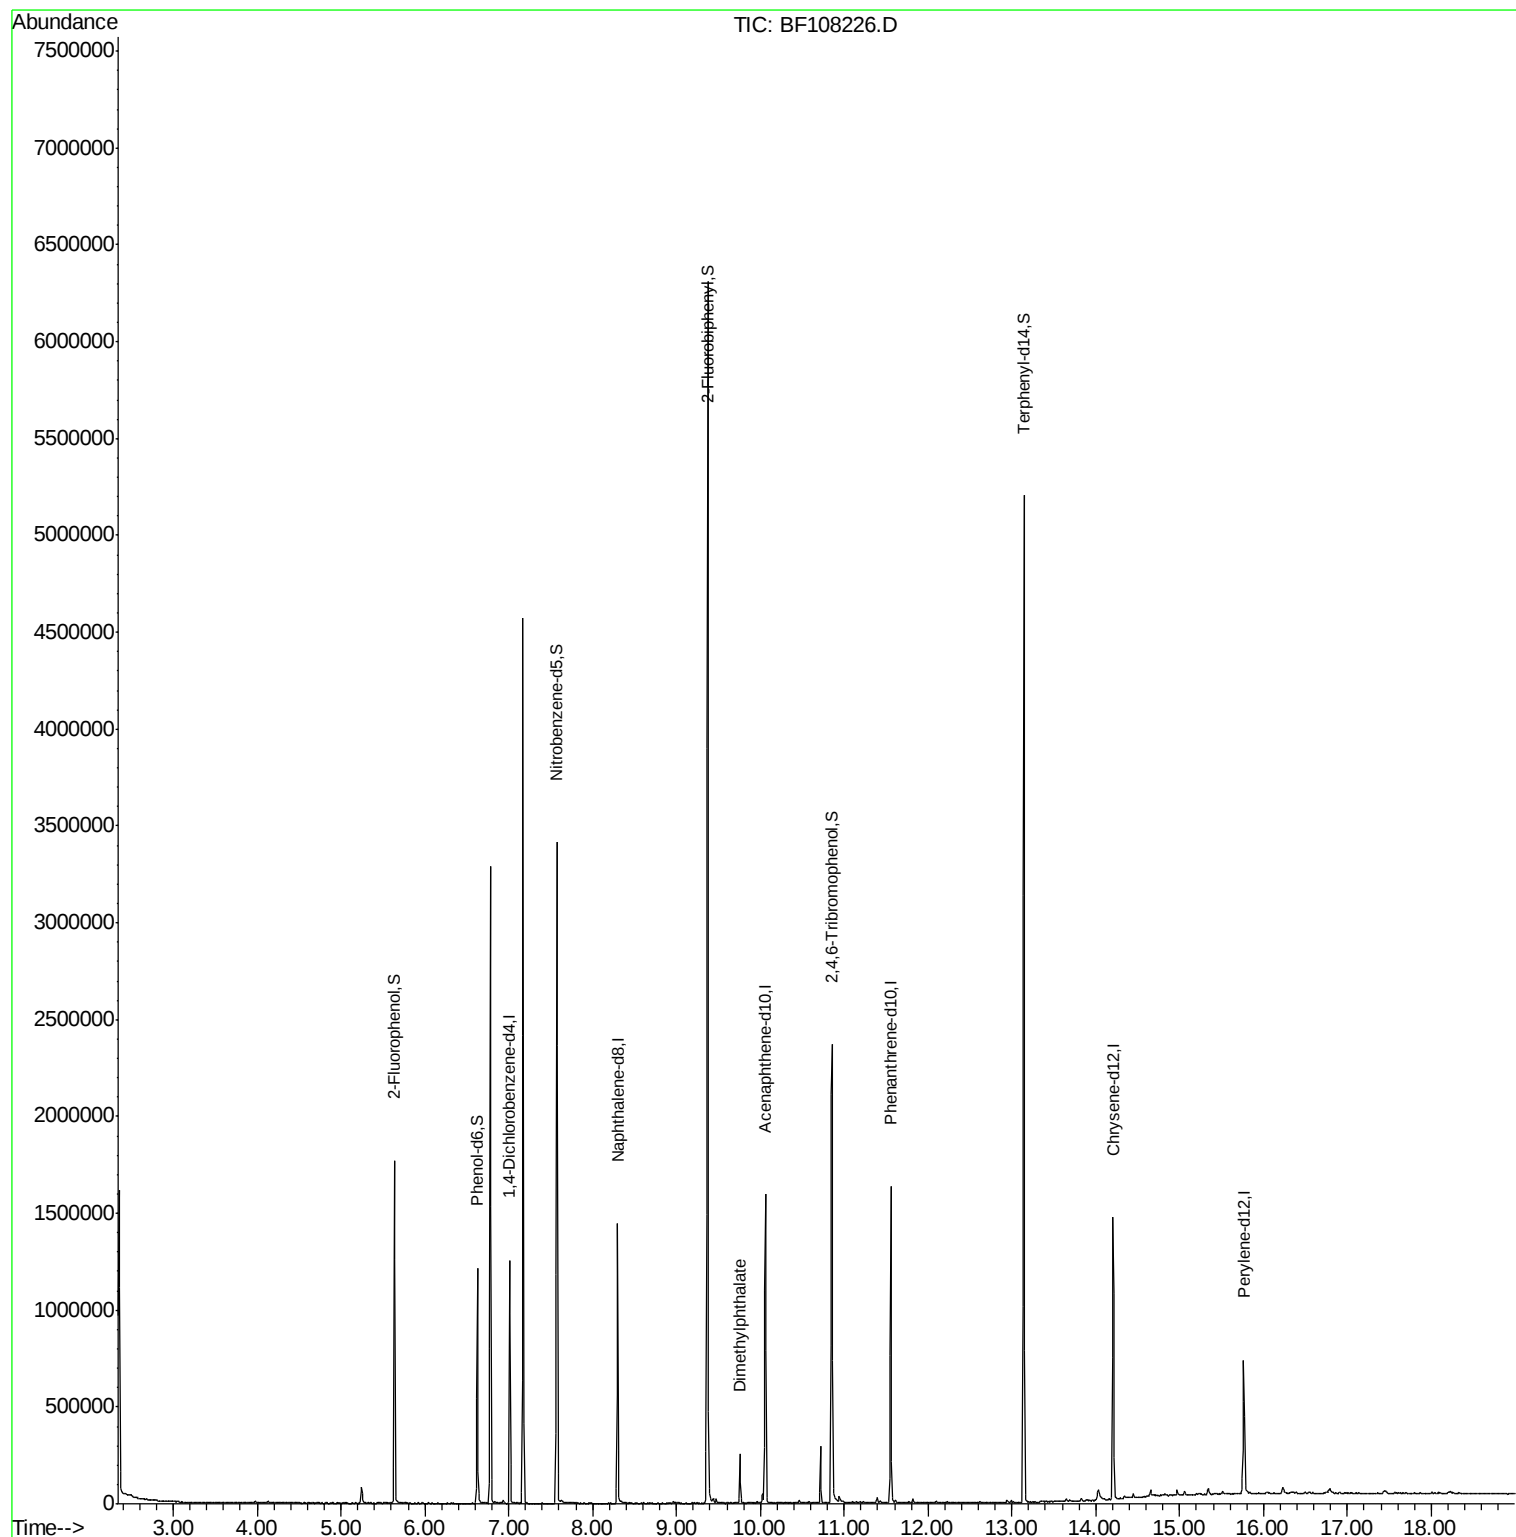




#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.01 min Scan# 795
Delta R.T. 0.00 min
Lab File: BF108226.D
Acq: 17 Aug 2018 5:32

Instrument :
BNA_F
ClientSampleId :
081418-DBRI-F-U-S

Tot Ion	Ratio	Lower	Upper
152	100		
150	157.2	124.6	186.8
115	60.5	50.1	75.1


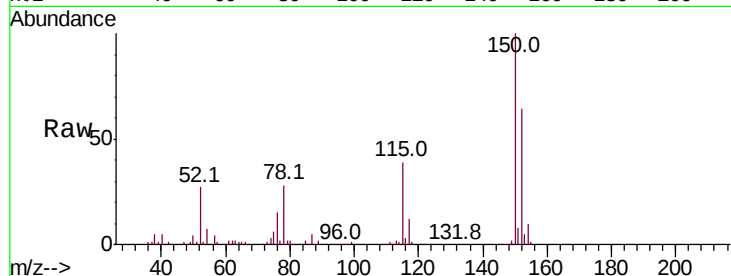


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

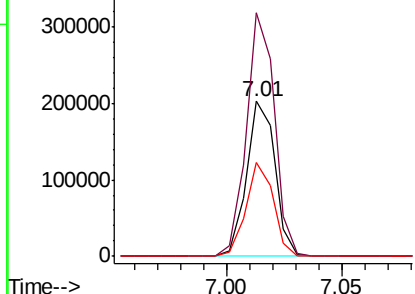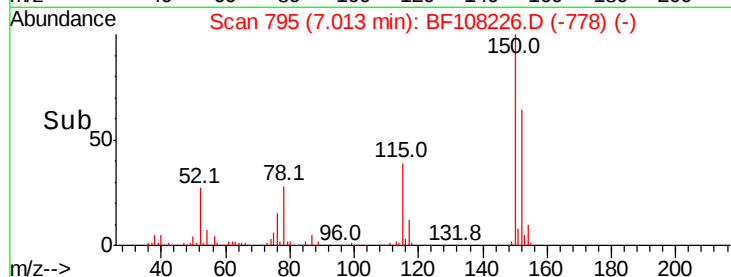

#5

2-Fluorophenol
Concen: 42.535 ng
RT: 5.64 min Scan# 561
Delta R.T. 0.01 min
Lab File: BF108226.D
Acq: 17 Aug 2018 5:32

Tgt Ion	Ratio	Lower	Upper
112	100		
64	70.3	47.9	71.9
63	36.7	23.7	35.5#


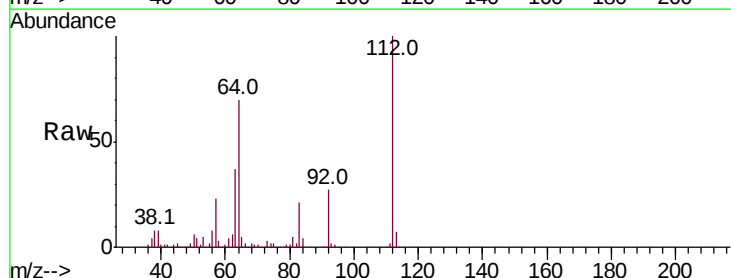


Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF1

Ion 63.00 (62.70 to 63.70): BF1

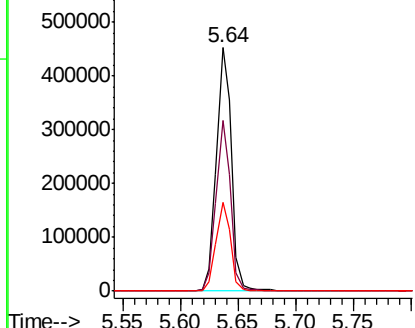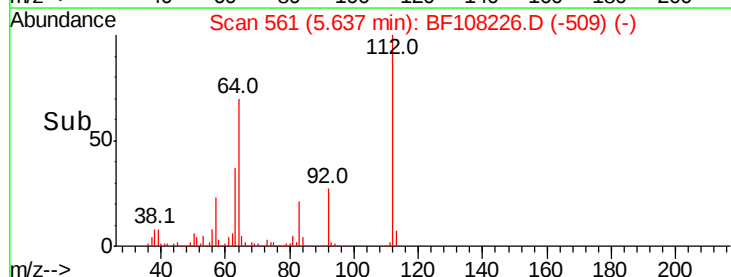



#7

Phenol-d6

Concen: 26.122 ng

RT: 6.62 min Scan# 729

Delta R.T. -0.01 min

Lab File: BF108226.D

Acq: 17 Aug 2018 5:32

Instrument :

BNA_F

ClientSampleId :

081418-DBRI-F-U-S


Tot Ion: 99 Resp: 335156

Ion Ratio Lower Upper




99 100

42 22.8 14.5 21.7#

71 34.8 25.4 38.0

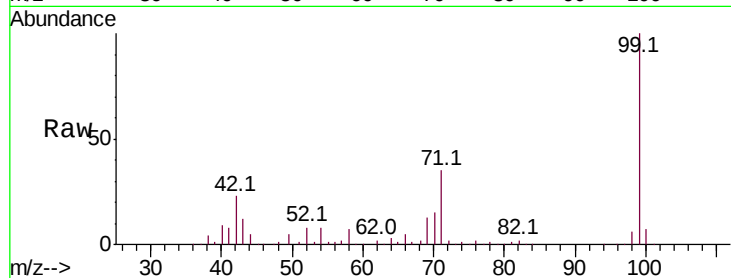

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

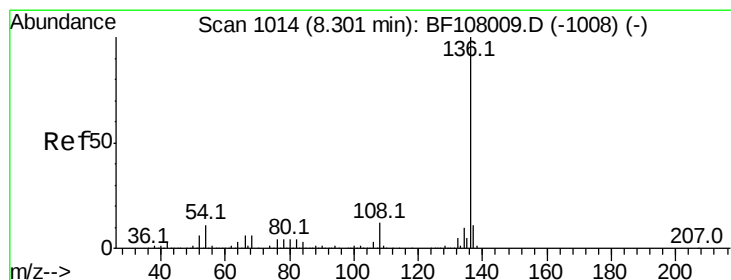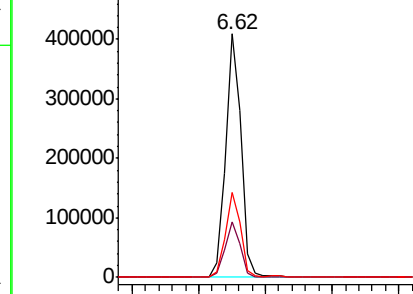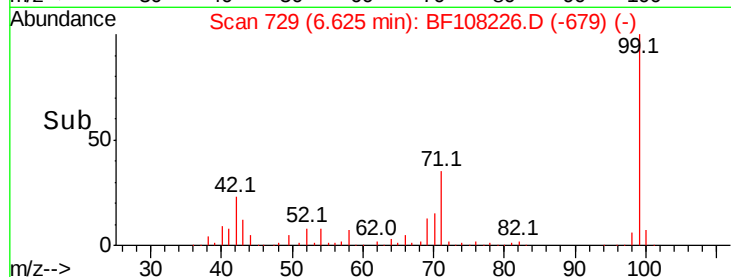

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.30 min Scan# 1013

Delta R.T. -0.01 min

Lab File: BF108226.D

Acq: 17 Aug 2018 5:32

Tgt Ion: 136 Resp: 631031


Ion Ratio Lower Upper

136 100



137 11.4 8.9 13.3

54 10.8 6.6 9.8#

68 6.4 5.0 7.4

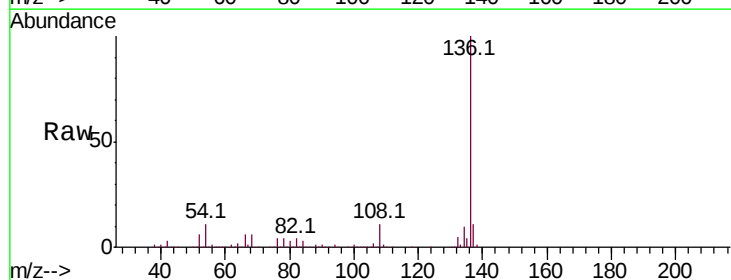

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

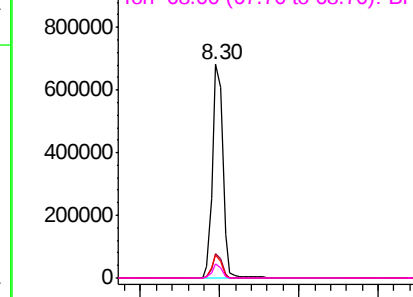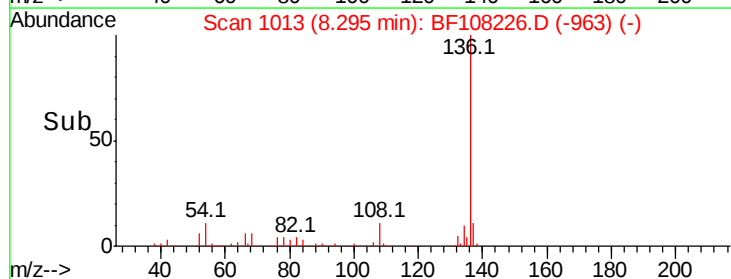



#23

Nitrobenzene-d5

Concen: 102.816 ng

RT: 7.58 min Scan# 891

Delta R.T. 0.00 min

Lab File: BF108226.D

Acq: 17 Aug 2018 5:32

Instrument :

BNA_F

ClientSampleId :

081418-DBRI-F-U-S


Tot Ion: 82 Resp: 1162693

Ion Ratio Lower Upper

82 100

128 41.2 36.1 54.1




54 58.9 41.4 62.2

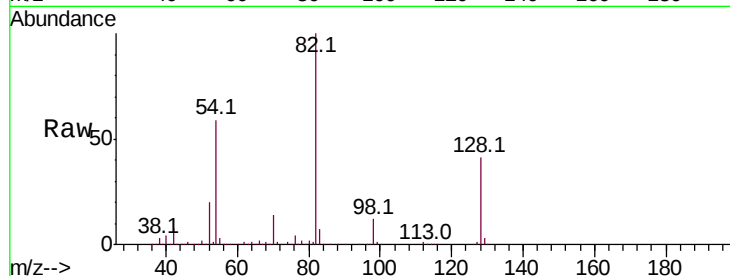

Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 128.00 (127.70 to 128.70): BF1

Ion 54.00 (53.70 to 54.70): BF1

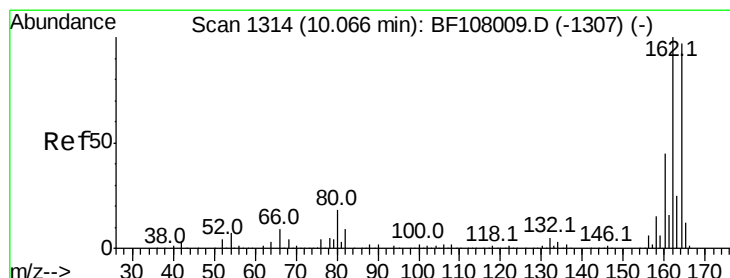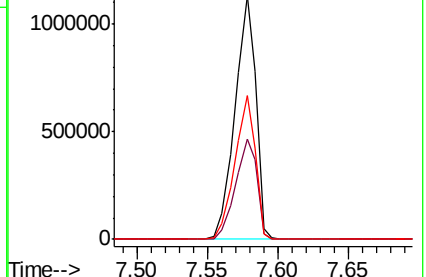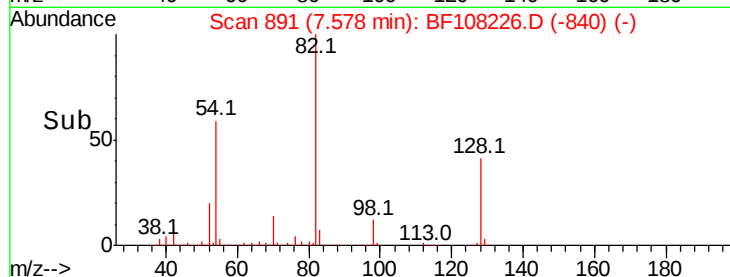

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 10.06 min Scan# 1313

Delta R.T. -0.01 min

Lab File: BF108226.D

Acq: 17 Aug 2018 5:32


Tgt Ion:164 Resp: 301089

Ion Ratio Lower Upper

164 100

162 100.1 86.1 129.1



160 46.4 38.3 57.5

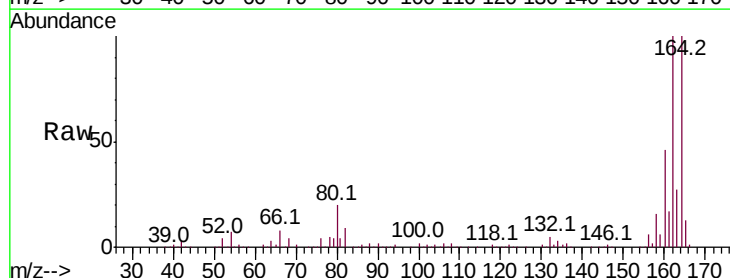

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

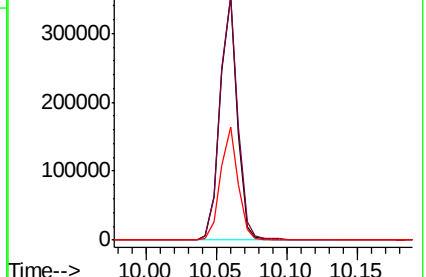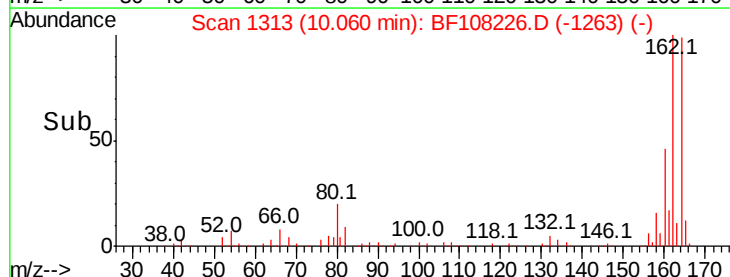






#41
 2,4,6-Tribromophenol
 Concen: 97.865 ng
 RT: 10.85 min Scan# 1448
 Delta R.T. -0.01 min
 Lab File: BF108226.D
 Acq: 17 Aug 2018 5:32

Instrument :
 BNA_F
 ClientSampleId :
 081418-DBRI-F-U-S

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.8	77.0	115.6
141	32.8	29.9	44.9

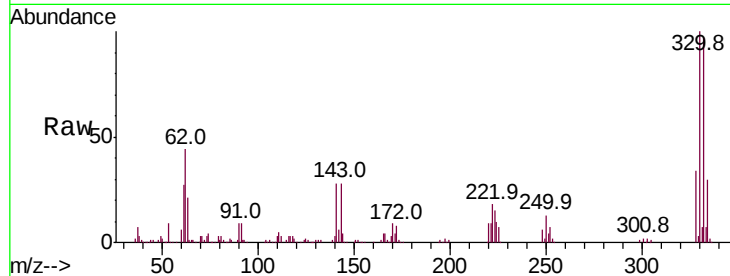


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

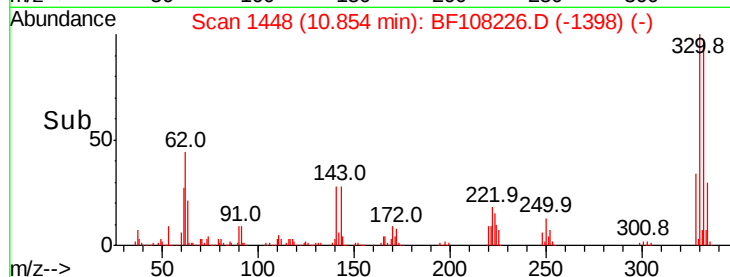
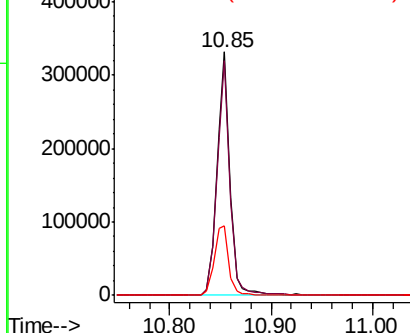


#44
 2-Fluorobiphenyl
 Concen: 109.008 ng
 RT: 9.37 min Scan# 1196
 Delta R.T. -0.01 min
 Lab File: BF108226.D
 Acq: 17 Aug 2018 5:32

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.5	29.7	44.5
170	25.6	19.6	29.4

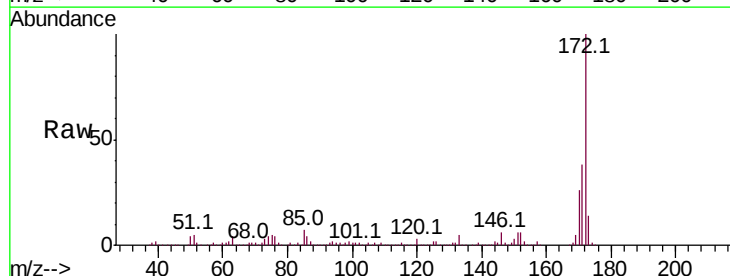

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

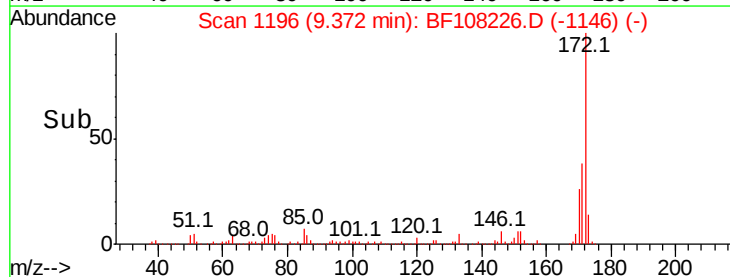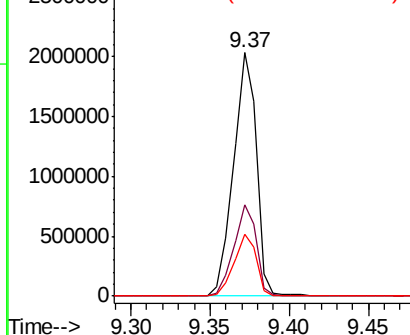







#49
Dimethylphthalate
Concen: 4.568 ng
RT: 9.76 min Scan# 1262
Delta R.T. -0.02 min
Lab File: BF108226.D
Acq: 17 Aug 2018 5:32

Instrument :
BNA_F
ClientSampleId :
081418-DBRI-F-U-S

Tot Ion:163 Resp: 95810
Ion Ratio Lower Upper
163 100
194 3.9 2.7 4.1
164 9.7 8.2 12.2

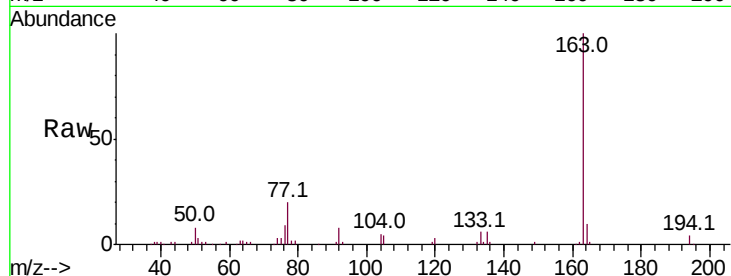


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

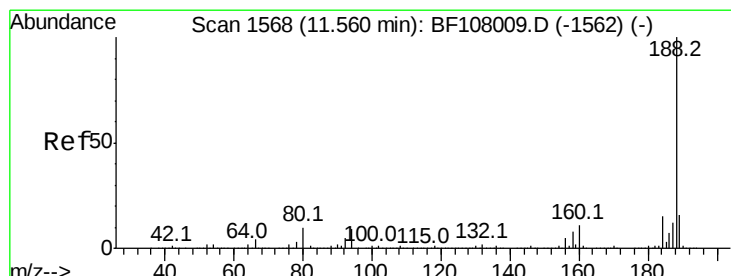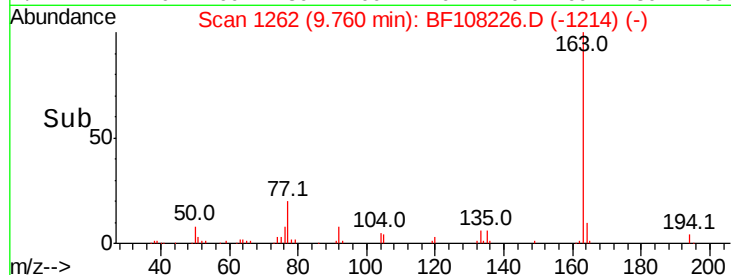
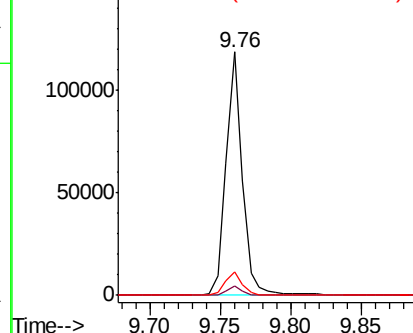



#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.55 min Scan# 1567
Delta R.T. -0.01 min
Lab File: BF108226.D
Acq: 17 Aug 2018 5:32

Tgt Ion:188 Resp: 557117
Ion Ratio Lower Upper
188 100
94 9.4 8.5 12.7
80 10.2 9.2 13.8

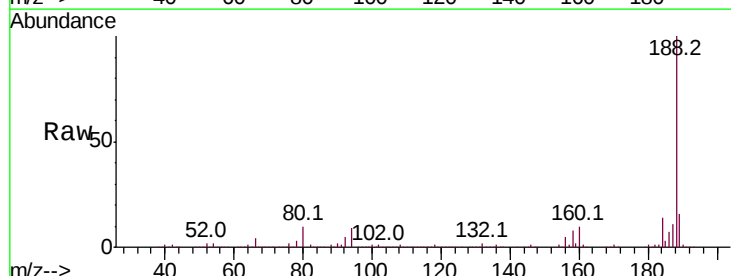

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1

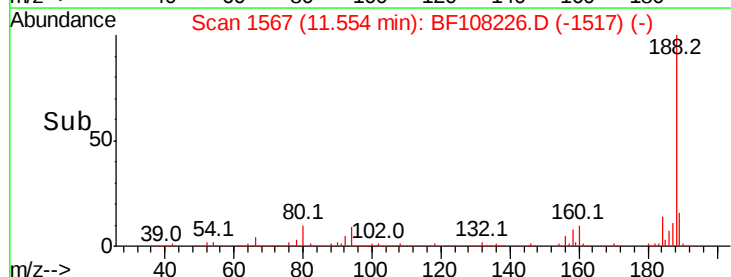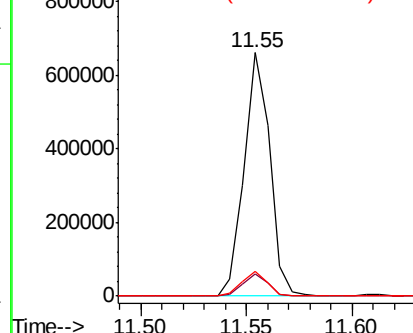

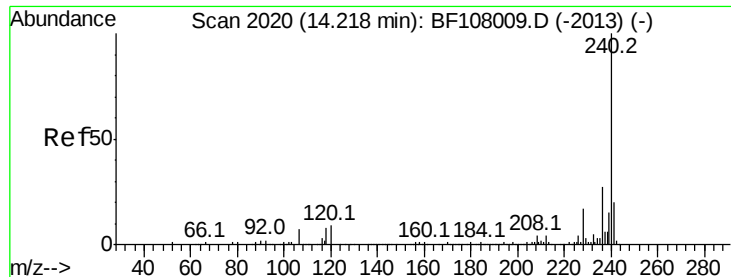

#75

Chrysene-d12

Concen: 20.000 ng

RT: 14.21 min Scan# 2018

Delta R.T. -0.01 min

Lab File: BF108226.D

Acq: 17 Aug 2018 5:32

Instrument :

BNA_F

ClientSampleId :

081418-DBRI-F-U-S


Tot Ion:240 Resp: 477576

Ion Ratio Lower Upper

240 100

120 10.7 9.5 14.3



236 26.3 20.7 31.1

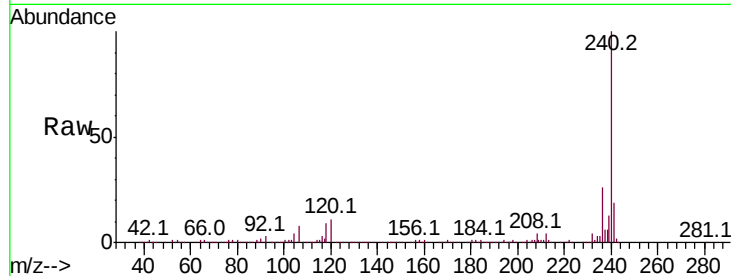

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

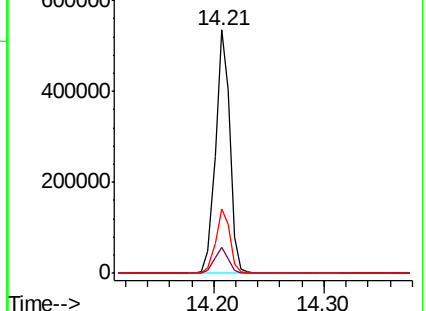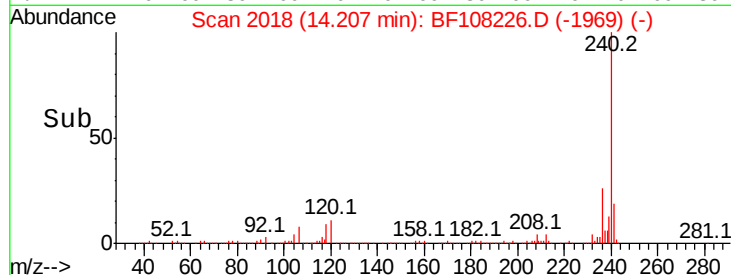

#78

Terphenyl-d14

Concen: 103.953 ng

RT: 13.14 min Scan# 1837

Delta R.T. -0.01 min

Lab File: BF108226.D

Acq: 17 Aug 2018 5:32


Tgt Ion:244 Resp: 1952569

Ion Ratio Lower Upper

244 100

212 7.6 5.4 8.0



122 11.4 11.0 16.4

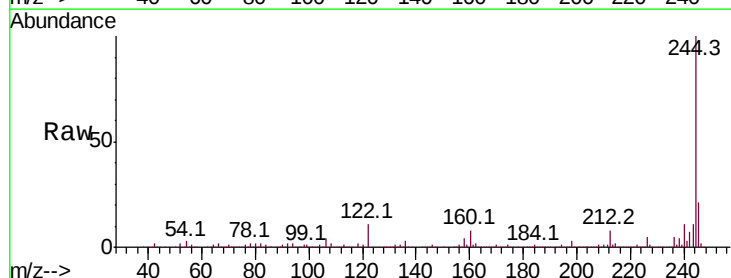

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

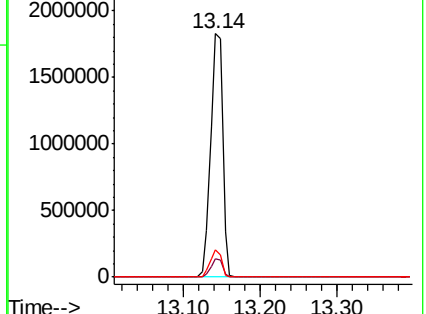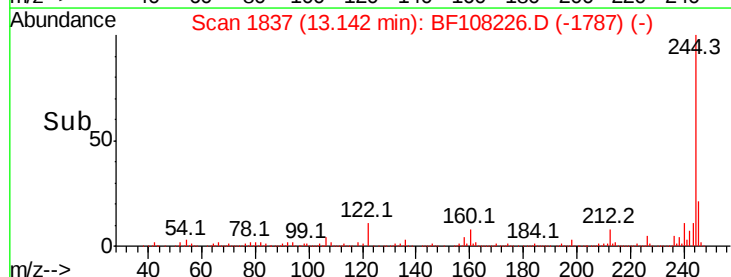



#86
Pervlene-d12
Concen: 20.000 ng
RT: 15.77 min Scan# 2284
Delta R.T. -0.01 min
Lab File: BF108226.D
Acq: 17 Aug 2018 5:32

Instrument :
BNA_F
ClientSampleId :
081418-DBRI-F-U-S

Tot Ion	Ratio	Lower	Upper
264	100		
260	24.3	19.2	28.8
265	21.4	17.5	26.3

