

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF081618\
 Data File : BF108211.D
 Acq On : 16 Aug 2018 22:41
 Operator : JU/SJ
 Sample : J4499-06 5X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 LSB-06(0-1)

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.243	490	494	498	rVB	28917	28936	2.21%	0.256%
2	5.631	556	560	568	rBV	582450	522757	39.87%	4.616%
3	6.625	725	729	742	rVB	672106	555862	42.39%	4.908%
4	6.778	752	755	759	rBV	650593	565605	43.14%	4.994%
5	7.013	792	795	799	rBV	1141088	988965	75.43%	8.733%
6	7.172	818	822	825	rBV	549027	452401	34.50%	3.995%
7	7.572	886	890	893	rBV	434345	348630	26.59%	3.079%
8	8.301	1010	1014	1017	rBV	1420241	1243651	94.85%	10.982%
9	9.372	1192	1196	1205	rBV	675809	656847	50.10%	5.800%
10	9.437	1205	1207	1210	rVB2	17984	15198	1.16%	0.134%
11	9.760	1257	1262	1267	rBV	43039	40578	3.09%	0.358%
12	9.966	1294	1297	1301	rVB	15716	14500	1.11%	0.128%
13	10.060	1309	1313	1324	rBV2	1459416	1311175	100.00%	11.578%
14	10.472	1380	1383	1387	rVB	18270	15521	1.18%	0.137%
15	10.848	1444	1447	1454	rBV	298896	293447	22.38%	2.591%
16	10.942	1461	1463	1469	rVB	18162	17534	1.34%	0.155%
17	11.395	1535	1540	1543	rBV	18821	13972	1.07%	0.123%
18	11.554	1564	1567	1571	rBV	1243291	1186189	90.47%	10.474%
19	11.825	1610	1613	1616	rBV	13703	14532	1.11%	0.128%
20	12.778	1771	1775	1777	rBV	39539	37418	2.85%	0.330%
21	13.007	1808	1814	1821	rVB2	34700	46029	3.51%	0.406%
22	13.136	1833	1836	1840	rBV	605857	560694	42.76%	4.951%
23	13.383	1875	1878	1883	rVB4	14849	16475	1.26%	0.145%
24	13.824	1950	1953	1955	rBV	24623	23928	1.82%	0.211%
25	14.030	1985	1988	1991	rBV4	18371	25735	1.96%	0.227%
26	14.213	2014	2019	2022	rBV	1199757	1219985	93.05%	10.773%
27	14.236	2022	2023	2029	rVB3	66207	50133	3.82%	0.443%
28	14.624	2086	2089	2092	rBV2	51846	58004	4.42%	0.512%
29	15.030	2155	2158	2162	rBV2	36927	48195	3.68%	0.426%
30	15.489	2234	2236	2240	rVB3	32490	35447	2.70%	0.313%
31	15.771	2279	2284	2294	rVB	688756	916224	69.88%	8.091%


Sum of corrected areas: 11324567

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF081618\
Data File : BF108211.D
Acq On : 16 Aug 2018 22:41
Operator : JU/SJ
Sample : J4499-06 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LSB-06(0-1)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

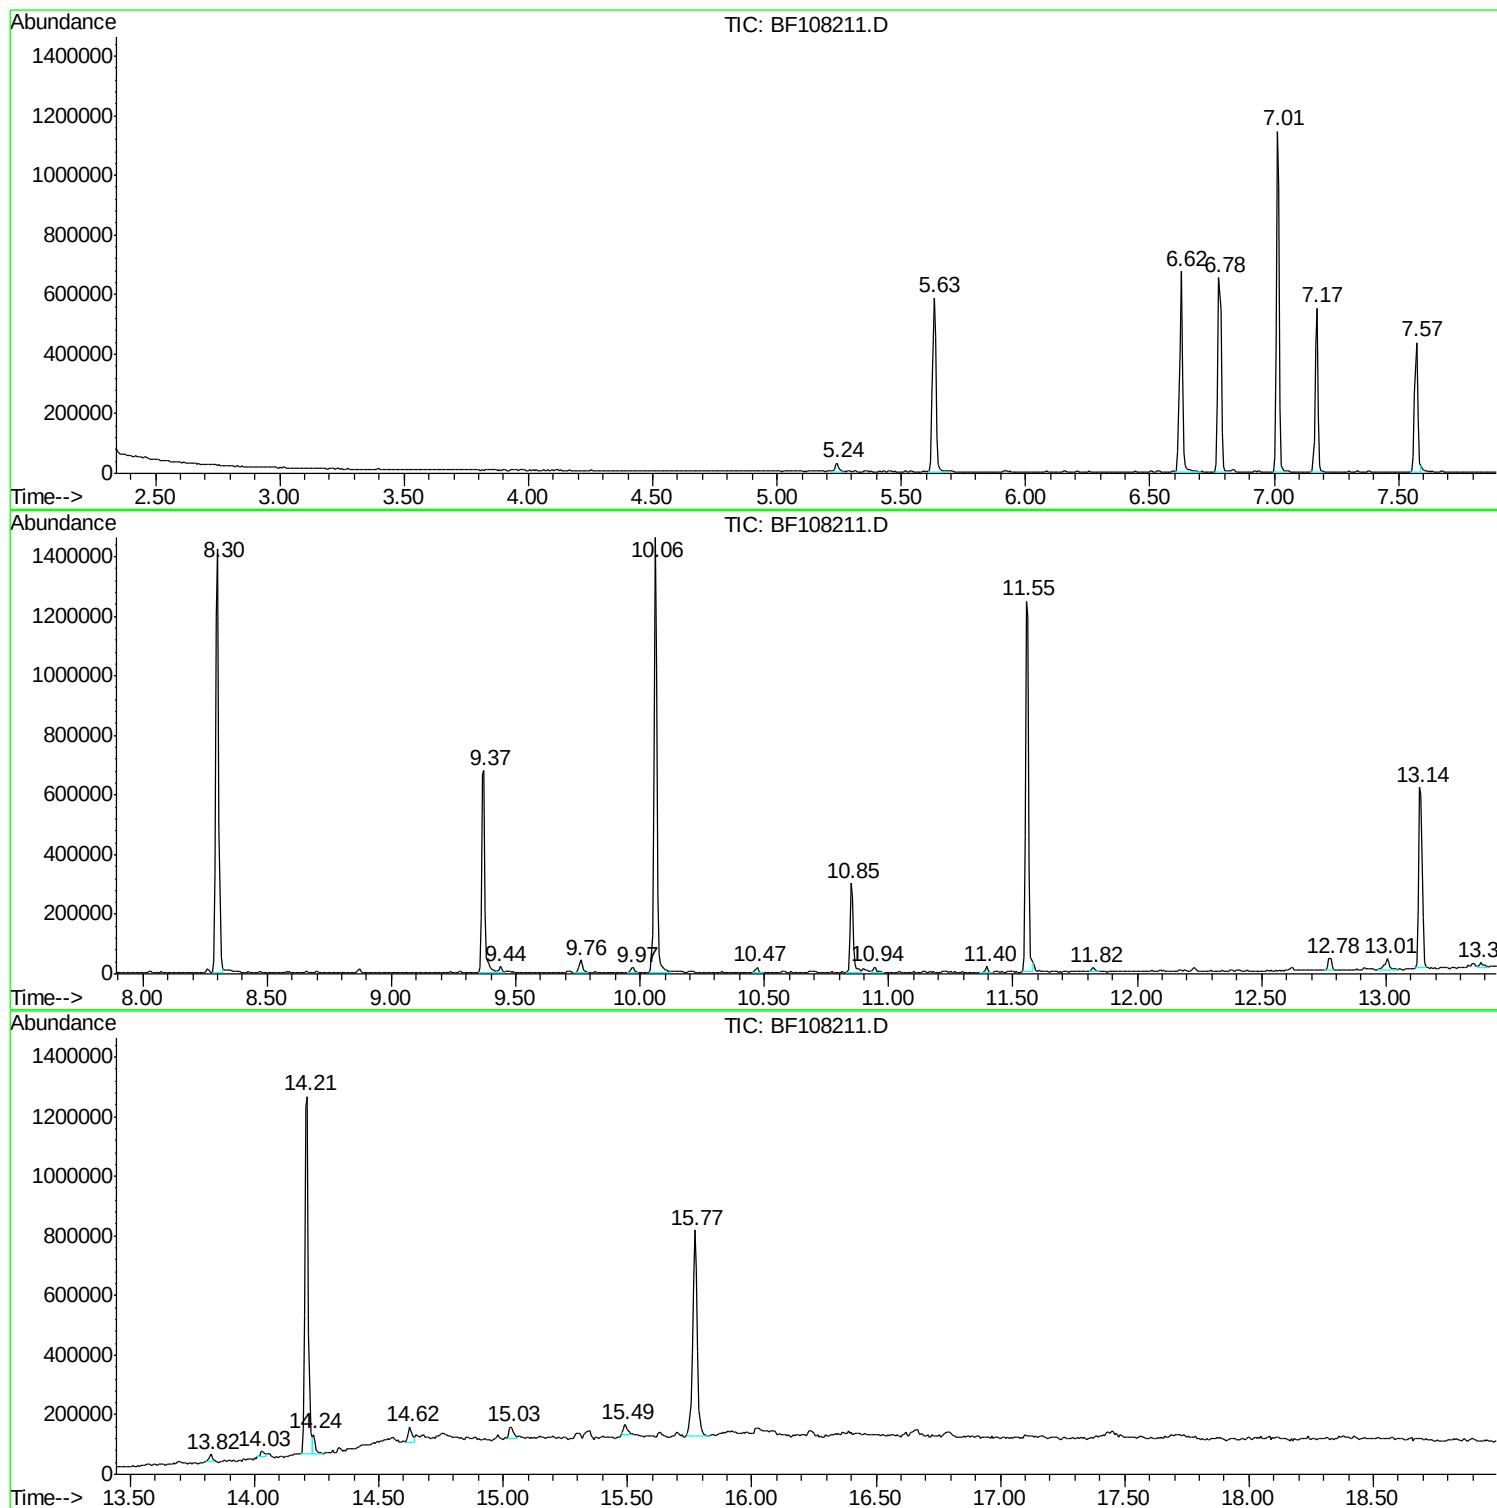

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF081618\
Data File : BF108211.D
Acq On : 16 Aug 2018 22:41
Operator : JU/SJ
Sample : J4499-06 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LSB-06(0-1)










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.78 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.78	11.44 ng	565605	1,4-Dichlorobenzene-d4	7.01

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
3		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	10
4		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
5		1,3,4-Thiadiazole-2(3H)-thione, ...	132	C3H4N2S2	029490-19-5	9

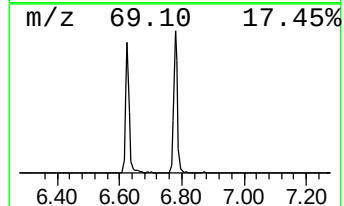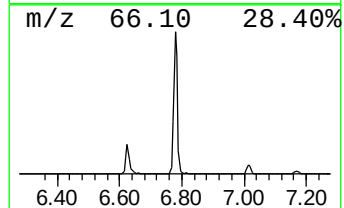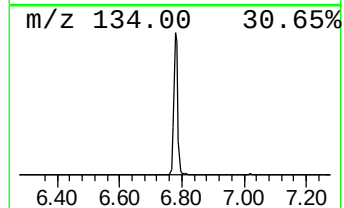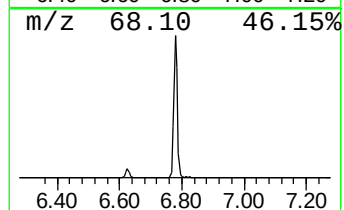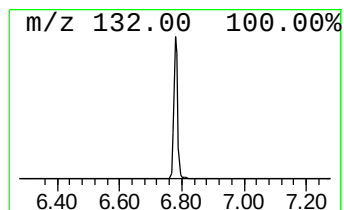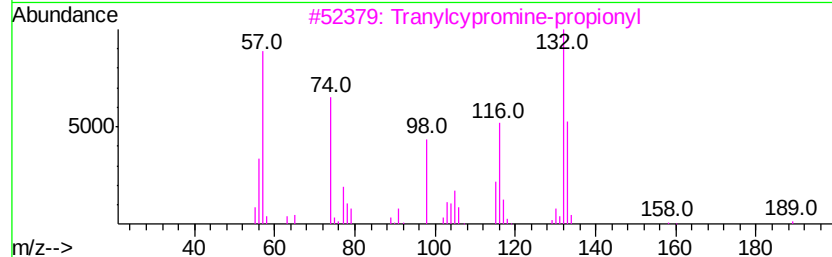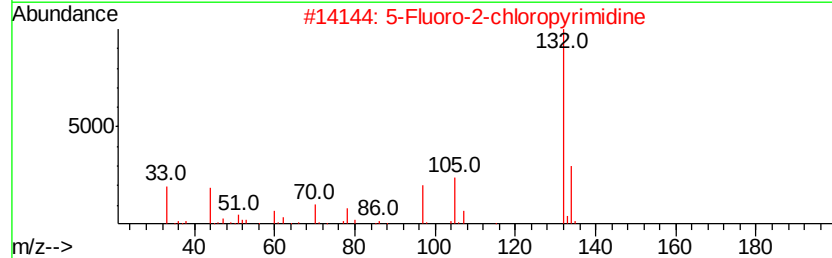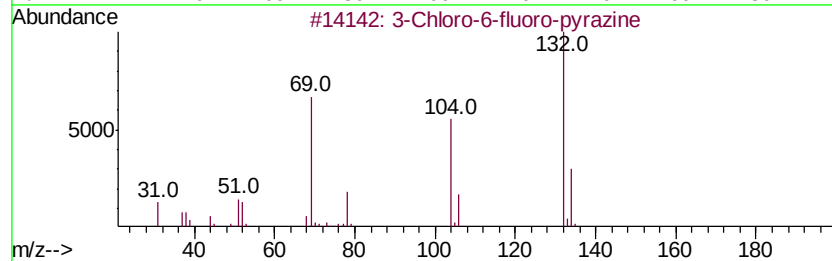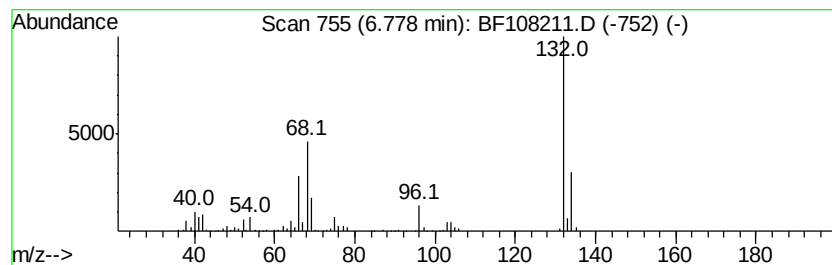

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF081618\
Data File : BF108211.D
Acq On : 16 Aug 2018 22:41
Operator : JU/SJ
Sample : J4499-06 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LSB-06(0-1)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.78	6.78	11.4	ng	565605	1	7.01	988965	20.0