

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081618\
 Data File : BF108222.D
 Acq On : 17 Aug 2018 3:43
 Operator : JU/SJ
 Sample : J4479-01
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DSN-001A-081418

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.366	3	5	13	rVB	1645313	1743452	31.95%	4.401%
2	5.254	492	496	503	rBV	371152	416270	7.63%	1.051%
3	5.643	555	562	565	rBV	2707569	2483922	45.51%	6.270%
4	5.878	598	602	605	rBV	932119	781810	14.33%	1.973%
5	5.907	605	607	613	rVB	160364	131409	2.41%	0.332%
6	6.631	725	730	733	rBV	1762521	1473552	27.00%	3.720%
7	6.784	752	756	760	rBV	3926227	3918292	71.80%	9.890%
8	7.013	792	795	799	rBV	1152919	994957	18.23%	2.511%
9	7.060	800	803	813	rVB2	108016	120541	2.21%	0.304%
10	7.172	818	822	826	rBV	3937178	3734474	68.43%	9.427%
11	7.266	834	838	842	rBV	390800	312153	5.72%	0.788%
12	7.354	851	853	859	rVB	76269	71513	1.31%	0.181%
13	7.413	859	863	866	rVB	61820	55880	1.02%	0.141%
14	7.578	886	891	894	rBV	3044409	3081229	56.46%	7.778%
15	7.842	934	936	939	rBV	76170	62926	1.15%	0.159%
16	7.942	949	953	958	rBV2	126420	154180	2.83%	0.389%
17	8.137	982	986	989	rBV	102123	92272	1.69%	0.233%
18	8.231	999	1002	1009	rVB	98403	101561	1.86%	0.256%
19	8.295	1009	1013	1016	rBV	1242302	1207927	22.13%	3.049%
20	8.578	1057	1061	1064	rBV	289619	257352	4.72%	0.650%
21	8.654	1070	1074	1081	rVB	98677	108355	1.99%	0.274%
22	8.972	1123	1128	1132	rBV	160160	175316	3.21%	0.443%
23	9.372	1191	1196	1199	rBV	5483047	5457436	100.00%	13.776%
24	10.060	1309	1313	1317	rBV	1522923	1277015	23.40%	3.223%
25	10.854	1443	1448	1460	rBV	3254598	3117619	57.13%	7.869%
26	11.554	1563	1567	1570	rBV	1335611	1227709	22.50%	3.099%
27	11.783	1601	1606	1609	rBV2	50223	63119	1.16%	0.159%
28	12.266	1685	1688	1698	rBV	67578	97711	1.79%	0.247%
29	13.148	1833	1838	1841	rBV	4756479	4844288	88.76%	12.228%
30	14.030	1985	1988	1992	rBV	41847	59217	1.09%	0.149%
31	14.207	2014	2018	2022	rBV	1216776	1127450	20.66%	2.846%
32	15.060	2161	2163	2167	rVB	55654	56991	1.04%	0.144%
33	15.771	2278	2284	2289	rBV	597364	808828	14.82%	2.042%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081618\
Data File : BF108222.D
Acq On : 17 Aug 2018 3:43
Operator : JU/SJ
Sample : J4479-01
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DSN-001A-081418

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION


Sum of corrected areas: 39616726

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081618\
Data File : BF108222.D
Acq On : 17 Aug 2018 3:43
Operator : JU/SJ
Sample : J4479-01
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DSN-001A-081418

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

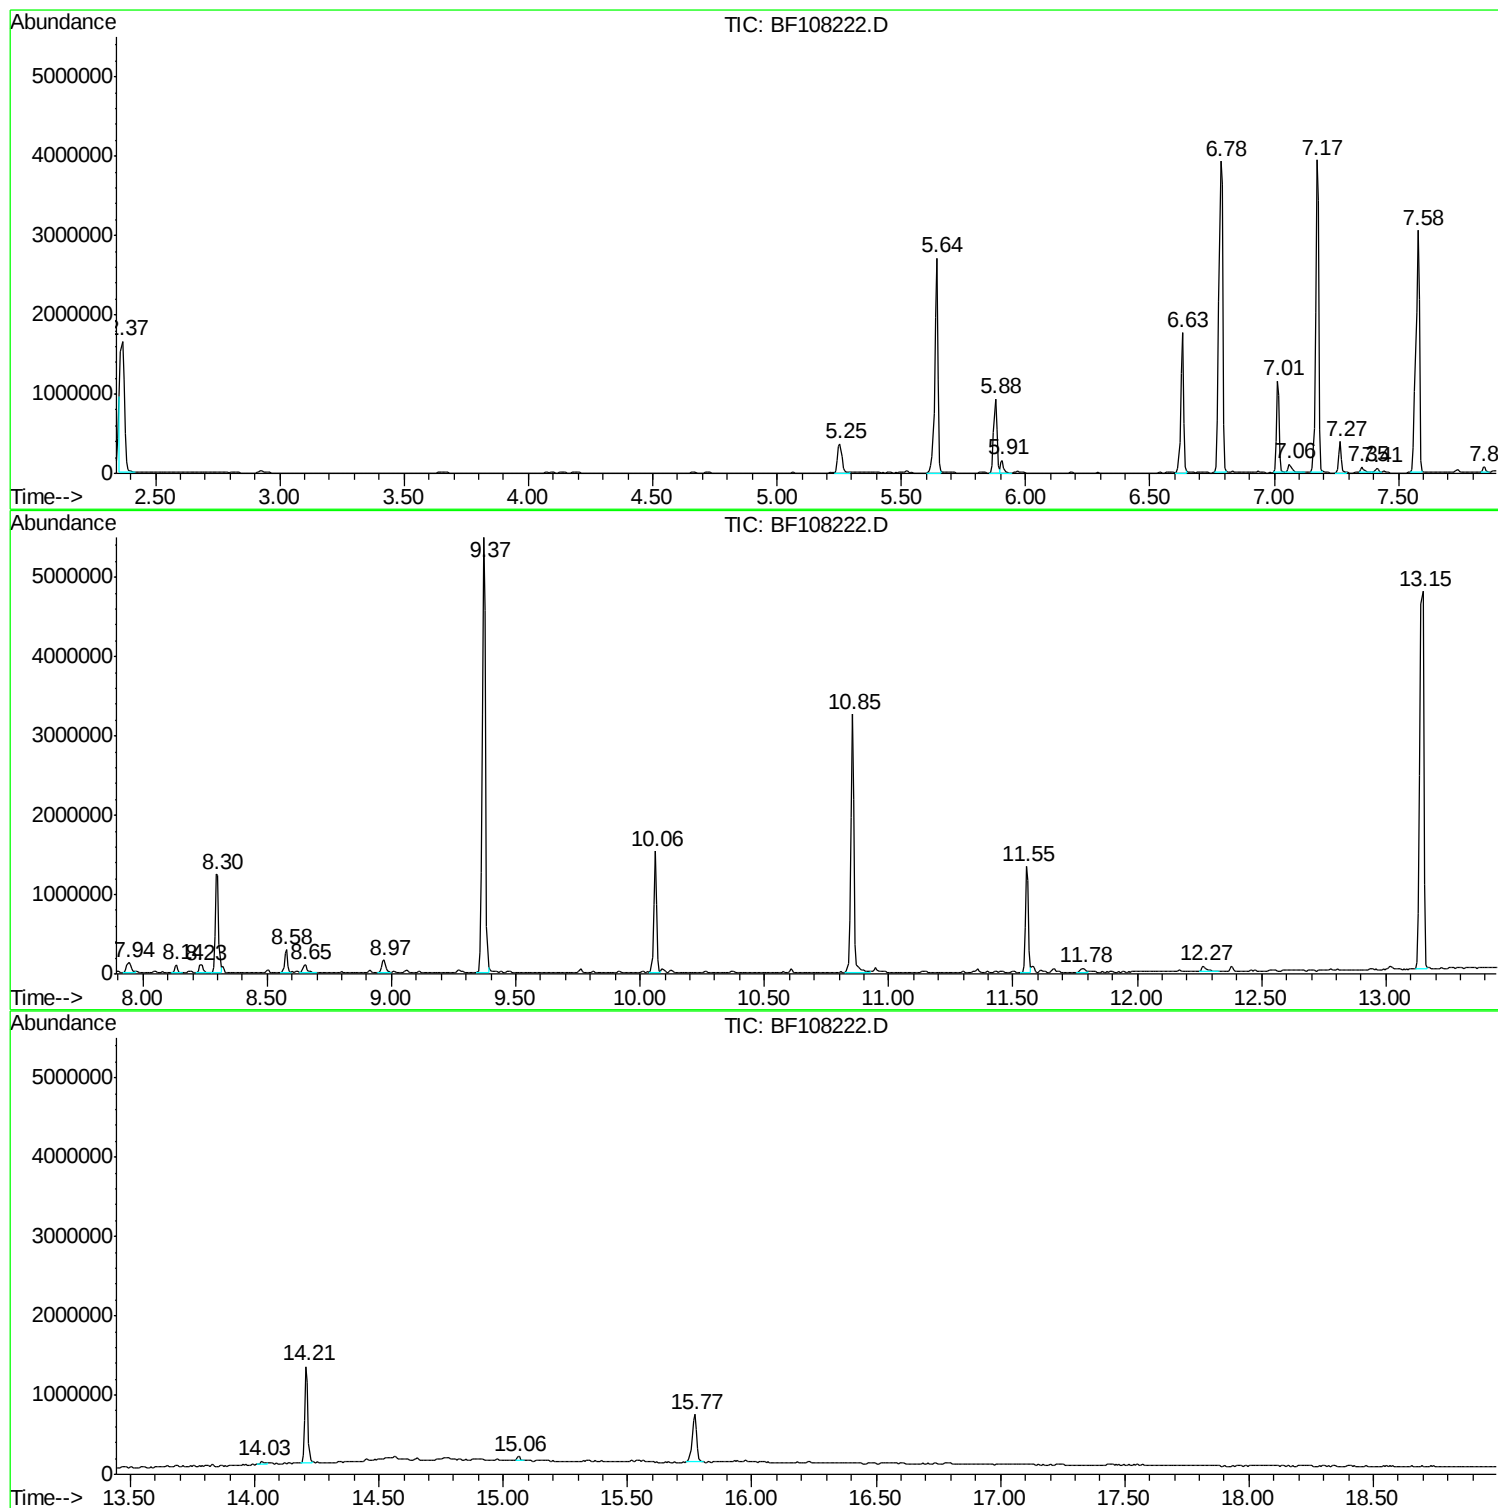

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081618\
Data File : BF108222.D
Acq On : 17 Aug 2018 3:43
Operator : JU/SJ
Sample : J4479-01
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DSN-001A-081418

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081618\
Data File : BF108222.D
Acq On : 17 Aug 2018 3:43
Operator : JU/SJ
Sample : J4479-01
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DSN-001A-081418

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc