

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF081618\
 Data File : BF108223.D
 Acq On : 17 Aug 2018 4:10
 Operator : JU/SJ
 Sample : J4504-01
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 081418-DBRI-F-D-B

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.248	492	495	503	rVB	97759	97903	1.75%	0.298%
2	5.636	557	561	565	rBV	1658911	1597305	28.62%	4.857%
3	6.625	725	729	734	rBV	1217084	1090859	19.55%	3.317%
4	6.783	752	756	759	rBV	3223698	2785272	49.90%	8.469%
5	7.013	792	795	799	rBV	1138231	981341	17.58%	2.984%
6	7.172	818	822	826	rBV	4208358	3863403	69.22%	11.747%
7	7.577	886	891	894	rBV	3169943	3198924	57.32%	9.727%
8	8.301	1009	1014	1017	rBV	1225623	1165263	20.88%	3.543%
9	9.372	1191	1196	1199	rBV	5701846	5581196	100.00%	16.970%
10	9.760	1258	1262	1266	rBV	183921	146258	2.62%	0.445%
11	10.060	1309	1313	1321	rVB	1423375	1229621	22.03%	3.739%
12	10.718	1421	1425	1428	rBV	662860	511538	9.17%	1.555%
13	10.854	1443	1448	1457	rBV	2140649	2072479	37.13%	6.302%
14	11.554	1563	1567	1571	rBV	1338073	1175032	21.05%	3.573%
15	13.148	1833	1838	1841	rBV	4678755	4833654	86.61%	14.697%
16	14.030	1984	1988	1999	rBV	165147	284879	5.10%	0.866%
17	14.206	2014	2018	2022	rBV	1303227	1230354	22.04%	3.741%
18	15.771	2278	2284	2294	rVB	683719	968362	17.35%	2.944%
19	16.236	2358	2363	2370	rBV	41900	74713	1.34%	0.227%


Sum of corrected areas: 32888356

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF081618\
Data File : BF108223.D
Acq On : 17 Aug 2018 4:10
Operator : JU/SJ
Sample : J4504-01
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
081418-DBRI-F-D-B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

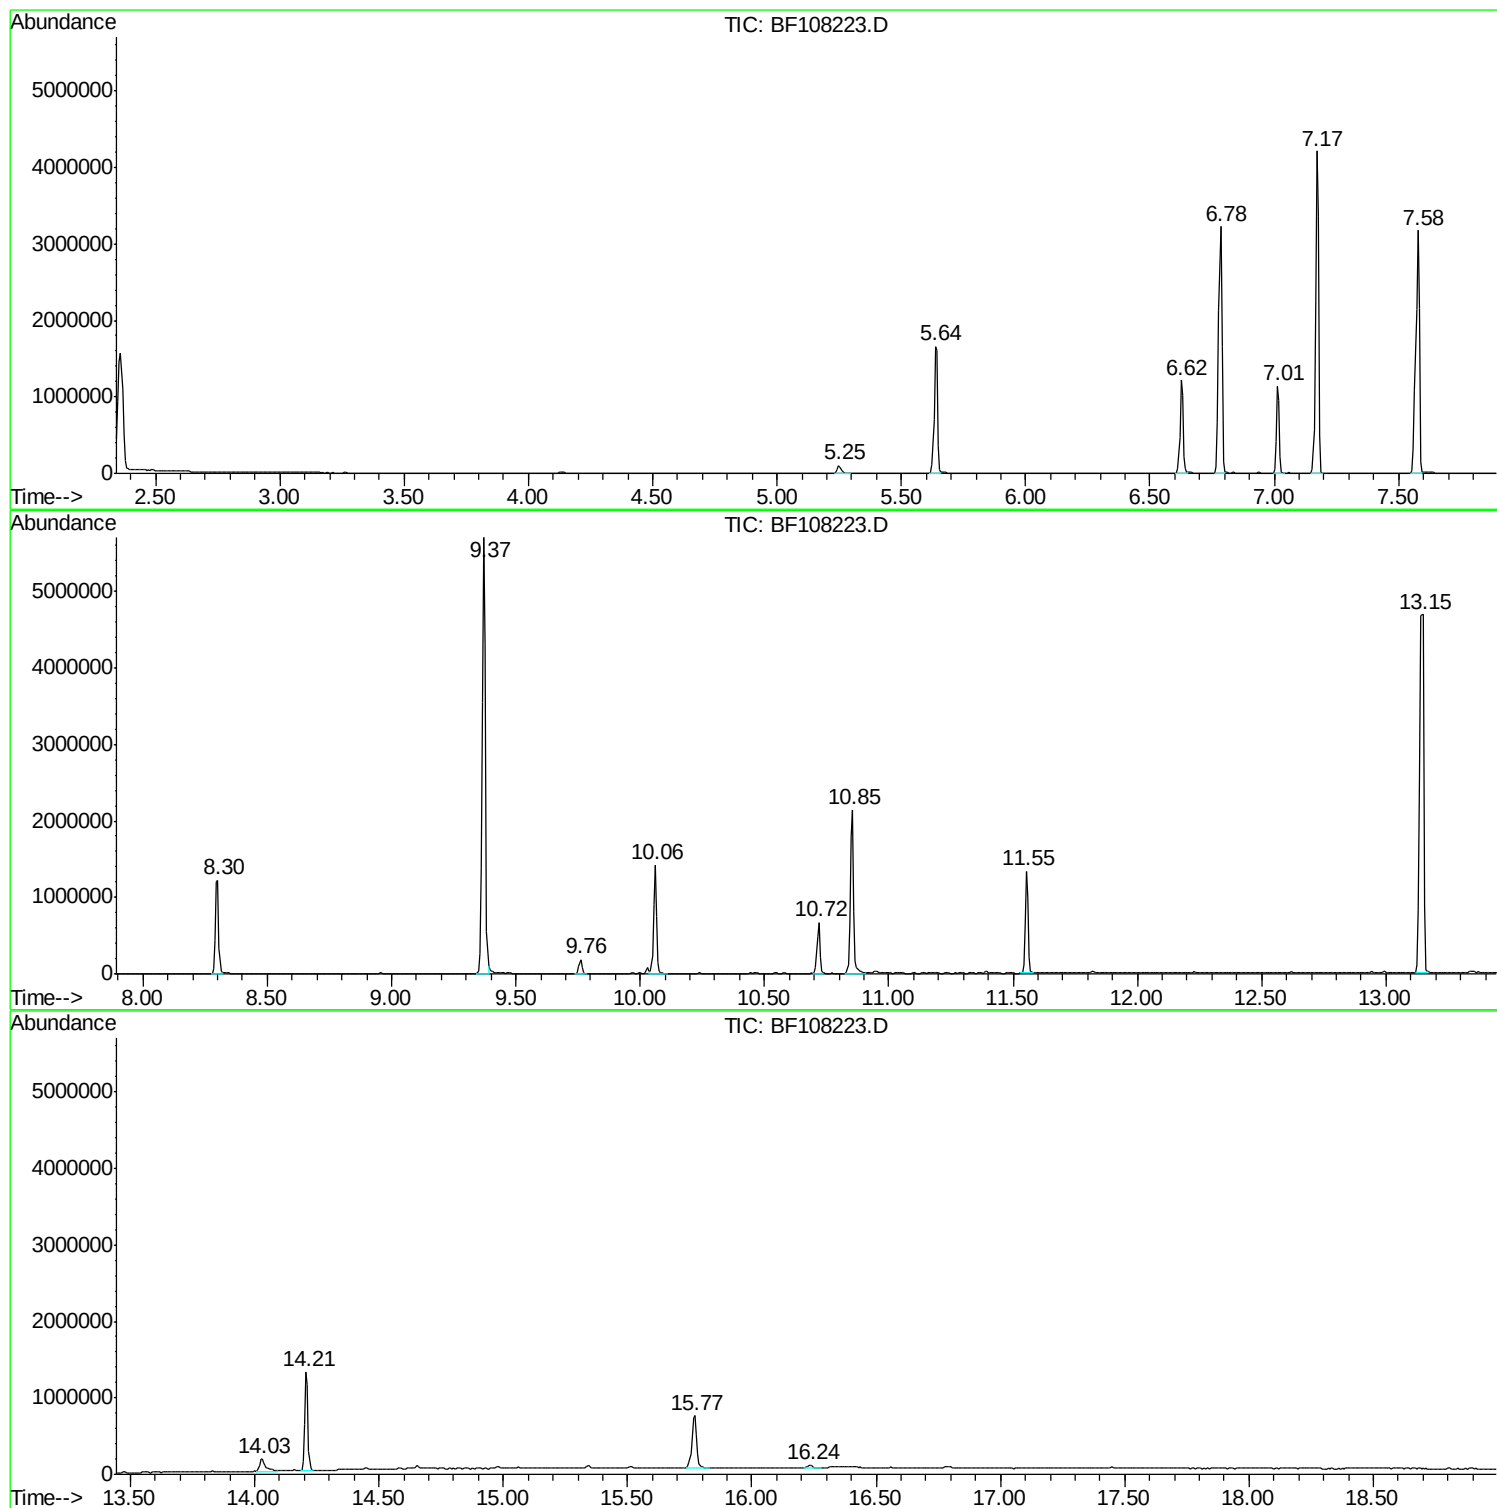

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF081618\
Data_File : BF108223.D
Acq_On : 17 Aug 2018 4:100
Operator : JU/SJJ
Sample : J4504-011
Misc :
ALS_Vial : 32 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
081418-DBRI-F-D-B

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
