

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF081618\
 Data File : BF108224.D
 Acq On : 17 Aug 2018 4:37
 Operator : JU/SJ
 Sample : J4504-02
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 081418-DBRI-F-D-S

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.248	492	495	503	rVB	103173	102399	1.64%	0.284%
2	5.637	557	561	565	rBV	1882121	1616184	25.84%	4.485%
3	6.625	725	729	734	rBV	1305854	1112663	17.79%	3.088%
4	6.784	752	756	759	rBV	3401541	2936140	46.94%	8.148%
5	7.013	792	795	799	rBV	1283094	1057643	16.91%	2.935%
6	7.172	818	822	826	rBV	4346018	4080211	65.23%	11.322%
7	7.578	886	891	894	rBV	3368309	3482561	55.67%	9.664%
8	8.301	1010	1014	1017	rBV	1447606	1312454	20.98%	3.642%
9	9.372	1191	1196	1200	rBV	6175269	6255235	100.00%	17.358%
10	9.760	1258	1262	1267	rBV	280086	222558	3.56%	0.618%
11	10.030	1305	1308	1310	rBV	78186	65861	1.05%	0.183%
12	10.060	1310	1313	1321	rVB	1731583	1478974	23.64%	4.104%
13	10.719	1421	1425	1428	rBV	477616	366062	5.85%	1.016%
14	10.854	1443	1448	1460	rBV	2620278	2509935	40.13%	6.965%
15	11.554	1563	1567	1571	rBV	1661324	1468378	23.47%	4.075%
16	13.148	1833	1838	1841	rBV	5260131	5500847	87.94%	15.264%
17	14.030	1984	1988	1998	rBV3	68551	126483	2.02%	0.351%
18	14.207	2014	2018	2022	rBV	1398006	1302876	20.83%	3.615%
19	15.771	2277	2284	2291	rBV	727162	1039752	16.62%	2.885%


Sum of corrected areas: 36037216

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF081618\
Data File : BF108224.D
Acq On : 17 Aug 2018 4:37
Operator : JU/SJ
Sample : J4504-02
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
081418-DBRI-F-D-S

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

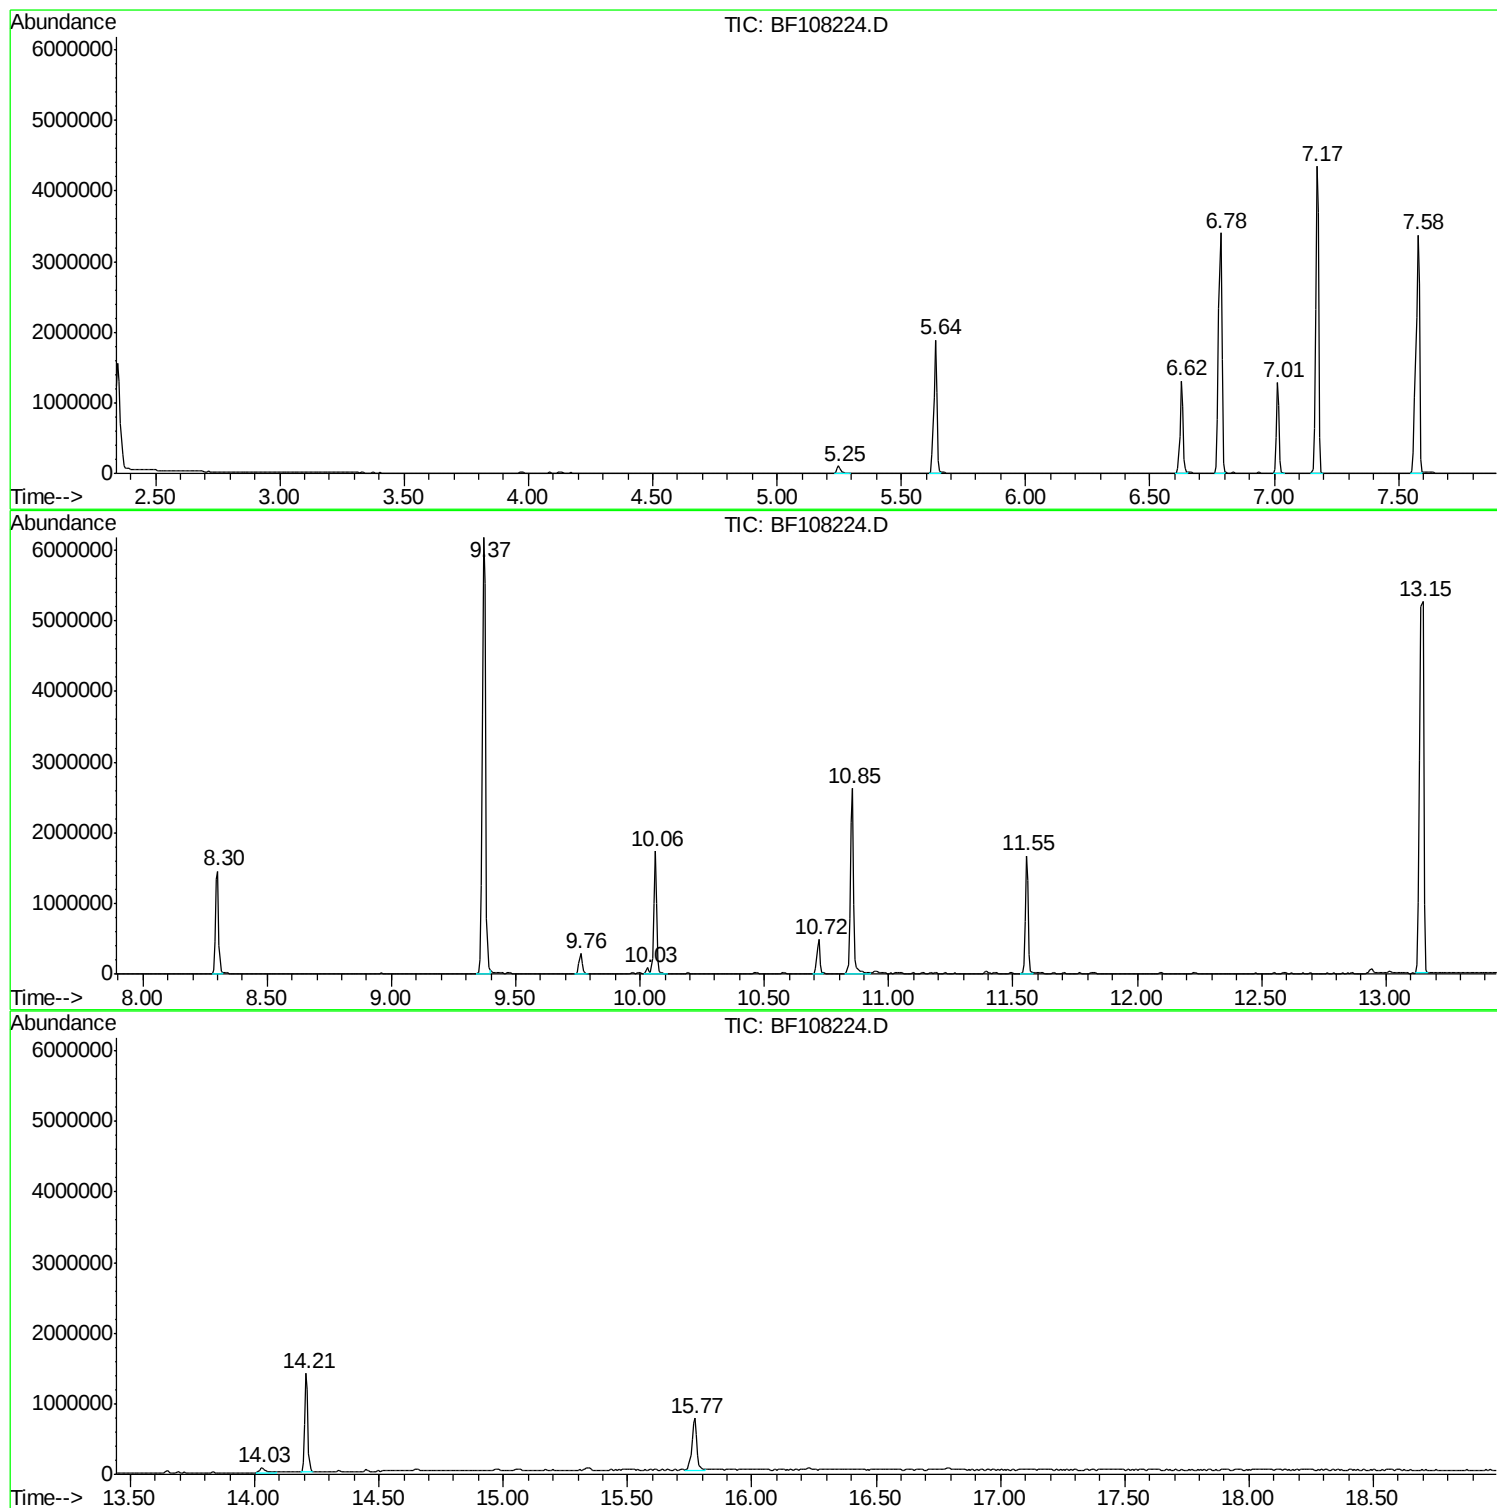

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF081618\
Data_File : BF108224.D
Acq_On : 17 Aug 2018 4:377
Operator : JU/SJJ
Sample : J4504-022
Misc :
ALS_Vial : 33 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
081418-DBRI-F-D-S

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
