

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF081618\
 Data File : BF108225.D
 Acq On : 17 Aug 2018 5:04
 Operator : JU/SJ
 Sample : J4504-03
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 081418-DBRI-F-U-B

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.248	491	495	502	rVB	93699	94051	1.59%	0.273%
2	5.636	557	561	565	rBV	1763492	1527485	25.82%	4.434%
3	6.625	725	729	734	rBV	1202433	1043767	17.64%	3.030%
4	6.783	752	756	759	rBV	3230929	2761828	46.69%	8.017%
5	7.013	792	795	799	rBV	1220391	1054365	17.82%	3.061%
6	7.172	818	822	826	rBV	4227152	3877508	65.55%	11.256%
7	7.578	886	891	894	rBV	3289055	3325222	56.21%	9.653%
8	8.295	1009	1013	1017	rBV	1386366	1291832	21.84%	3.750%
9	9.372	1191	1196	1199	rBV	6132751	5915426	100.00%	17.171%
10	9.760	1259	1262	1267	rBV	320251	249380	4.22%	0.724%
11	10.030	1305	1308	1310	rBV	82077	65729	1.11%	0.191%
12	10.060	1310	1313	1320	rVB	1680293	1429061	24.16%	4.148%
13	10.719	1422	1425	1428	rBV	352547	270222	4.57%	0.784%
14	10.854	1443	1448	1460	rBV	2400054	2293902	38.78%	6.659%
15	11.554	1563	1567	1571	rBV	1556414	1404427	23.74%	4.077%
16	13.142	1833	1837	1841	rBV	5066474	5194173	87.81%	15.078%
17	14.030	1984	1988	1999	rBV	192687	337080	5.70%	0.978%
18	14.207	2014	2018	2022	rBV	1336018	1284097	21.71%	3.727%
19	15.771	2277	2284	2292	rBV	751801	1029752	17.41%	2.989%


Sum of corrected areas: 34449307

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF081618\
Data File : BF108225.D
Acq On : 17 Aug 2018 5:04
Operator : JU/SJ
Sample : J4504-03
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
081418-DBRI-F-U-B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

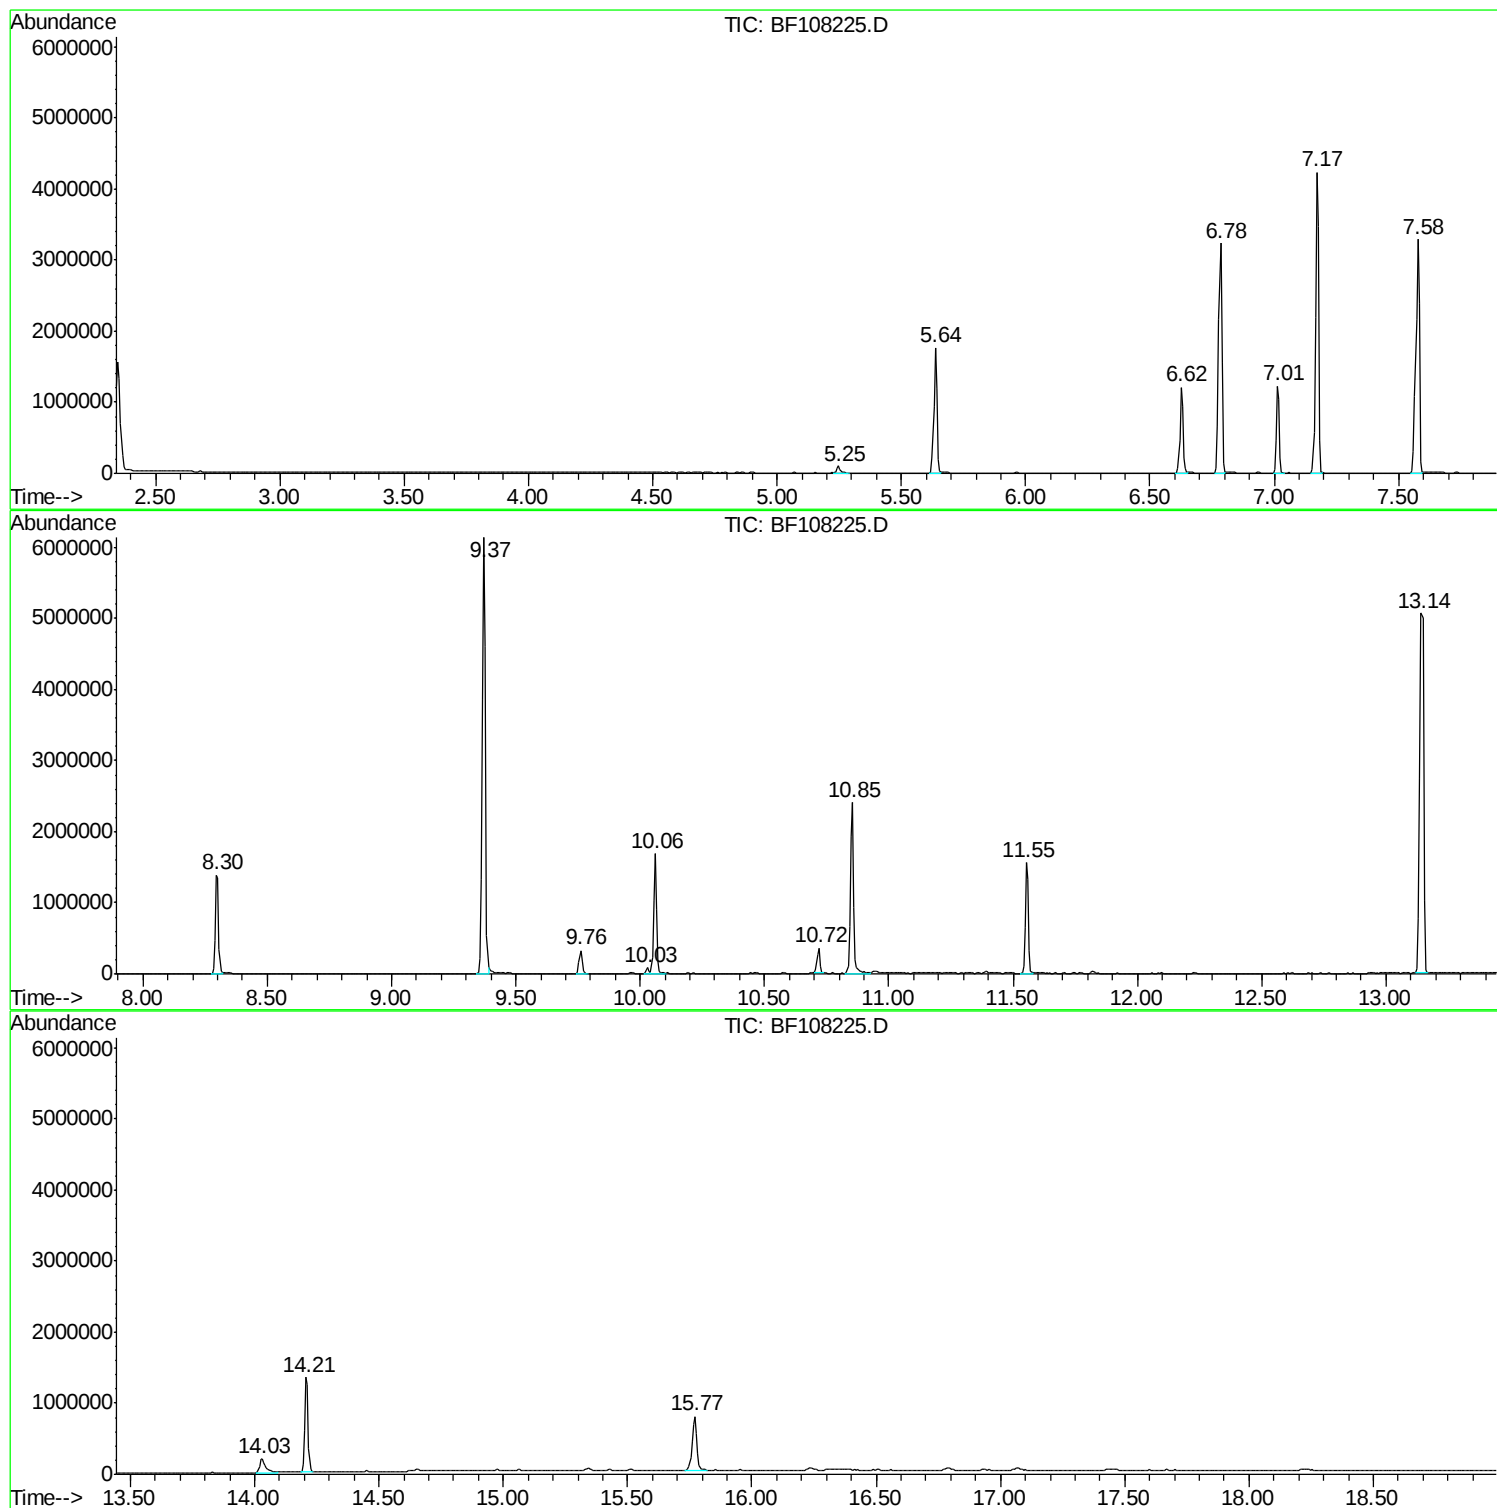

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF081618\
Data_File : BF108225.D
Acq_On : 17 Aug 2018 5:044
Operator : JU/SJJ
Sample : J4504-033
Misc :
ALS_Vial : 34 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
081418-DBRI-F-U-B

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
