

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF081618\
 Data File : BF108227.D
 Acq On : 17 Aug 2018 5:59
 Operator : JU/SJ
 Sample : J4504-05
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 081418-TIPC-F-D-B

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.248	491	495	503	rVB	78085	80360	1.39%	0.246%
2	5.636	557	561	565	rBV	1729053	1527582	26.47%	4.682%
3	6.624	725	729	734	rBV	1194068	1033945	17.92%	3.169%
4	6.783	752	756	759	rBV	3318100	2805066	48.61%	8.597%
5	7.013	792	795	799	rBV	1211306	1035046	17.94%	3.172%
6	7.172	818	822	826	rBV	4290166	3967938	68.77%	12.162%
7	7.577	886	891	894	rBV	3266907	3340794	57.90%	10.239%
8	8.295	1009	1013	1017	rBV	1350868	1226227	21.25%	3.758%
9	9.371	1191	1196	1199	rBV	5992866	5770100	100.00%	17.685%
10	9.760	1258	1262	1266	rBV	89923	71553	1.24%	0.219%
11	10.030	1305	1308	1310	rBV	71444	57964	1.00%	0.178%
12	10.060	1310	1313	1320	rVB	1479683	1283963	22.25%	3.935%
13	10.718	1421	1425	1428	rBV	364025	289622	5.02%	0.888%
14	10.854	1443	1448	1460	rBV	2143843	2033293	35.24%	6.232%
15	11.554	1563	1567	1571	rBV	1433350	1196412	20.73%	3.667%
16	12.942	1800	1803	1806	rVB	78214	61971	1.07%	0.190%
17	13.142	1833	1837	1840	rBV	4927265	4631172	80.26%	14.194%
18	14.030	1984	1988	1997	rBV3	56075	115637	2.00%	0.354%
19	14.206	2014	2018	2022	rBV	1319183	1203773	20.86%	3.690%
20	15.765	2278	2283	2291	rVB	628494	894534	15.50%	2.742%


Sum of corrected areas: 32626952

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF081618\
Data File : BF108227.D
Acq On : 17 Aug 2018 5:59
Operator : JU/SJ
Sample : J4504-05
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
081418-TIPC-F-D-B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

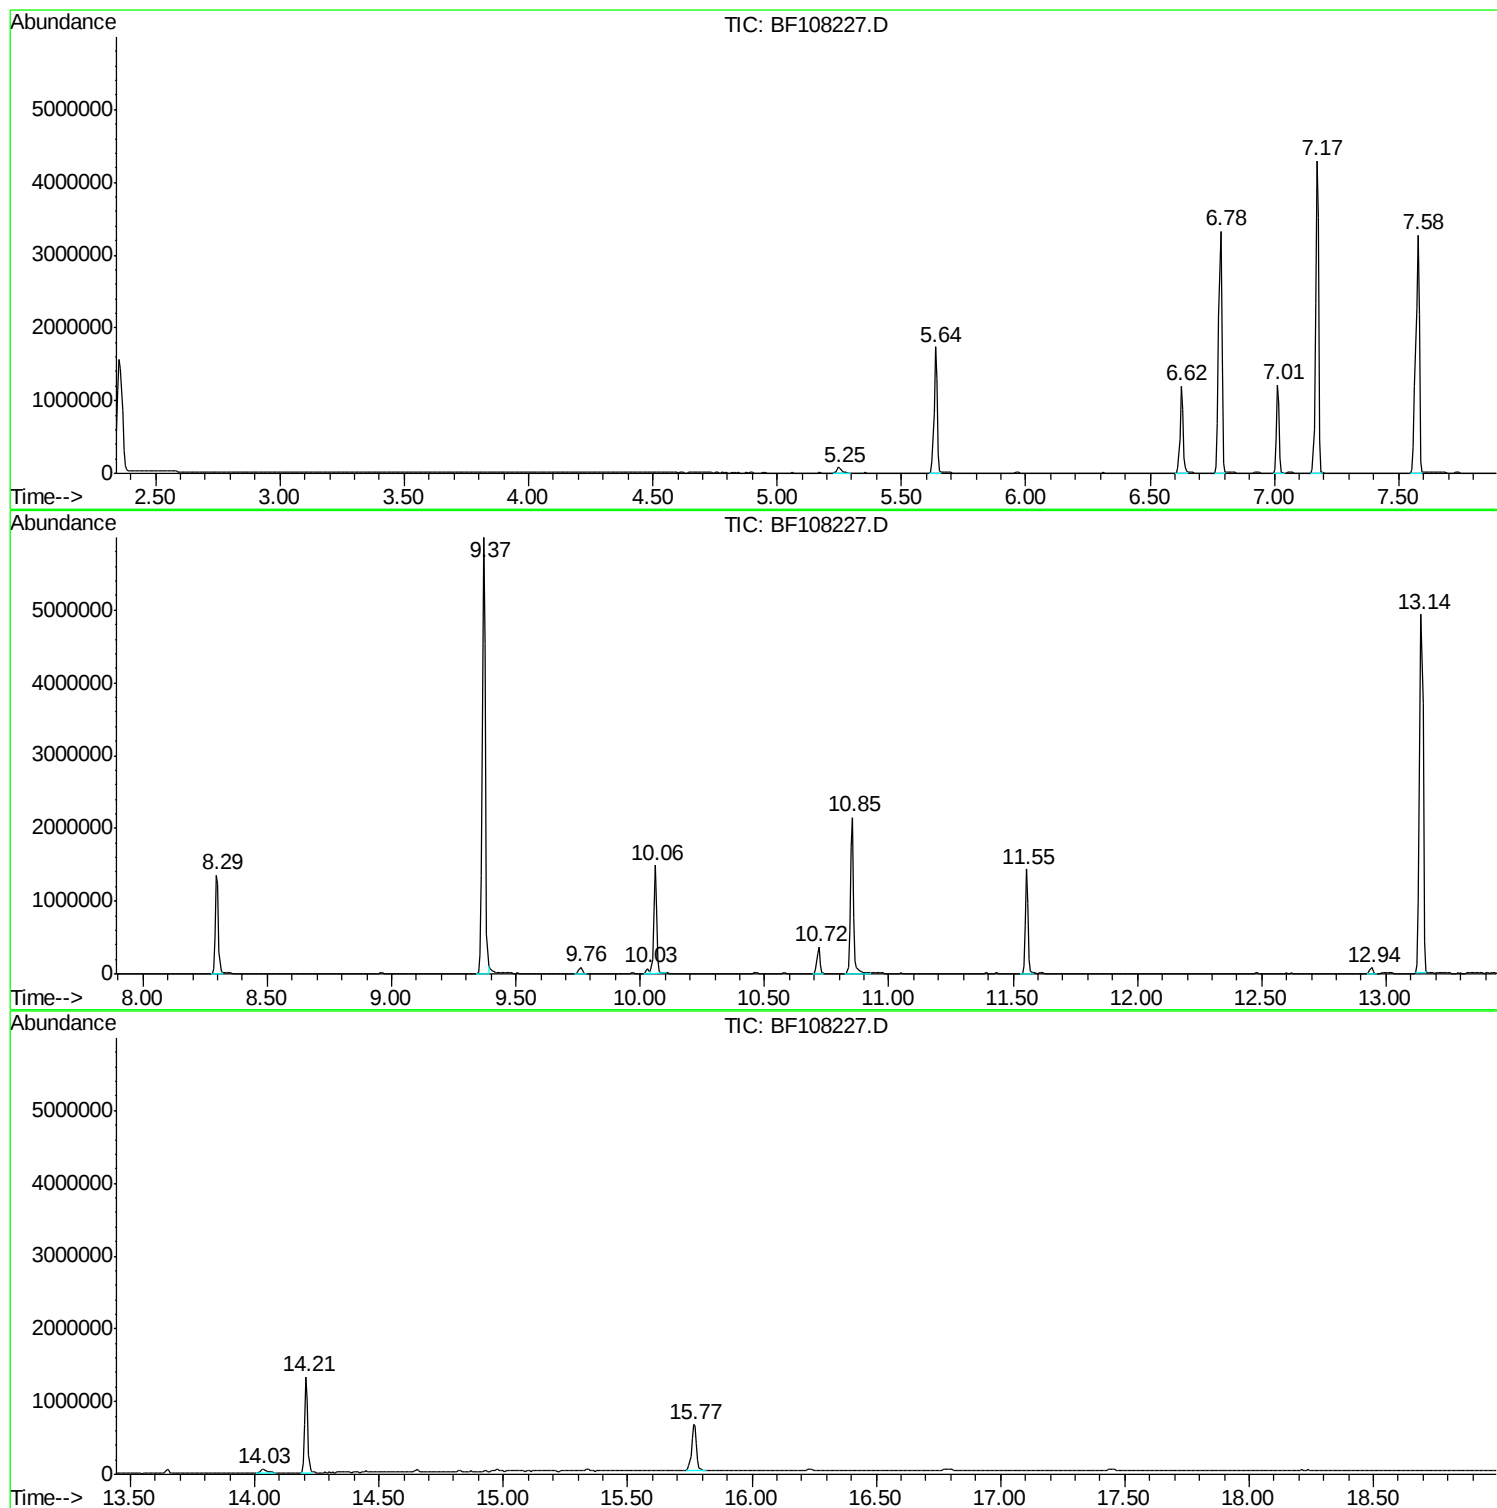

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF081618\
Data_File : BF108227.D
Acq_On : 17 Aug 2018 5:59
Operator : JU/SJJ
Sample : J4504-055
Misc :
ALS_Vial : 36 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
081418-TIPC-F-D-B

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
