


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081618\
 Data File : BF108190.D
 Acq On : 16 Aug 2018 12:11
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 08 12:24:24 2018

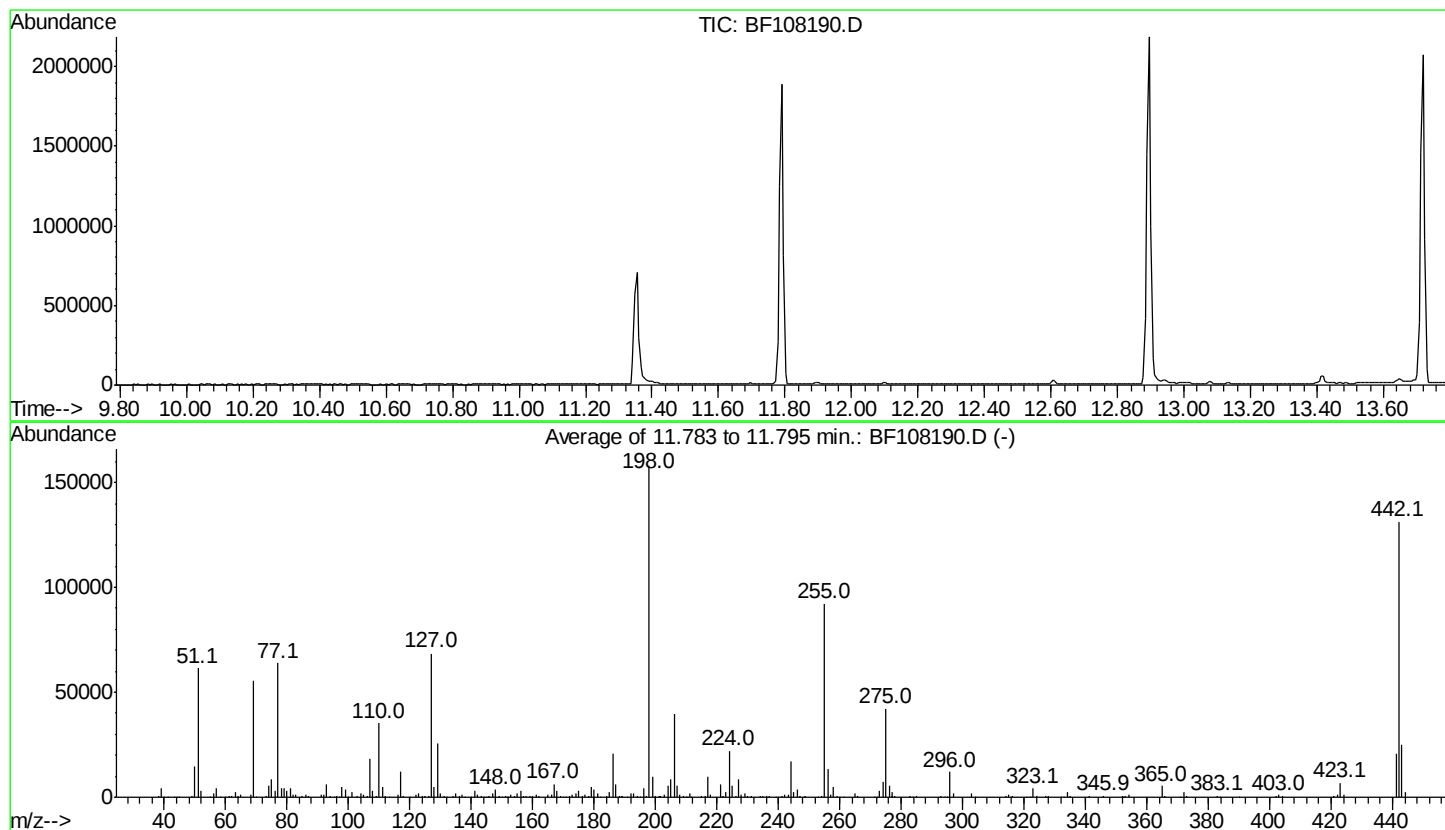

AutoFind: Scans 1606, 1607, 1608; Background Corrected with Scan 1600

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.9	61472	PASS
68	69	0.00	2	1.7	939	PASS
69	198	0.00	100	35.0	55360	PASS
70	69	0.00	2	0.5	268	PASS
127	198	10	80	43.4	68530	PASS
197	198	0.00	2	0.3	518	PASS
198	198	100	100	100.0	158018	PASS
199	198	5	9	6.4	10071	PASS
275	198	10	60	26.7	42157	PASS
365	198	1	100	3.4	5362	PASS
441	198	0.01	100	13.1	20744	PASS
442	198	50	100	83.0	131160	PASS
443	442	15	24	18.9	24777	PASS