


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081618\
 Data File : BF108215.D
 Acq On : 17 Aug 2018 00:31
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 08 12:24:24 2018

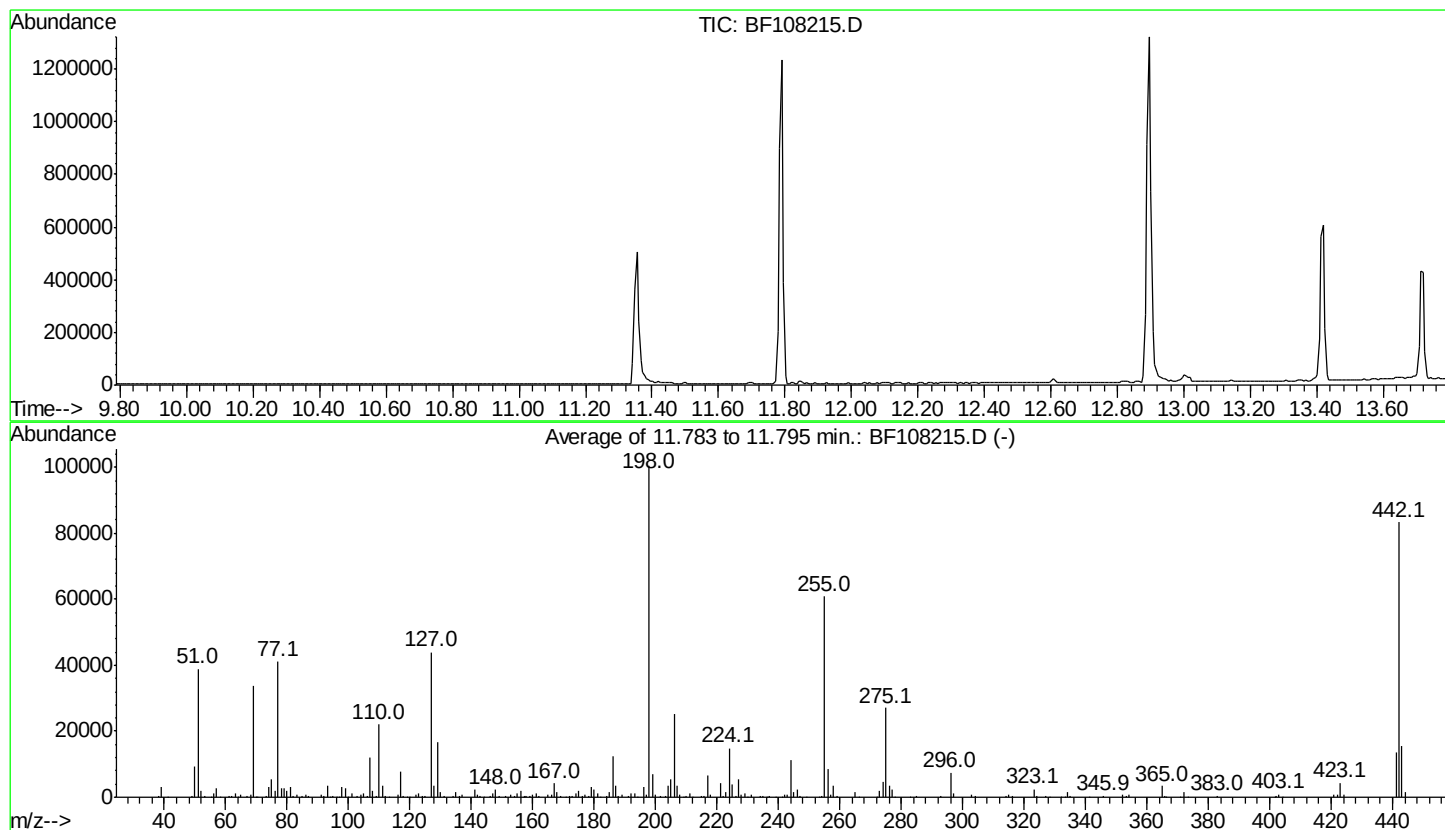

AutoFind: Scans 1606, 1607, 1608; Background Corrected with Scan 1601

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.8	38964	PASS
68	69	0.00	2	1.8	604	PASS
69	198	0.00	100	33.7	33904	PASS
70	69	0.00	2	0.4	135	PASS
127	198	10	80	43.6	43849	PASS
197	198	0.00	2	0.6	616	PASS
198	198	100	100	100.0	100490	PASS
199	198	5	9	6.9	6978	PASS
275	198	10	60	27.0	27140	PASS
365	198	1	100	3.3	3356	PASS
441	198	0.01	100	13.4	13468	PASS
442	198	50	100	82.9	83269	PASS
443	442	15	24	18.7	15569	PASS