

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF081619\
 Data File : BF116345.D
 Acq On : 17 Aug 2019 3:58
 Operator : HP/JU
 Sample : K4090-09 10X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OR-02-081519

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF073019.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.246	25	27	35	rVB2	13001	21071	1.86%	0.279%
2	2.404	51	54	67	rVB3	12775	24775	2.18%	0.328%
3	5.475	573	576	589	rBV	43490	116784	10.29%	1.546%
4	6.481	745	747	765	rBV	62464	169785	14.96%	2.247%
5	6.604	765	768	786	rVB	141101	228353	20.13%	3.023%
6	6.816	801	804	828	rBV	814907	788687	69.51%	10.440%
7	6.975	828	831	845	rBV	146158	174567	15.38%	2.311%
8	7.404	901	904	926	rBV	43252	108798	9.59%	1.440%
9	8.098	1018	1022	1045	rBV	994333	1045808	92.17%	13.843%
10	9.175	1201	1205	1216	rBV	190433	240236	21.17%	3.180%
11	9.575	1267	1273	1283	rBV	18852	28760	2.53%	0.381%
12	9.845	1316	1319	1334	rBV	1099395	1134670	100.00%	15.019%
13	10.651	1453	1456	1469	rBV	57525	80317	7.08%	1.063%
14	11.333	1569	1572	1583	rBV	936421	993158	87.53%	13.146%
15	12.404	1749	1754	1755	rBV3	14093	17006	1.50%	0.225%
16	12.421	1755	1757	1764	rVB3	24287	24284	2.14%	0.321%
17	12.557	1777	1780	1787	rBV	46611	47958	4.23%	0.635%
18	12.786	1813	1819	1826	rBV	46445	58124	5.12%	0.769%
19	12.915	1837	1841	1847	rVB	192480	194778	17.17%	2.578%
20	13.804	1987	1992	1995	rBV3	19939	30426	2.68%	0.403%
21	13.833	1995	1997	2004	rVB2	20674	27848	2.45%	0.369%
22	13.980	2017	2022	2030	rBV	675756	814092	71.75%	10.776%
23	14.121	2043	2046	2048	rBV3	17267	16735	1.47%	0.222%
24	14.421	2094	2097	2100	rBV3	25589	27738	2.44%	0.367%
25	14.721	2146	2148	2151	rVB	27551	23270	2.05%	0.308%
26	15.027	2196	2200	2201	rBV	26116	34095	3.00%	0.451%
27	15.045	2201	2203	2206	rVB	43160	44606	3.93%	0.590%
28	15.321	2247	2250	2253	rBV	19838	22303	1.97%	0.295%
29	15.386	2258	2261	2263	rVV	25930	34776	3.06%	0.460%
30	15.433	2263	2269	2283	rVB	571421	877294	77.32%	11.613%
31	15.833	2334	2337	2341	rVB2	35422	41801	3.68%	0.553%
32	16.321	2415	2420	2427	rBV4	29752	61813	5.45%	0.818%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF081619\
Data File : BF116345.D
Acq On : 17 Aug 2019 3:58
Operator : HP/JU
Sample : K4090-09 10X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OR-02-081519

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF073019.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION


Sum of corrected areas: 7554716

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF081619\
Data File : BF116345.D
Acq On : 17 Aug 2019 3:58
Operator : HP/JU
Sample : K4090-09 10X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OR-02-081519

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF073019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

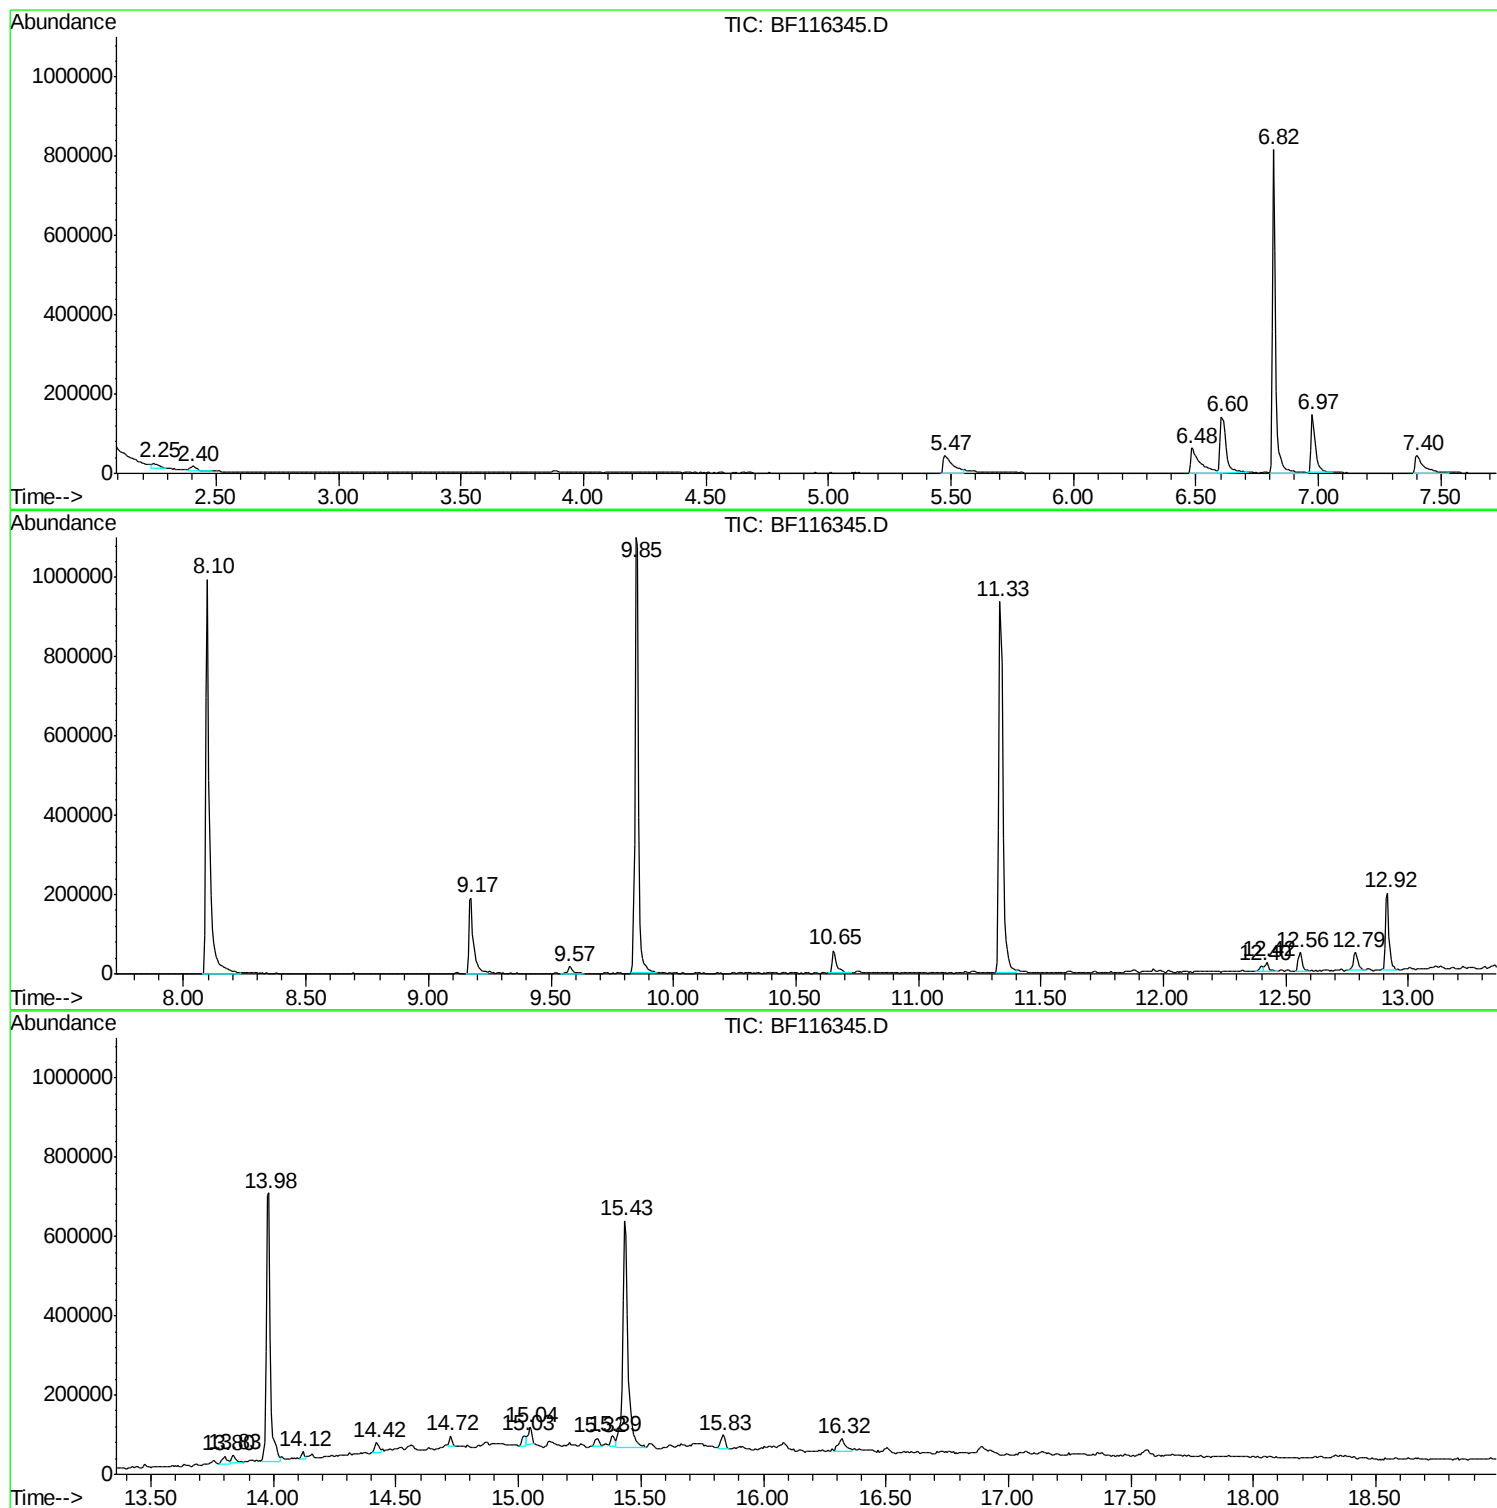

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF081619\
Data File : BF116345.D
Acq On : 17 Aug 2019 3:58
Operator : HP/JU
Sample : K4090-09 10X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OR-02-081519










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF073019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.60 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.60	5.79 ng	228353	1,4-Dichlorobenzene-d4	6.82

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	16
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	12
3		Amphetaminil	250	C17H18N2	017590-01-1	10
4		5-Aminoindole	132	C8H8N2	005192-03-0	10
5		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	9

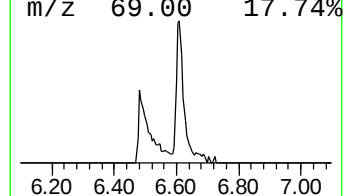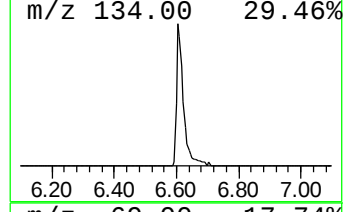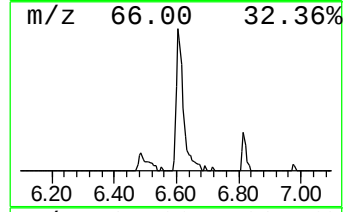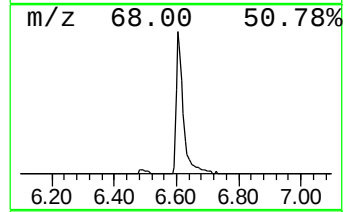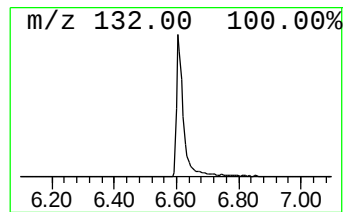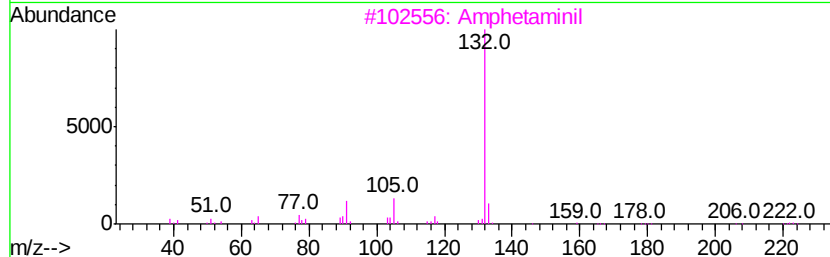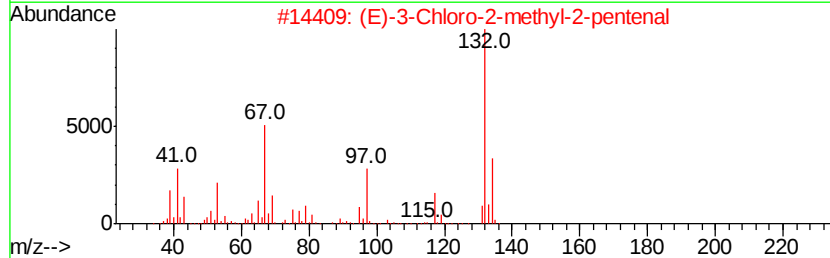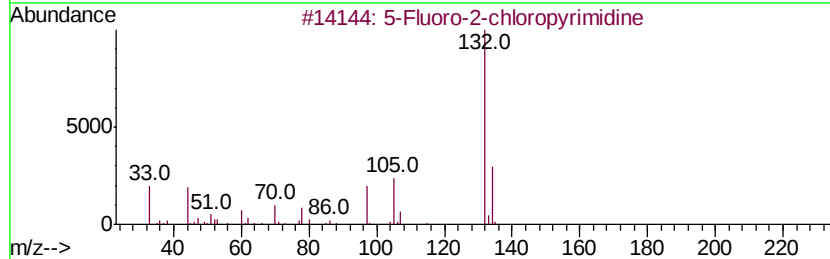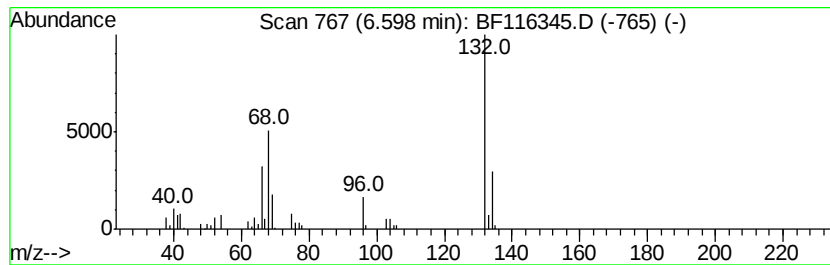

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF081619\
Data File : BF116345.D
Acq On : 17 Aug 2019 3:58
Operator : HP/JU
Sample : K4090-09 10X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OR-02-081519

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF073019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.60	6.60	5.8	ng	228353	1	6.82	788687	20.0