

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF081619\
 Data File : BF116346.D
 Acq On : 17 Aug 2019 4:26
 Operator : HP/JU
 Sample : K4319-05DL 5X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TEST-PIT-1DL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF073019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.475	573	576	600	rBV	187271	518188	28.07%	3.726%
2	6.492	746	749	766	rBV	207146	606183	32.84%	4.358%
3	6.610	766	769	791	rVB	463463	752489	40.77%	5.410%
4	6.816	801	804	822	rVB	912255	824759	44.68%	5.930%
5	6.975	827	831	849	rVB	524901	537280	29.11%	3.863%
6	7.386	898	901	917	rBV	243999	389856	21.12%	2.803%
7	8.098	1018	1022	1042	rBV	1019266	1064729	57.69%	7.655%
8	9.169	1200	1204	1216	rBV	773542	748205	40.54%	5.380%
9	9.574	1269	1273	1285	rBV	39539	50704	2.75%	0.365%
10	9.845	1316	1319	1343	rVB	1132207	1179559	63.91%	8.481%
11	10.645	1452	1455	1470	rBV	304265	390898	21.18%	2.811%
12	11.333	1569	1572	1586	rBV	1022675	1119620	60.66%	8.050%
13	11.857	1657	1661	1664	rBV	41259	55098	2.99%	0.396%
14	11.886	1664	1666	1670	rVB2	26489	26831	1.45%	0.193%
15	12.557	1777	1780	1785	rBV	82614	85458	4.63%	0.614%
16	12.780	1813	1818	1825	rVB2	106869	121132	6.56%	0.871%
17	12.910	1837	1840	1848	rBV	684435	608739	32.98%	4.377%
18	13.386	1916	1921	1924	rBV	2005514	1845759	100.00%	13.271%
19	13.833	1987	1997	2003	rBV9	32671	96512	5.23%	0.694%
20	13.939	2011	2015	2018	rBV	1013809	844570	45.76%	6.072%
21	13.980	2018	2022	2034	rVB	710299	828198	44.87%	5.955%
22	14.421	2093	2097	2100	rBV4	23648	33587	1.82%	0.241%
23	14.580	2121	2124	2127	rVB	38877	35846	1.94%	0.258%
24	14.721	2145	2148	2150	rBV	23475	22338	1.21%	0.161%
25	15.021	2196	2199	2201	rBV	38515	50642	2.74%	0.364%
26	15.051	2201	2204	2210	rVB	59107	73573	3.99%	0.529%
27	15.321	2246	2250	2256	rBV	21444	31274	1.69%	0.225%
28	15.386	2258	2261	2263	rVV	26405	35168	1.91%	0.253%
29	15.433	2263	2269	2287	rVB	489760	785922	42.58%	5.651%
30	15.833	2333	2337	2342	rVB	41885	58243	3.16%	0.419%
31	16.321	2416	2420	2429	rVB2	34042	58128	3.15%	0.418%
32	16.892	2512	2517	2520	rBV2	16045	28631	1.55%	0.206%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF081619\
Data File : BF116346.D
Acq On : 17 Aug 2019 4:26
Operator : HP/JU
Sample : K4319-05DL 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TEST-PIT-1DL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF073019.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION


Sum of corrected areas: 13908119

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF081619\
Data File : BF116346.D
Acq On : 17 Aug 2019 4:26
Operator : HP/JU
Sample : K4319-05DL 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TEST-PIT-1DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF073019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

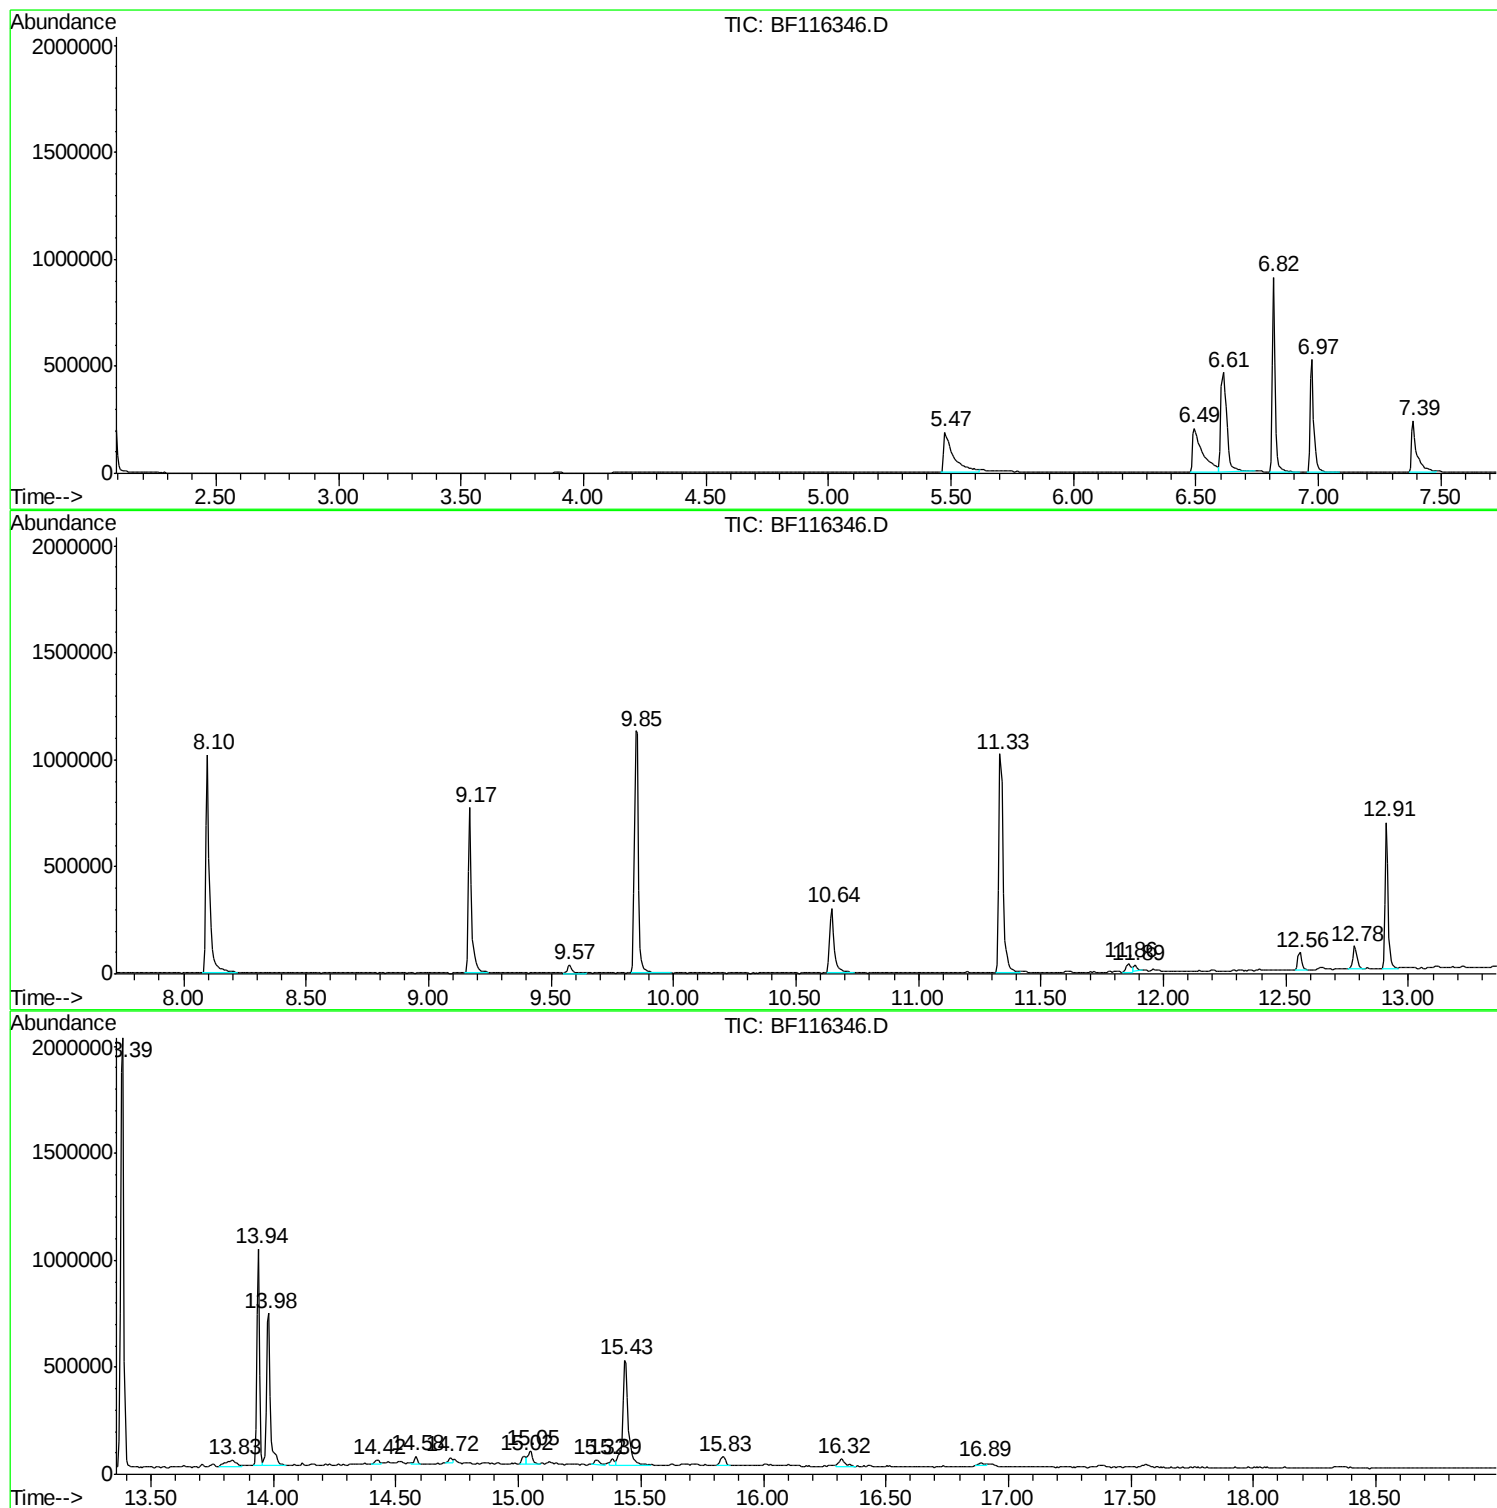

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF081619\
Data File : BF116346.D
Acq On : 17 Aug 2019 4:26
Operator : HP/JU
Sample : K4319-05DL 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TEST-PIT-1DL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF073019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.61 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.61	18.25 ng	752489	1,4-Dichlorobenzene-d4	6.82

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	16
3		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
4		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9
5		1-Methylpyrrolo[1,2-a]pyrazine	132	C8H8N2	064608-59-9	9

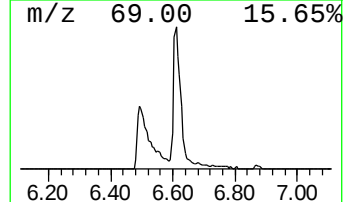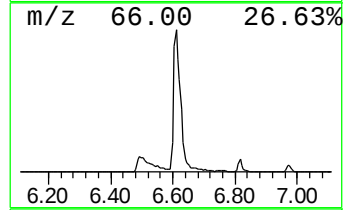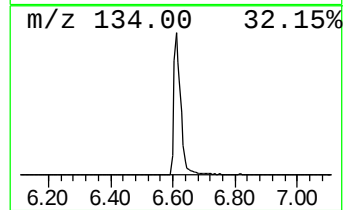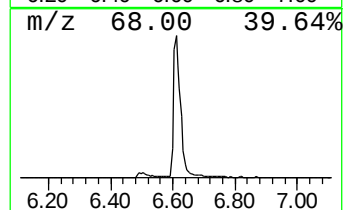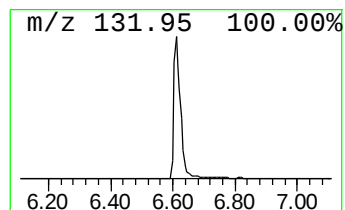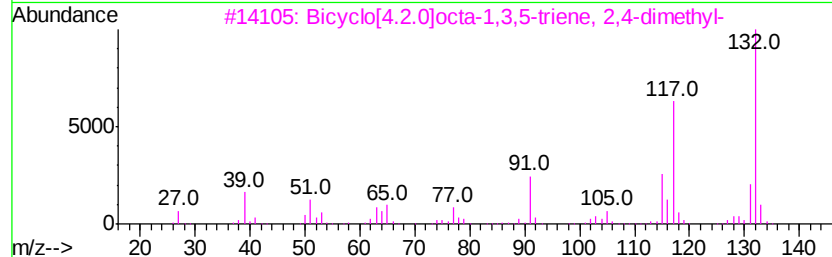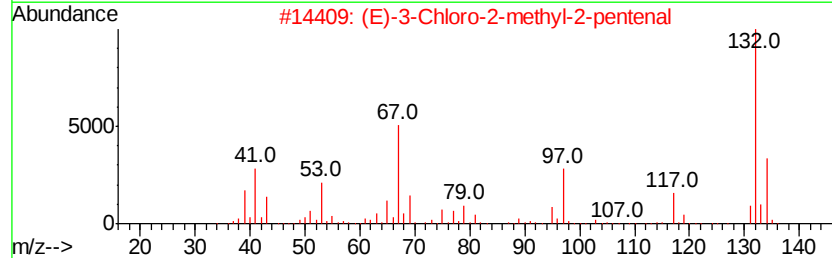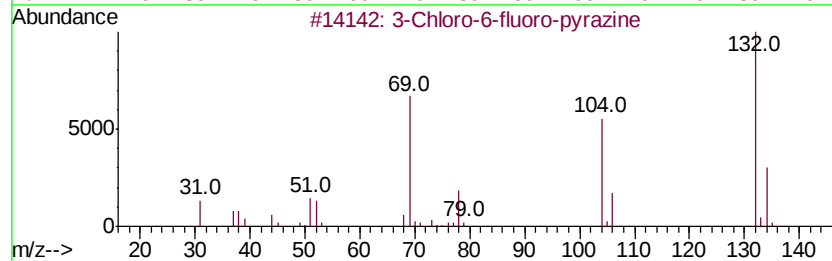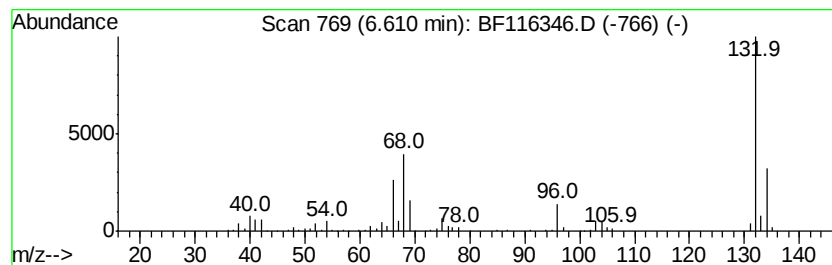

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF081619\
Data File : BF116346.D
Acq On : 17 Aug 2019 4:26
Operator : HP/JU
Sample : K4319-05DL 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
TEST-PIT-1DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF073019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 4 Oxazolidine, 3-phenyl- Concentration Rank 4

R.T.	EstConc	Area	Relative to ISTD	R.T.	
13.83	2.33 ng	96512	Chrysene-d12	13.98	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Oxazolidine, 3-phenyl-	149	C9H11NO	020503-92-8	59
2	2,2'-(Ethane-1,2-diylbis(oxv))bi...	358	C20H22O6	1000366-99-4	59
3	2-(2-(2-Methoxvethoxv)ethoxv)eth...	268	C14H20O5	1000366-99-1	59
4	3,6,9,12-Tetraoxatetradecane-1,1...	446	C24H30O8	1000366-97-0	45
5	Diethylene glycol dibenzoate	314	C18H18O5	000120-55-8	45

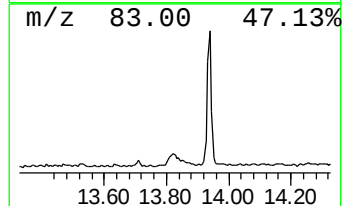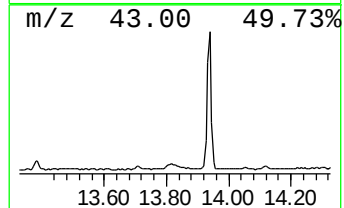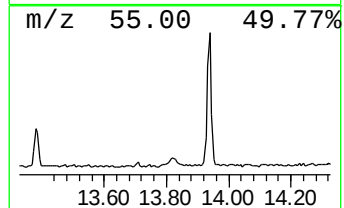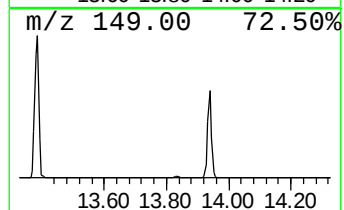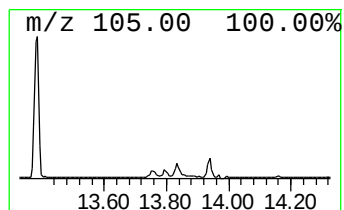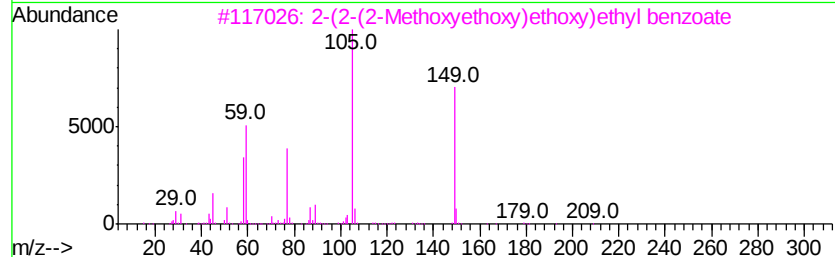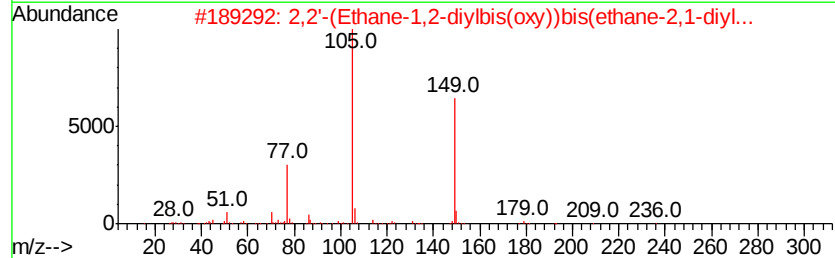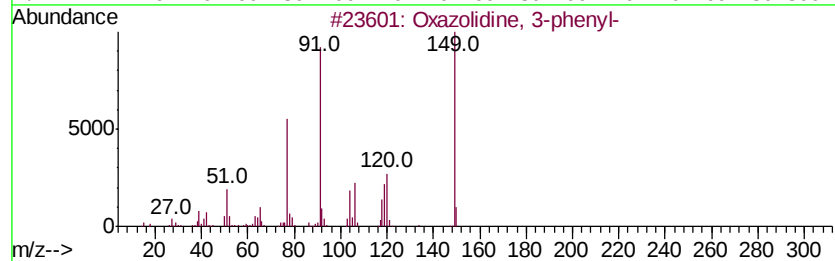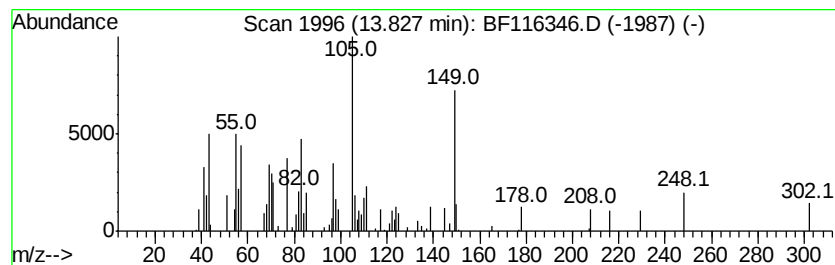

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF081619\
Data File : BF116346.D
Acq On : 17 Aug 2019 4:26
Operator : HP/JU
Sample : K4319-05DL 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TEST-PIT-1DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF073019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.61	6.61	18.3	ng	752489	1	6.82	824759	20.0
Oxazolidine, 3-ph...	13.83	2.3	ng	96512	5	13.98	828198	20.0