


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081619\
 Data File : BF116307.D
 Acq On : 16 Aug 2019 7:53
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF073019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 19 06:03:31 2019

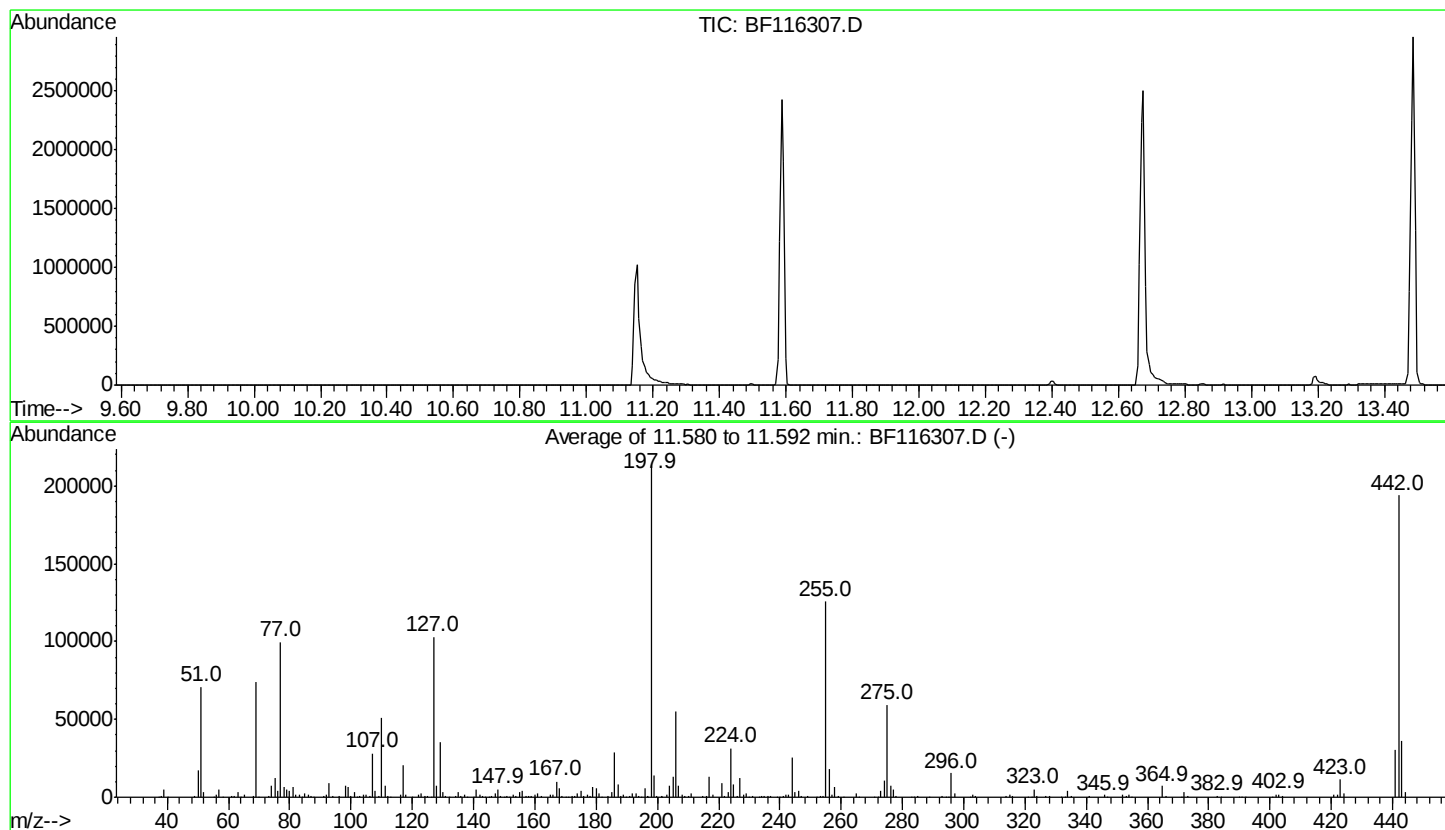

AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.2	70768	PASS
68	69	0.00	2	1.6	1210	PASS
69	198	0.00	100	34.8	74109	PASS
70	69	0.00	2	0.5	387	PASS
127	198	10	80	48.3	102968	PASS
197	198	0.00	2	0.6	1199	PASS
198	198	100	100	100.0	212992	PASS
199	198	5	9	6.7	14248	PASS
275	198	10	60	27.9	59517	PASS
365	198	1	100	3.4	7267	PASS
441	198	0.01	100	14.3	30557	PASS
442	198	50	100	90.9	193669	PASS
443	442	15	24	18.8	36453	PASS