
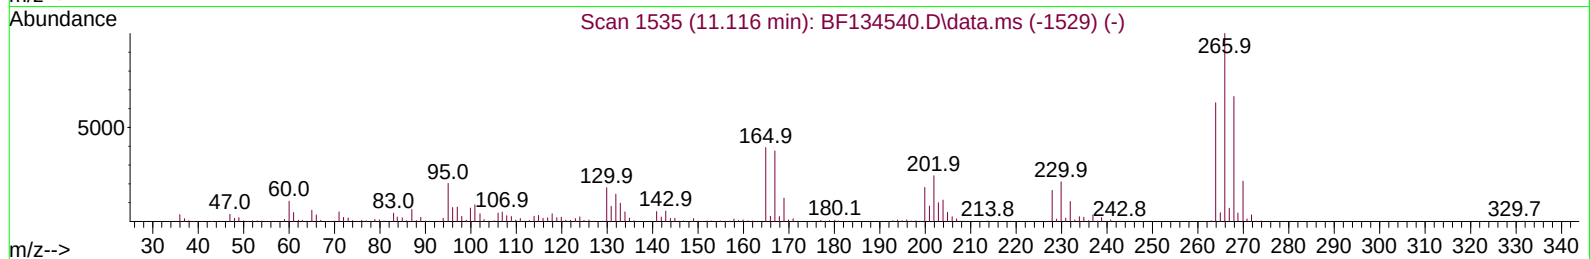
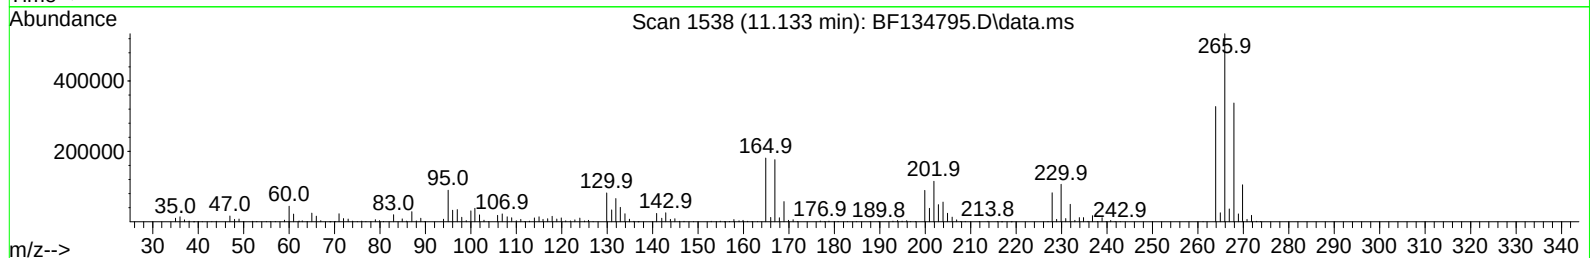


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081623\
Data File : BF134795.D
Acq On : 16 Aug 2023 07:09
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 17 02:50:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 04 09:29:15 2023
Response via : Initial Calibration

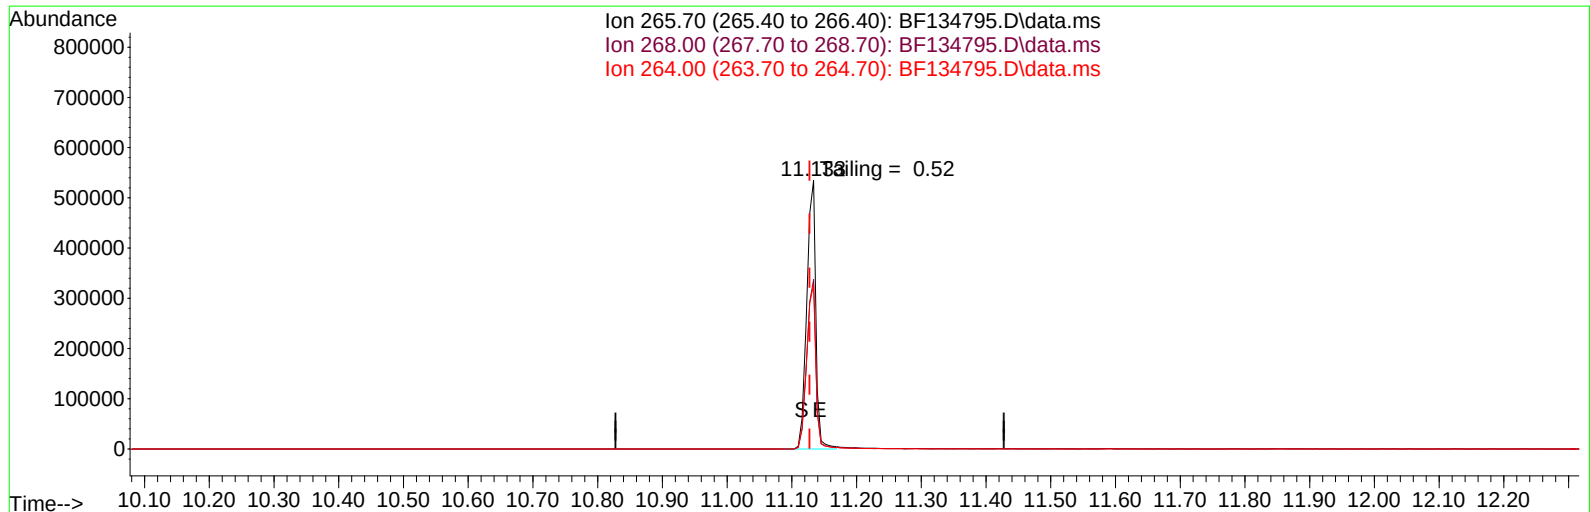

TIC: BF134795.D\data.ms

(70) Pentachlorophenol (C)




11.133min (+ 0.006) 1214058.24 ng

response 530056

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.10	63.09
264.00	59.70	61.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081623\
Data File : BF134795.D
Acq On : 16 Aug 2023 07:09
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 17 02:50:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 04 09:29:15 2023
Response via : Initial Calibration

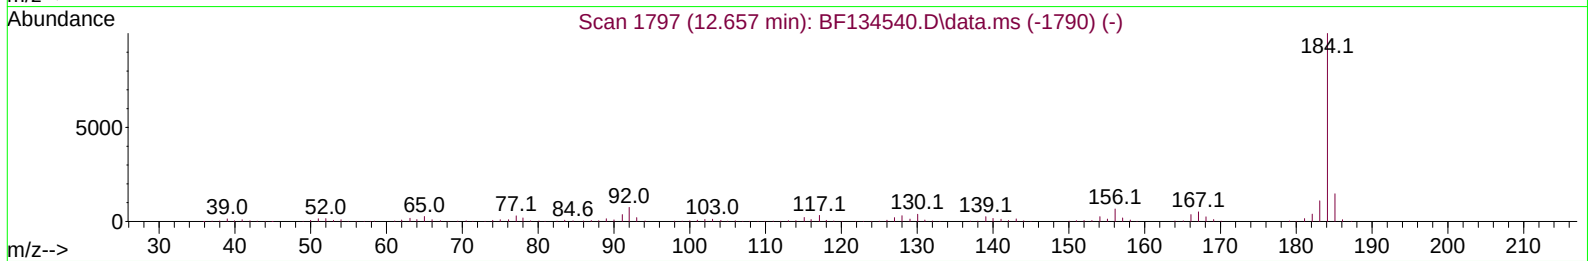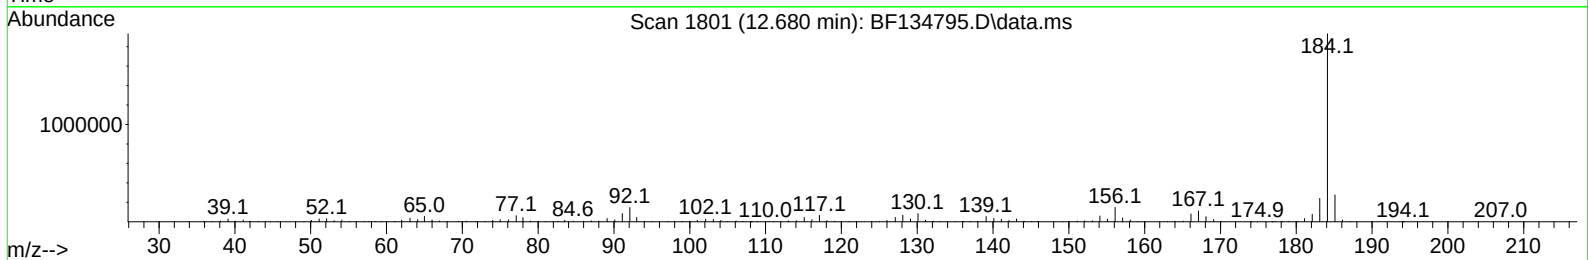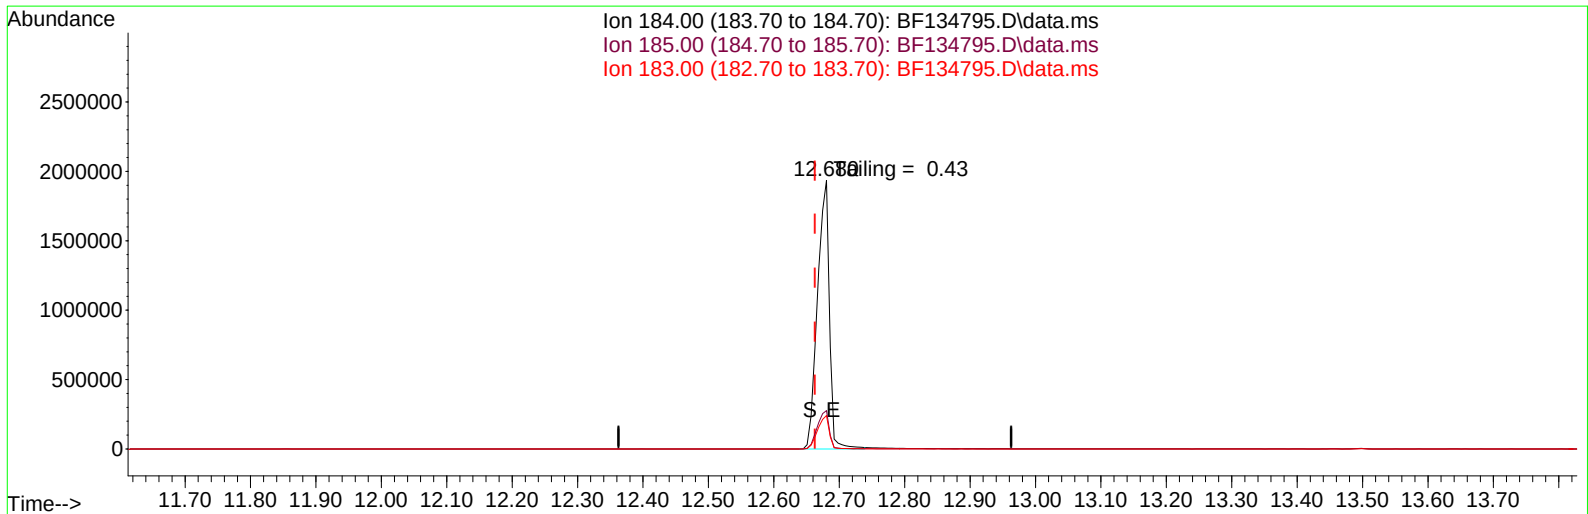

TIC: BF134795.D\data.ms

(77) Benzidine

12.680min (+ 0.018) 216514.56 ng

response 2472238

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.30
183.00	10.80	12.43
0.00	0.00	0.00