

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081623\
 Data File : BF134797.D
 Acq On : 16 Aug 2023 08:45
 Operator : CG\JU
 Sample : PB154844BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB154844BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF134797.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.157	5	12	18	rVB	60010	89577	1.42%	0.234%
2	2.269	25	31	36	rBV	53403	65106	1.03%	0.170%
3	5.075	503	508	519	rVB	65536	98154	1.55%	0.257%
4	5.446	565	571	574	rBV	4388061	4851234	76.69%	12.682%
5	6.440	733	740	743	rBV	4034888	4836121	76.45%	12.643%
6	6.798	797	801	804	rBV	1405831	1125416	17.79%	2.942%
7	7.363	890	897	900	rBV	3023309	3338229	52.77%	8.727%
8	8.075	1013	1018	1021	rBV	1716490	1525739	24.12%	3.989%
9	9.157	1195	1202	1205	rBV	5524125	5829927	92.16%	15.241%
10	9.833	1311	1317	1320	rBV	1952551	1771852	28.01%	4.632%
11	10.628	1445	1452	1455	rBV	3900526	3877319	61.29%	10.136%
12	11.322	1566	1570	1573	rBV	2155374	1825514	28.86%	4.772%
13	12.921	1837	1842	1845	rBV	5702642	6326066	100.00%	16.538%
14	13.968	2016	2020	2031	rBV	1447837	1420768	22.46%	3.714%
15	15.445	2265	2271	2285	rBV	707866	1082353	17.11%	2.830%
16	17.204	2565	2570	2589	rVB5	40184	188112	2.97%	0.492%




Sum of corrected areas: 38251487

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081623\
Data File : BF134797.D
Acq On : 16 Aug 2023 08:45
Operator : CG\JU
Sample : PB154844BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB154844BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

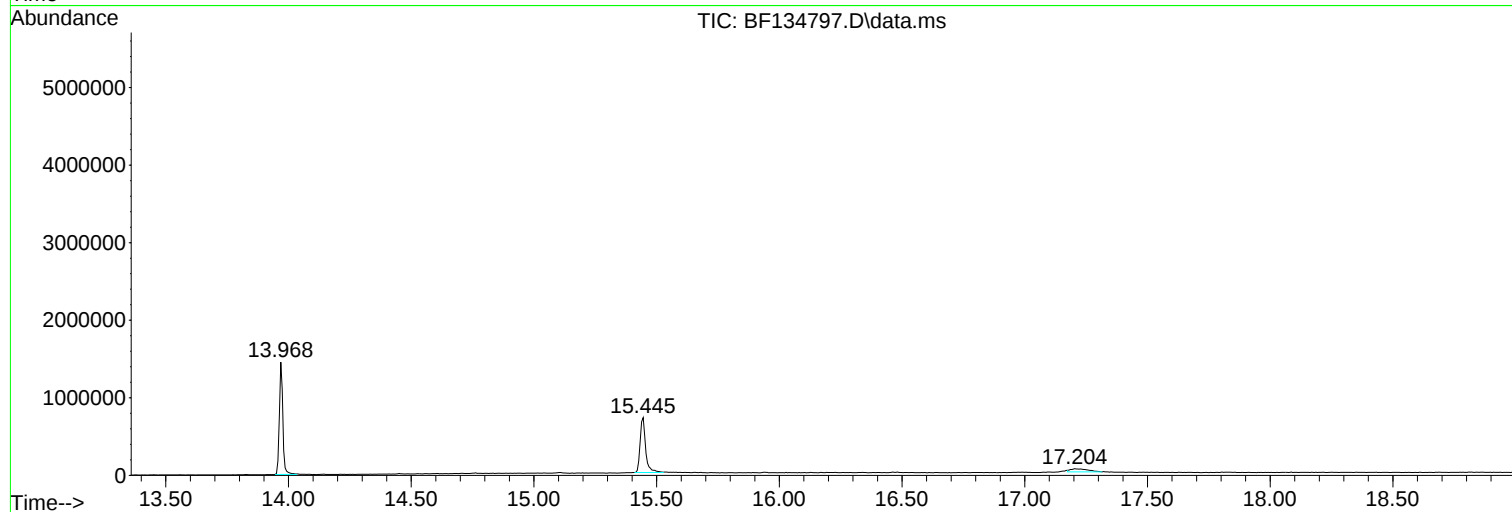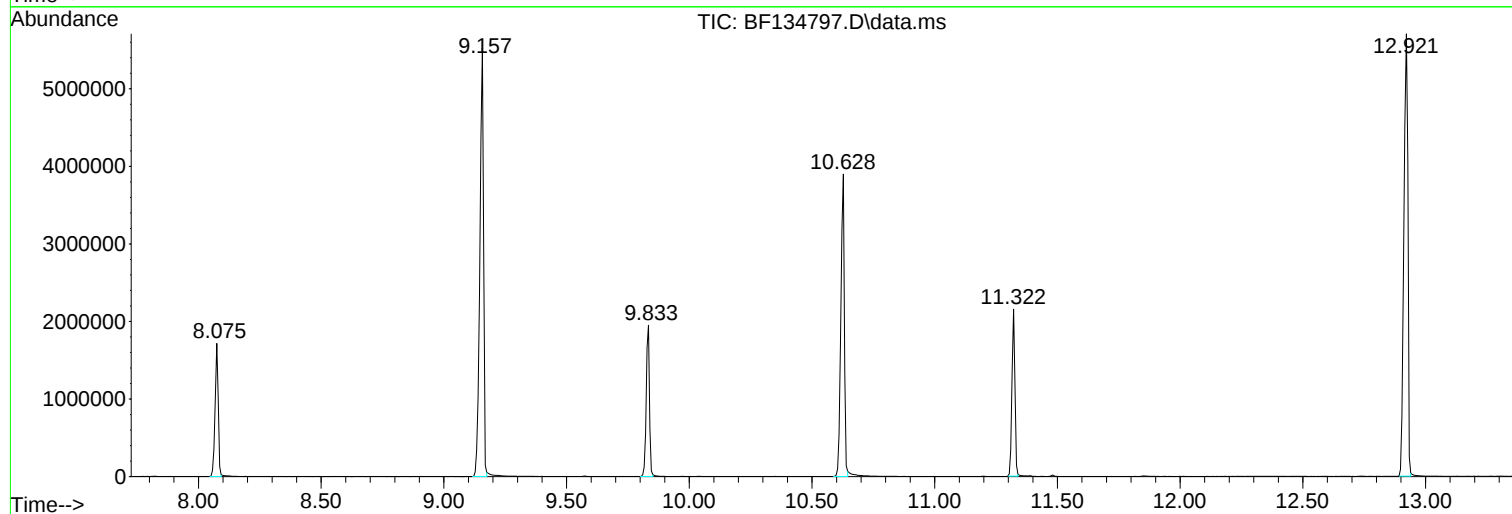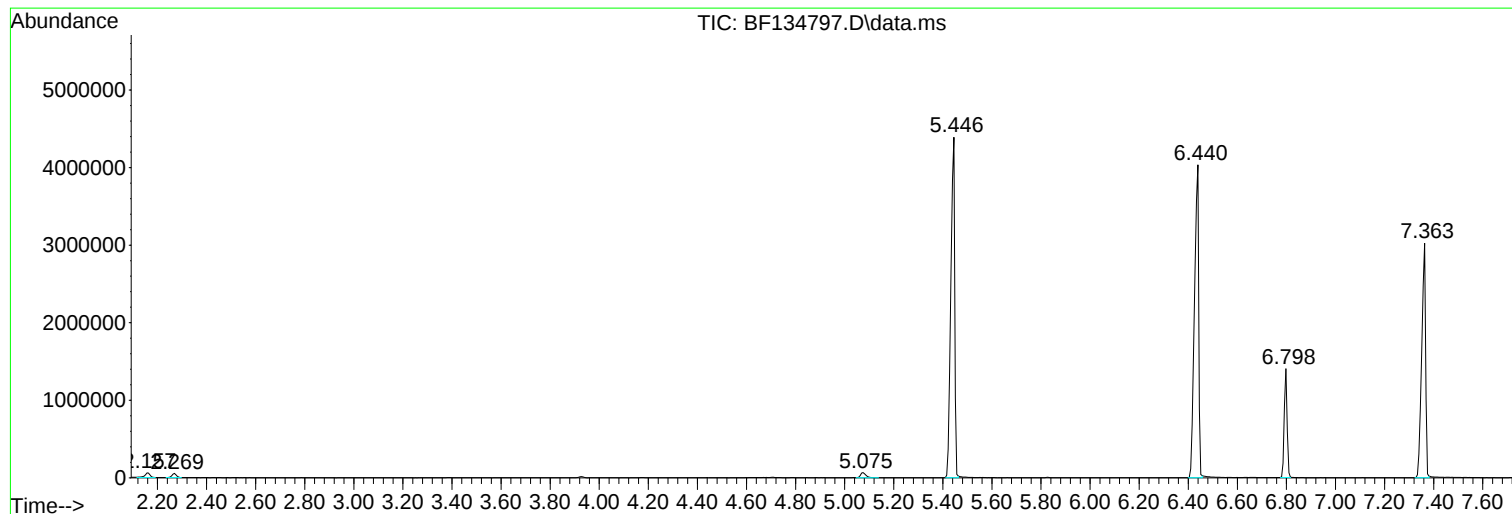

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081623\
Data File : BF134797.D
Acq On : 16 Aug 2023 08:45
Operator : CG\JU
Sample : PB154844BL
Misc :
ALS Vial : 3 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
PB154844BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (1,1'-Biphenyl)-4,4'-diamin... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
17.204	3.48 ng	188112	Perylene-d12	15.445	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	(1,1'-Biphenyl)-4,4'-diamine, N,N'-di-2-Naphthyl-p-phenylenediamine	360	C26H20N2	006311-48-4	87
2	[.mu.-Fulvalene]bis(cyclopentadiene)	360	C20H18V2	1000163-45-2	46
3	N,N'-di-2-Naphthyl-p-phenylenediamine	360	C26H20N2	000093-46-9	43
4	2,4-Dinitro-11-phenyl-5H-dibenzo[1,2-b:4,5-b']dipyrrolo[2,3-d:2',3'-d']indole	360	C19H12N4O4	071354-26-2	38
5	1H-isindole-1,3(2H)-dione, 2-[5-phenyl-2H-pyridin-2-ylidene]	360	C21H16N2O4	1000398-48-8	38

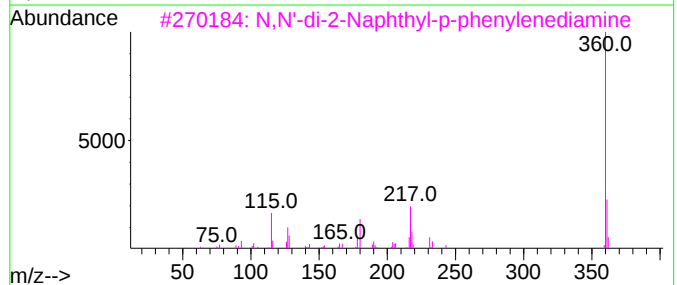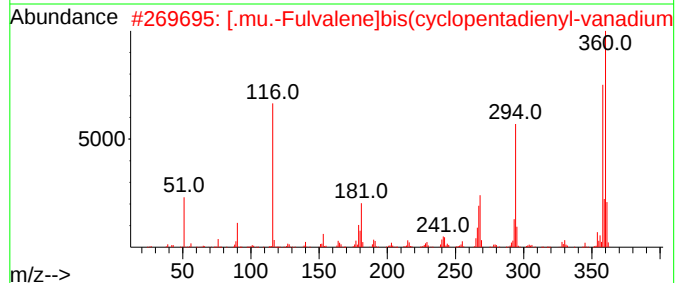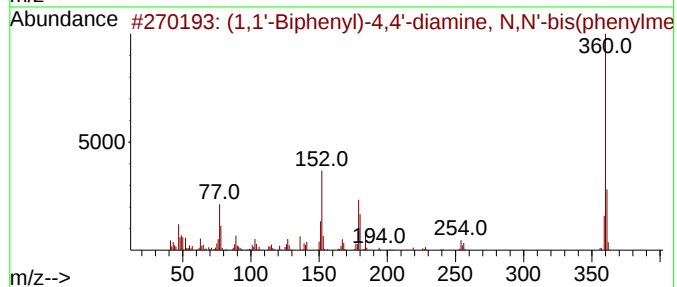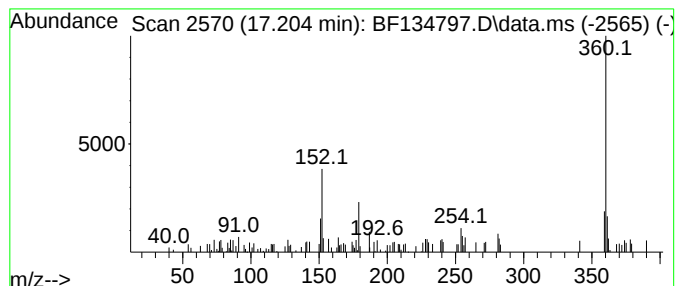

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081623\
Data File : BF134797.D
Acq On : 16 Aug 2023 08:45
Operator : CG\JU
Sample : PB154844BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB154844BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(1,1'-Biphenyl)...	17.204	3.5	ng	188112	6	15.445	1082350	20.0