
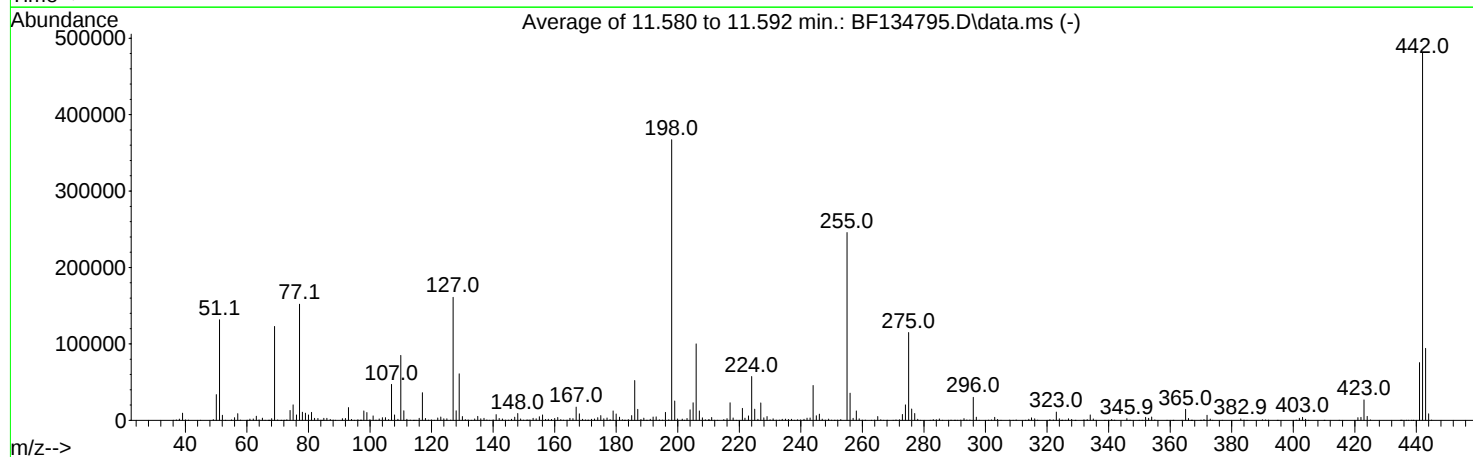


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081623\
Data File : BF134795.D
Acq On : 16 Aug 2023 07:09
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Aug 04 09:29:15 2023

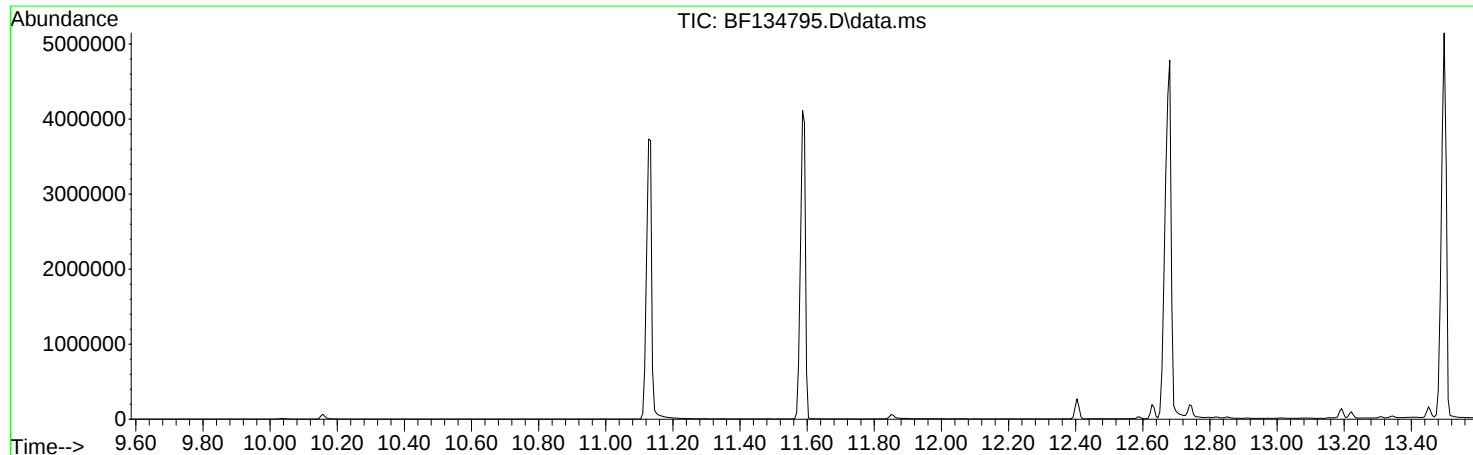




AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.9	131773	PASS
68	69	0.00	2	1.9	2308	PASS
69	198	0.00	100	33.5	122872	PASS
70	69	0.00	2	0.5	669	PASS
127	198	10	80	43.9	161045	PASS
197	198	0.00	2	0.2	825	PASS
198	198	100	100	100.0	367211	PASS
199	198	5	9	6.9	25368	PASS
275	198	10	60	31.3	114877	PASS
365	198	1	100	3.9	14386	PASS
441	198	0.01	100	20.6	75523	PASS
442	442	50	100	100.0	481301	PASS
443	442	15	24	19.6	94232	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081623\
Data File : BF134795.D
Acq On : 16 Aug 2023 07:09
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 17 02:50:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 04 09:29:15 2023
Response via : Initial Calibration

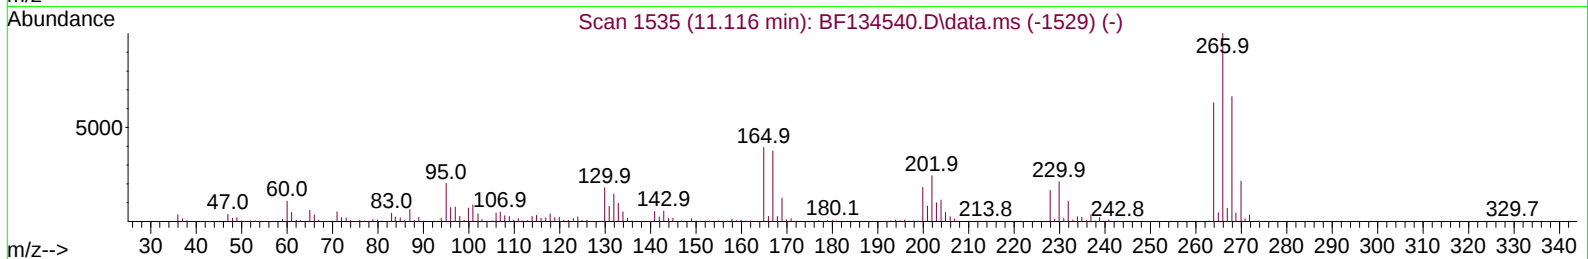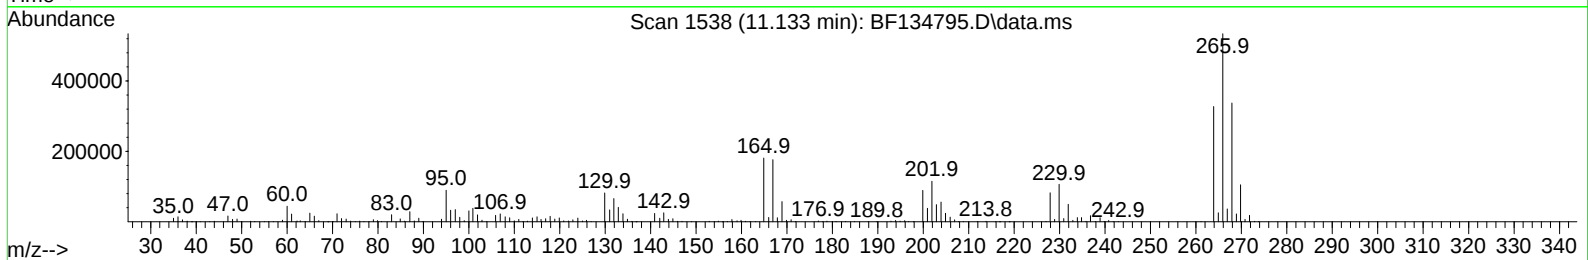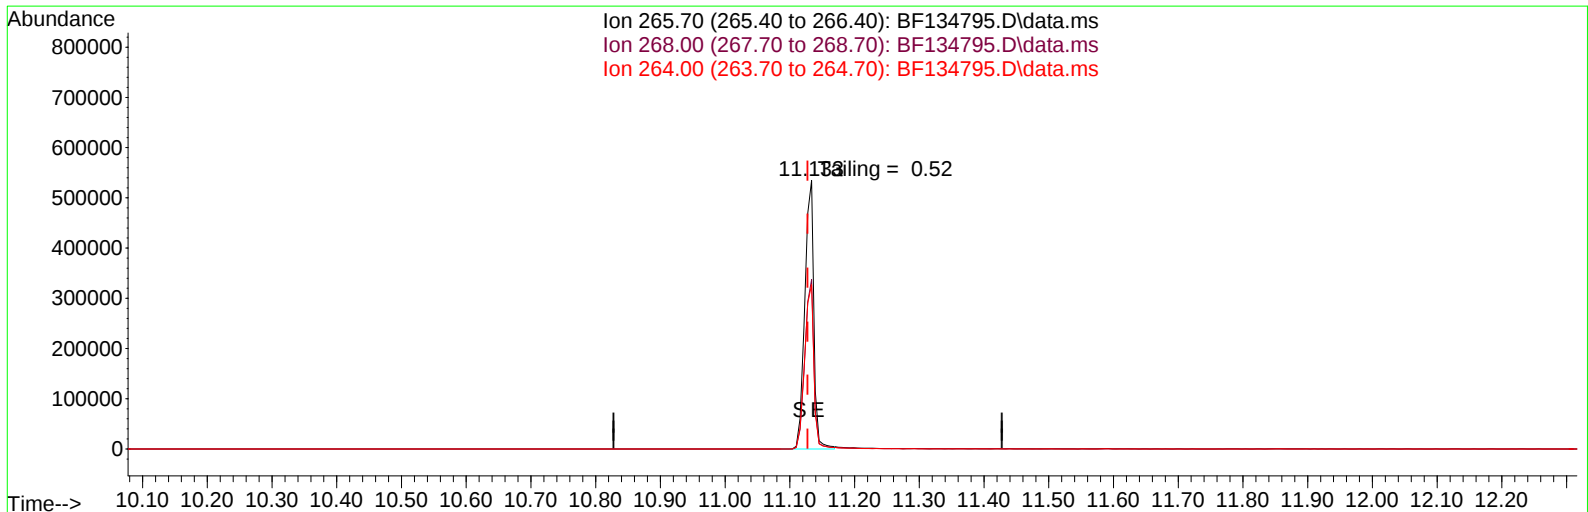

TIC: BF134795.D\data.ms

(70) Pentachlorophenol (C)

11.133min (+ 0.006) 1214058.24 ng




response 530056

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.10	63.09
264.00	59.70	61.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081623\
Data File : BF134795.D
Acq On : 16 Aug 2023 07:09
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 17 02:50:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 04 09:29:15 2023
Response via : Initial Calibration

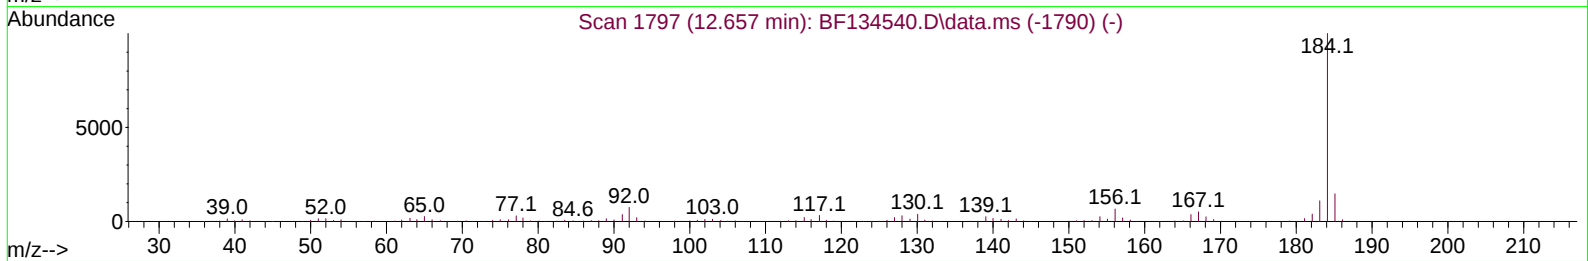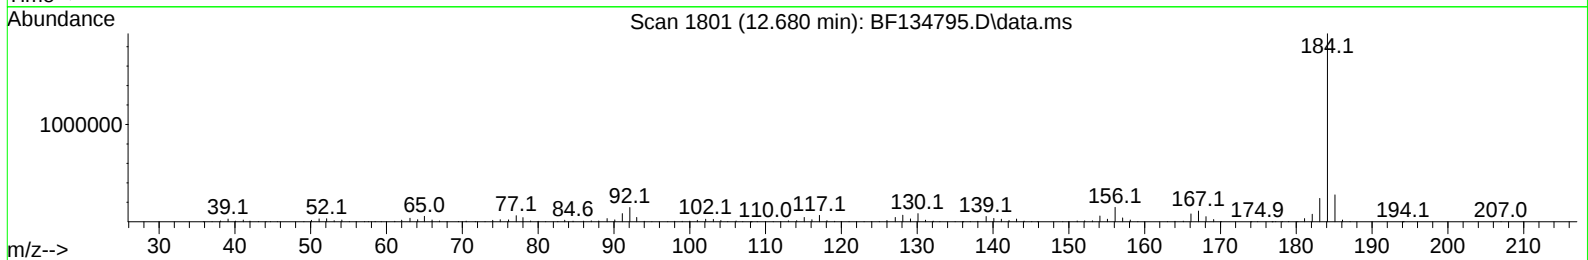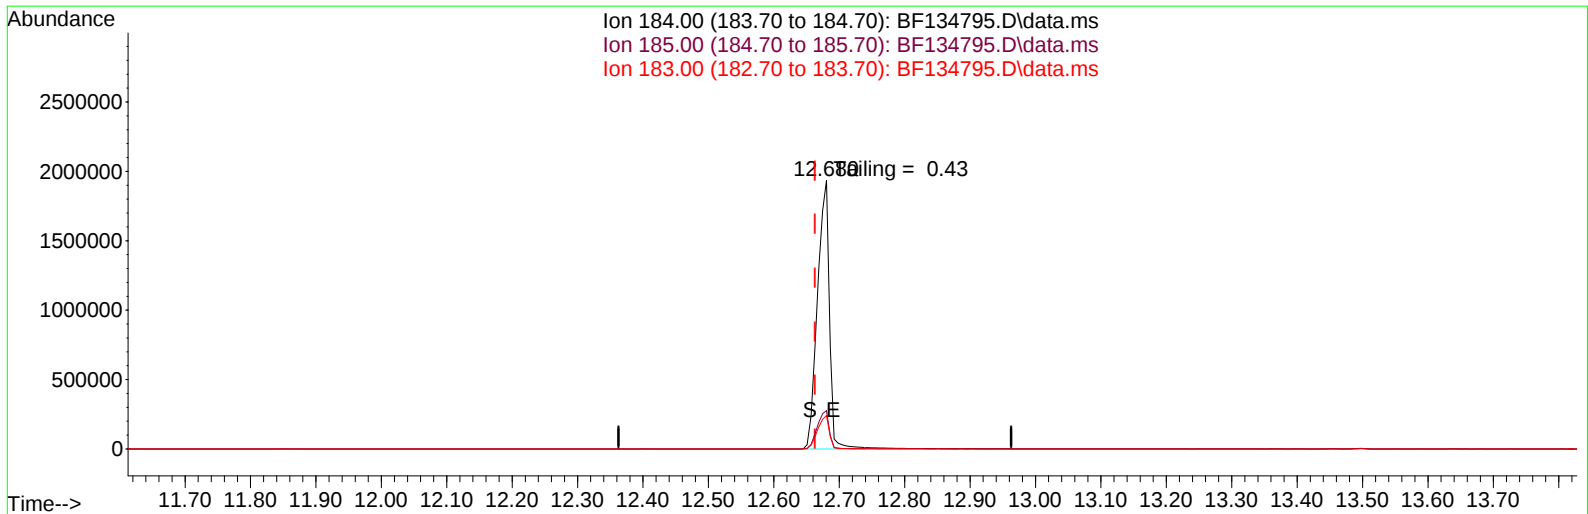

TIC: BF134795.D\data.ms

(77) Benzidine

12.680min (+ 0.018) 216514.56 ng

response 2472238

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.30
183.00	10.80	12.43
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/16/2023	BNA_F	<u>BF134795.D</u>
Compound Name	Response	Retention Time
DDT	1049935	13.498
DDD	35348	13.192
DDE	1678	12.851
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
37026	1086961	3.41

Instrument :
BNA_F
ClientSampleId :
DFTPP