


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081723\
Data File : BF134816.D
Acq On : 17 Aug 2023 09:25
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Aug 04 09:29:15 2023

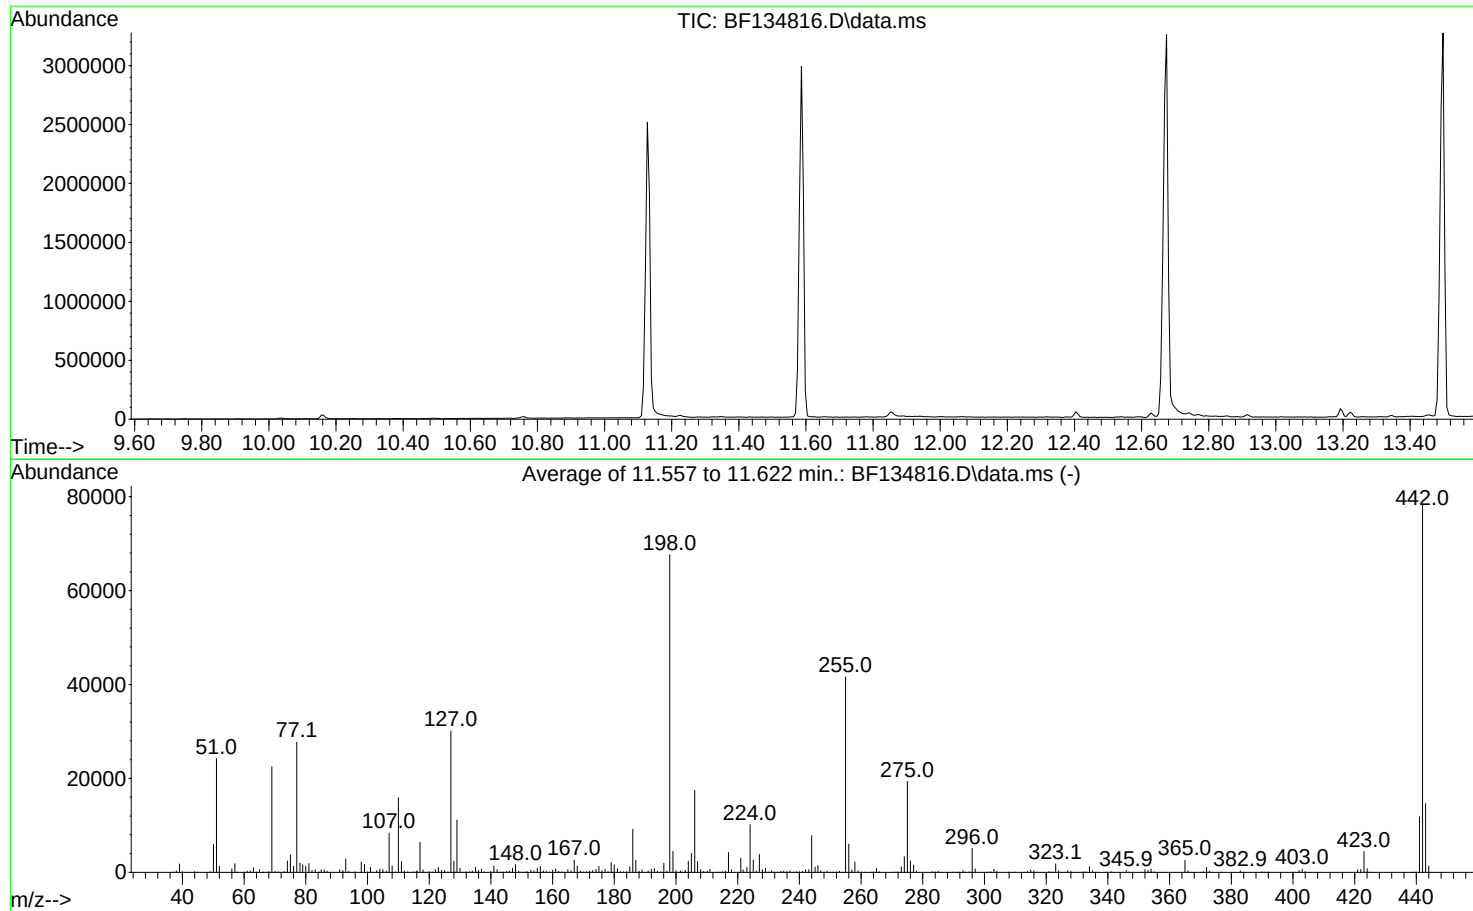




Spectrum Information: Average of 11.557 to 11.622 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.8	24215	PASS
68	69	0.00	2	0.7	162	PASS
69	198	0.00	100	33.3	22499	PASS
70	69	0.00	2	0.9	212	PASS
127	198	10	80	44.5	30091	PASS
197	198	0.00	2	0.4	257	PASS
198	198	100	100	100.0	67646	PASS
199	198	5	9	6.6	4480	PASS
275	198	10	60	28.6	19380	PASS
365	198	1	100	3.8	2604	PASS
441	198	0.01	100	17.5	11811	PASS
442	442	50	100	100.0	78337	PASS
443	442	15	24	18.7	14628	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081723\
Data File : BF134816.D
Acq On : 17 Aug 2023 09:25
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 17 09:50:56 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 04 09:29:15 2023
Response via : Initial Calibration

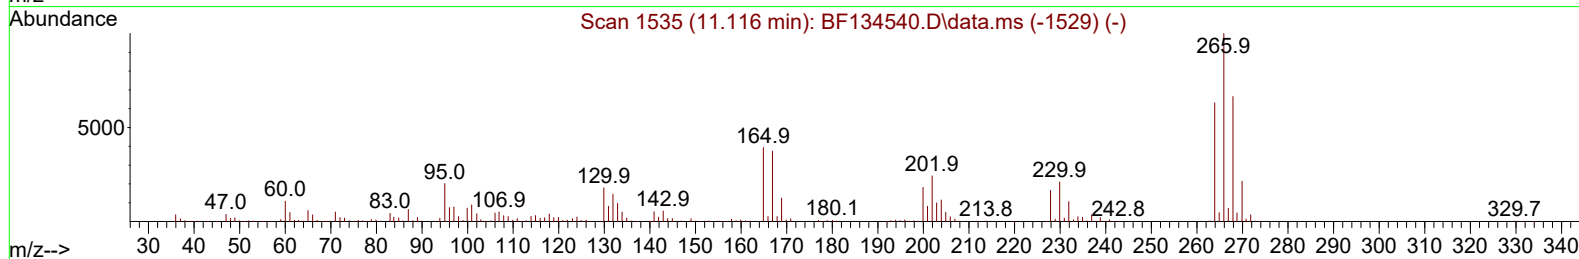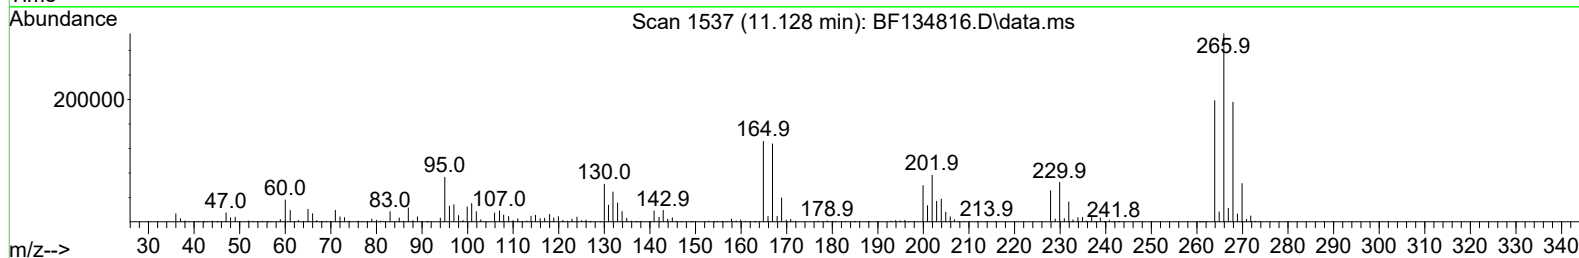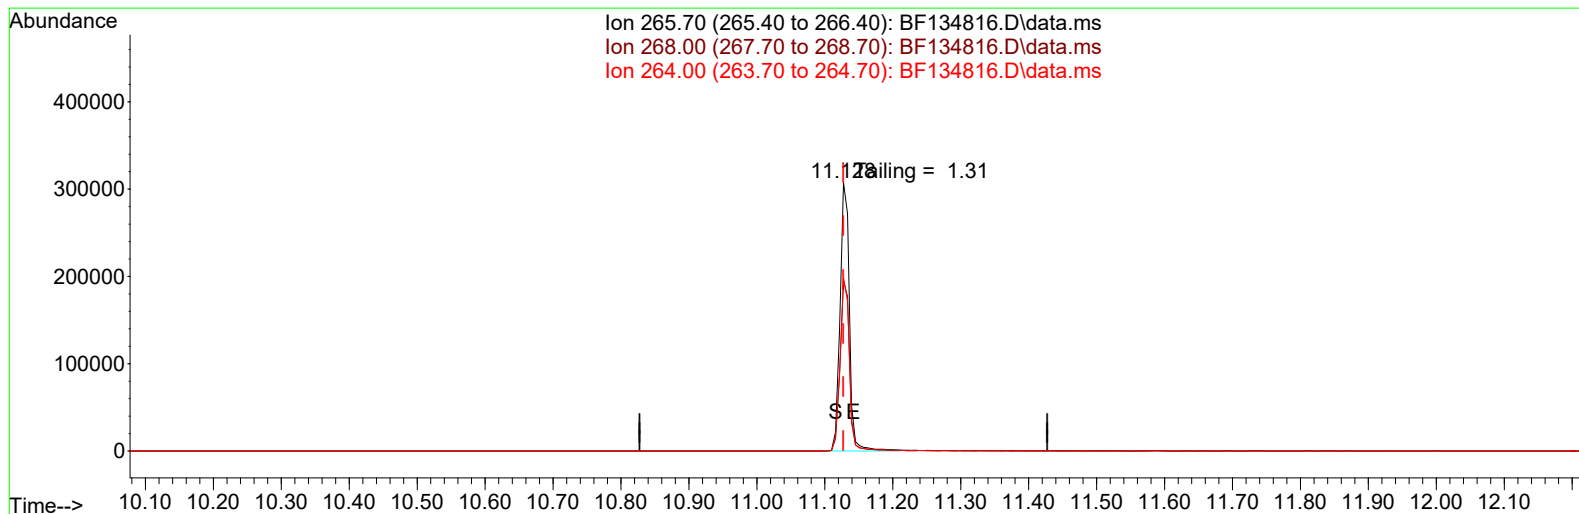

TIC: BF134816.D\data.ms

(70) Pentachlorophenol (C)

11.128min (+ 0.000) 695153.37 ng




response 293552

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.10	63.59
264.00	59.70	64.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081723\
Data File : BF134816.D
Acq On : 17 Aug 2023 09:25
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 17 09:50:56 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 04 09:29:15 2023
Response via : Initial Calibration

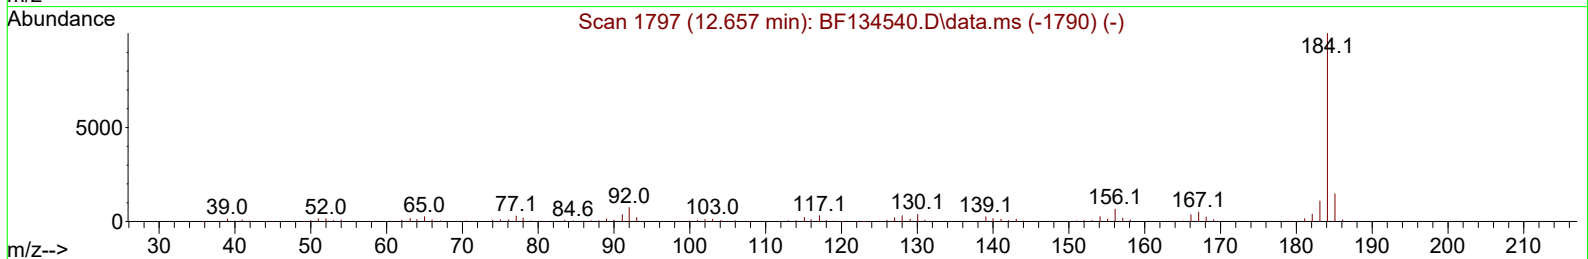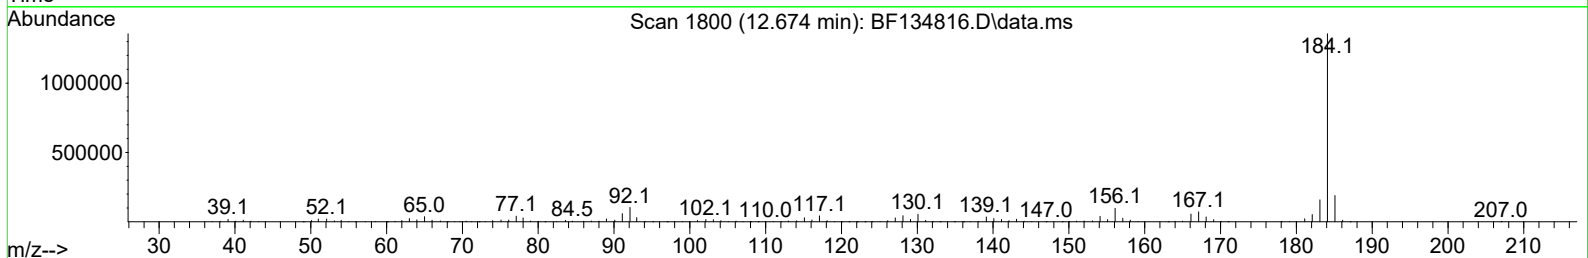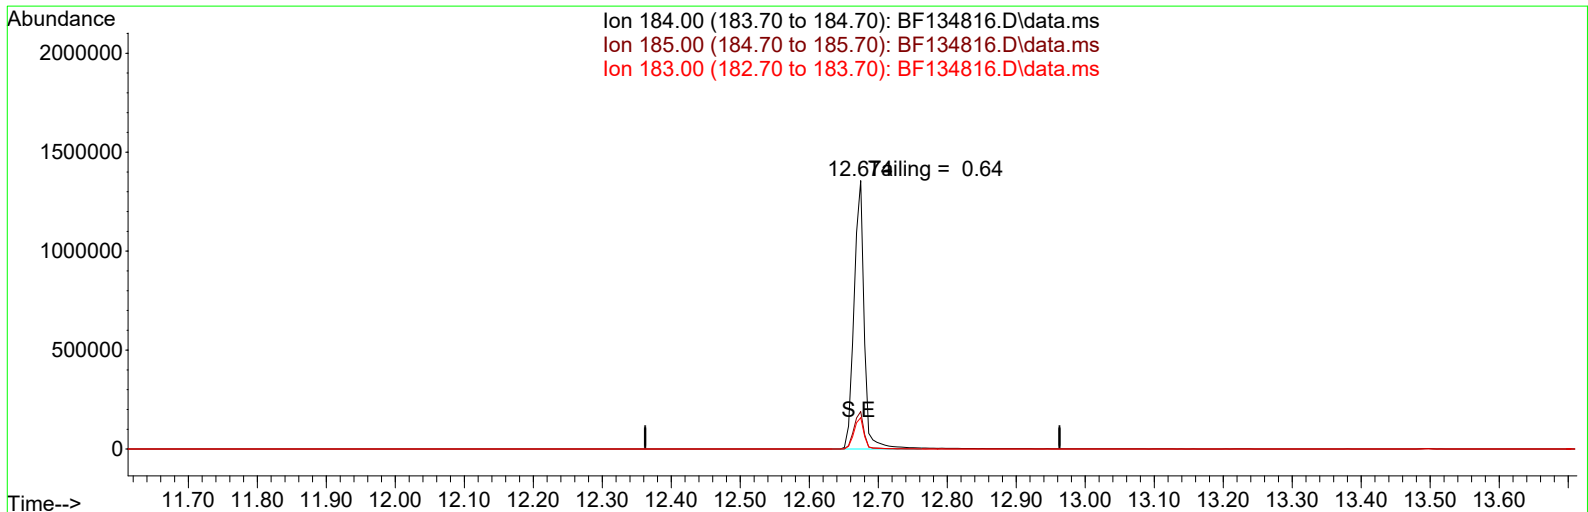

TIC: BF134816.D\data.ms

(77) Benzidine

12.674min (+ 0.012) 6793.80 ng m

response 1374061

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.98
183.00	10.80	11.70
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/17/2023	BNA_F	<u>BF134816.D</u>
Compound Name	Response	Retention Time
DDT	604655	13.498
DDD	17969	13.192
DDE	1074	12.857
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19043	623698	3.05

Instrument :
BNA_F
ClientSampleId :
DFTPP