
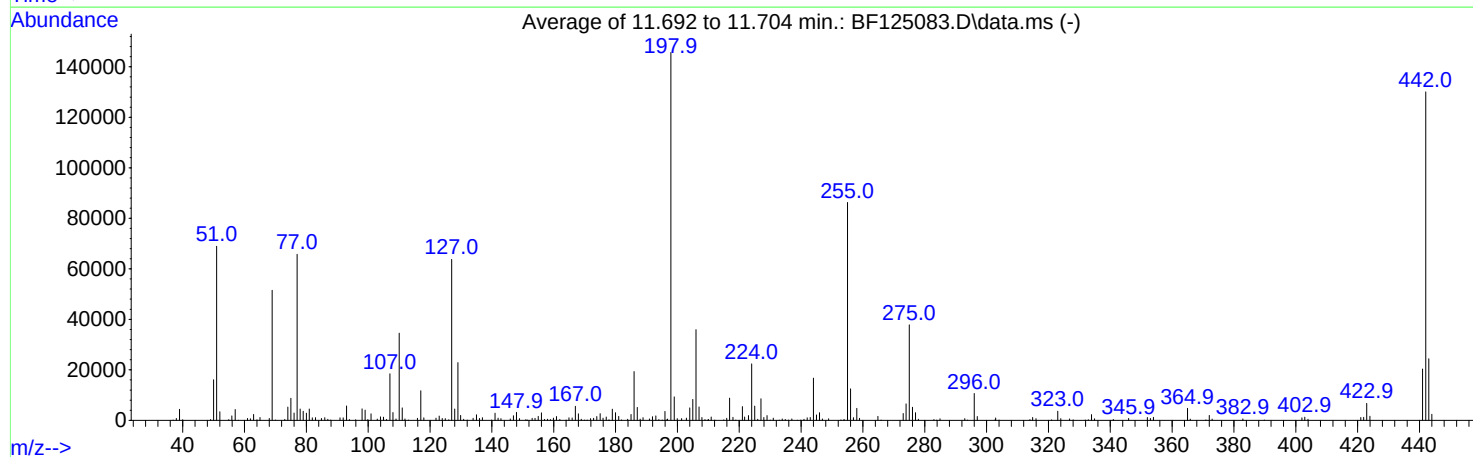


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081821\
 Data File : BF125083.D
 Acq On : 18 Aug 2021 11:53
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 18 17:03:50 2021

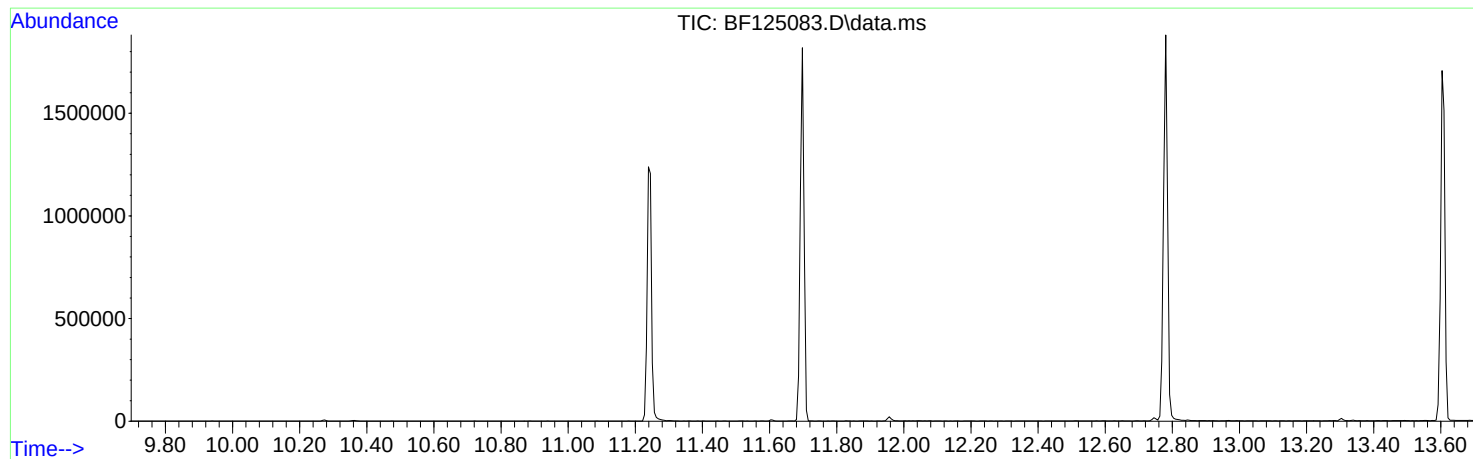




AutoFind: Scans 1633, 1634, 1635; Background Corrected with Scan 1628

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.3	68909	PASS
68	69	0.00	2	1.5	772	PASS
69	198	0.00	100	35.4	51509	PASS
70	69	0.00	2	0.2	104	PASS
127	198	10	80	43.8	63757	PASS
197	198	0.00	2	0.3	483	PASS
198	198	100	100	100.0	145659	PASS
199	198	5	9	6.4	9346	PASS
275	198	10	60	26.0	37837	PASS
365	198	1	100	3.3	4749	PASS
441	198	0.01	100	14.0	20368	PASS
442	442	50	100	100.0	130051	PASS
443	442	15	24	18.7	24371	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081821\
 Data File : BF125083.D
 Acq On : 18 Aug 2021 11:53
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Aug 18 14:25:36 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 18 14:16:18 2021
 Response via : Initial Calibration

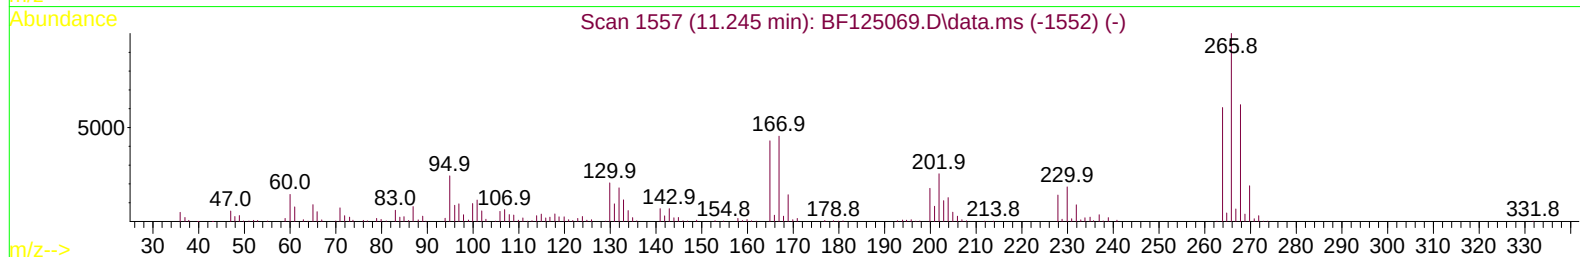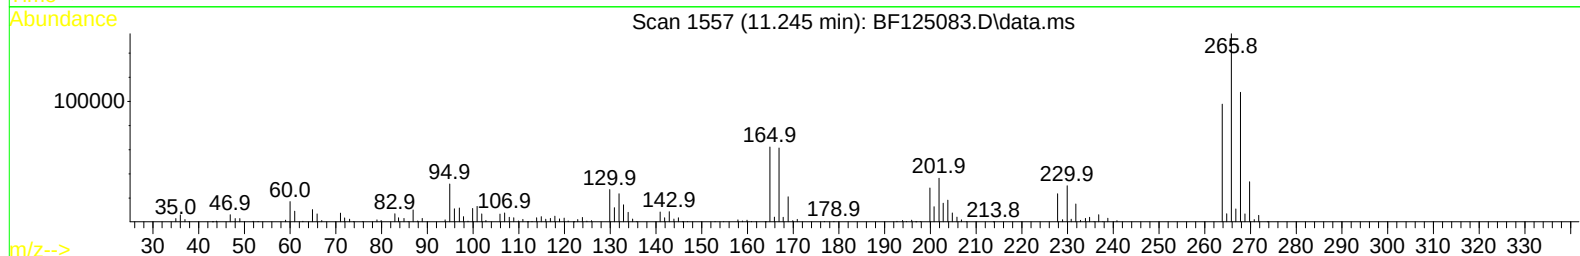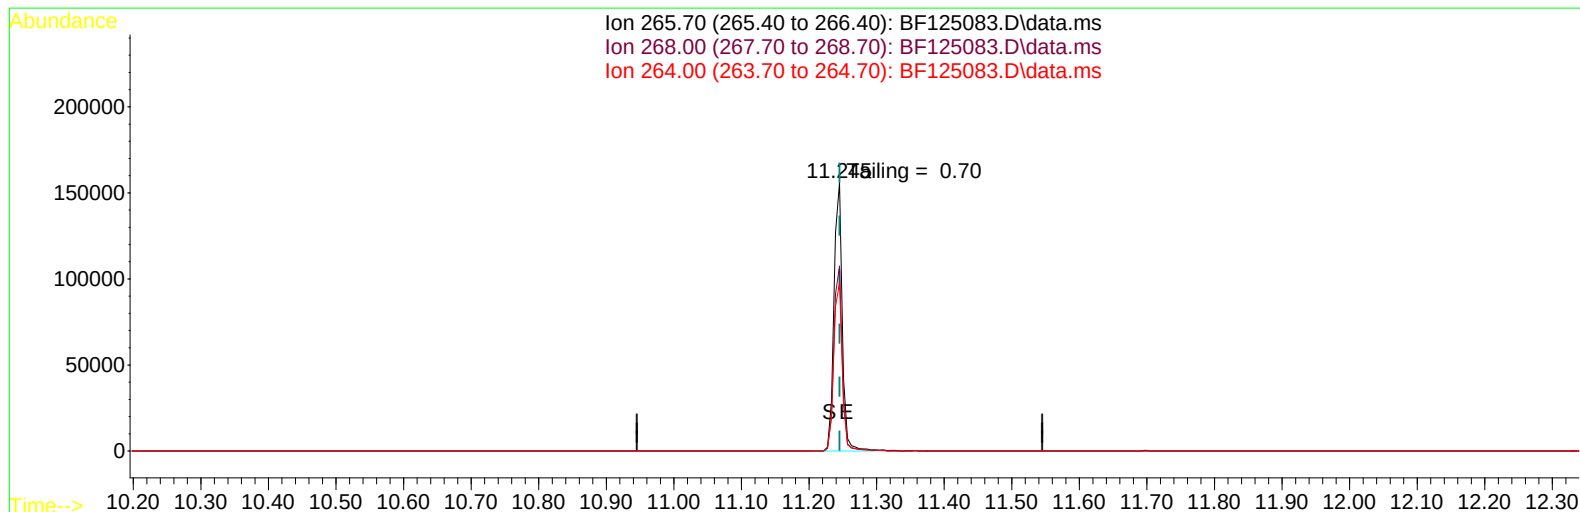

TIC: BF125083.D\data.ms

(70) Pentachlorophenol (C)

11.245min (-0.000) 35021.99 ng




response 132852

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	68.91
264.00	69.90	62.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081821\
Data File : BF125083.D
Acq On : 18 Aug 2021 11:53
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 18 14:25:36 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 18 14:16:18 2021
Response via : Initial Calibration

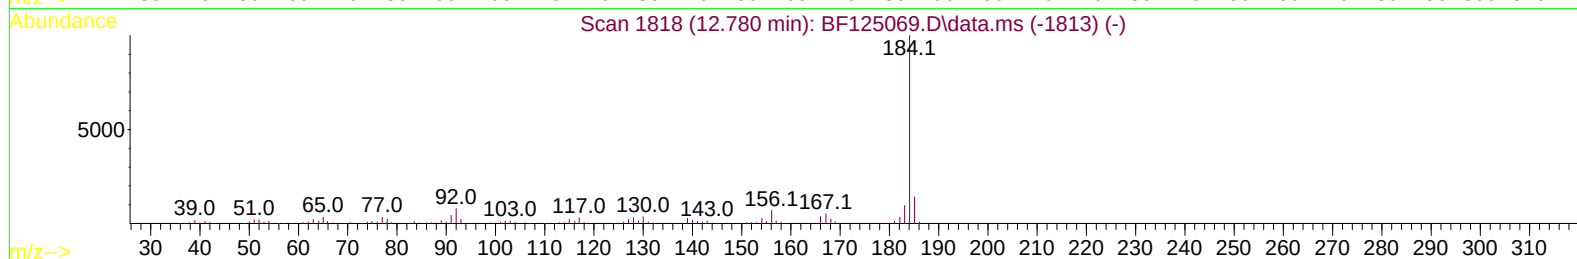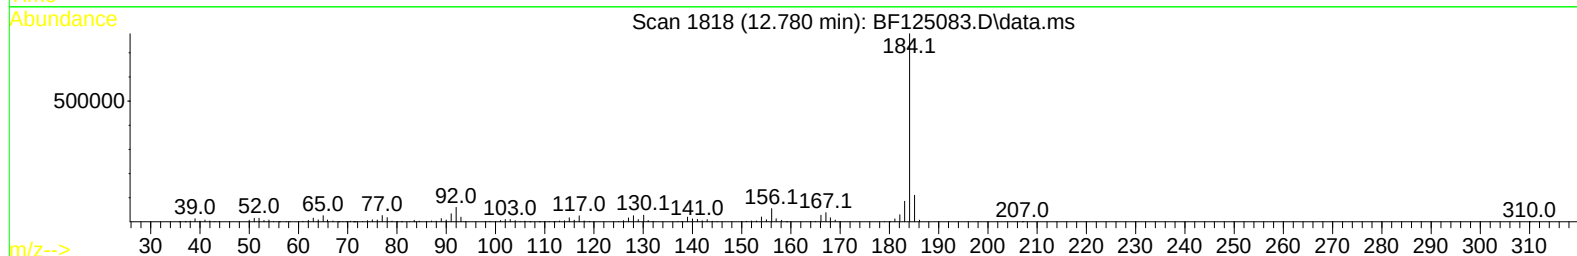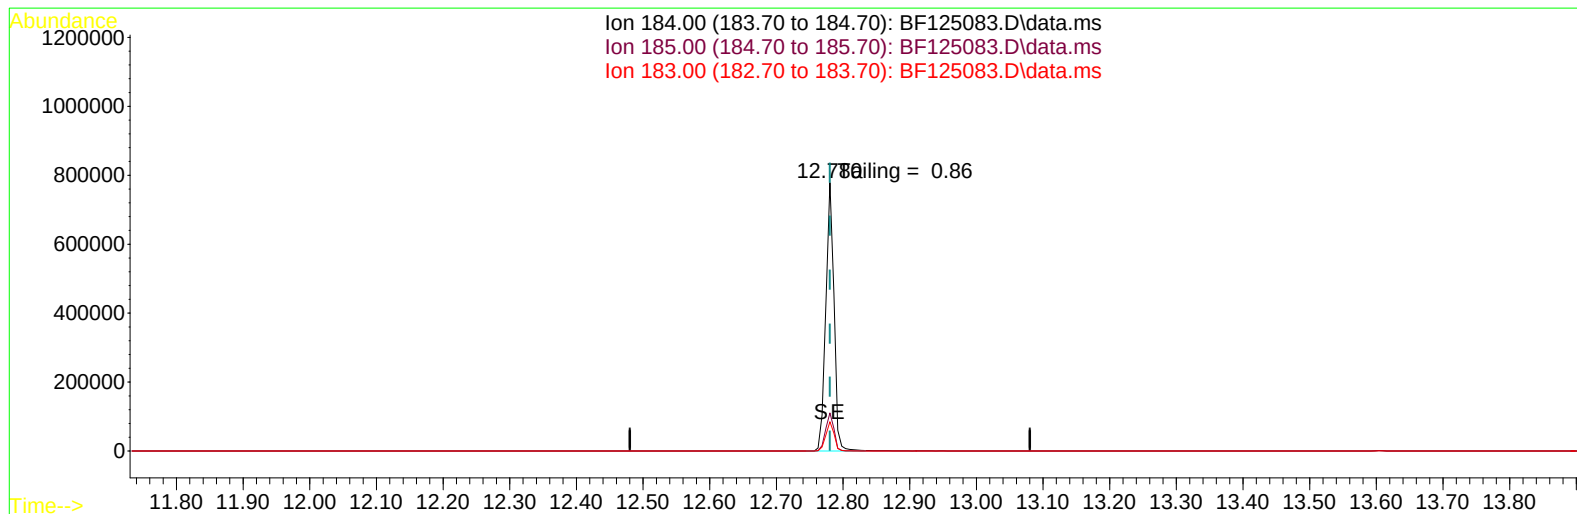

TIC: BF125083.D\data.ms

(77) Benzidine

12.780min (-0.000) 0.00 ng

response 670226

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.17
183.00	10.10	10.92
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/16/2021	BNA_F	<u>BF125083.D</u>
Compound Name	Response	Retention Time
DDT	289148	13.61
DDD	2687	13.3
DDE	465	12.96
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3152	292300	1.08