
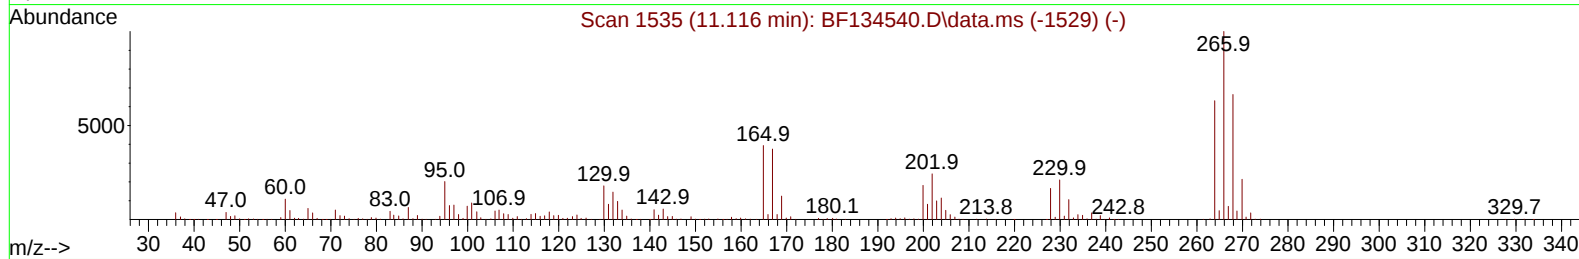
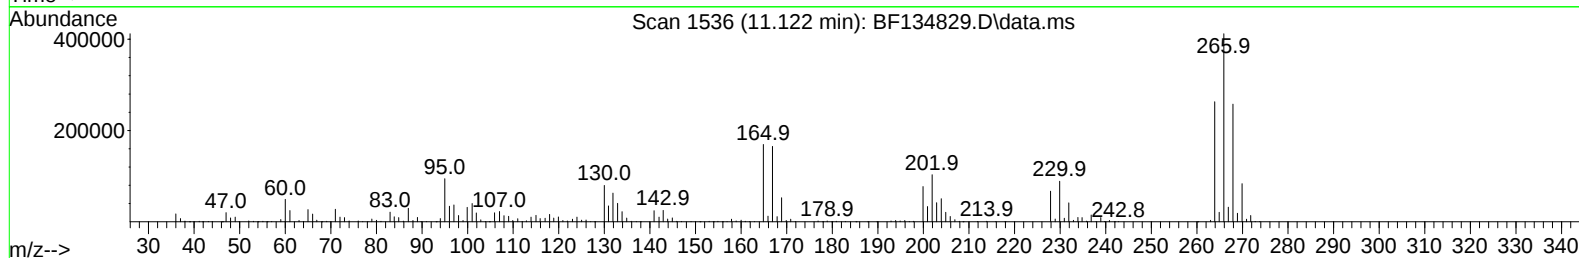


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081823\
Data File : BF134829.D
Acq On : 18 Aug 2023 07:49
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 18 08:26:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 04 09:29:15 2023
Response via : Initial Calibration

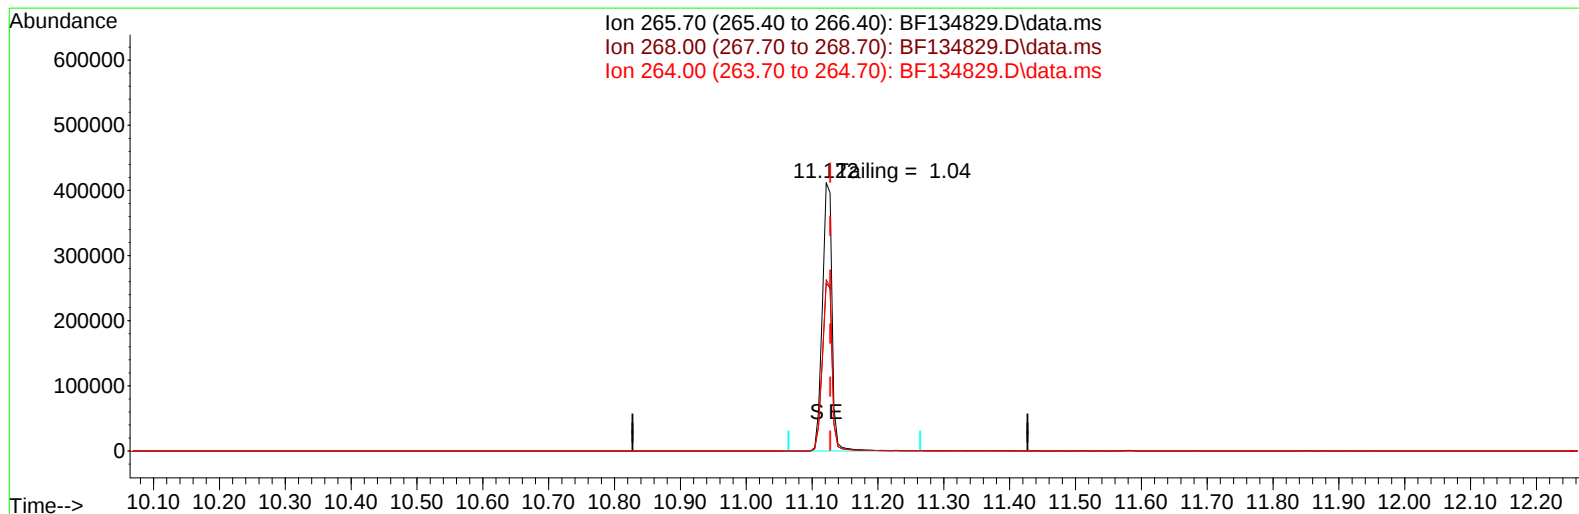

TIC: BF134829.D\data.ms

(70) Pentachlorophenol (C)




11.122min (-0.006) 32874.85 ng m

response 426358

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.10	62.54
264.00	59.70	63.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081823\
Data File : BF134829.D
Acq On : 18 Aug 2023 07:49
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 18 08:26:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 04 09:29:15 2023
Response via : Initial Calibration

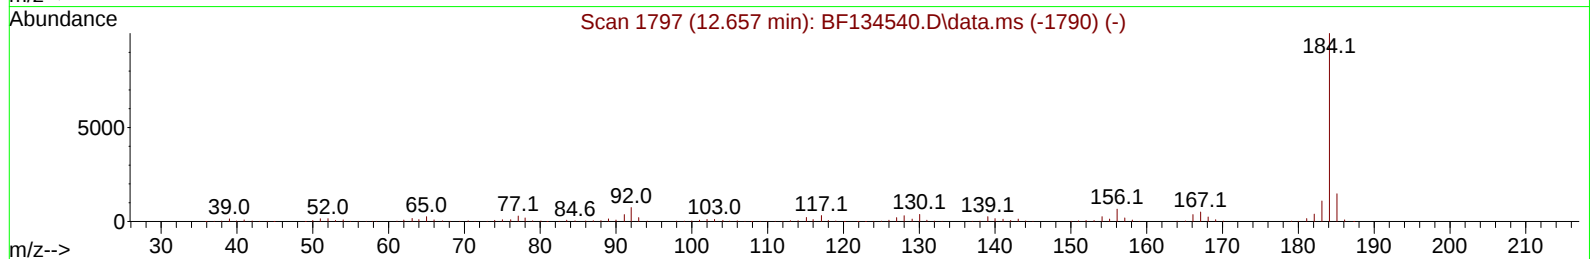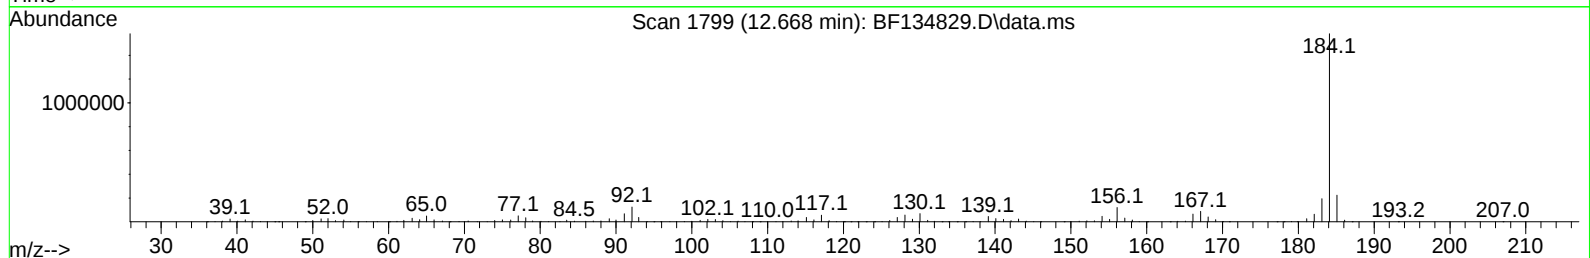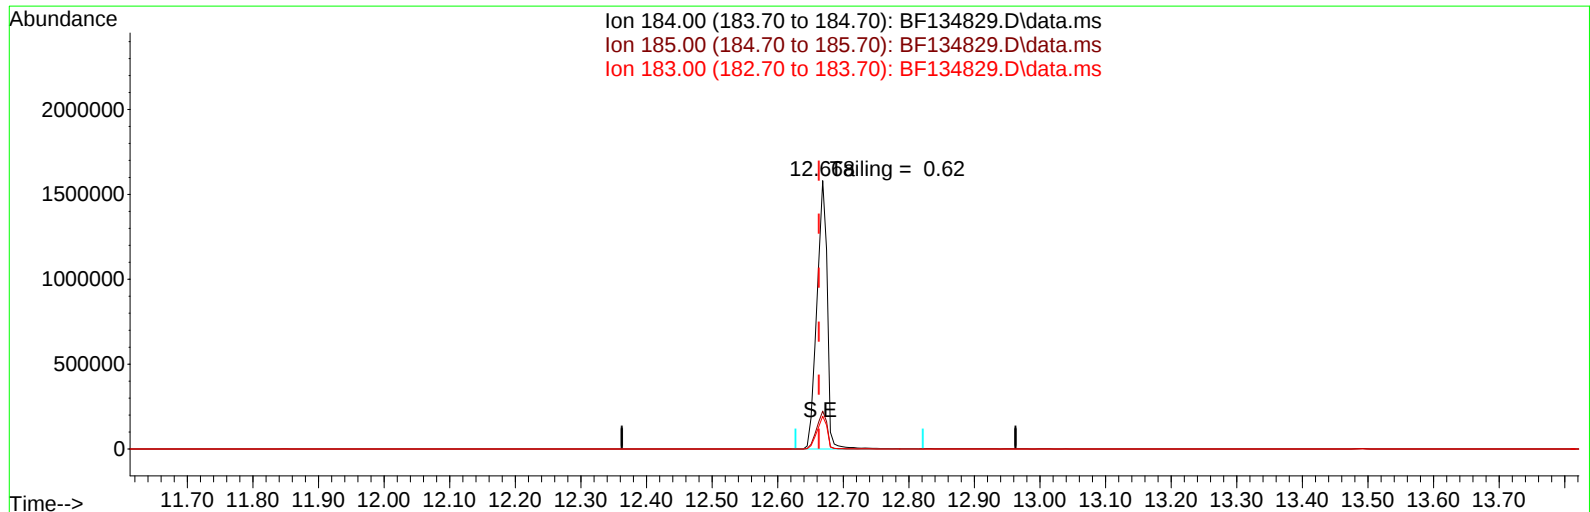

TIC: BF134829.D\data.ms

(77) Benzidine

12.668min (+ 0.006) 41501.56 ng

response 1729749

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.16
183.00	10.80	12.24
0.00	0.00	0.00