
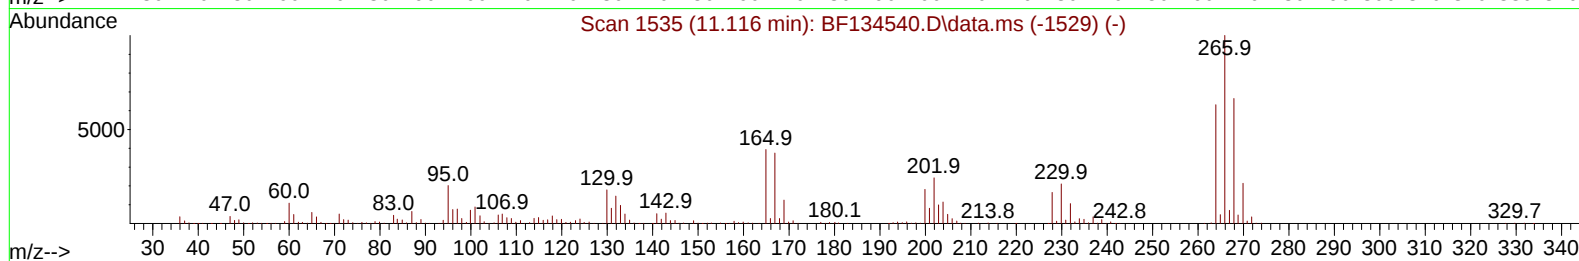
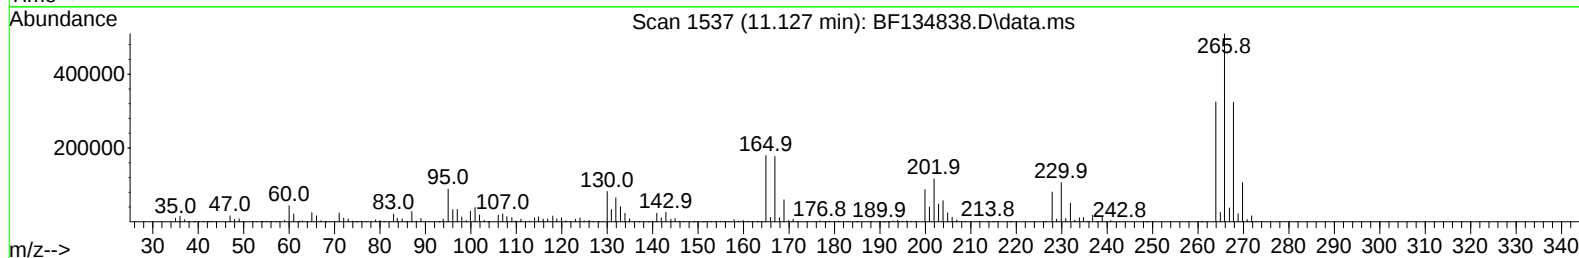


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081823\
Data File : BF134838.D
Acq On : 18 Aug 2023 13:22
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 18 13:50:22 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 04 09:29:15 2023
Response via : Initial Calibration

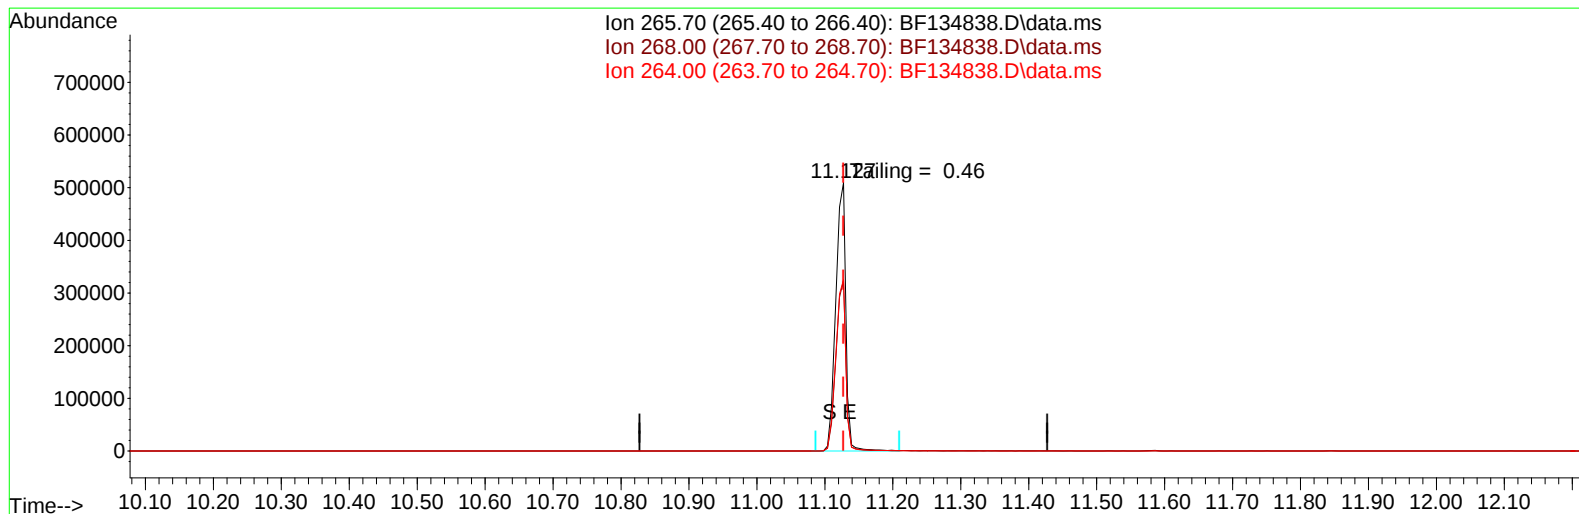

TIC: BF134838.D\data.ms

(70) Pentachlorophenol (C)




11.127min (-0.000) 30316.28 ng

response 524234

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.10	63.54
264.00	59.70	63.80
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081823\
Data File : BF134838.D
Acq On : 18 Aug 2023 13:22
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 18 13:50:22 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 04 09:29:15 2023
Response via : Initial Calibration

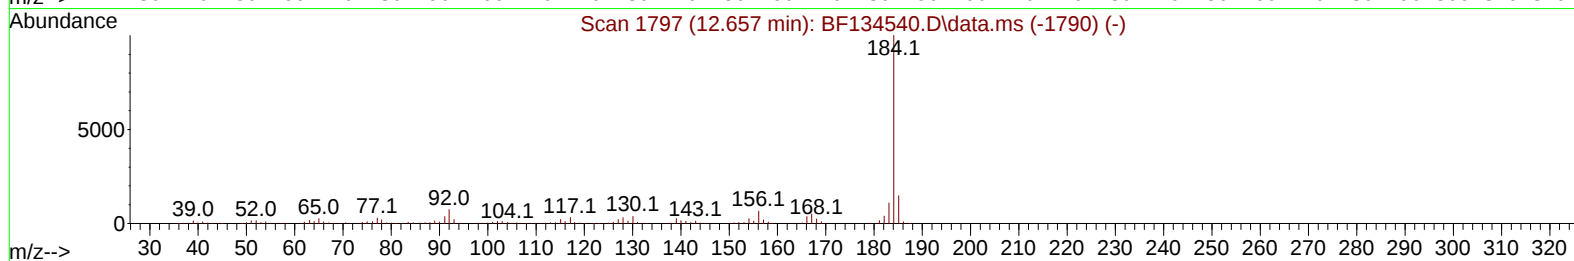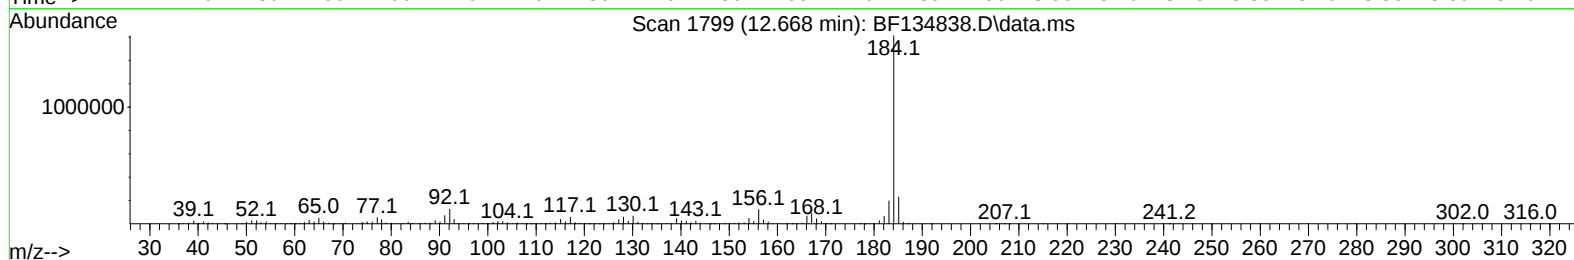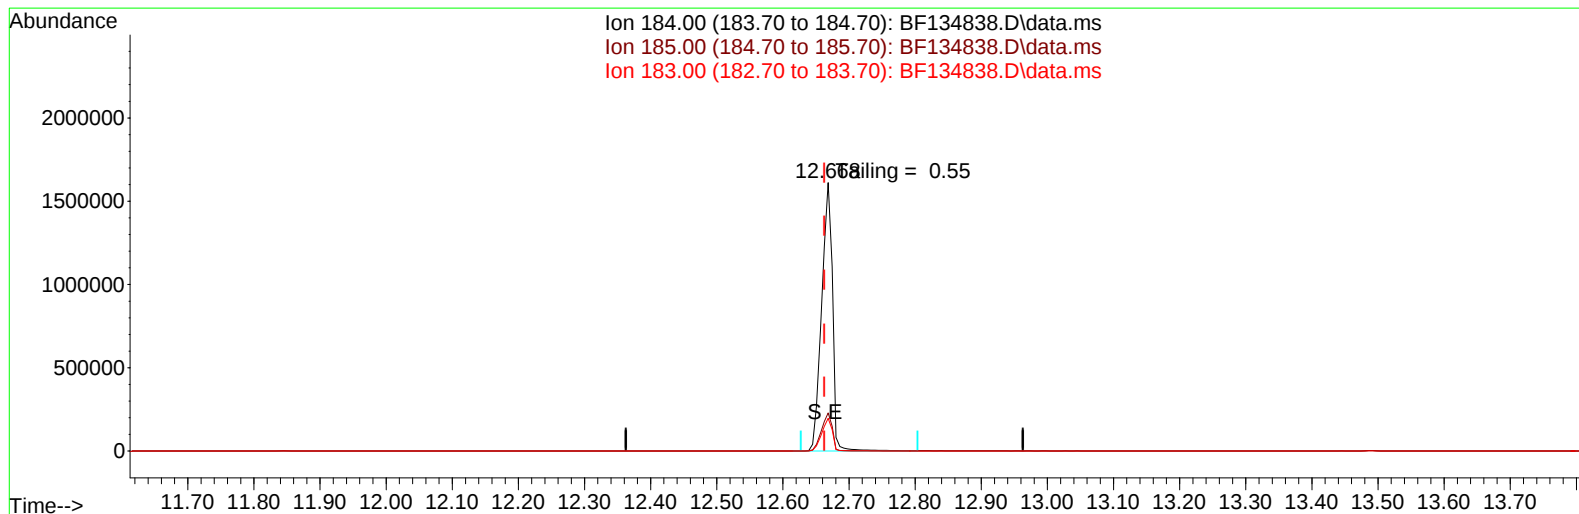

TIC: BF134838.D\data.ms

(77) Benzidine

12.668min (+ 0.006) 33791.05 ng

response 1837498

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.22
183.00	10.80	12.21
0.00	0.00	0.00