

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081823\
 Data File : BF134833.D
 Acq On : 18 Aug 2023 10:32
 Operator : CG\JU
 Sample : 04047-04 20X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 NEVINS-SB05-Z83-84

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/21/2023
 Supervised By :mohammad ahmed 08/21/2023

Quant Time: Aug 18 11:15:52 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 04 09:29:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.792	152	9105	20.000	ng	0.00
21) Naphthalene-d8	8.081	136	26601	20.000	ng	# 0.00
39) Acenaphthene-d10	9.827	164	30217	20.000	ng	0.00
64) Phenanthrene-d10	11.321	188	25063	20.000	ng	# 0.00
76) Chrysene-d12	13.968	240	16162	20.000	ng	# 0.00
86) Perylene-d12	15.433	264	15558	20.000	ng	# 0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.416	112	34507	57.610	ng	-0.01
7) Phenol-d6	6.422	99	45890	59.934	ng	-0.02
23) Nitrobenzene-d5	7.351	82	29914	70.276	ng	-0.02
42) 2,4,6-Tribromophenol	10.616	330	8355	27.124	ng	-0.01
45) 2-Fluorobiphenyl	9.145	172	60162	33.104	ng	-0.02
79) Terphenyl-d14	12.910	244	42013	45.826	ng	-0.01
Target Compounds						Qvalue
31) Naphthalene	8.133	128	10188586	7620.959	ng	96
37) 2-Methylnaphthalene	8.810	142	3895201	4395.601	ng	98
38) 1-Methylnaphthalene	8.904	142	2762597	3352.534	ng	96
46) 1,1'-Biphenyl	9.251	154	977741	416.102	ng	99
49) Acenaphthylene	9.704	152	3033838	1096.199	ng	97
52) Acenaphthene	9.863	154	548901	306.044	ng	99
55) Dibenzofuran	10.033	168	271832	106.467	ng	# 87
58) Fluorene	10.386	166	1505296	809.429	ng	94
71) Phenanthrene	11.357	178	3912641	2939.085	ng	98
72) Anthracene	11.404	178	1471279	1081.982	ng	98
73) Carbazole	11.551	167	58774	48.408	ng	# 88
75) Fluoranthene	12.539	202	1581496	1124.649	ng	96
78) Pyrene	12.774	202	2255711	1612.926	ng	97
81) Benzo(a)anthracene	13.957	228	964726m	834.784	ng	
83) Chrysene	13.998	228	819436	727.794	ng	98
87) Indeno(1,2,3-cd)pyrene	16.915	276	143080	156.371	ng	# 95
88) Benzo(b)fluoranthene	15.009	252	542498m	571.733	ng	
89) Benzo(k)fluoranthene	15.033	252	168990m	178.782	ng	
90) Benzo(a)pyrene	15.374	252	568391	642.463	ng	# 95
91) Dibenzo(a,h)anthracene	16.927	278	40419	54.660	ng	# 89
92) Benzo(g,h,i)perylene	17.362	276	160070	212.209	ng	# 93

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081823\
Data File : BF134833.D
Acq On : 18 Aug 2023 10:32
Operator : CG\JU
Sample : 04047-04 20X
Misc :
ALS Vial : 5 Sample Multiplier: 1


Instrument :
BNA_F
ClientSampleId :
NEVINS-SB05-Z83-84

Quant Time: Aug 18 11:15:52 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 04 09:29:15 2023
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 08/21/2023
Supervised By :mohammad ahmed 08/21/2023

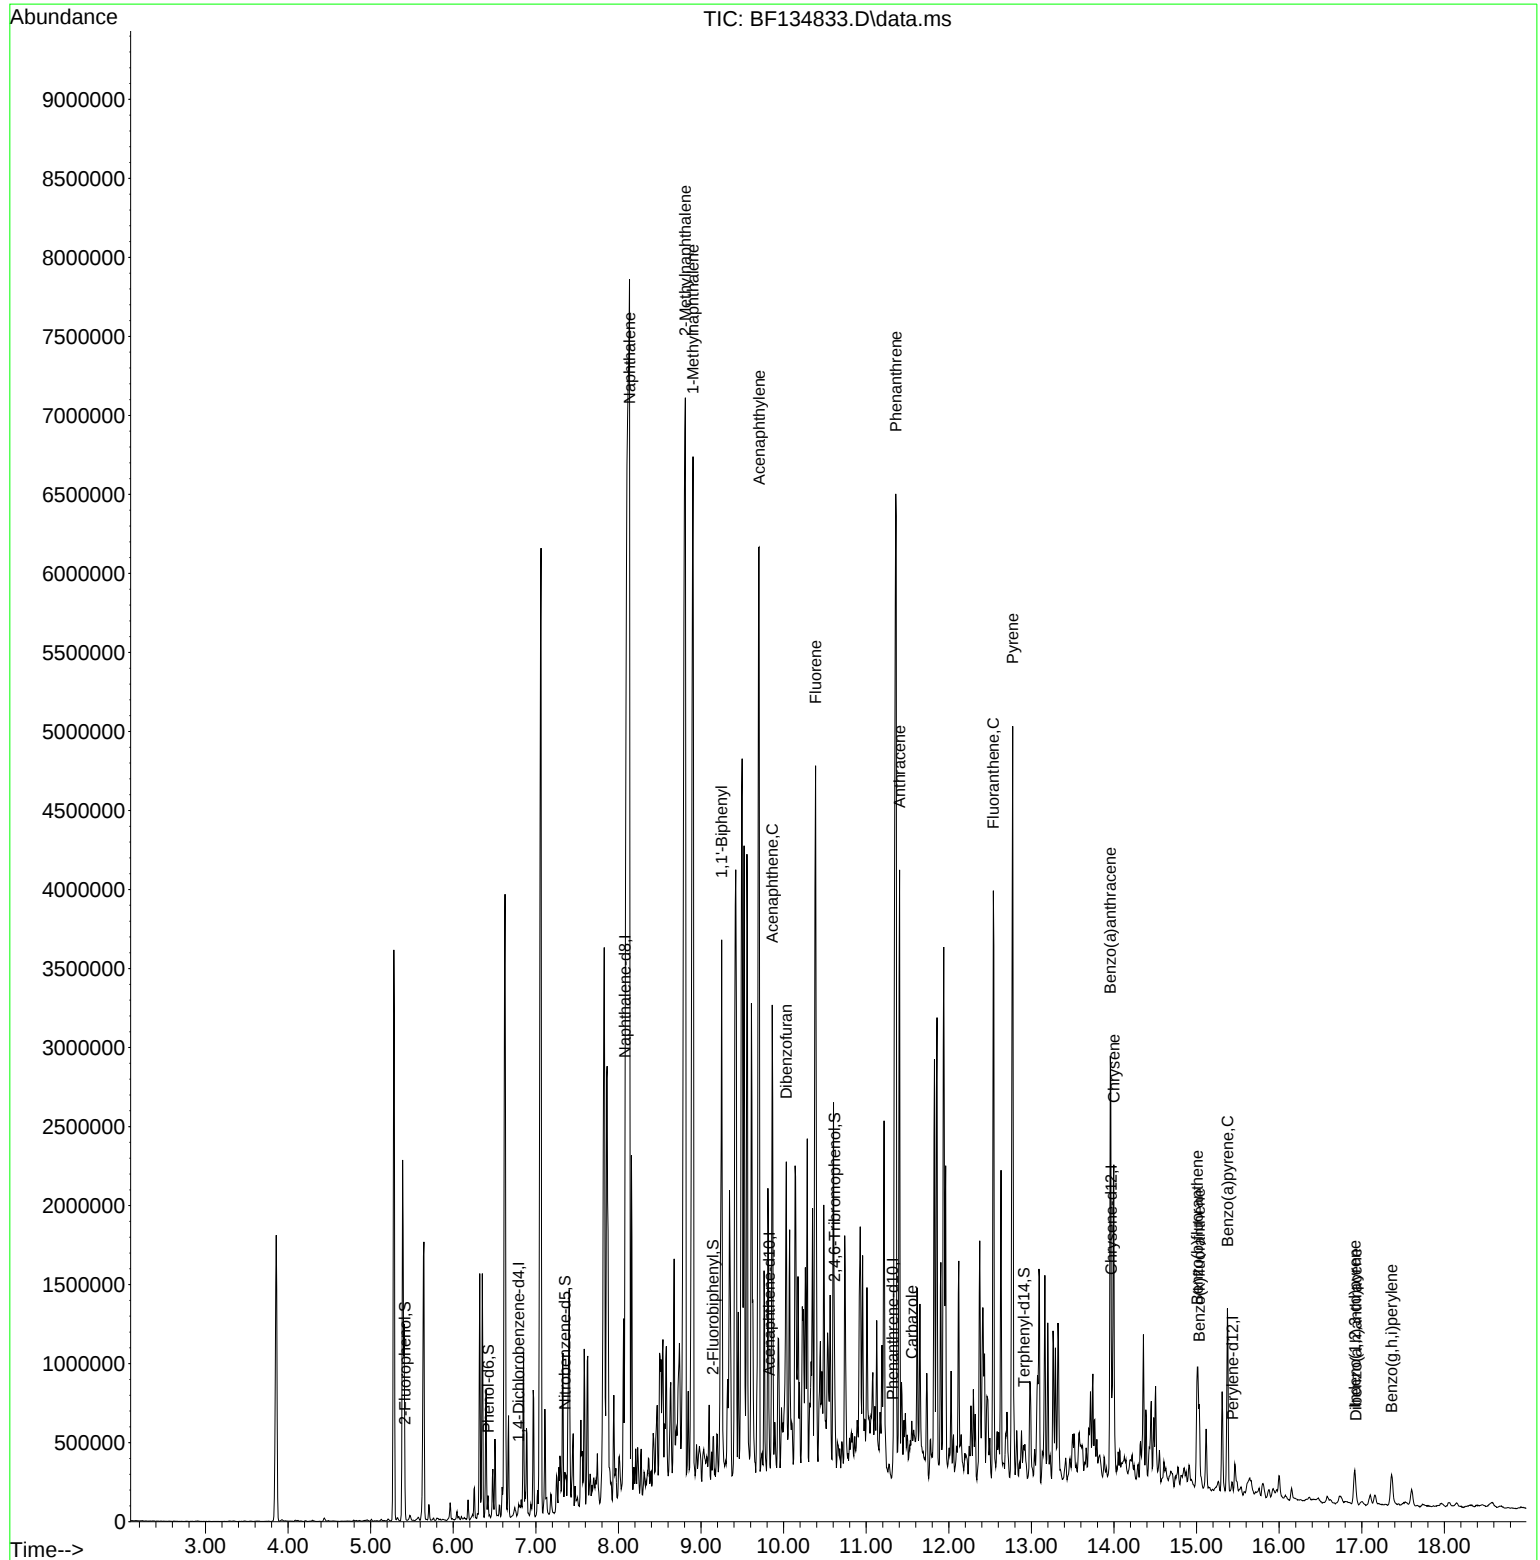



#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.792 min Scan# 800
Delta R.T. -0.006 min
Lab File: BF134833.D
Acq: 18 Aug 2023 10:32




Instrument :
BNA_F
Client SampleId :
NEVINS-SB05-Z83-84

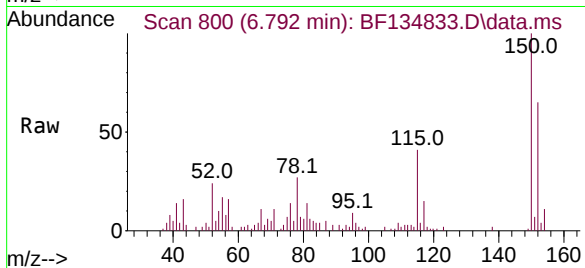

Tgt Ion:152 Resp: 9105
Ion Ratio Lower Upper
152 100
150 152.8 128.3 192.5
115 62.6 52.4 78.6




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 08/21/2023
Supervised By :mohammad ahmed 08/21/2023

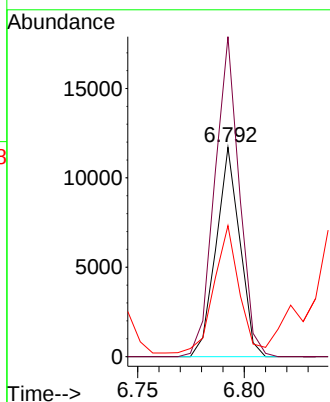

#5
2-Fluorophenol
Concen: 57.610 ng
RT: 5.416 min Scan# 566
Delta R.T. -0.012 min
Lab File: BF134833.D
Acq: 18 Aug 2023 10:32


Tgt Ion:112 Resp: 34507
Ion Ratio Lower Upper
112 100
64 58.5 44.9 67.3
63 31.4 25.4 38.0

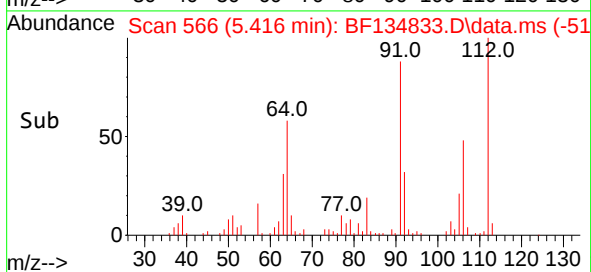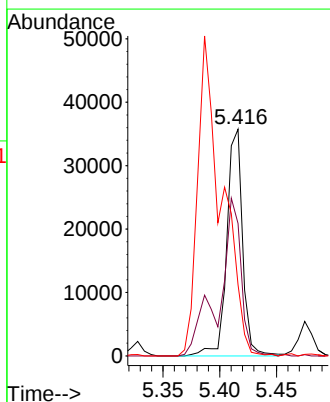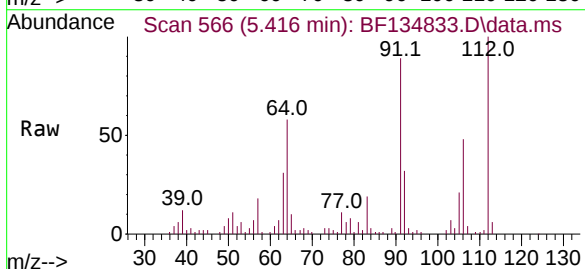



#7
Phenol-d6
Concen: 59.934 ng
RT: 6.422 min Scan# 738
Delta R.T. -0.018 min
Lab File: BF134833.D
Acq: 18 Aug 2023 10:32




Instrument :
BNA_F
ClientSampleId :
NEVINS-SB05-Z83-84



Tgt Ion: 99 Resp: 45890
Ion Ratio Lower Upper
99 100
42 18.7 18.7 28.1
71 31.7 36.4 54.6




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 08/21/2023
Supervised By :mohammad ahmed 08/21/2023

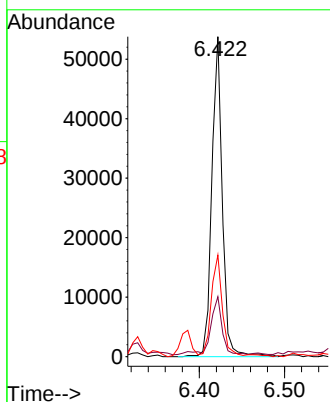

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.081 min Scan# 1019
Delta R.T. -0.000 min
Lab File: BF134833.D
Acq: 18 Aug 2023 10:32


Tgt Ion:136 Resp: 26601
Ion Ratio Lower Upper
136 100
137 20.2 8.4 12.6#
54 18.8 5.2 7.8#
68 23.2 2.9 4.3#

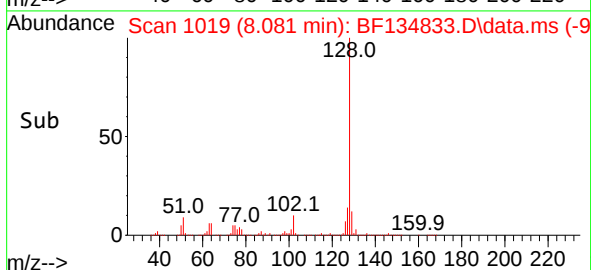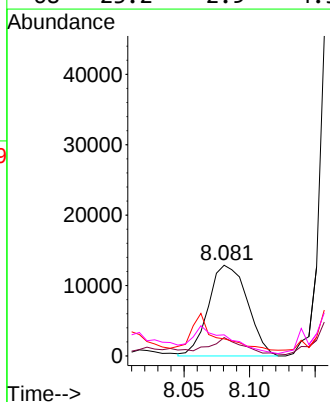



#23
Nitrobenzene-d5
Concen: 70.276 ng
RT: 7.351 min Scan# 896
Delta R.T. -0.018 min
Lab File: BF134833.D
Acq: 18 Aug 2023 10:32




Instrument :
BNA_F
ClientSampleId :
NEVINS-SB05-Z83-84

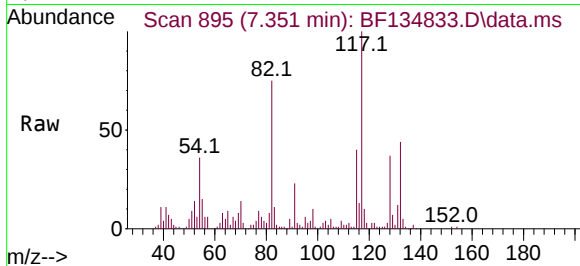

Tgt Ion: 82 Resp: 29914
Ion Ratio Lower Upper
82 100
128 49.4 34.3 51.5
54 48.5 43.8 65.6




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 08/21/2023
Supervised By :mohammad ahmed 08/21/2023



#31
Naphthalene
Concen: 7620.959 ng
RT: 8.133 min Scan# 1028
Delta R.T. 0.029 min
Lab File: BF134833.D
Acq: 18 Aug 2023 10:32

Tgt Ion:128 Resp:10188586
Ion Ratio Lower Upper
128 100
129 12.1 8.4 12.6
127 14.9 10.7 16.1

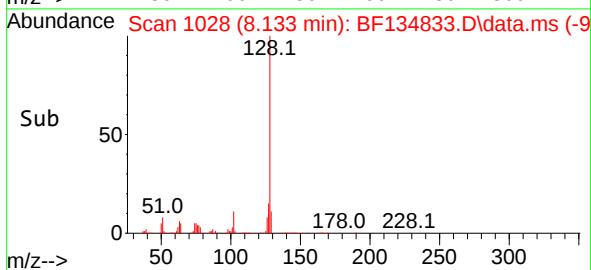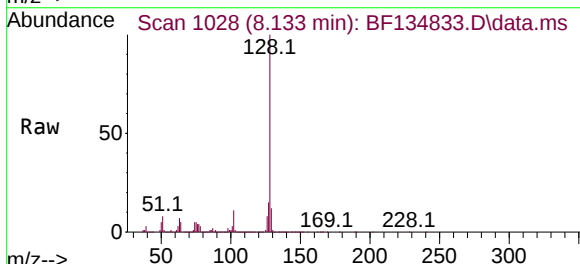



#37

2-Methylnaphthalene

Concen: 4395.601 ng

RT: 8.810 min Scan# 1143

Delta R.T. 0.018 min

Lab File: BF134833.D

Acq: 18 Aug 2023 10:32

Instrument :

BNA_F

ClientSampleId :

NEVINS-SB05-Z83-84

Tgt Ion:142 Resp: 389520

Ion Ratio Lower Upper

142 100





141 90.8 70.8 106.2

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 08/21/2023

Supervised By :mohammad ahmed 08/21/2023

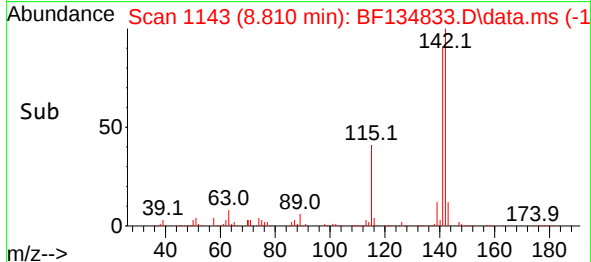

#38

1-Methylnaphthalene

Concen: 3352.534 ng

RT: 8.904 min Scan# 1159

Delta R.T. 0.012 min

Lab File: BF134833.D




Acq: 18 Aug 2023 10:32


Tgt Ion:142 Resp: 2762597

Ion Ratio Lower Upper

142 100


141 92.7 71.4 107.2

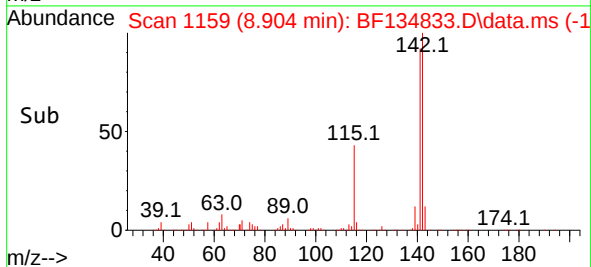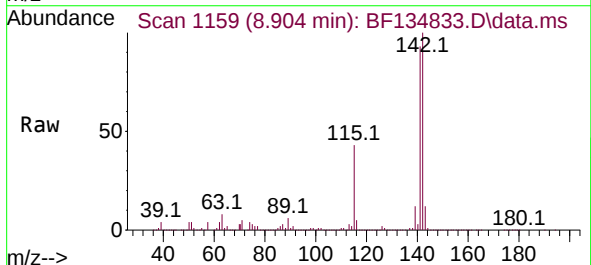



#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.827 min Scan# 1316
Delta R.T. -0.006 min
Lab File: BF134833.D
Acq: 18 Aug 2023 10:32




Instrument :
BNA_F
ClientSampleId :
NEVINS-SB05-Z83-84




Tgt Ion:164 Resp: 3021
Ion Ratio Lower Upper
164 100
162 109.8 82.6 123.8
160 48.4 37.2 55.8

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 08/21/2023
Supervised By :mohammad ahmed 08/21/2023




#42
2,4,6-Tribromophenol
Concen: 27.124 ng
RT: 10.616 min Scan# 1450
Delta R.T. -0.012 min
Lab File: BF134833.D
Acq: 18 Aug 2023 10:32



Tgt Ion:330 Resp: 8355
Ion Ratio Lower Upper
330 100
332 97.8 78.8 118.2
141 109.3 25.4 38.2#

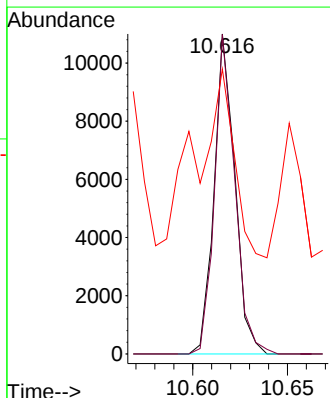



#45

2-Fluorobiphenyl

Concen: 33.104 ng

RT: 9.145 min Scan# 1200

Delta R.T. -0.018 min

Lab File: BF134833.D

Acq: 18 Aug 2023 10:32

Instrument :

BNA_F

ClientSampleId :

NEVINS-SB05-Z83-84





Tgt Ion:	172	Resp:	60162
Ion Ratio	Lower	Upper	
172	100		
171	33.1	28.8	43.2
170	21.8	18.7	28.1

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 08/21/2023

Supervised By :mohammad ahmed 08/21/2023

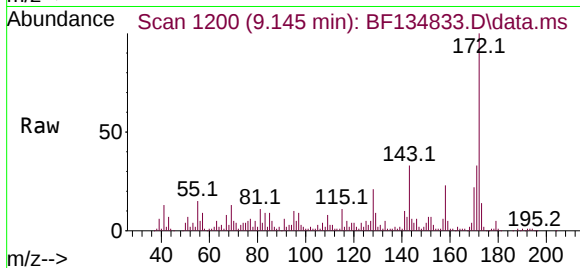

#46

1,1'-Biphenyl

Concen: 416.102 ng




RT: 9.251 min Scan# 1218


Delta R.T. -0.012 min

Lab File: BF134833.D

Acq: 18 Aug 2023 10:32


Tgt Ion:	154	Resp:	977741
Ion Ratio	Lower	Upper	
154	100		
153	40.9	20.8	60.8
76	12.1	0.0	30.2

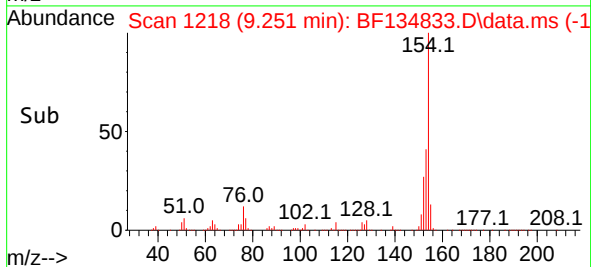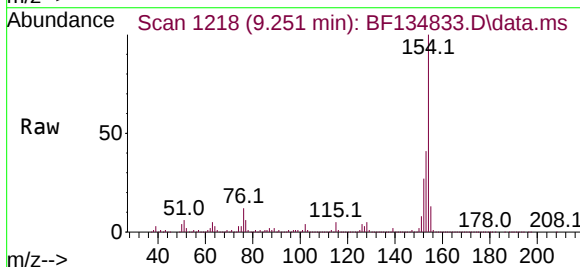



#49
Acenaphthylene
Concen: 1096.199 ng
RT: 9.704 min Scan# 1295
Delta R.T. 0.006 min
Lab File: BF134833.D
Acq: 18 Aug 2023 10:32




Instrument :
BNA_F
ClientSampleId :
NEVINS-SB05-Z83-84



Tgt Ion:152 Resp: 3033838
Ion Ratio Lower Upper
152 100
151 21.1 16.4 24.6
153 15.4 10.9 16.3




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 08/21/2023
Supervised By :mohammad ahmed 08/21/2023

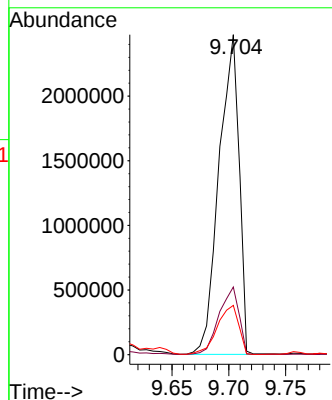

#52
Acenaphthene
Concen: 306.044 ng
RT: 9.863 min Scan# 1322
Delta R.T. -0.012 min
Lab File: BF134833.D
Acq: 18 Aug 2023 10:32


Tgt Ion:154 Resp: 548901
Ion Ratio Lower Upper
154 100
153 113.9 90.0 135.0
152 52.9 42.4 63.6

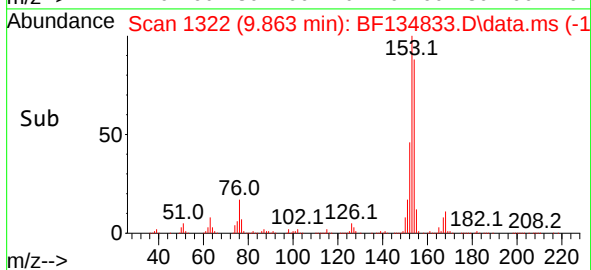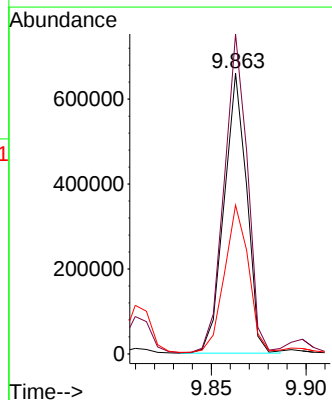



#55
Dibenzenofuran
Concen: 106.467 ng
RT: 10.033 min Scan# 1351
Delta R.T. -0.012 min
Lab File: BF134833.D
Acq: 18 Aug 2023 10:32




Instrument :
BNA_F
ClientSampleId :
NEVINS-SB05-Z83-84




Tgt Ion:168 Resp: 271832
Ion Ratio Lower Upper
168 100
139 41.3 33.4 50.2
169 34.5 10.6 15.8

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 08/21/2023
Supervised By :mohammad ahmed 08/21/2023




#58
Fluorene
Concen: 809.429 ng
RT: 10.386 min Scan# 1411
Delta R.T. -0.000 min
Lab File: BF134833.D
Acq: 18 Aug 2023 10:32




Tgt Ion:166 Resp: 1505296
Ion Ratio Lower Upper
166 100
165 99.8 74.5 111.7
167 14.4 10.6 16.0

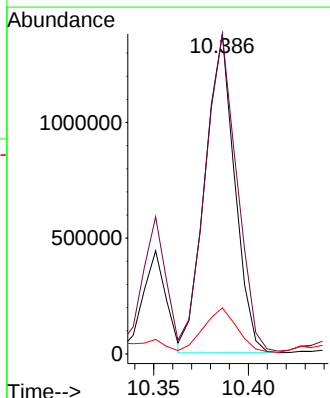



#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.321 min Scan# 1570
Delta R.T. -0.000 min
Lab File: BF134833.D
Acq: 18 Aug 2023 10:32




Instrument :
BNA_F
ClientSampleId :
NEVINS-SB05-Z83-84



Tgt Ion:188 Resp: 25063
Ion Ratio Lower Upper
188 100
94 12.4 5.1 7.7
80 14.3 6.6 9.8




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 08/21/2023
Supervised By :mohammad ahmed 08/21/2023

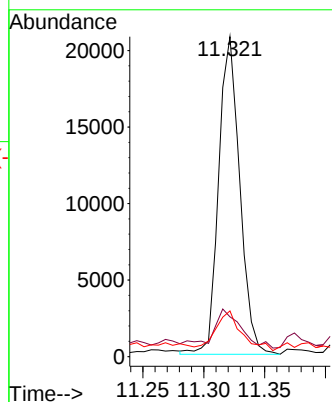

#71
Phenanthrene
Concen: 2939.085 ng
RT: 11.357 min Scan# 1576
Delta R.T. 0.006 min
Lab File: BF134833.D
Acq: 18 Aug 2023 10:32

Tgt Ion:178 Resp: 3912641
Ion Ratio Lower Upper
178 100
176 20.8 15.8 23.6
179 16.5 12.7 19.1

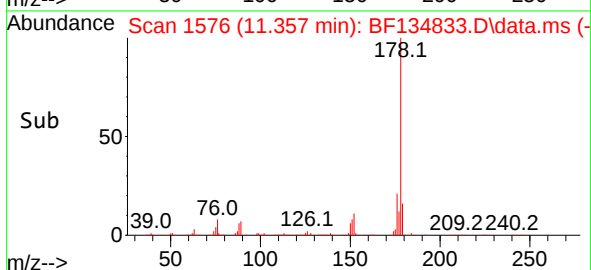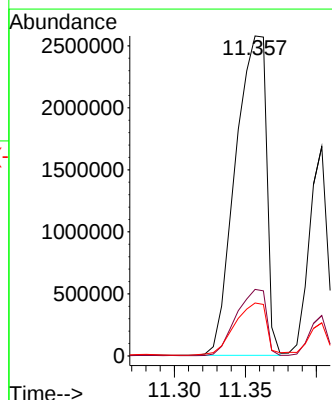

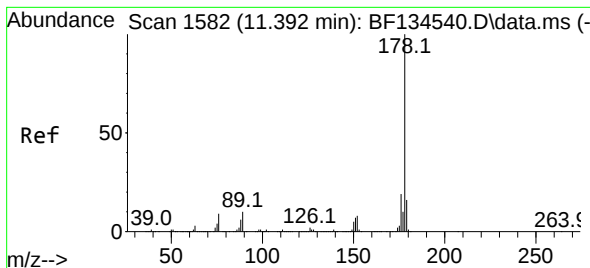

#72

Anthracene

Concen: 1081.982 ng

RT: 11.404 min Scan# 11

Delta R.T. -0.000 min

Lab File: BF134833.D

Acq: 18 Aug 2023 10:32

Instrument :

BNA_F

ClientSampleId :

NEVINS-SB05-Z83-84

Tgt Ion:178 Resp: 1471279

Ion Ratio Lower Upper

178 100

176 19.3 14.6 21.8





179 15.8 12.3 18.5

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 08/21/2023

Supervised By :mohammad ahmed 08/21/2023

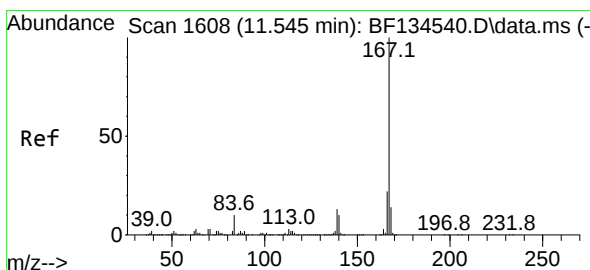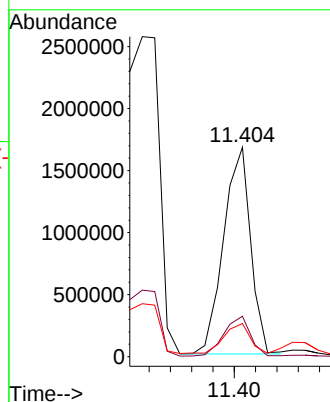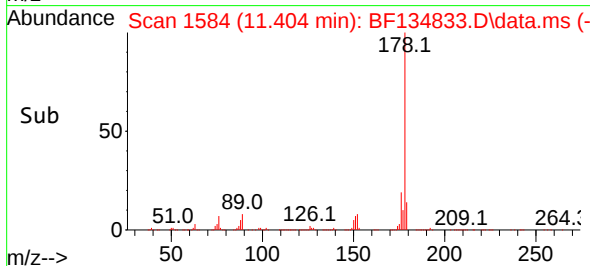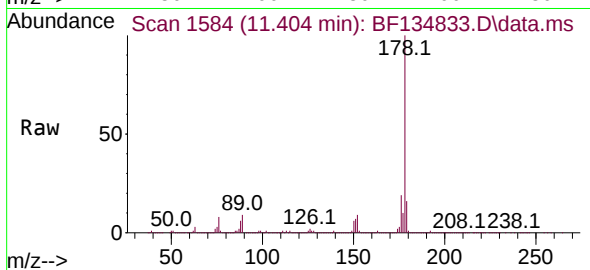

#73

Carbazole

Concen: 48.408 ng

RT: 11.551 min Scan# 1609

Delta R.T. -0.006 min

Lab File: BF134833.D

Acq: 18 Aug 2023 10:32




Tgt Ion:167 Resp: 58774


Ion Ratio Lower Upper

167 100

166 29.4 17.5 26.3


139 16.2 11.0 16.4

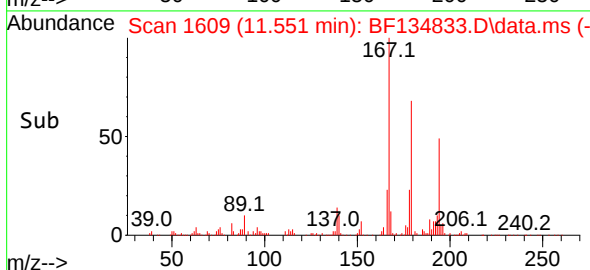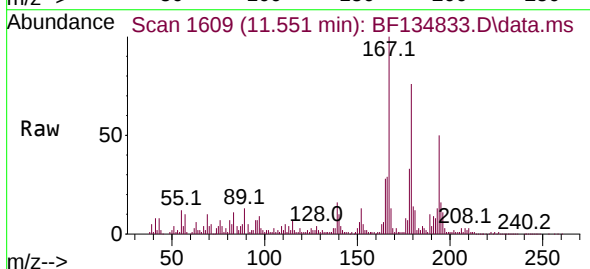

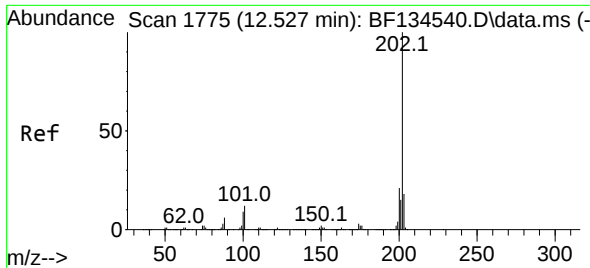

#75
Fluoranthene
Concen: 1124.649 ng
RT: 12.539 min Scan# 11
Delta R.T. -0.000 min
Lab File: BF134833.D
Acq: 18 Aug 2023 10:32




Instrument :
BNA_F
ClientSampleId :
NEVINS-SB05-Z83-84

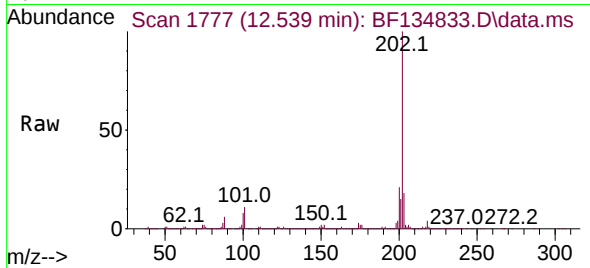

Tgt Ion:202 Resp: 1581496
Ion Ratio Lower Upper
202 100
101 11.4 0.0 28.5
203 18.3 0.0 37.5




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 08/21/2023
Supervised By :mohammad ahmed 08/21/2023

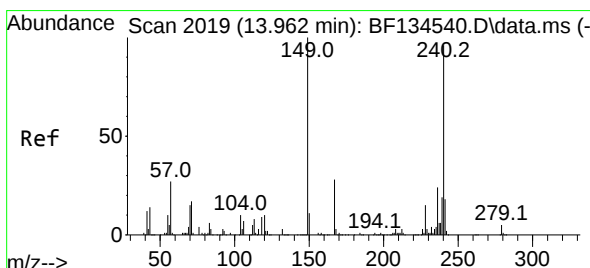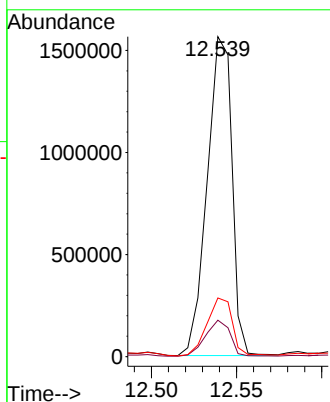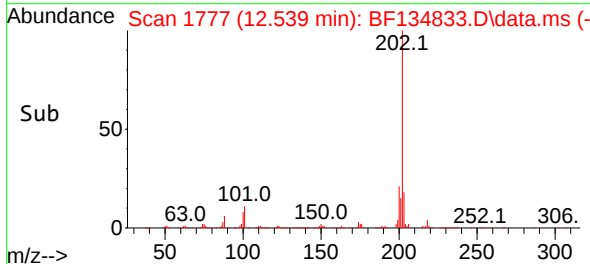

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.968 min Scan# 2020
Delta R.T. -0.006 min
Lab File: BF134833.D
Acq: 18 Aug 2023 10:32


Tgt Ion:240 Resp: 16162
Ion Ratio Lower Upper
240 100
120 19.3 6.6 10.0#
236 30.1 20.2 30.2

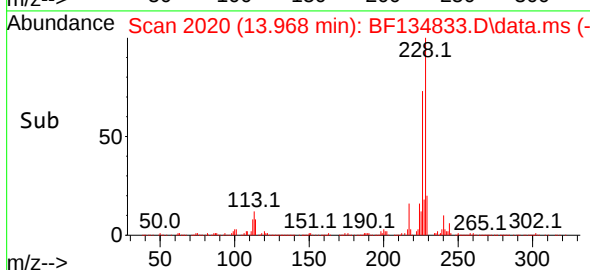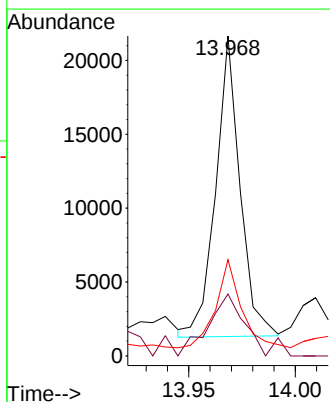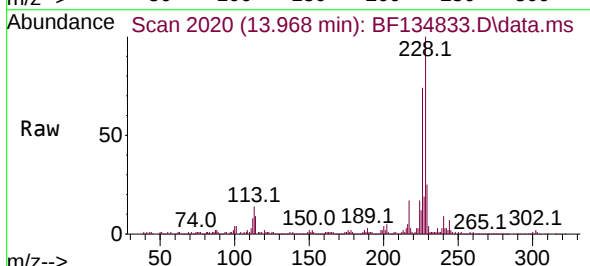



#78
Pyrene
Concen: 1612.926 ng
RT: 12.774 min Scan# 1817
Delta R.T. 0.006 min
Lab File: BF134833.D
Acq: 18 Aug 2023 10:32




Instrument :
BNA_F
ClientSampleId :
NEVINS-SB05-Z83-84

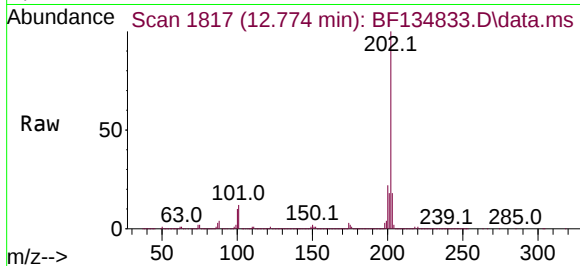

Tgt Ion:202 Resp: 2255711
Ion Ratio Lower Upper
202 100
200 21.6 15.8 23.8
203 18.1 13.5 20.3




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 08/21/2023
Supervised By :mohammad ahmed 08/21/2023

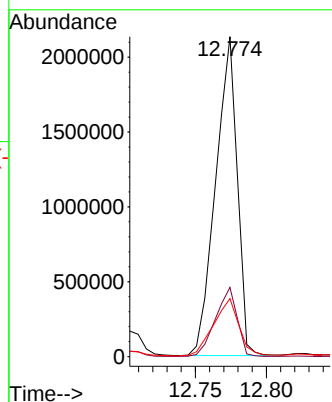

#79
Terphenyl-d14
Concen: 45.826 ng
RT: 12.910 min Scan# 1840
Delta R.T. -0.012 min
Lab File: BF134833.D
Acq: 18 Aug 2023 10:32


Tgt Ion:244 Resp: 42013
Ion Ratio Lower Upper
244 100
212 7.0 5.6 8.4
122 10.2 8.0 12.0

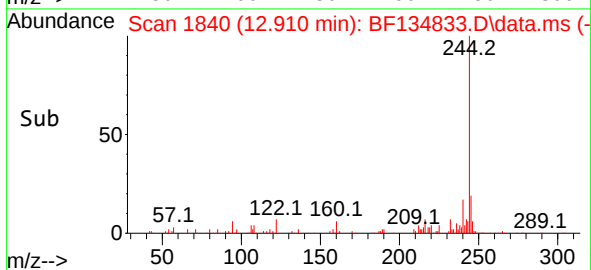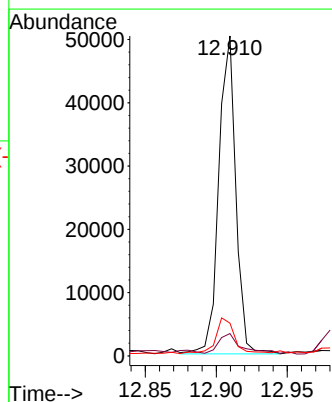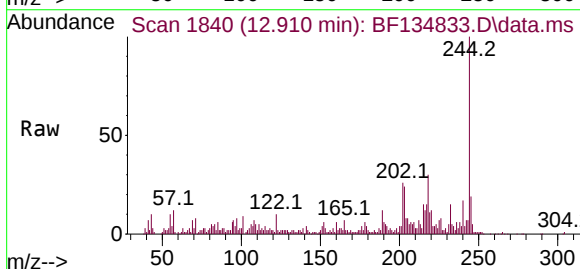



#81
Benzo(a)anthracene
Concen: 834.784 ng m
RT: 13.957 min Scan# 20
Delta R.T. -0.006 min
Lab File: BF134833.D
Acq: 18 Aug 2023 10:32




Instrument :
BNA_F
ClientSampleId :
NEVINS-SB05-Z83-84

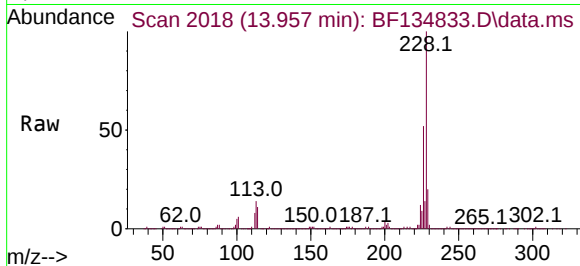


Tgt Ion:228 Resp: 964726
Ion Ratio Lower Upper
228 100
226 52.4 22.3 33.5
229 20.5 15.8 23.6

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 08/21/2023
Supervised By :mohammad ahmed 08/21/2023

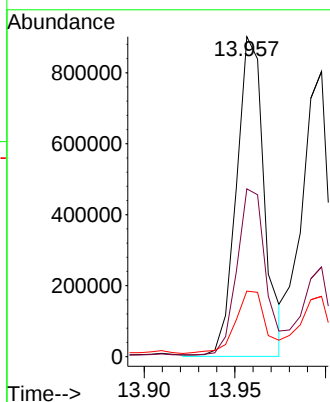


#83
Chrysene
Concen: 727.794 ng
RT: 13.998 min Scan# 2025
Delta R.T. -0.000 min
Lab File: BF134833.D
Acq: 18 Aug 2023 10:32

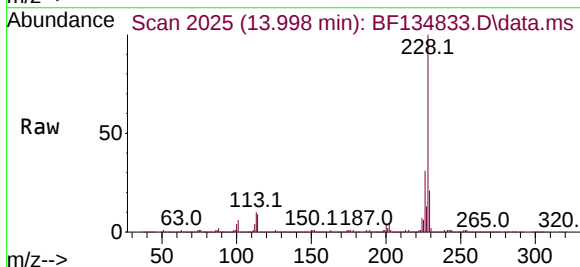

Tgt Ion:228 Resp: 819436
Ion Ratio Lower Upper
228 100
226 31.5 24.5 36.7
229 21.1 15.8 23.8

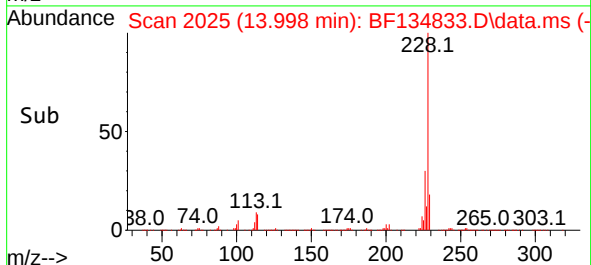







#86
Perylene-d12
Concen: 20.000 ng
RT: 15.433 min Scan# 21
Delta R.T. -0.006 min
Lab File: BF134833.D
Acq: 18 Aug 2023 10:32

Instrument :
BNA_F
ClientSampleId :
NEVINS-SB05-Z83-84

Tgt Ion:264 Resp: 15558
Ion Ratio Lower Upper
264 100
260 22.4 18.4 27.6
265 62.6 15.8 23.8




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 08/21/2023
Supervised By :mohammad ahmed 08/21/2023

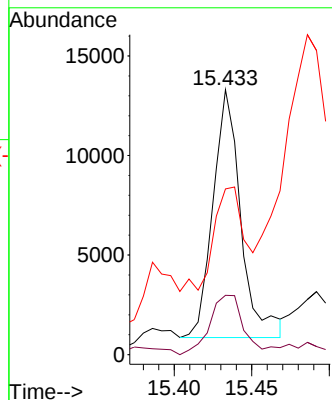

#87
Indeno(1,2,3-cd)pyrene
Concen: 156.371 ng
RT: 16.915 min Scan# 2521
Delta R.T. -0.012 min
Lab File: BF134833.D
Acq: 18 Aug 2023 10:32


Tgt Ion:276 Resp: 143080
Ion Ratio Lower Upper
276 100
138 22.5 14.2 21.4
277 25.2 19.9 29.9

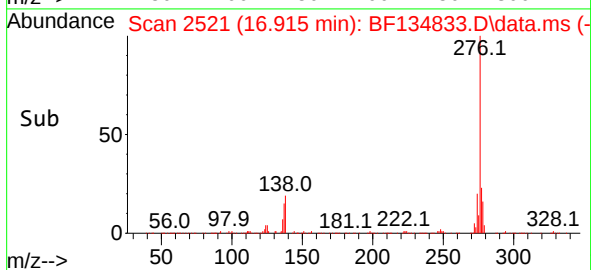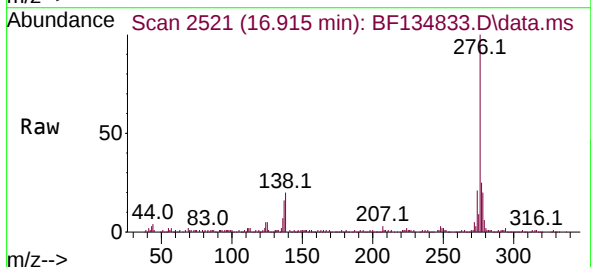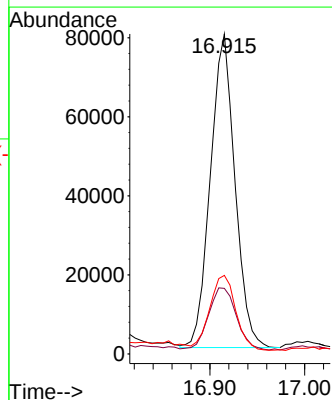



#88
Benzo(b)fluoranthene
Concen: 571.733 ng m
RT: 15.009 min Scan# 21
Delta R.T. -0.000 min
Lab File: BF134833.D
Acq: 18 Aug 2023 10:32




Instrument :
BNA_F
ClientSampleId :
NEVINS-SB05-Z83-84



Tgt Ion:252 Resp: 542498
Ion Ratio Lower Upper
252 100
253 23.1 17.3 25.9
125 11.7 6.0 9.0




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 08/21/2023
Supervised By :mohammad ahmed 08/21/2023

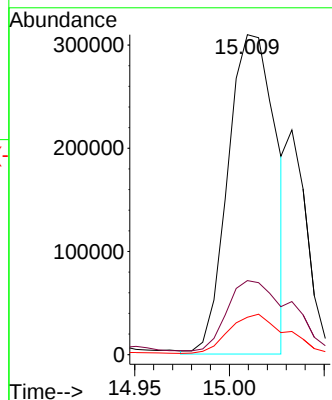

#89
Benzo(k)fluoranthene
Concen: 178.782 ng m
RT: 15.033 min Scan# 2201
Delta R.T. -0.006 min
Lab File: BF134833.D
Acq: 18 Aug 2023 10:32


Tgt Ion:252 Resp: 168990
Ion Ratio Lower Upper
252 100
253 23.6 17.9 26.9
125 10.3 6.3 9.5

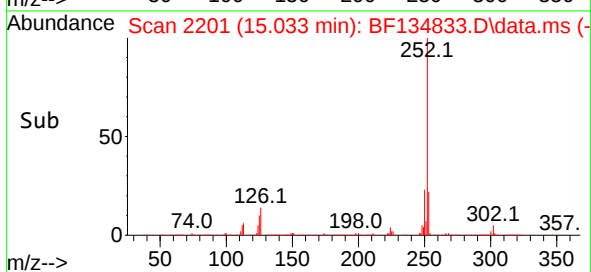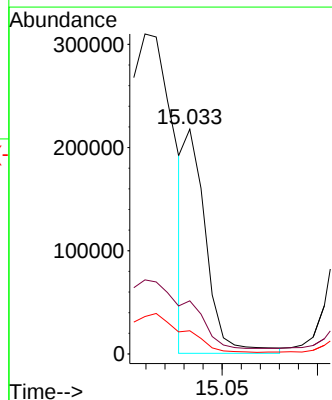



#90
Benzo(a)pyrene
Concen: 642.463 ng
RT: 15.374 min Scan# 21
Delta R.T. -0.006 min
Lab File: BF134833.D
Acq: 18 Aug 2023 10:32




Instrument :
BNA_F
ClientSampleId :
NEVINS-SB05-Z83-84



Tgt Ion:252 Resp: 56839
Ion Ratio Lower Upper
252 100
253 22.6 17.0 25.4
125 11.4 6.2 9.4




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 08/21/2023
Supervised By :mohammad ahmed 08/21/2023

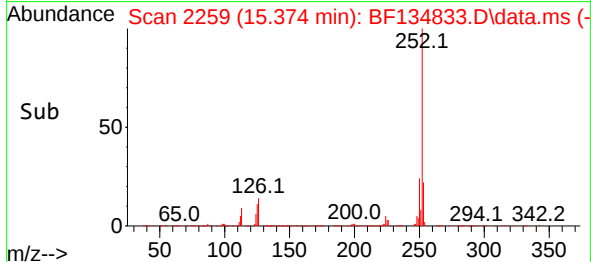

#91
Dibenzo(a,h)anthracene
Concen: 54.660 ng
RT: 16.927 min Scan# 2523
Delta R.T. -0.024 min
Lab File: BF134833.D
Acq: 18 Aug 2023 10:32


Tgt Ion:278 Resp: 40419
Ion Ratio Lower Upper
278 100
139 17.9 10.0 15.0#
279 29.3 19.7 29.5

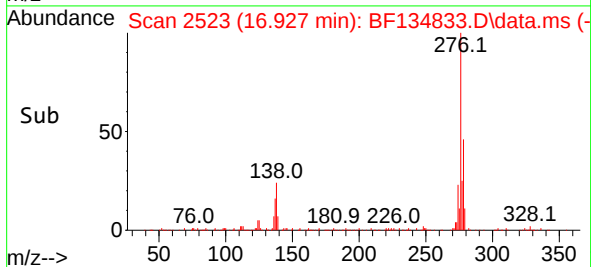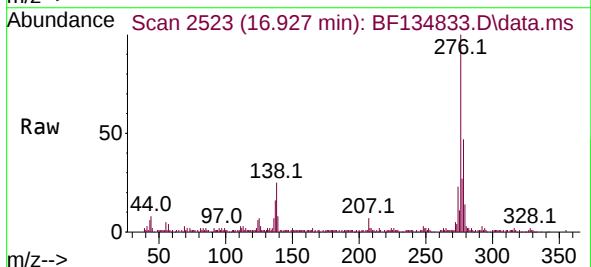

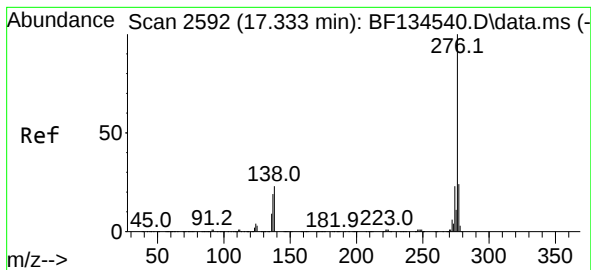

#92
 Benzo(g,h,i)perylene
 Concen: 212.209 ng
 RT: 17.362 min Scan# 2597
 Delta R.T. -0.012 min
 Lab File: BF134833.D
 Acq: 18 Aug 2023 10:32

Instrument : BNA_F
 ClientSampleId : NEVINS-SB05-Z83-84

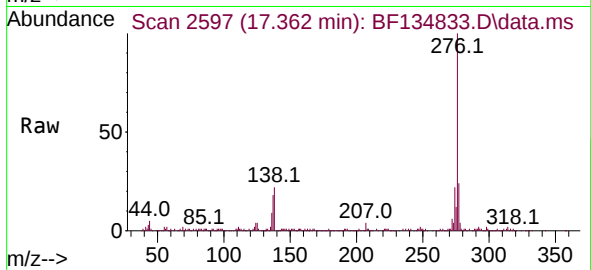

Tgt Ion: 276 Resp: 160076

Ion	Ratio	Lower	Upper
276	100		
277	23.7	19.0	28.6
138	22.1	12.2	18.2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/21/2023
 Supervised By :mohammad ahmed 08/21/2023

