

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081823\
 Data File : BF134835.D
 Acq On : 18 Aug 2023 11:35
 Operator : CG\JU
 Sample : 04046-01 10X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-02(0-5)

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF134835.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.410	561	565	574	rBV	295352	261331	21.99%	3.301%
2	6.416	733	736	745	rBV	315672	266998	22.47%	3.373%
3	6.793	796	800	803	rBV	992941	813442	68.44%	10.276%
4	7.346	890	894	900	rBV	200436	168491	14.18%	2.129%
5	8.069	1013	1017	1020	rBV	1334776	1099007	92.47%	13.884%
6	9.145	1196	1200	1208	rBV	395008	331583	27.90%	4.189%
7	9.822	1312	1315	1319	rBV	1348526	1188506	100.00%	15.014%
8	9.857	1319	1321	1328	rVB	19234	20642	1.74%	0.261%
9	10.610	1446	1449	1461	rVB	213192	178758	15.04%	2.258%
10	11.316	1565	1569	1571	rBV	1129059	1002806	84.38%	12.668%
11	11.333	1571	1572	1576	rVV	104669	85407	7.19%	1.079%
12	11.386	1579	1581	1584	rVB	19871	17590	1.48%	0.222%
13	11.845	1655	1659	1665	rBV	76789	72978	6.14%	0.922%
14	11.928	1670	1673	1676	rBV2	16989	16203	1.36%	0.205%
15	12.528	1772	1775	1779	rBV	161606	130763	11.00%	1.652%
16	12.633	1788	1793	1798	rBV7	17841	25282	2.13%	0.319%
17	12.757	1808	1814	1817	rBV	151126	146732	12.35%	1.854%
18	12.904	1836	1839	1847	rVB	268526	235138	19.78%	2.970%
19	12.980	1847	1852	1856	rBV6	8314	17487	1.47%	0.221%
20	13.192	1884	1888	1890	rBV	12377	13515	1.14%	0.171%
21	13.416	1918	1926	1929	rBV8	6923	20652	1.74%	0.261%
22	13.710	1973	1976	1979	rBV3	9033	13758	1.16%	0.174%
23	13.816	1990	1994	1998	rVB5	15162	21773	1.83%	0.275%
24	13.963	2014	2019	2022	rBV	985420	906448	76.27%	11.451%
25	13.986	2022	2023	2025	rVB	52025	27845	2.34%	0.352%
26	14.069	2032	2037	2040	rBV2	15934	21695	1.83%	0.274%
27	14.827	2163	2166	2171	rBV	51523	58564	4.93%	0.740%
28	15.004	2192	2196	2198	rBV	41778	58273	4.90%	0.736%
29	15.304	2244	2247	2251	rVB	20635	26830	2.26%	0.339%
30	15.369	2254	2258	2262	rVB	31591	39901	3.36%	0.504%
31	15.427	2264	2268	2276	rBV	484501	627411	52.79%	7.926%




Sum of corrected areas: 7915809

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081823\
Data File : BF134835.D
Acq On : 18 Aug 2023 11:35
Operator : CG\JU
Sample : 04046-01 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-02(0-5)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

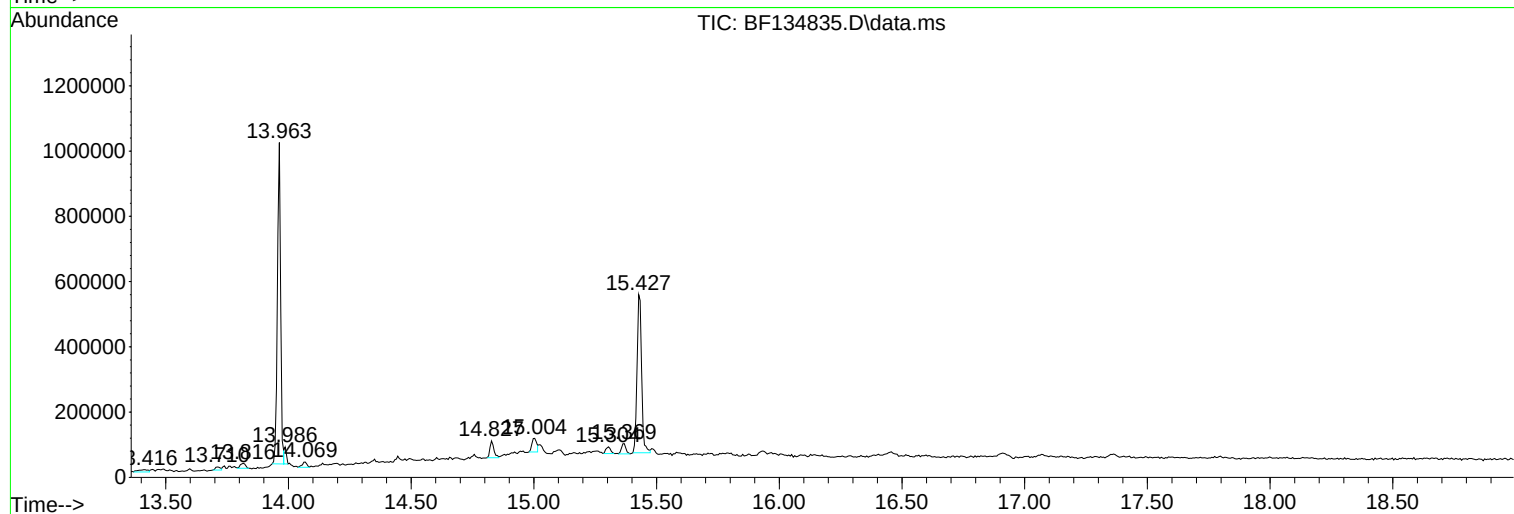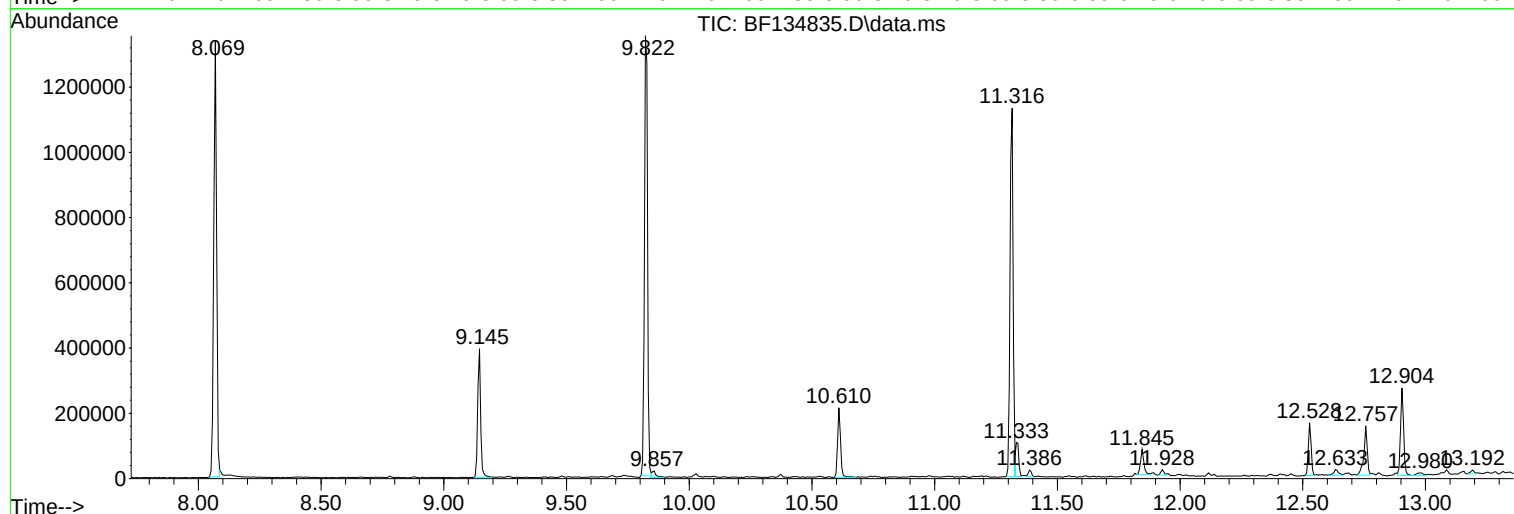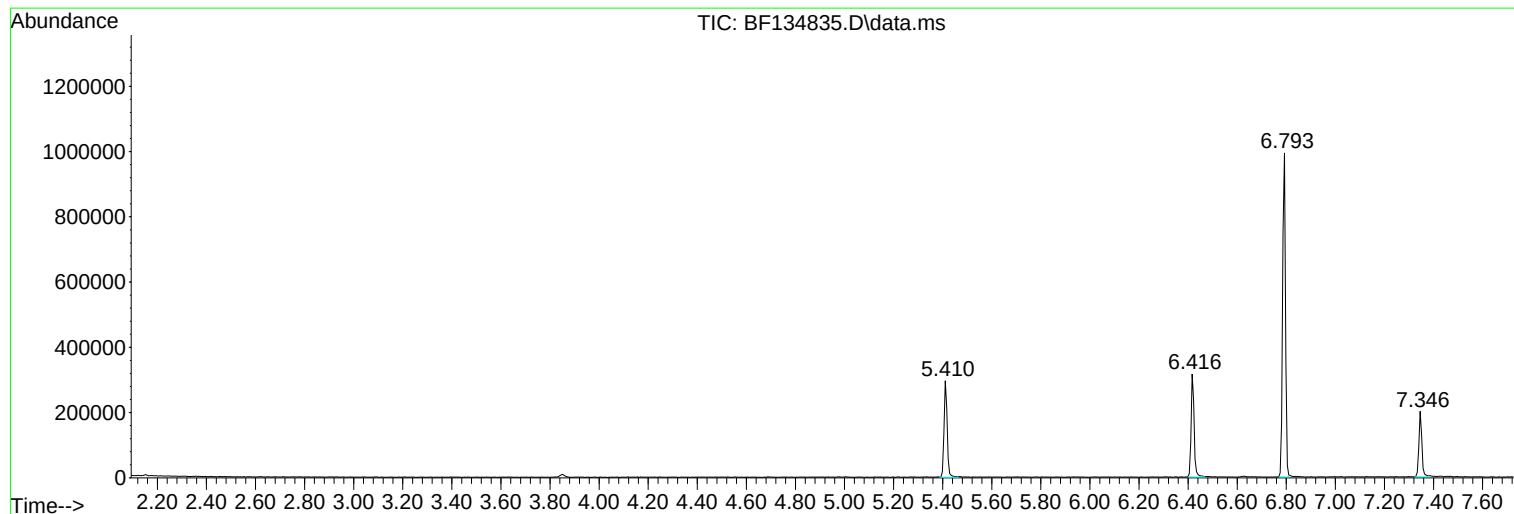

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081823\
Data File : BF134835.D
Acq On : 18 Aug 2023 11:35
Operator : CG\JU
Sample : 04046-01 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-02(0-5)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081823\
Data File : BF134835.D
Acq On : 18 Aug 2023 11:35
Operator : CG\JU
Sample : 04046-01 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-02(0-5)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------