

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081823\
 Data File : BF134840.D
 Acq On : 18 Aug 2023 14:57
 Operator : CG\JU
 Sample : PB154882BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB154882BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF134840.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.134	4	8	14	rVB	57762	77994	1.61%	0.264%
2	5.434	564	569	572	rBV	3855291	4367160	89.97%	14.760%
3	6.434	732	739	742	rBV	3655046	4304893	88.69%	14.550%
4	6.793	796	800	803	rBV	1077890	884565	18.22%	2.990%
5	7.351	889	895	898	rBV	2548528	2894432	59.63%	9.783%
6	8.069	1012	1017	1020	rBV	1321357	1177406	24.26%	3.979%
7	9.151	1194	1201	1204	rBV	4714923	4854030	100.00%	16.406%
8	9.822	1310	1315	1319	rBV	1395542	1264763	26.06%	4.275%
9	10.616	1445	1450	1454	rBV	2812119	2902144	59.79%	9.809%
10	11.316	1565	1569	1572	rBV	1387179	1166196	24.03%	3.942%
11	12.916	1836	1841	1844	rBV	3876391	3881704	79.97%	13.120%
12	13.963	2015	2019	2038	rVB	920551	894929	18.44%	3.025%
13	15.433	2263	2269	2275	rBV	760564	916662	18.88%	3.098%




Sum of corrected areas: 29586878

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081823\
Data File : BF134840.D
Acq On : 18 Aug 2023 14:57
Operator : CG\JU
Sample : PB154882BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB154882BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

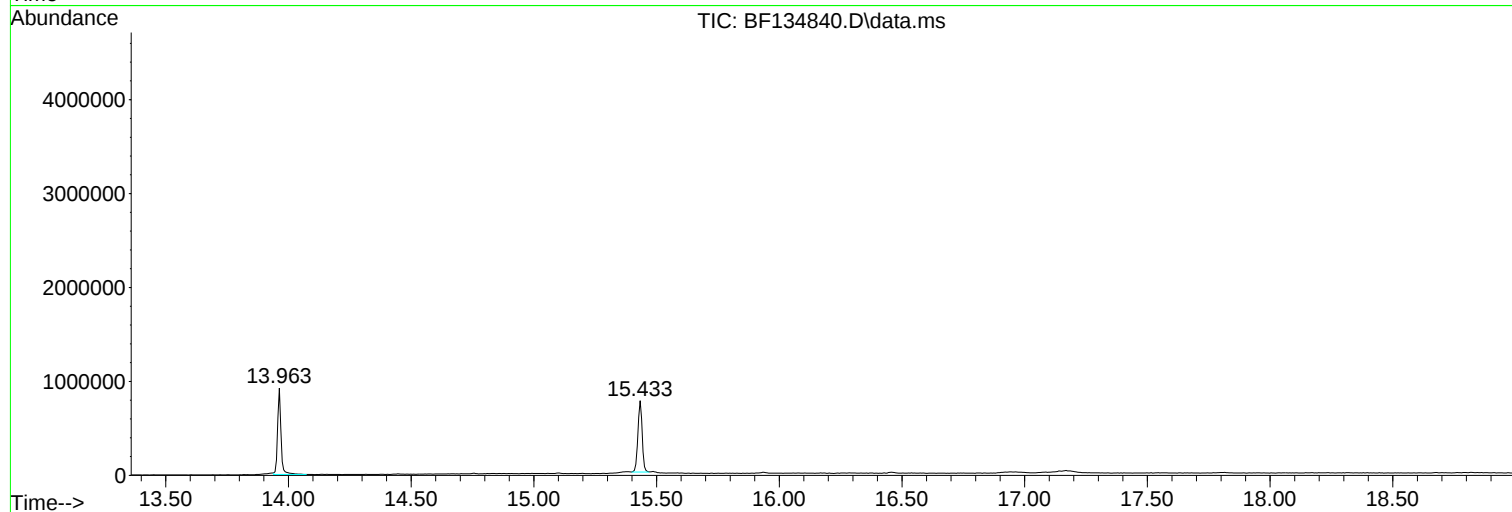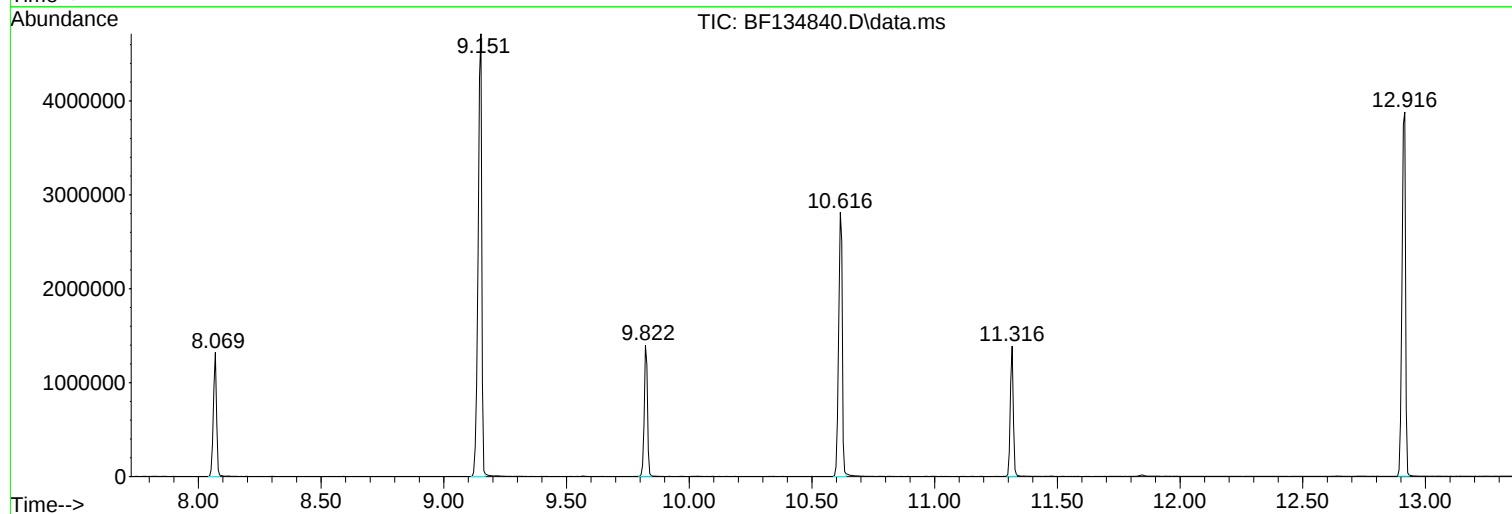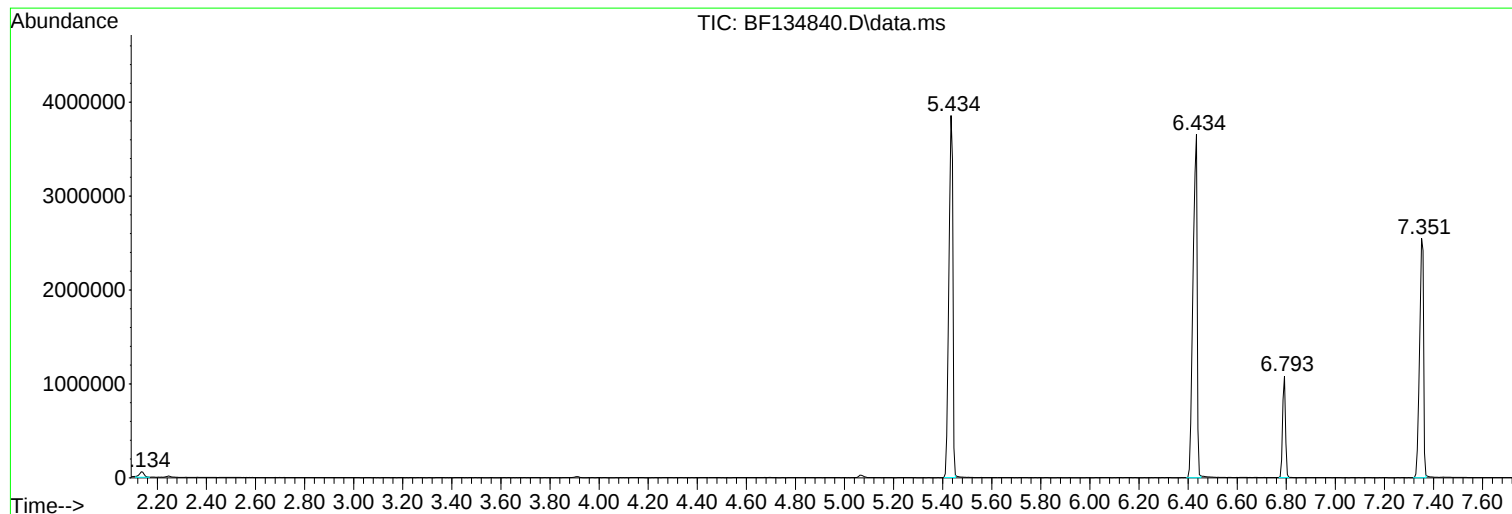

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081823\
Data File : BF134840.D
Acq On : 18 Aug 2023 14:57
Operator : CG\JU
Sample : PB154882BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB154882BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081823\
Data File : BF134840.D
Acq On : 18 Aug 2023 14:57
Operator : CG\JU
Sample : PB154882BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB154882BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------