

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081823\
 Data File : BF134846.D
 Acq On : 18 Aug 2023 18:14
 Operator : CG\JU
 Sample : 04020-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 E-2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF134846.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.810	118	123	130	rVB	299234	418342	10.10%	1.648%
2	3.681	266	271	278	rVB	46691	66801	1.61%	0.263%
3	4.063	332	336	343	rBV	69882	84928	2.05%	0.335%
4	4.428	394	398	403	rBV	73523	81492	1.97%	0.321%
5	4.622	427	431	436	rBV	141804	143345	3.46%	0.565%
6	4.693	439	443	448	rVB	101699	106425	2.57%	0.419%
7	5.057	499	505	513	rVB2	357535	512977	12.38%	2.021%
8	5.440	564	570	573	rBV	3546622	3558742	85.90%	14.023%
9	6.434	733	739	742	rBV	3152214	3208767	77.45%	12.644%
10	6.792	797	800	803	rBV	1119161	839958	20.28%	3.310%
11	7.357	890	896	899	rBV	2499676	2519464	60.82%	9.928%
12	8.069	1013	1017	1021	rBV	1322432	1108737	26.76%	4.369%
13	8.316	1057	1059	1067	rVB	76605	67311	1.62%	0.265%
14	9.151	1195	1201	1204	rBV	4149528	4142805	100.00%	16.325%
15	9.263	1216	1220	1224	rBV	141097	124951	3.02%	0.492%
16	9.822	1311	1315	1319	rBV	1154095	1079170	26.05%	4.252%
17	10.616	1445	1450	1453	rBV	2364302	2041810	49.29%	8.046%
18	11.316	1565	1569	1572	rBV	982099	814225	19.65%	3.208%
19	11.845	1654	1659	1669	rBV2	52649	80272	1.94%	0.316%
20	12.910	1836	1840	1844	rBV	3303416	3032915	73.21%	11.951%
21	13.963	2015	2019	2028	rVB	877340	808519	19.52%	3.186%
22	15.433	2264	2269	2275	rBV	438677	535704	12.93%	2.111%




Sum of corrected areas: 25377660

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081823\
Data File : BF134846.D
Acq On : 18 Aug 2023 18:14
Operator : CG\JU
Sample : 04020-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
E-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

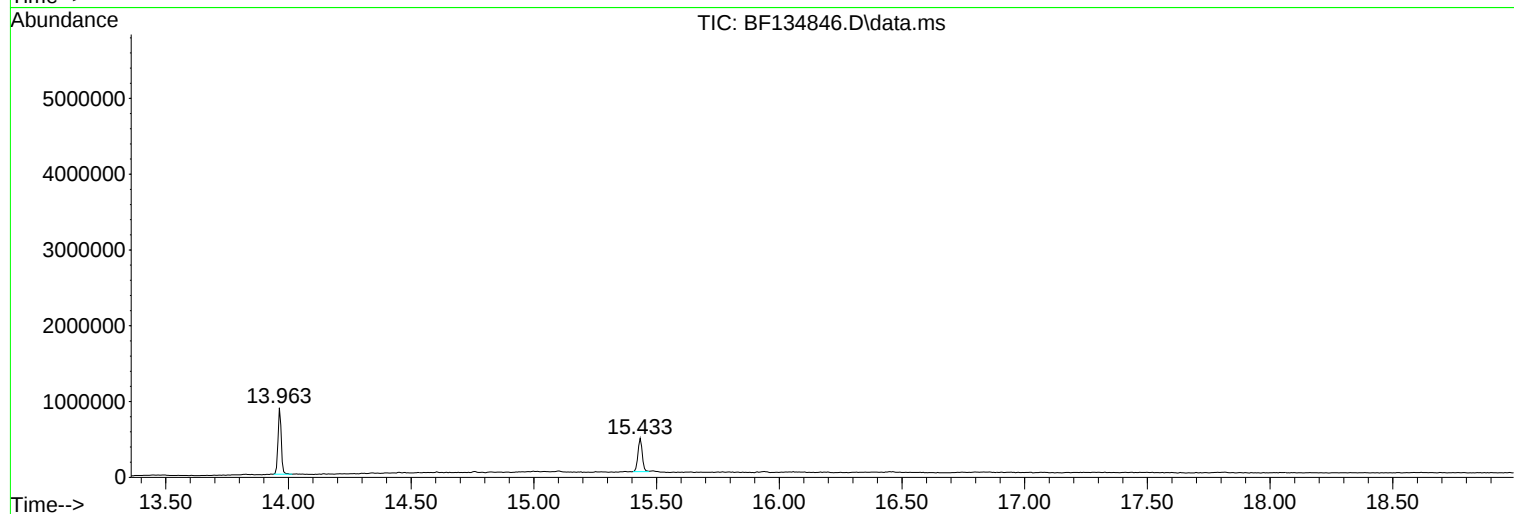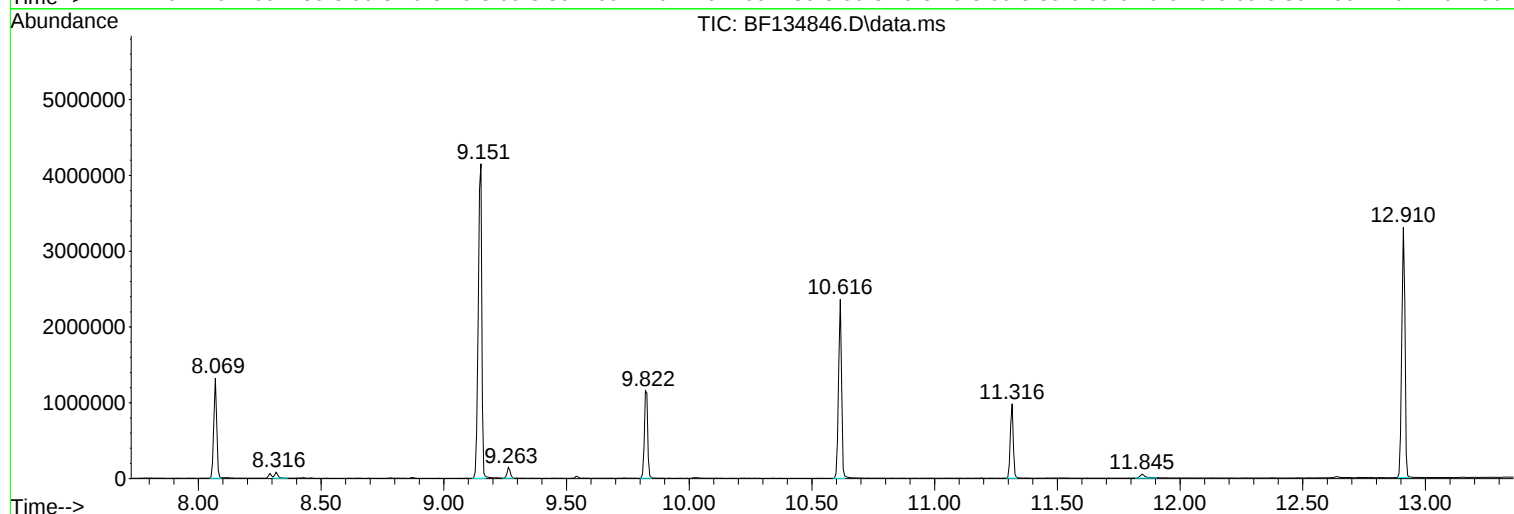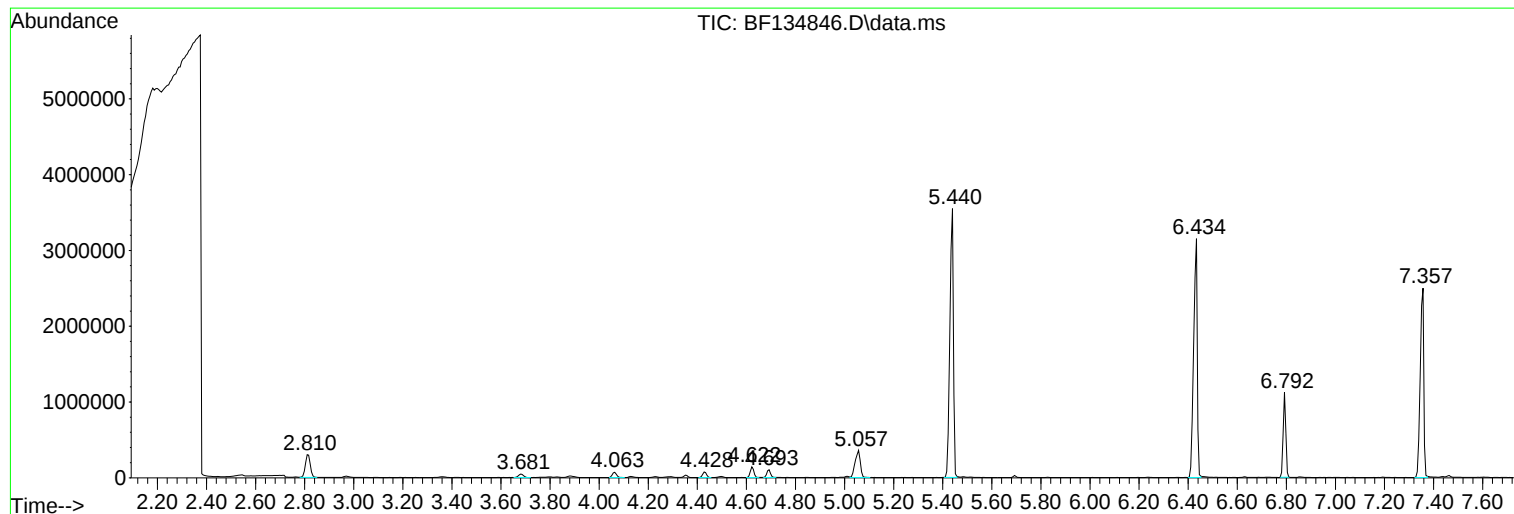

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081823\
Data File : BF134846.D
Acq On : 18 Aug 2023 18:14
Operator : CG\JU
Sample : 04020-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
E-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081823\
Data File : BF134846.D
Acq On : 18 Aug 2023 18:14
Operator : CG\JU
Sample : 04020-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
E-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------