
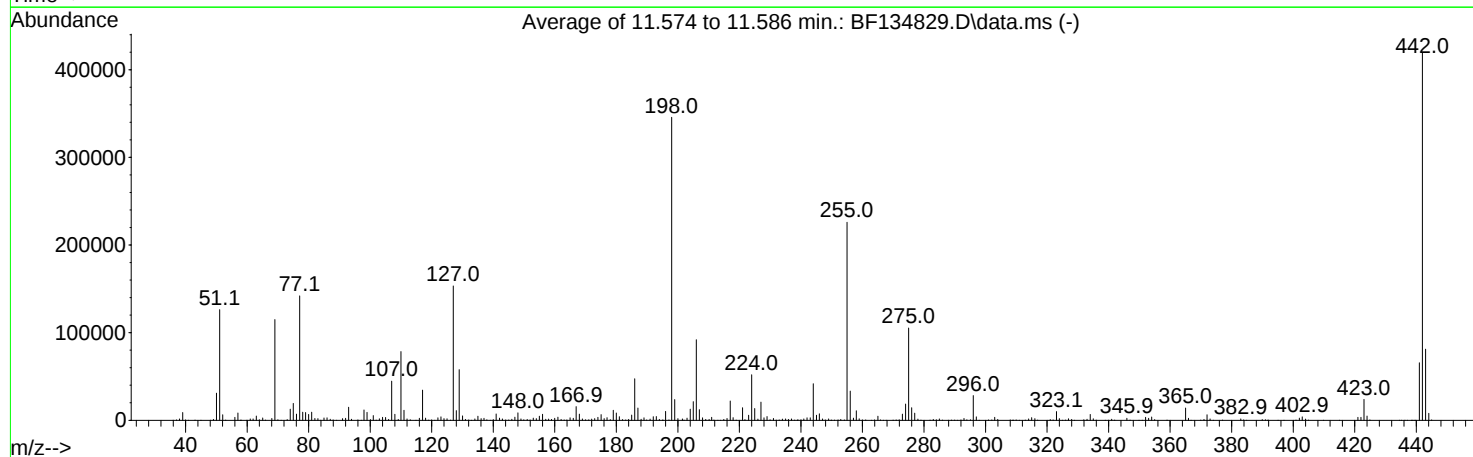


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081823\
 Data File : BF134829.D
 Acq On : 18 Aug 2023 07:49
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 04 09:29:15 2023

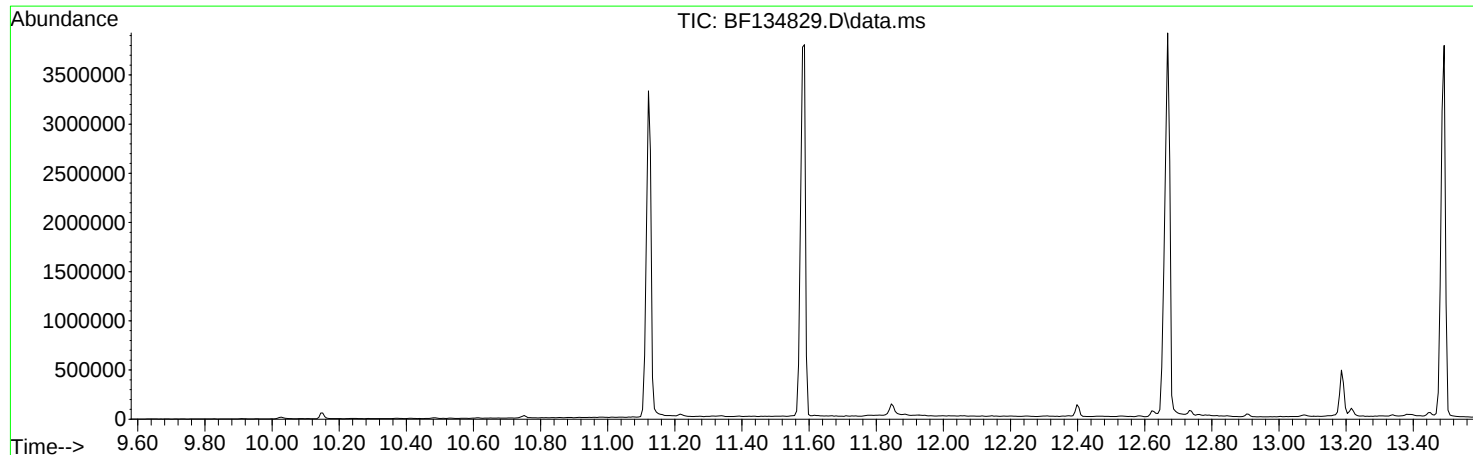




AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.5	126277	PASS
68	69	0.00	2	1.9	2128	PASS
69	198	0.00	100	33.2	114871	PASS
70	69	0.00	2	0.6	687	PASS
127	198	10	80	44.3	153256	PASS
197	198	0.00	2	0.1	469	PASS
198	198	100	100	100.0	345707	PASS
199	198	5	9	6.8	23672	PASS
275	198	10	60	30.4	105184	PASS
365	198	1	100	4.0	13931	PASS
441	198	0.01	100	19.0	65568	PASS
442	442	50	100	100.0	419776	PASS
443	442	15	24	19.3	81128	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081823\
Data File : BF134829.D
Acq On : 18 Aug 2023 07:49
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 18 08:26:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 04 09:29:15 2023
Response via : Initial Calibration

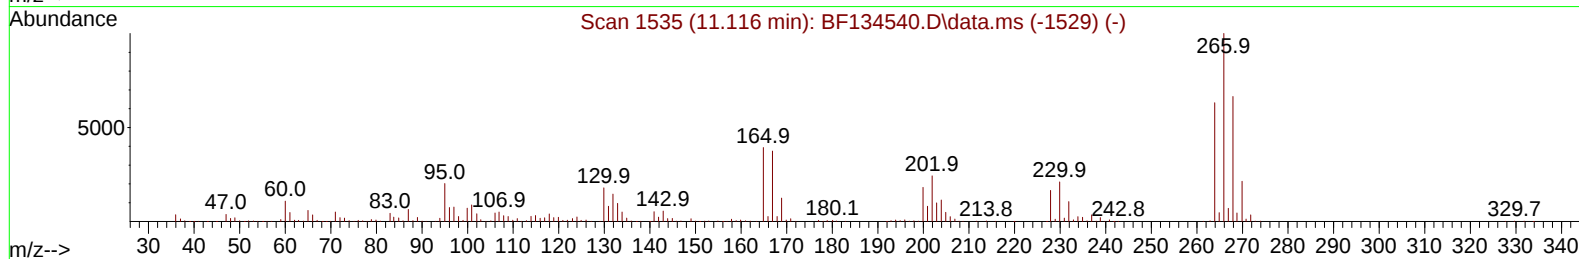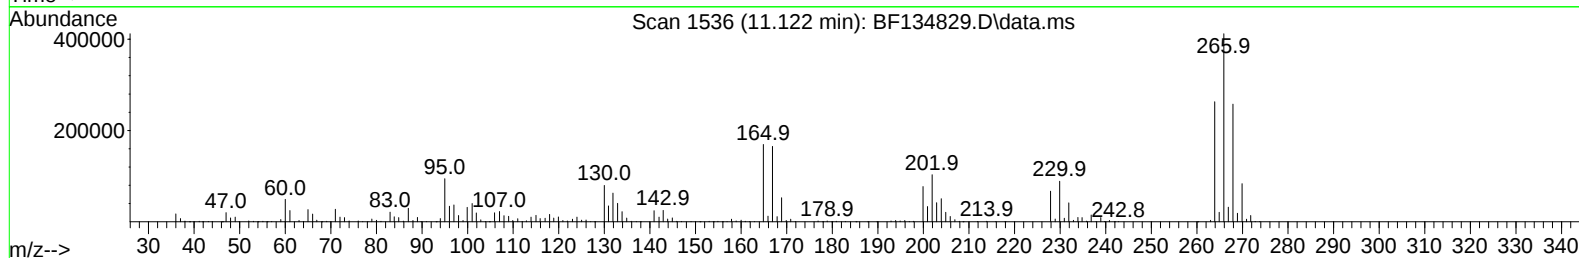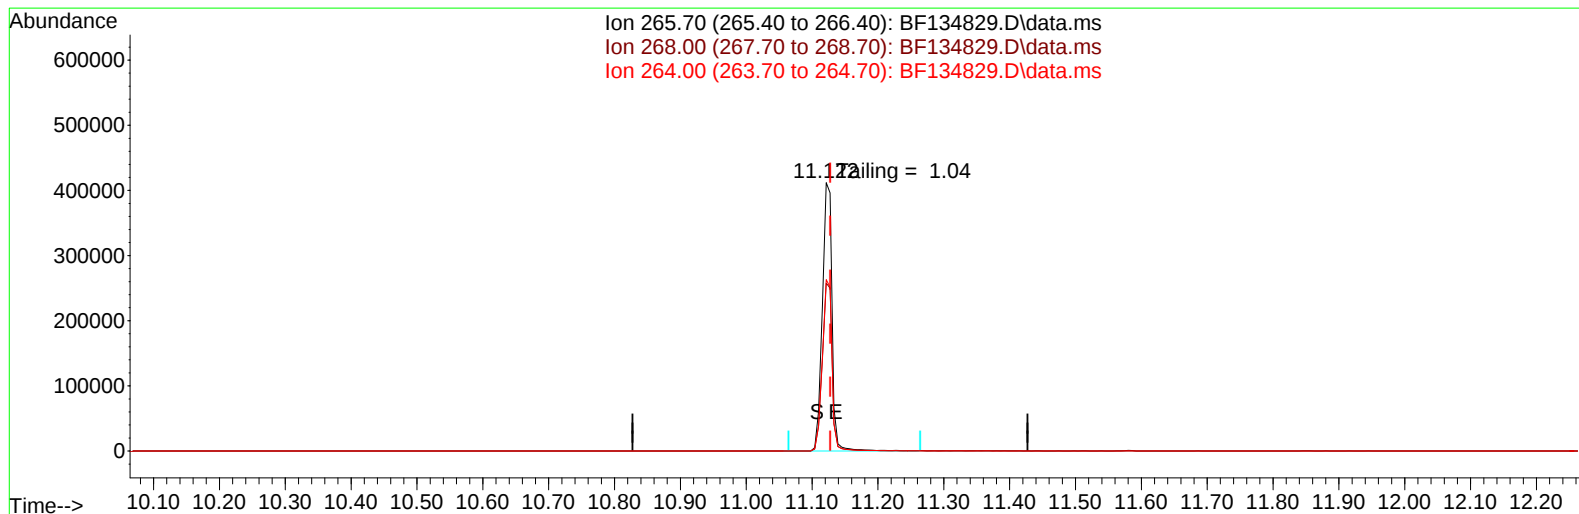

TIC: BF134829.D\data.ms

(70) Pentachlorophenol (C)

11.122min (-0.006) 32874.85 ng m




response 426358

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.10	62.54
264.00	59.70	63.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081823\
Data File : BF134829.D
Acq On : 18 Aug 2023 07:49
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 18 08:26:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 04 09:29:15 2023
Response via : Initial Calibration

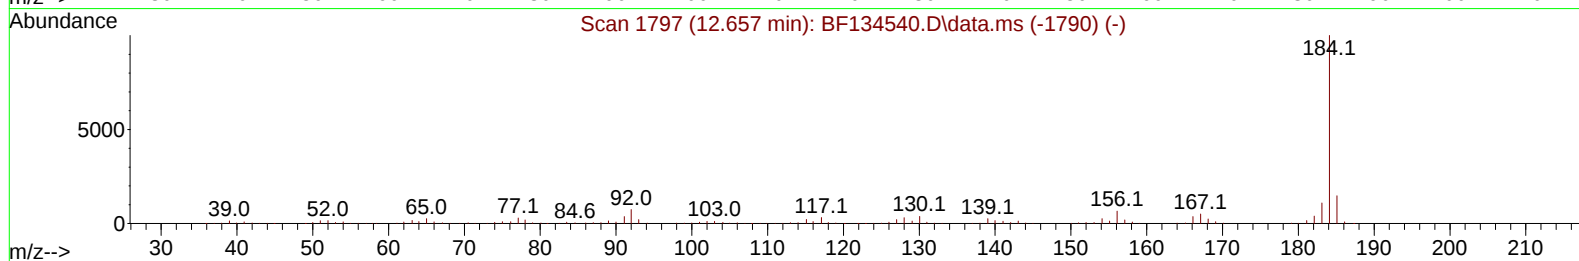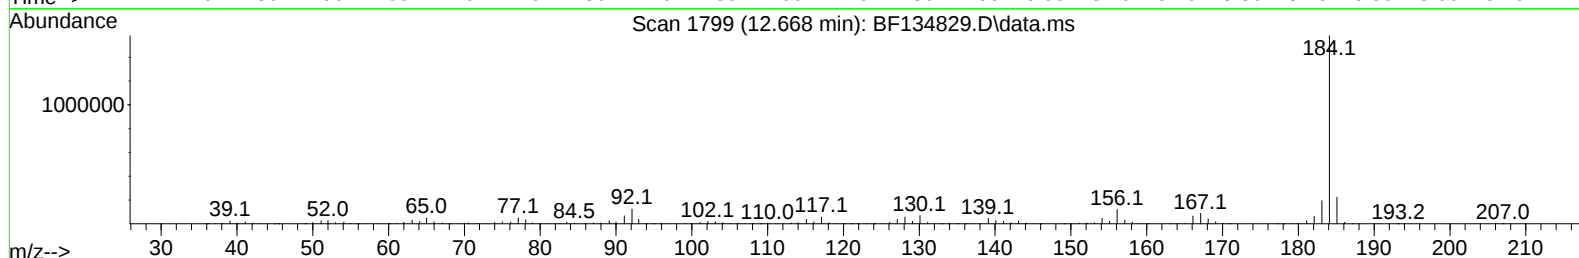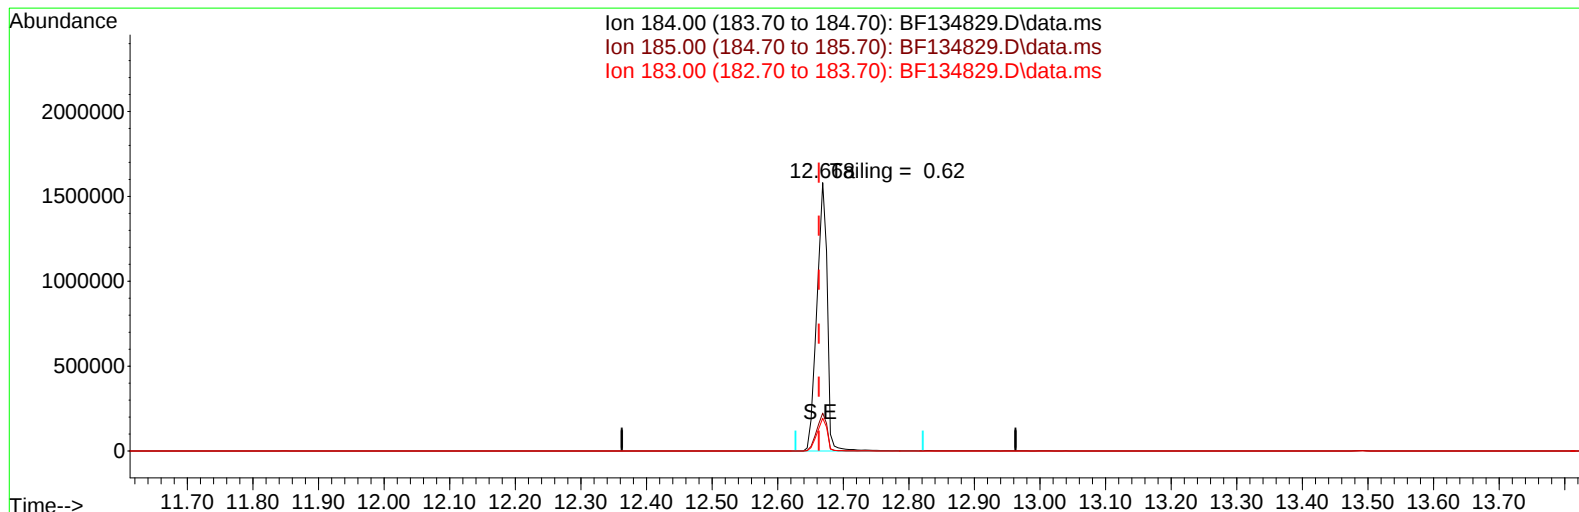

TIC: BF134829.D\data.ms

(77) Benzidine

12.668min (+ 0.006) 41501.56 ng

response 1729749

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.16
183.00	10.80	12.24
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/18/2023	BNA_F	<u>BF134829.D</u>
Compound Name	Response	Retention Time
DDT	703476	13.492
DDD	90195	13.186
DDE	868	12.851
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
91063	794539	11.46

Instrument :
BNA_F
ClientSampleId :
DFTPP