


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081823\
 Data File : BF134838.D
 Acq On : 18 Aug 2023 13:22
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 04 09:29:15 2023

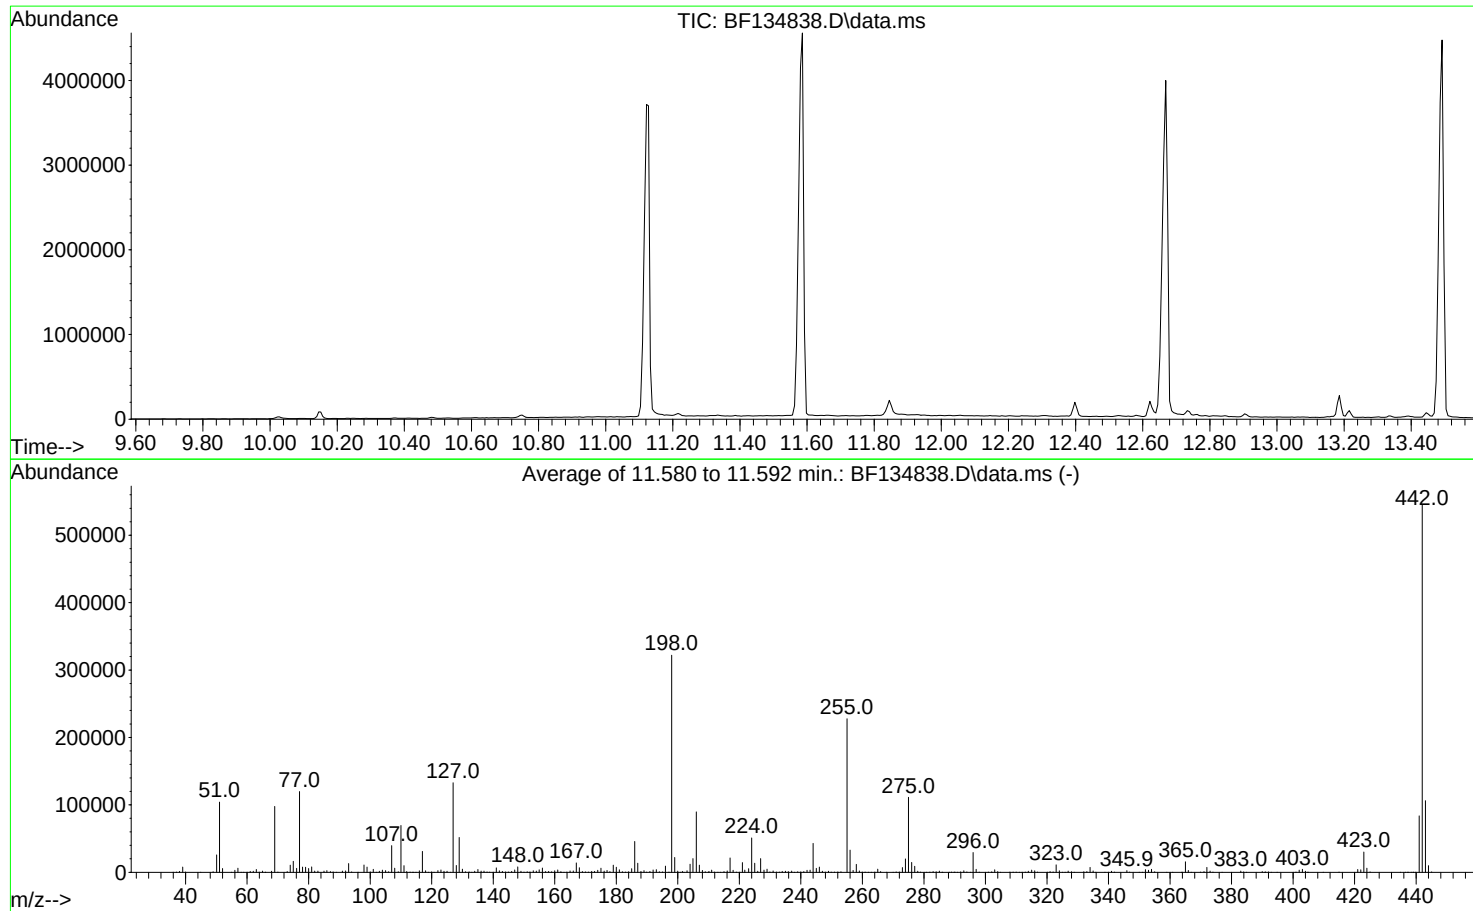




AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.3	104034	PASS
68	69	0.00	2	1.7	1653	PASS
69	198	0.00	100	30.3	97682	PASS
70	69	0.00	2	0.5	498	PASS
127	198	10	80	41.2	132799	PASS
197	198	0.00	2	0.1	336	PASS
198	198	100	100	100.0	322067	PASS
199	198	5	9	6.8	21899	PASS
275	198	10	60	34.5	111139	PASS
365	198	1	100	4.9	15671	PASS
441	198	0.01	100	26.0	83699	PASS
442	442	50	100	100.0	545728	PASS
443	442	15	24	19.5	106352	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081823\
Data File : BF134838.D
Acq On : 18 Aug 2023 13:22
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 18 13:50:22 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 04 09:29:15 2023
Response via : Initial Calibration

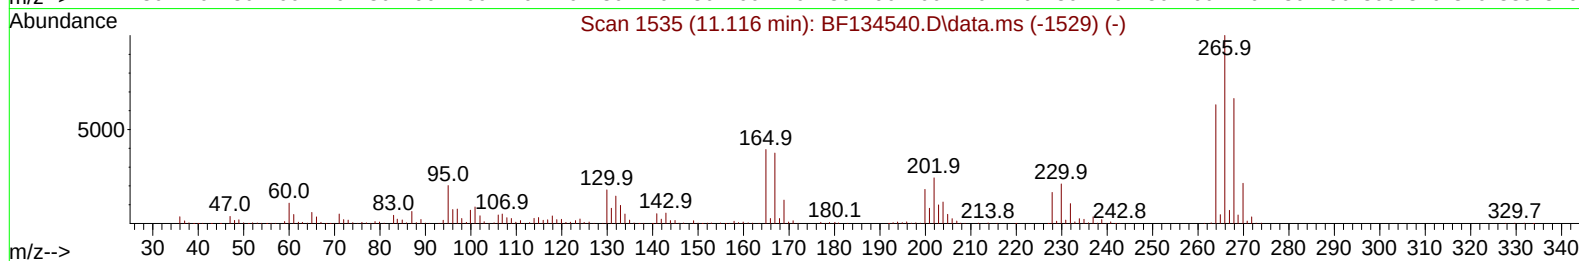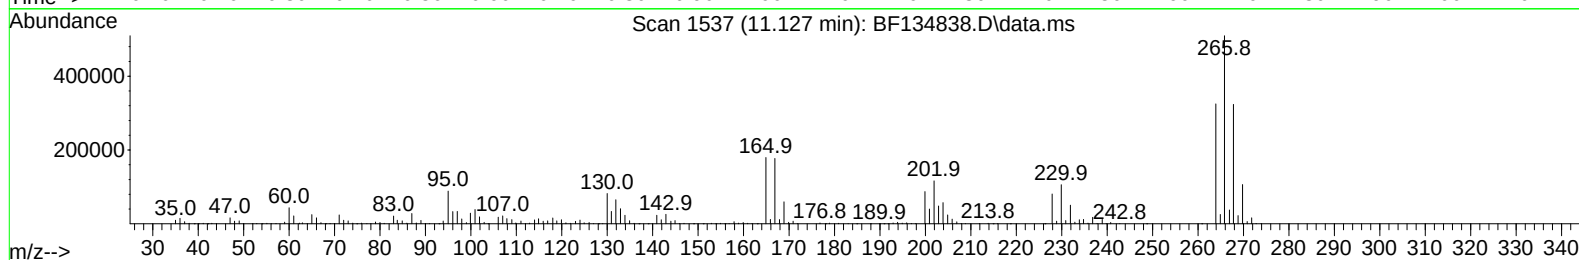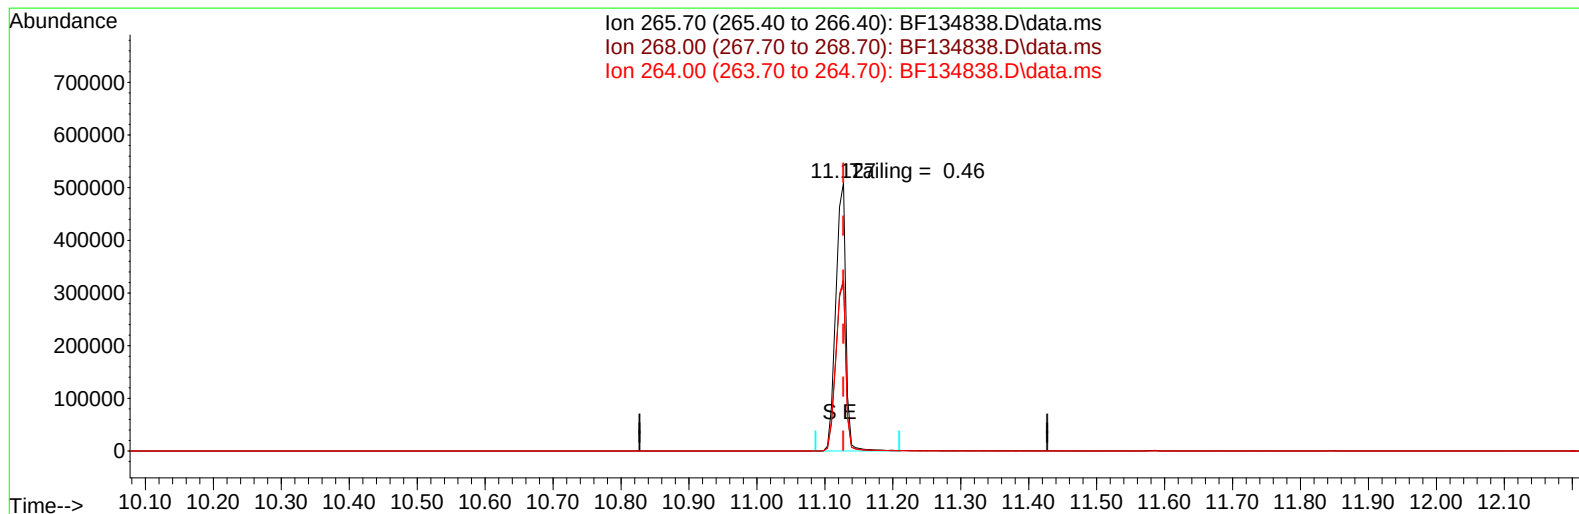

TIC: BF134838.D\data.ms

(70) Pentachlorophenol (C)

11.127min (-0.000) 30316.28 ng




response 524234

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.10	63.54
264.00	59.70	63.80
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081823\
Data File : BF134838.D
Acq On : 18 Aug 2023 13:22
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 18 13:50:22 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 04 09:29:15 2023
Response via : Initial Calibration

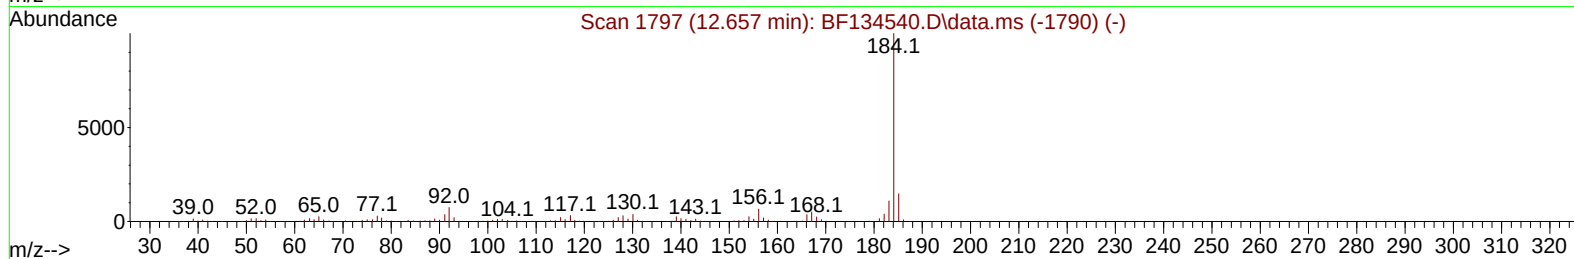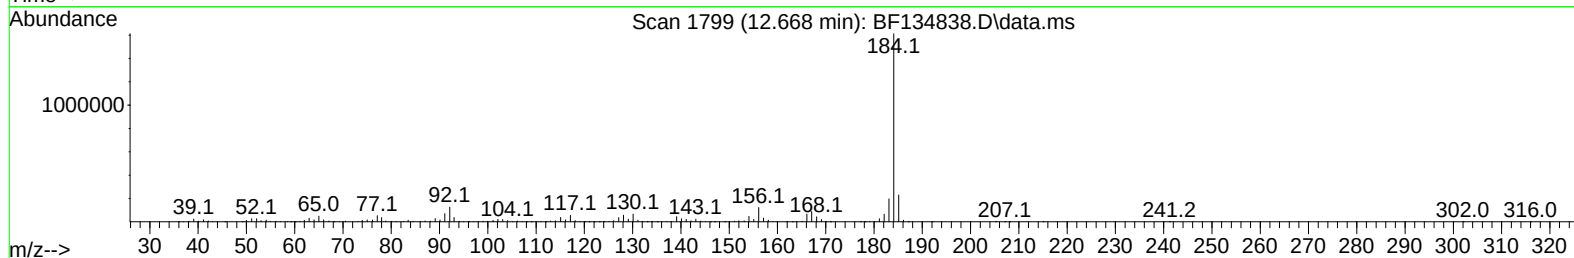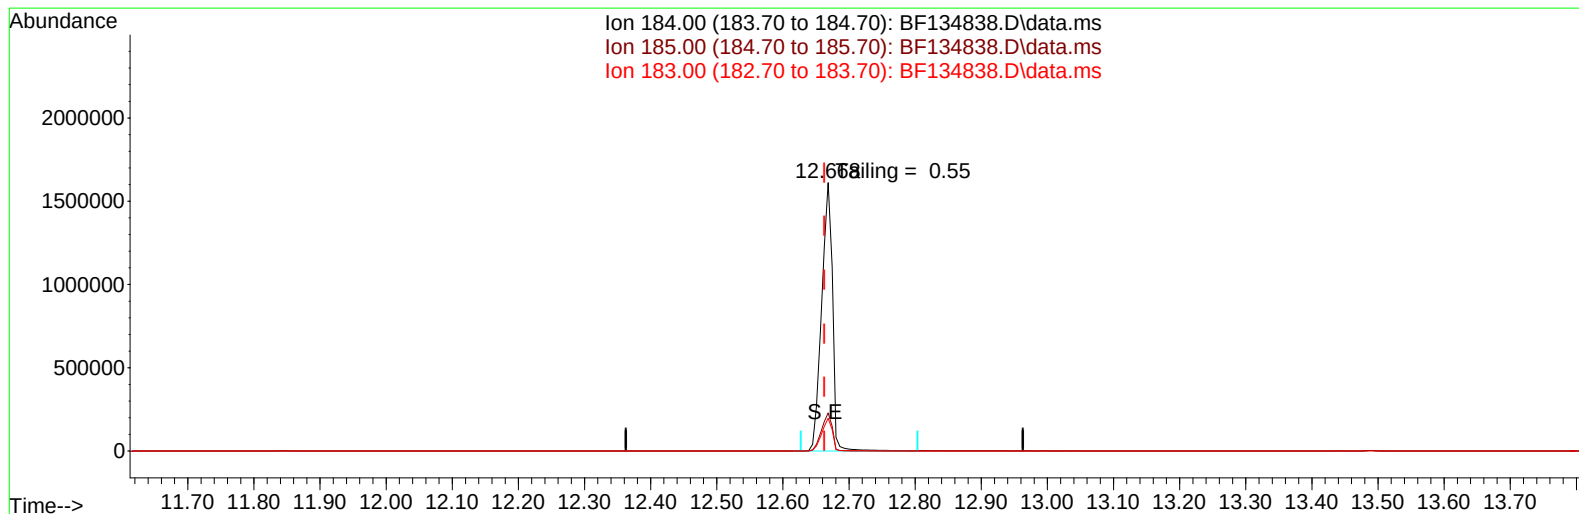

TIC: BF134838.D\data.ms

(77) Benzidine

12.668min (+ 0.006) 33791.05 ng

response 1837498

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.22
183.00	10.80	12.21
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/18/2023	BNA_F	<u>BF134838.D</u>
Compound Name	Response	Retention Time
DDT	898188	13.492
DDD	54312	13.186
DDE	944	12.851
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
55256	953444	5.80

Instrument :
BNA_F
ClientSampleId :
DFTPP