
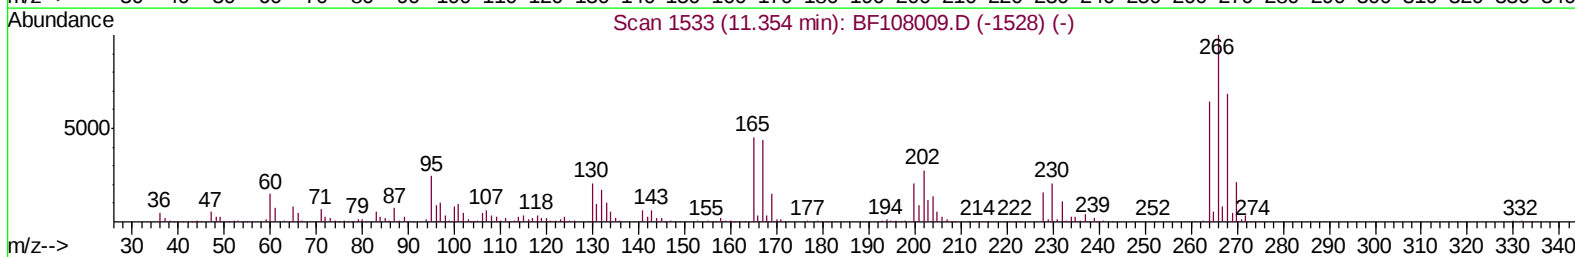
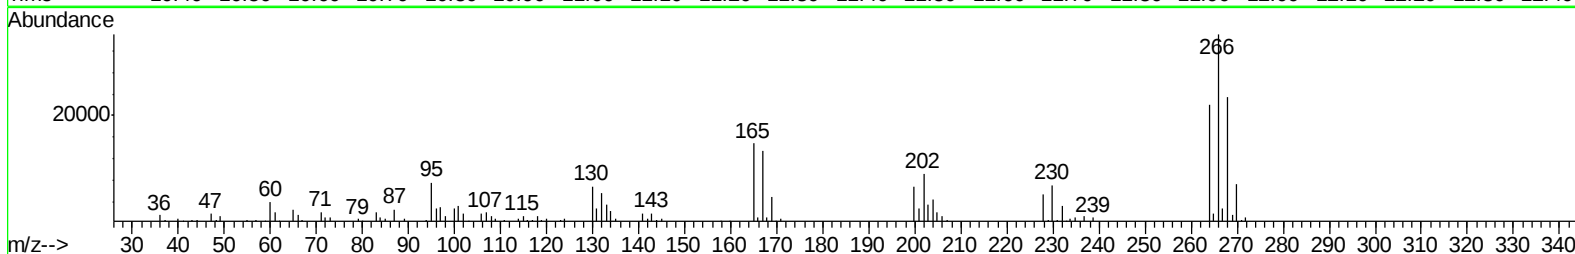


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082018\
Data File : BF108316.D
Acq On : 21 Aug 2018 3:32
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 21 07:42:20 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 08 12:24:24 2018
Response via : Initial Calibration

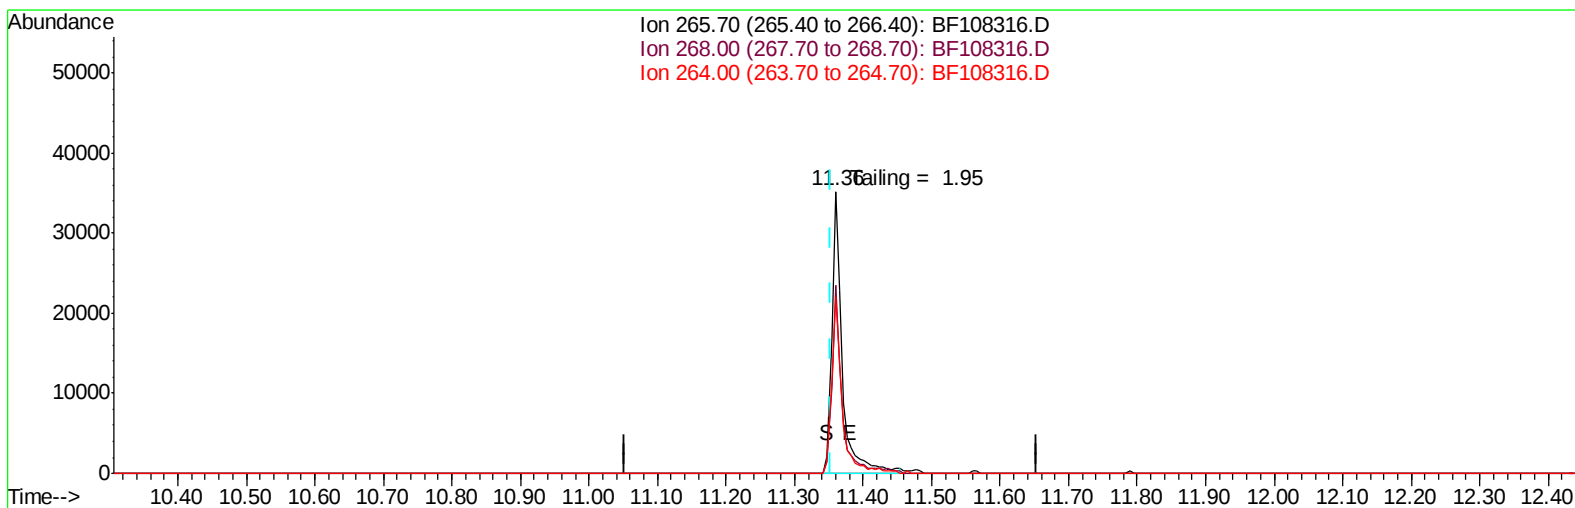

TIC: BF108316.D

(69) Pentachlorophenol (C)




11.359min (+0.006) 29750.25ng

response 36960

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	66.88
264.00	61.90	62.76
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082018\
Data File : BF108316.D
Acq On : 21 Aug 2018 3:32
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 21 07:42:20 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 08 12:24:24 2018
Response via : Initial Calibration

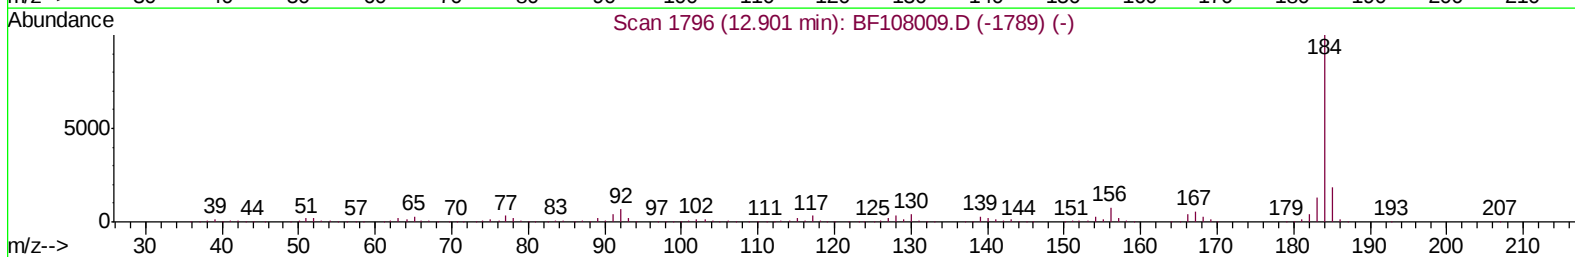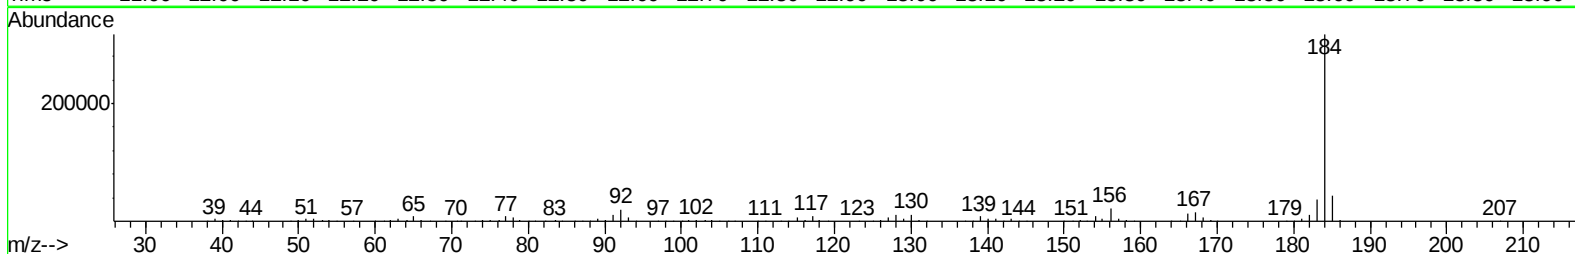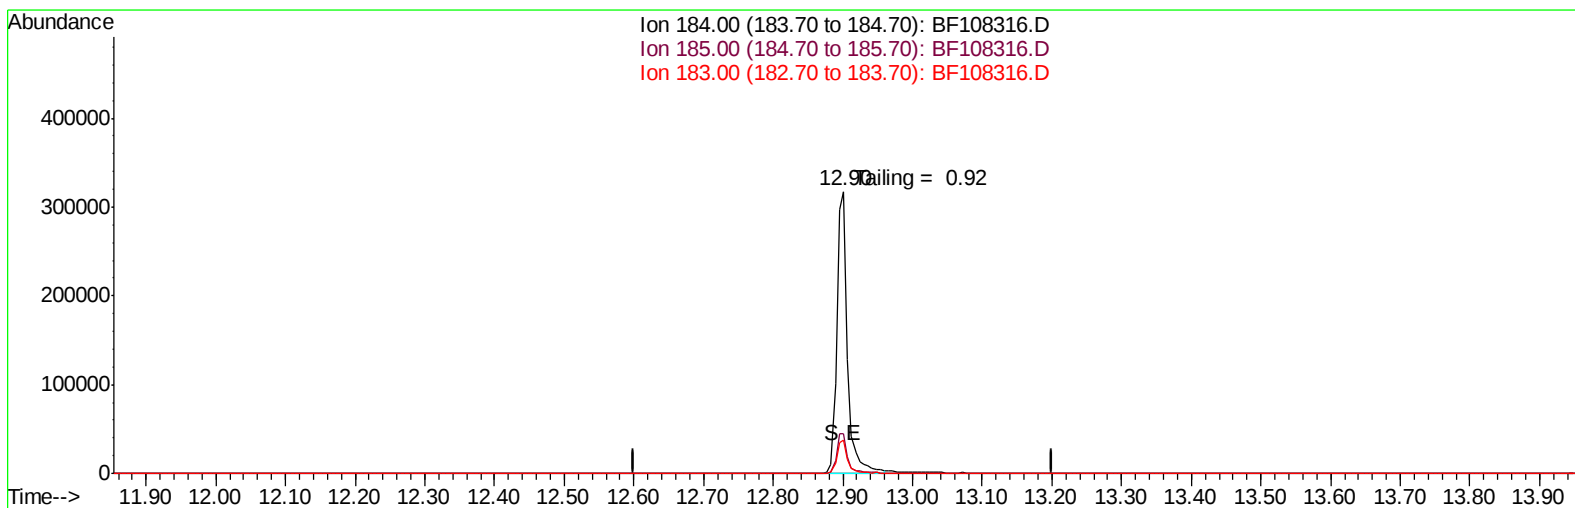

TIC: BF108316.D

(76) Benzidine

12.901min (-0.000) 84534.77ng m

response 341110

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	13.99
183.00	11.60	11.93
0.00	0.00	0.00