

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082018\
 Data File : BF108279.D
 Acq On : 20 Aug 2018 10:25
 Operator : JU/SJ
 Sample : PB112152BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB112152BL

Quant Time: Aug 20 11:22:43 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 12:24:24 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.01	152	191570	20.00	ng	0.00
21) Naphthalene-d8	8.30	136	735407	20.00	ng	0.00
38) Acenaphthene-d10	10.06	164	379789	20.00	ng	0.00
63) Phenanthrene-d10	11.56	188	779514	20.00	ng	0.00
75) Chrysene-d12	14.21	240	669328	20.00	ng	0.00
86) Perylene-d12	15.78	264	567763	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.65	112	1257912	118.88	ng	0.02
7) Phenol-d6	6.64	99	1665174	118.42	ng	0.01
23) Nitrobenzene-d5	7.58	82	1133102	85.98	ng	0.00
41) 2,4,6-Tribromophenol	10.86	330	536579	141.64	ng	0.00
44) 2-Fluorobiphenyl	9.38	172	2110370	89.21	ng	0.00
78) Terphenyl-d14	13.15	244	2447423	92.97	ng	0.00


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082018\
Data File : BF108279.D
Acq On : 20 Aug 2018 10:25
Operator : JU/SJ
Sample : PB112152BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB112152BL

Quant Time: Aug 20 11:22:43 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 08 12:24:24 2018
Response via : Initial Calibration

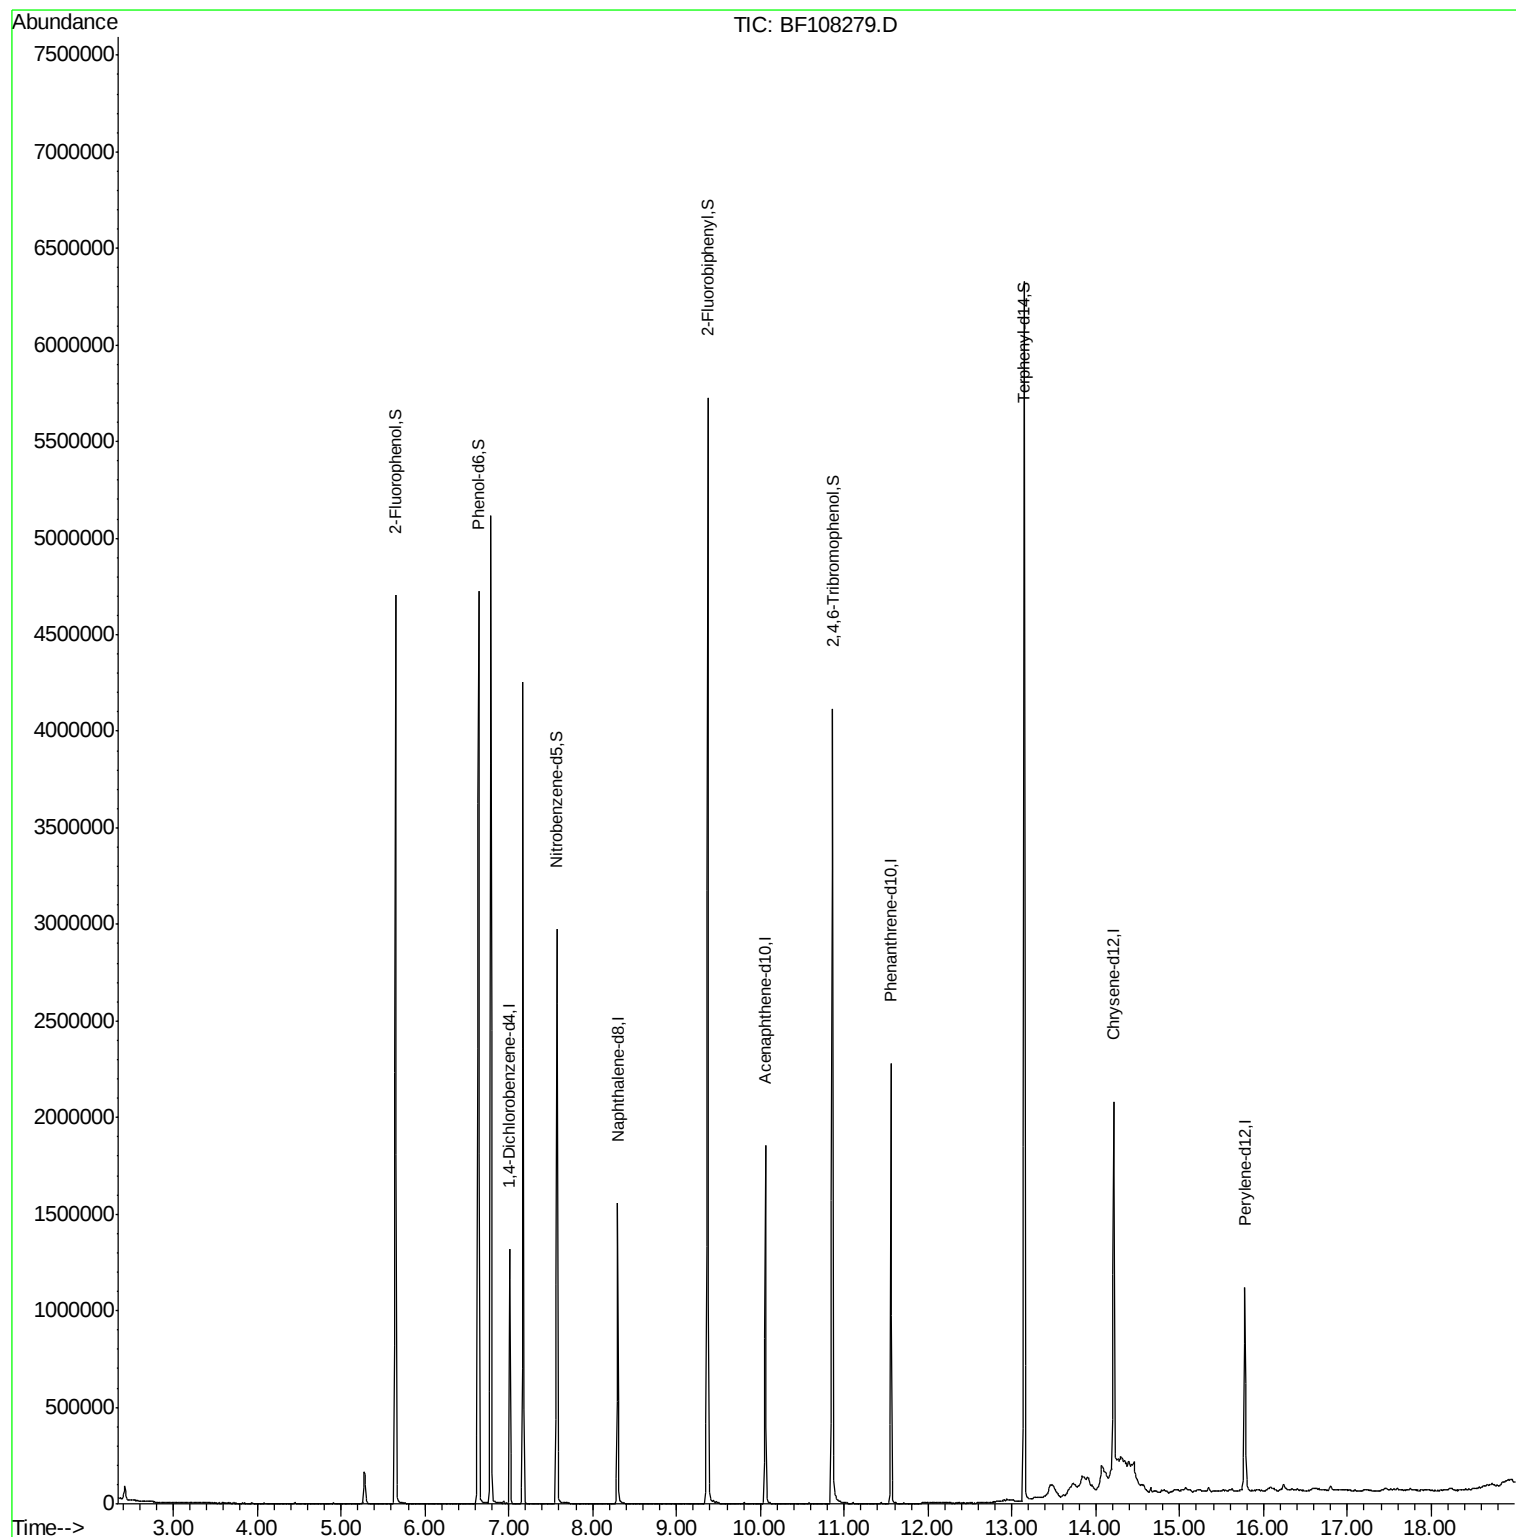




#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.01 min Scan# 795
Delta R.T. 0.00 min
Lab File: BF108279.D
Acq: 20 Aug 2018 10:25

Instrument :
BNA_F
ClientSampleId :
PB112152BL

Tot Ion:152 Resp: 191570
Ion Ratio Lower Upper
152 100
150 160.8 124.6 186.8
115 63.6 50.1 75.1

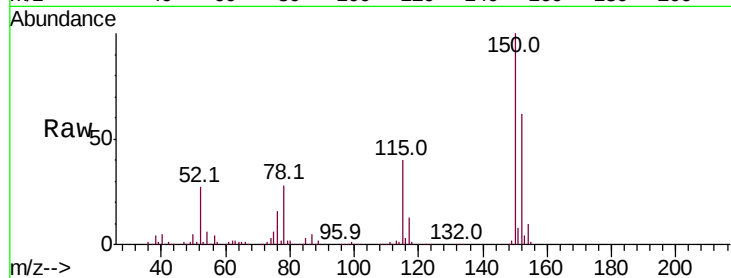


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

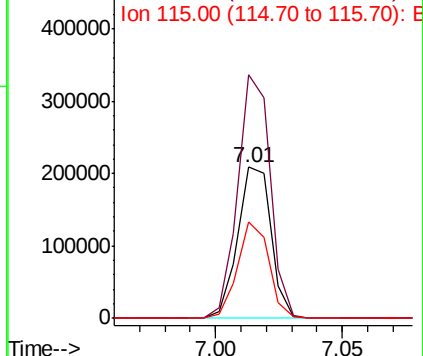



#5


2-Fluorophenol
Concen: 118.880 ng
RT: 5.65 min Scan# 564
Delta R.T. 0.02 min
Lab File: BF108279.D
Acq: 20 Aug 2018 10:25

Tgt Ion:112 Resp: 1257912
Ion Ratio Lower Upper
112 100
64 69.0 47.9 71.9
63 36.9 23.7 35.5#

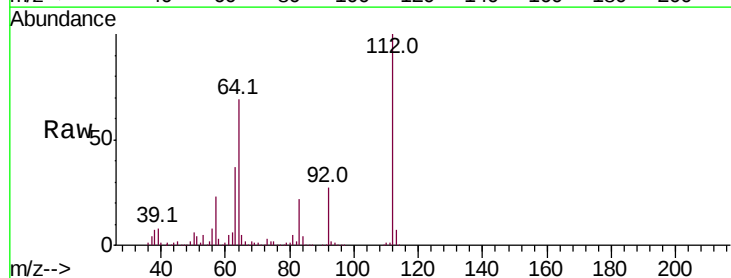

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

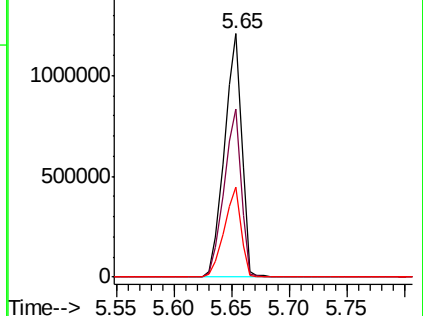

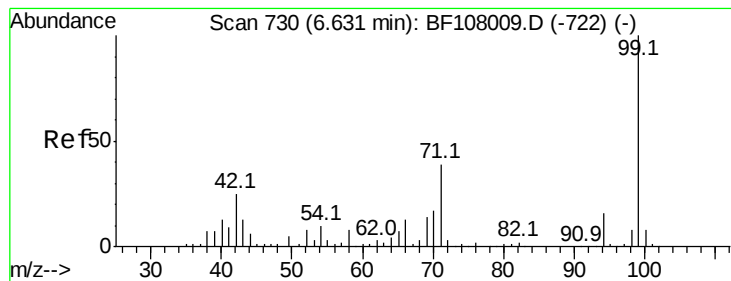

#7

Phenol-d6

Concen: 118.424 ng

RT: 6.64 min Scan# 732

Delta R.T. 0.01 min

Lab File: BF108279.D

Acq: 20 Aug 2018 10:25

Instrument :


BNA_F

ClientSampleId :




PB112152BL

Tot Ion: 99 Resp: 1665174

Ion	Ratio	Lower	Upper
99	100		
42	22.7	14.5	21.7#
71	37.9	25.4	38.0

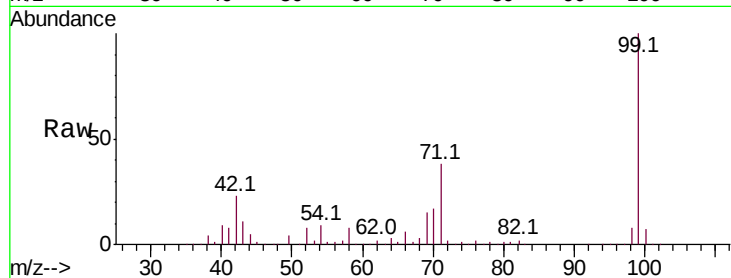

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

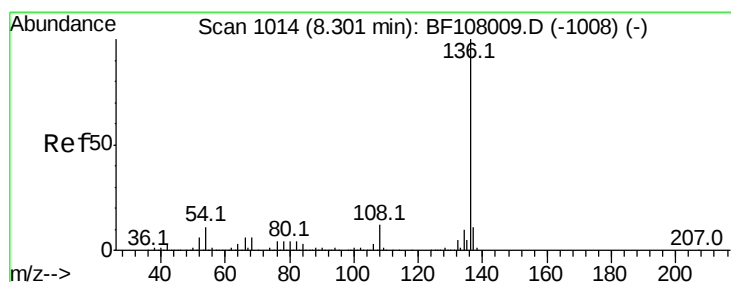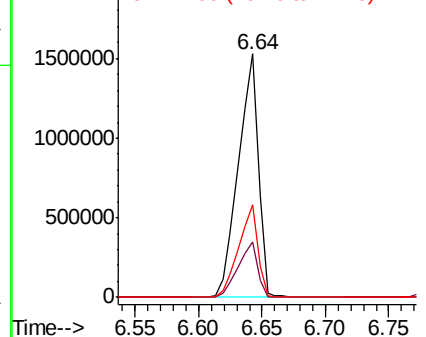

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.30 min Scan# 1014


Delta R.T. 0.00 min

Lab File: BF108279.D



Acq: 20 Aug 2018 10:25

Tgt Ion: 136 Resp: 735407

Ion	Ratio	Lower	Upper
136	100		
137	11.1	8.9	13.3
54	8.9	6.6	9.8
68	5.8	5.0	7.4

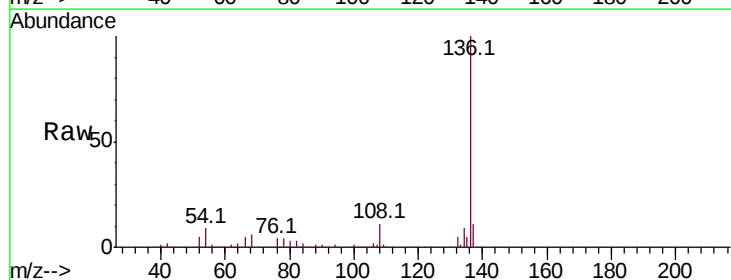

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

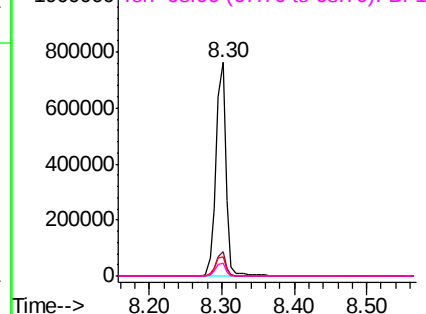







#23
 Nitrobenzene-d5
 Concen: 85.978 ng
 RT: 7.58 min Scan# 891
 Delta R.T. 0.00 min
 Lab File: BF108279.D
 Acq: 20 Aug 2018 10:25

Instrument :
 BNA_F
 ClientSampleId :
 PB112152BL

Tot Ion: 82 Resp: 1133102
 Ion Ratio Lower Upper
 82 100
 128 42.0 36.1 54.1
 54 57.9 41.4 62.2

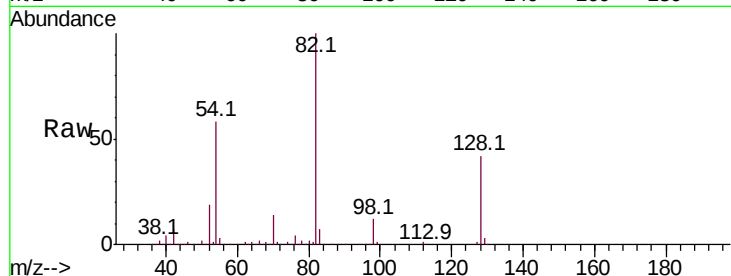


Abundance Ion 82.00 (81.70 to 82.70): BF1
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BF1

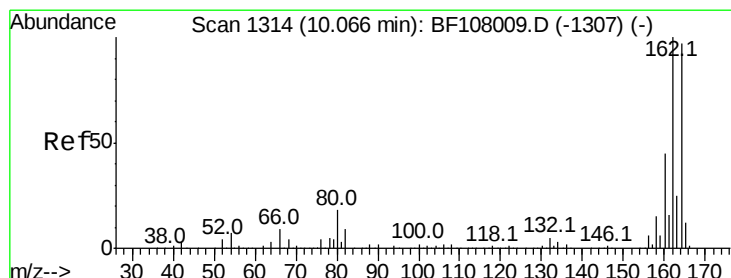
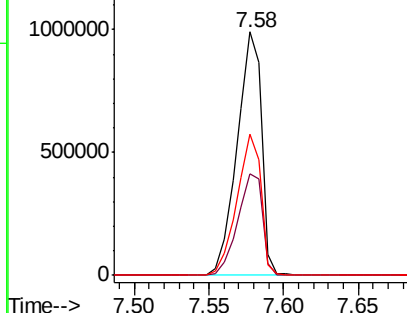



#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 10.06 min Scan# 1313
 Delta R.T. -0.01 min
 Lab File: BF108279.D
 Acq: 20 Aug 2018 10:25

Tgt Ion:164 Resp: 379789
 Ion Ratio Lower Upper
 164 100
 162 101.9 86.1 129.1
 160 46.4 38.3 57.5

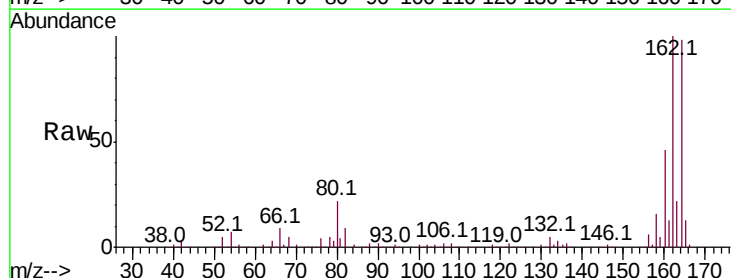

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

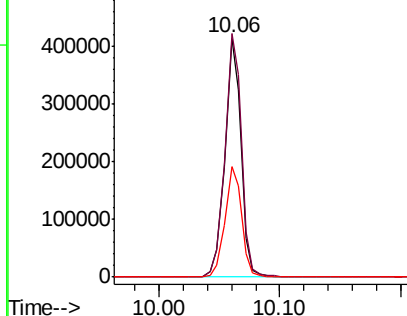







#41
 2,4,6-Tribromophenol
 Concen: 141.641 ng
 RT: 10.86 min Scan# 1449
 Delta R.T. 0.00 min
 Lab File: BF108279.D
 Acq: 20 Aug 2018 10:25

Instrument :
 BNA_F
 ClientSampleId :
 PB112152BL

Tot Ion:330 Resp: 536579
 Ion Ratio Lower Upper
 330 100
 332 95.5 77.0 115.6
 141 32.2 29.9 44.9

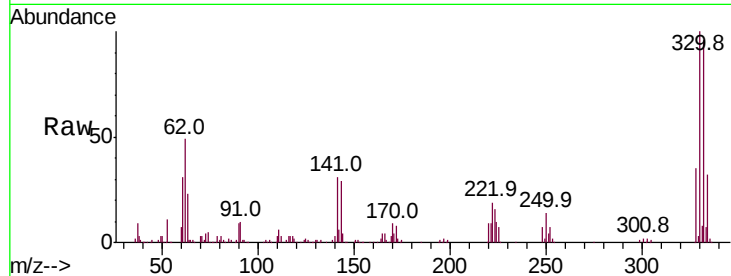


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

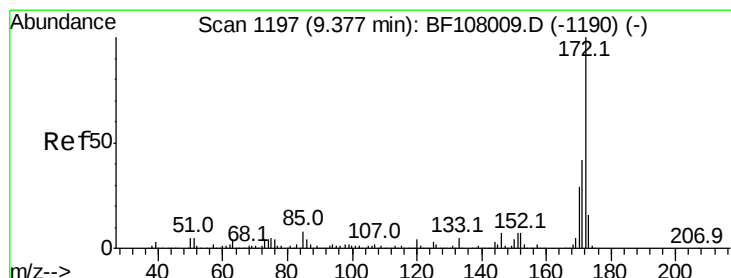
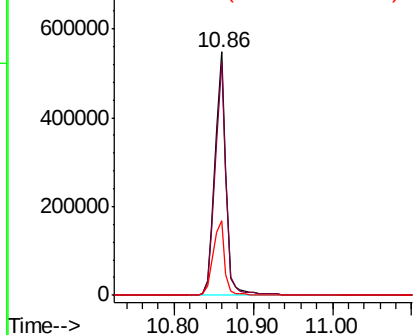



#44
 2-Fluorobiphenyl
 Concen: 89.211 ng
 RT: 9.38 min Scan# 1197
 Delta R.T. 0.00 min
 Lab File: BF108279.D
 Acq: 20 Aug 2018 10:25

Tgt Ion:172 Resp: 2110370
 Ion Ratio Lower Upper
 172 100
 171 37.8 29.7 44.5
 170 25.9 19.6 29.4

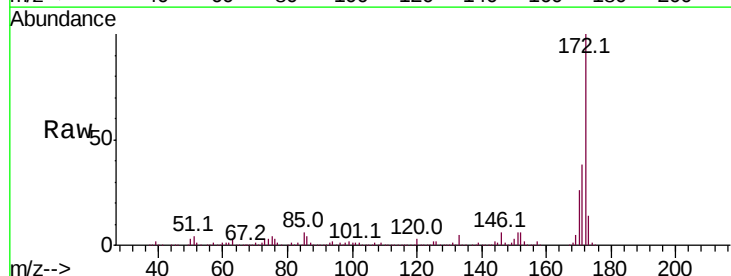

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

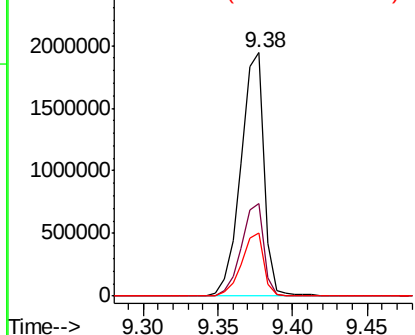


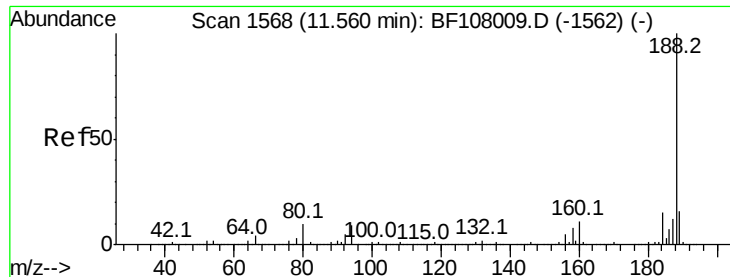




#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.56 min Scan# 1568
Delta R.T. 0.00 min
Lab File: BF108279.D
Acq: 20 Aug 2018 10:25

Instrument :
BNA_F
ClientSampleId :
PB112152BL

Tot Ion:188 Resp: 779514
Ion Ratio Lower Upper
188 100
94 8.6 8.5 12.7
80 9.5 9.2 13.8

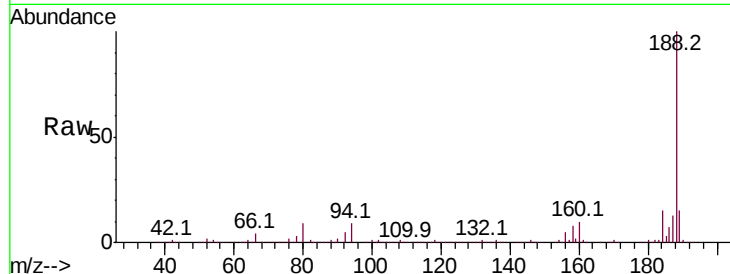


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1

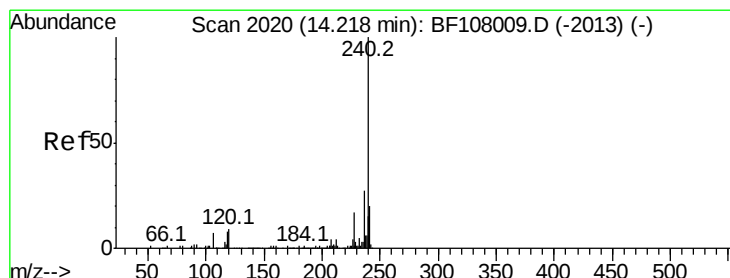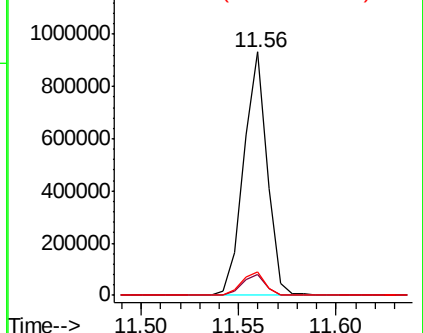
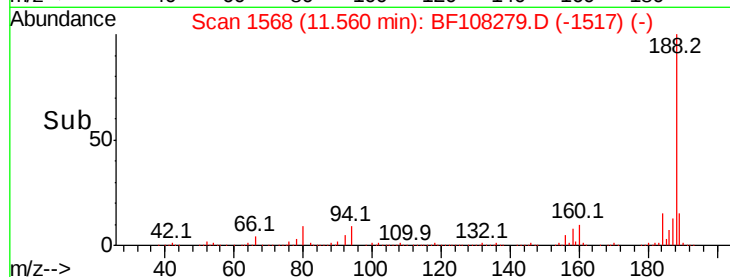



#75
Chrysene-d12
Concen: 20.000 ng
RT: 14.21 min Scan# 2019
Delta R.T. -0.01 min
Lab File: BF108279.D
Acq: 20 Aug 2018 10:25

Tgt Ion:240 Resp: 669328
Ion Ratio Lower Upper
240 100
120 10.9 9.5 14.3
236 26.9 20.7 31.1

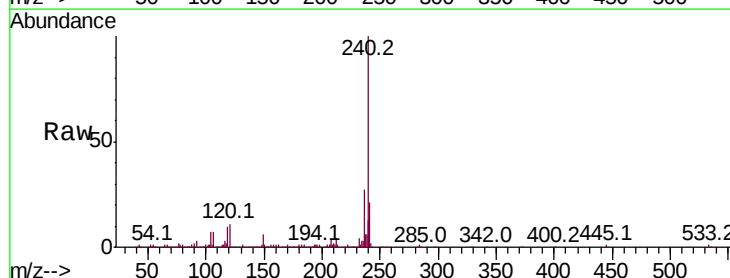

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

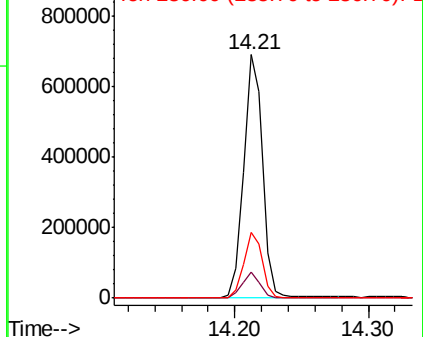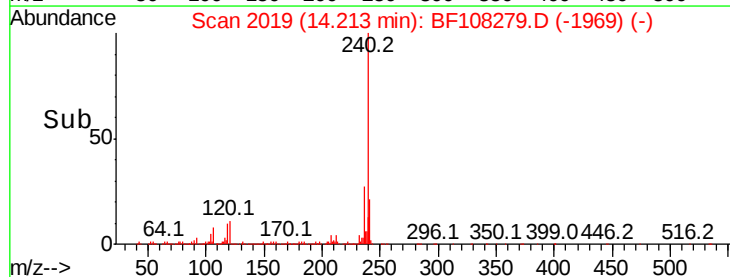

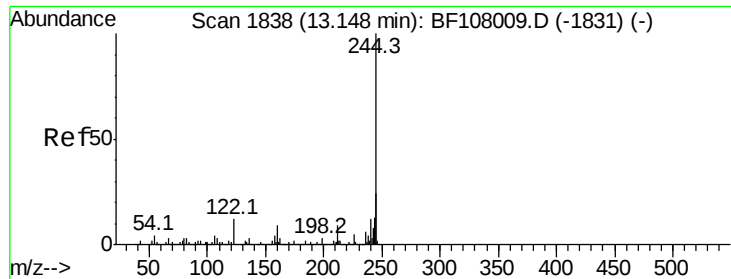

#78

Terphenyl-d14

Concen: 92.970 ng

RT: 13.15 min Scan# 1838

Delta R.T. 0.00 min

Lab File: BF108279.D

Acq: 20 Aug 2018 10:25

Instrument :

BNA_F

ClientSampleId :

PB112152BL


Tot Ion:244 Resp: 2447423

Ion Ratio Lower Upper

244 100

212 7.7 5.4 8.0




122 11.9 11.0 16.4

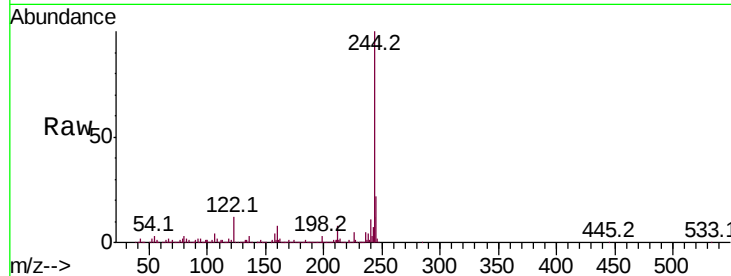

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

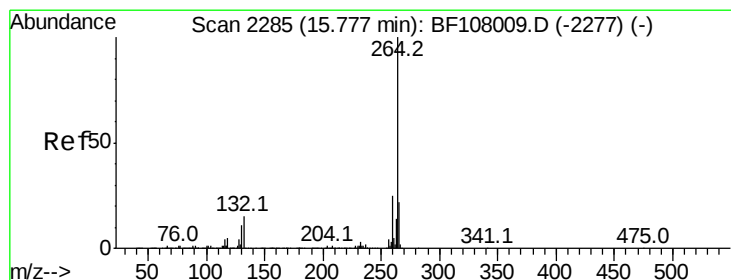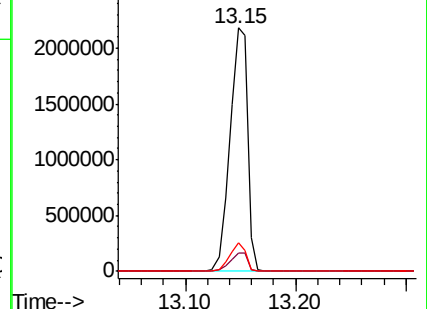

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.78 min Scan# 2285

Delta R.T. 0.00 min

Lab File: BF108279.D

Acq: 20 Aug 2018 10:25


Tgt Ion:264 Resp: 567763

Ion Ratio Lower Upper

264 100

260 24.3 19.2 28.8

265 21.9 17.5 26.3

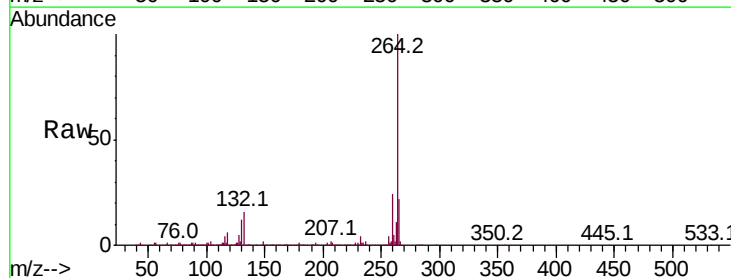

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

