


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082018\
 Data File : BF108316.D
 Acq On : 21 Aug 2018 3:32
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 08 12:24:24 2018

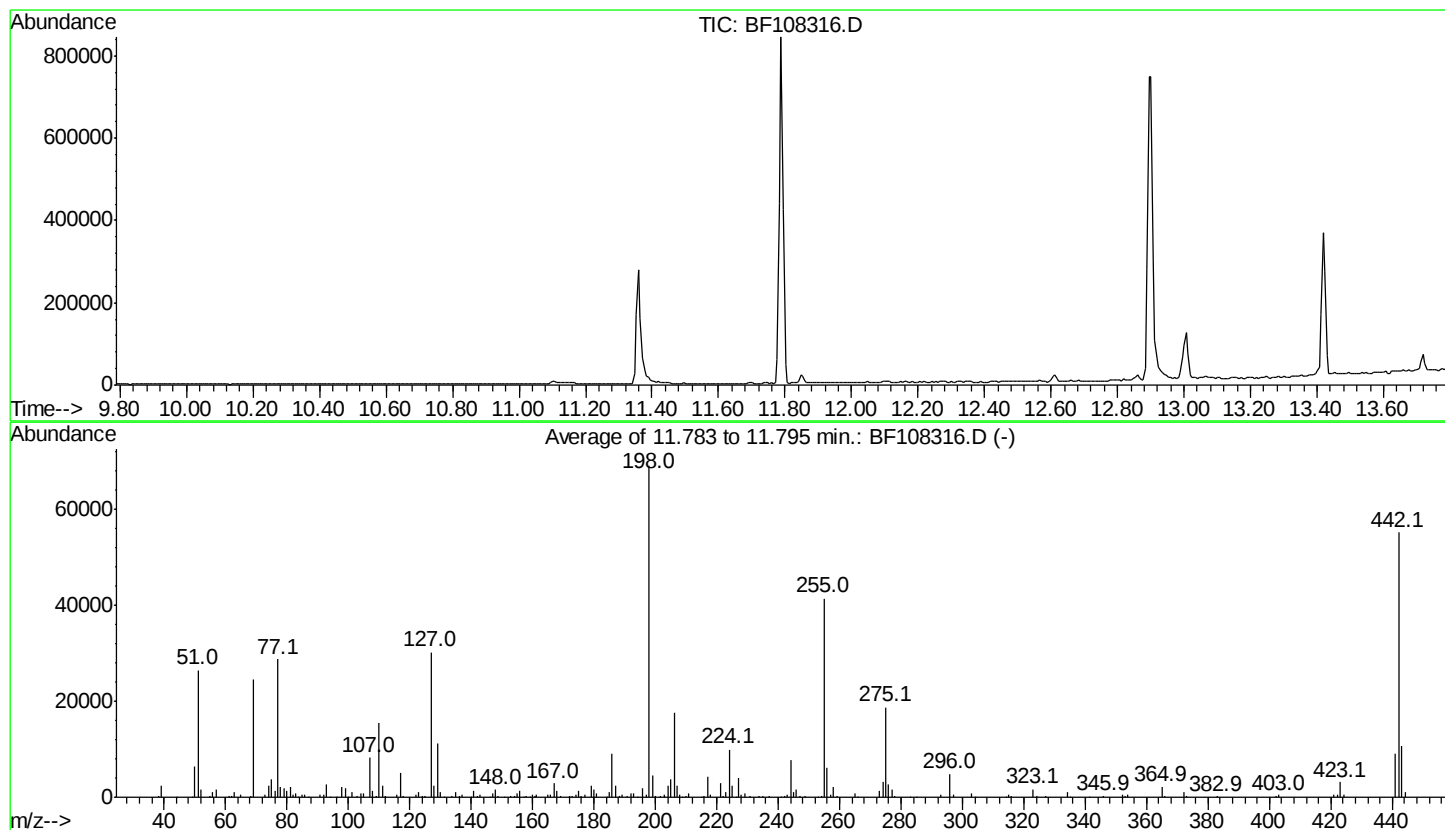

AutoFind: Scans 1606, 1607, 1608; Background Corrected with Scan 1601

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.3	26415	PASS
68	69	0.00	2	1.5	377	PASS
69	198	0.00	100	35.4	24392	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.7	30114	PASS
197	198	0.00	2	0.7	476	PASS
198	198	100	100	100.0	68989	PASS
199	198	5	9	6.4	4429	PASS
275	198	10	60	27.1	18671	PASS
365	198	1	100	3.2	2198	PASS
441	198	0.01	100	13.3	9193	PASS
442	198	50	100	79.9	55098	PASS
443	442	15	24	19.3	10620	PASS