

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082019\
 Data File : BF116439.D
 Acq On : 20 Aug 2019 19:31
 Operator : HP/JU
 Sample : K4096-06
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Aug 21 01:15:02 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF073019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 19 06:03:31 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.80	152	91464	20.00	ng	-0.01
21) Naphthalene-d8	8.09	136	354951	20.00	ng	-0.01
39) Acenaphthene-d10	9.83	164	192836	20.00	ng	-0.02
64) Phenanthrene-d10	11.32	188	367718	20.00	ng	-0.02
76) Chrysene-d12	13.96	240	316651	20.00	ng	-0.02
87) Perylene-d12	15.42	264	337200	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.44	112	677524	124.01	ng	0.00
7) Phenol-d6	6.45	99	800672	116.15	ng	-0.01
23) Nitrobenzene-d5	7.37	82	618759	100.62	ng	-0.02
42) 2,4,6-Tribromophenol	10.63	330	283981	151.89	ng	-0.02
45) 2-Fluorobiphenyl	9.16	172	1099388	106.79	ng	-0.01
79) Terphenyl-d14	12.90	244	1398171	93.04	ng	-0.01
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.37	70	82302	19.267	ng	# 79
25) Isophorone	7.37	82	618759	52.624	ng	# 65
50) Dimethylphthalate	9.56	163	42114	3.207	ng	# 99
51) 2,6-Dinitrotoluene	9.83	165	24715	8.662	ng	# 29
57) 2,4-Dinitrotoluene	9.83	165	24715	6.506	ng	# 20
67) 4-Bromophenyl-phenylether	10.63	248	17250	4.382	ng	# 1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082019\
Data File : BF116439.D
Acq On : 20 Aug 2019 19:31
Operator : HP/JU
Sample : K4096-06
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Aug 21 01:15:02 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF073019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 19 06:03:31 2019
Response via : Initial Calibration

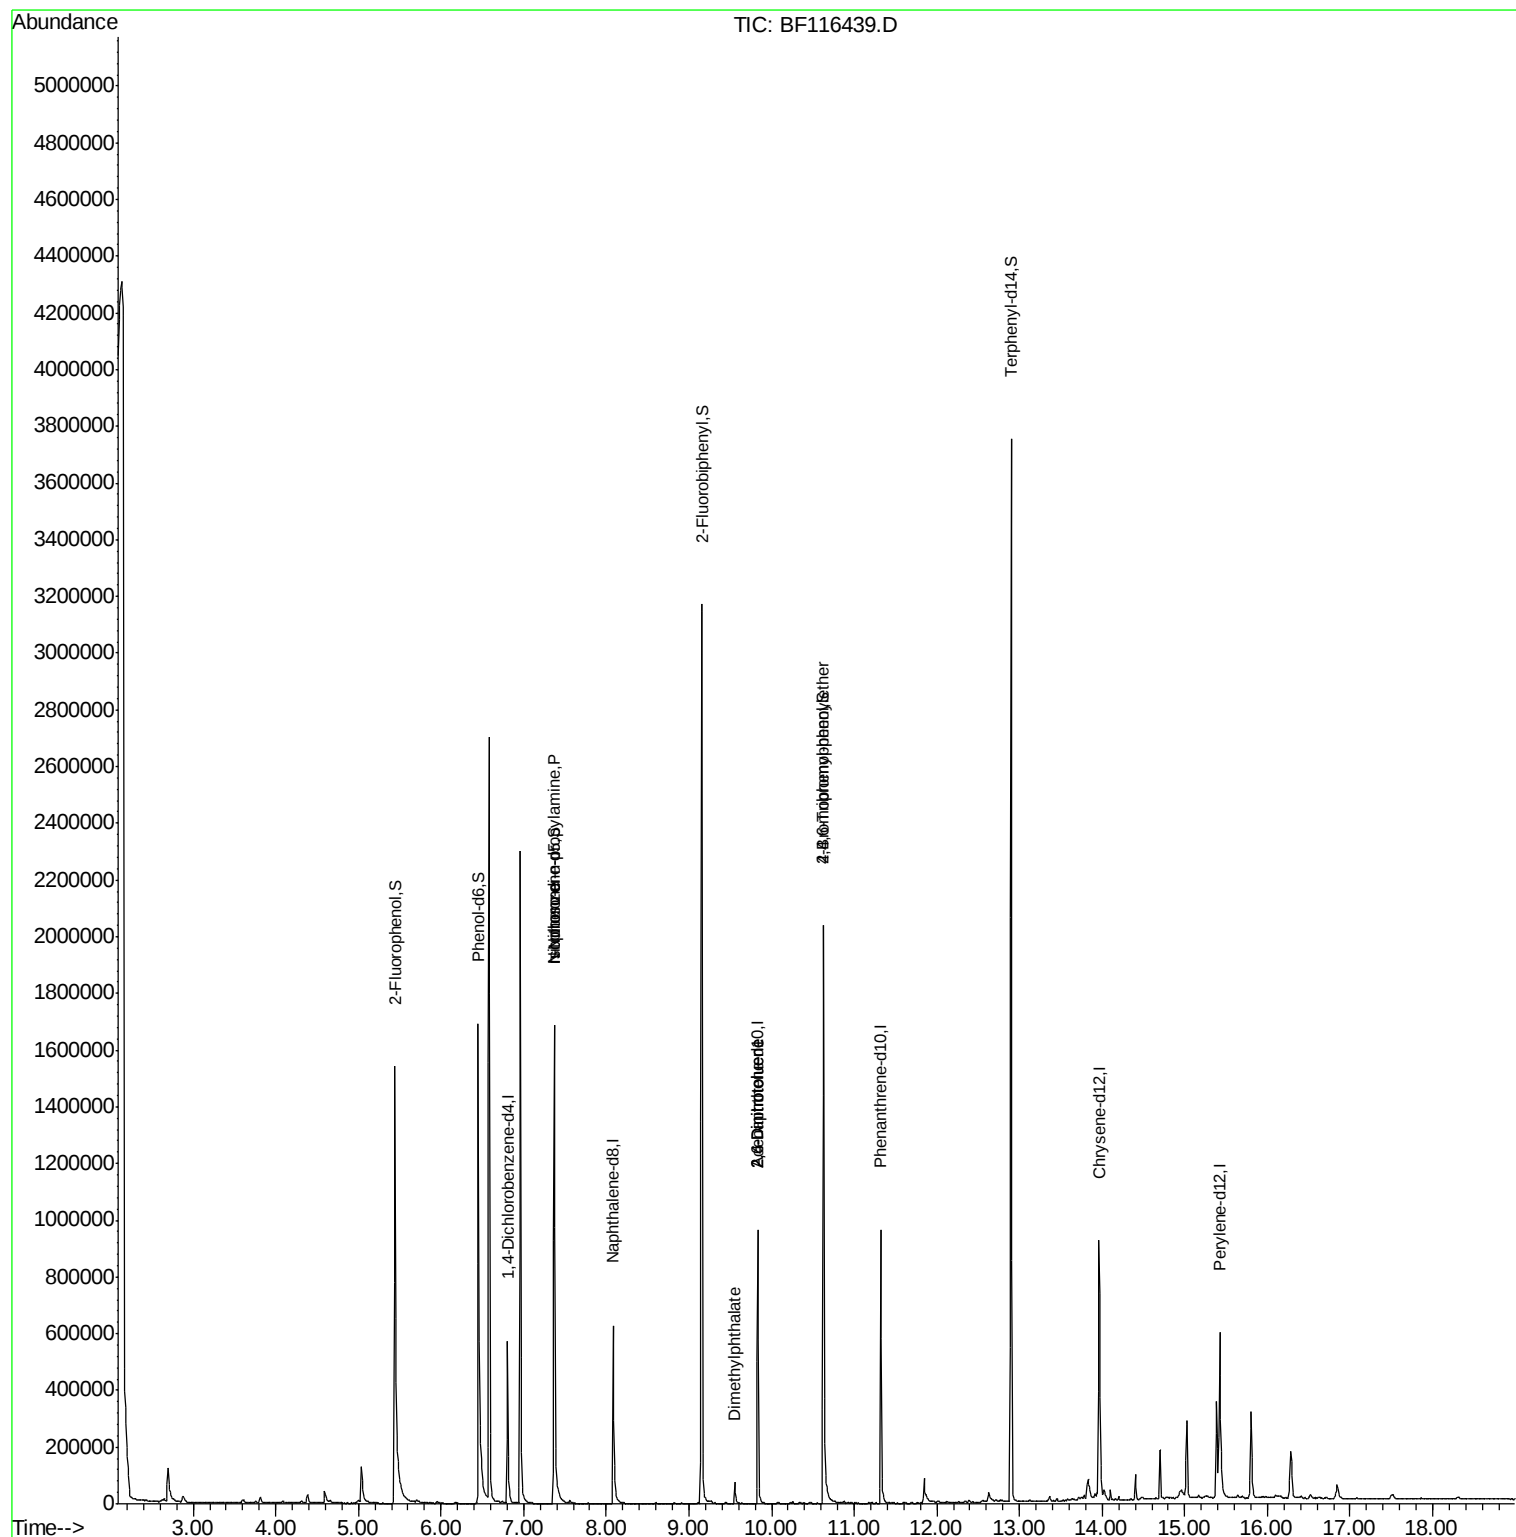




#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.80 min Scan# 802
Delta R.T. -0.01 min
Lab File: BF116439.D
Acq: 20 Aug 2019 19:31

Instrument :
BNA_F
ClientSampleId :

Tot Ion:152 Resp: 91464
Ion Ratio Lower Upper
152 100
150 159.3 126.2 189.2
115 63.8 49.9 74.9

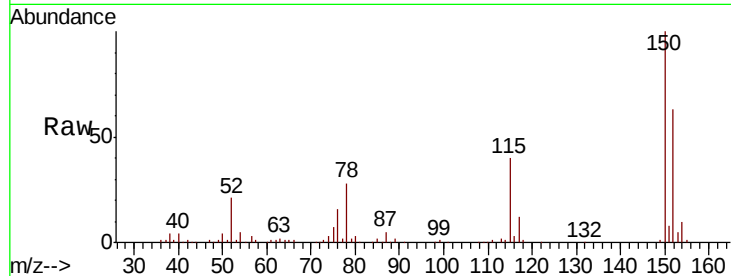


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

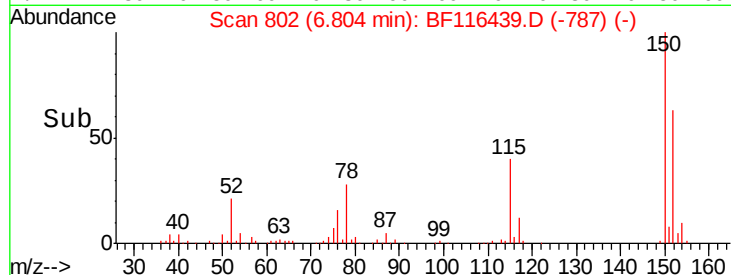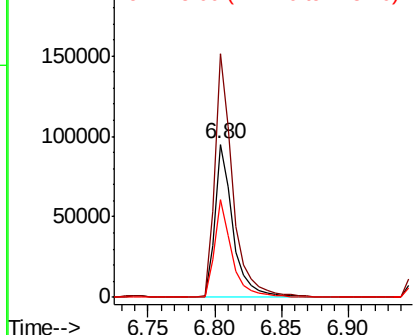



#5

2-Fluorophenol
Concen: 124.007 ng
RT: 5.44 min Scan# 570
Delta R.T. 0.00 min
Lab File: BF116439.D
Acq: 20 Aug 2019 19:31

Tgt Ion:112 Resp: 677524
Ion Ratio Lower Upper
112 100
64 57.6 45.4 68.2
63 30.0 23.7 35.5



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

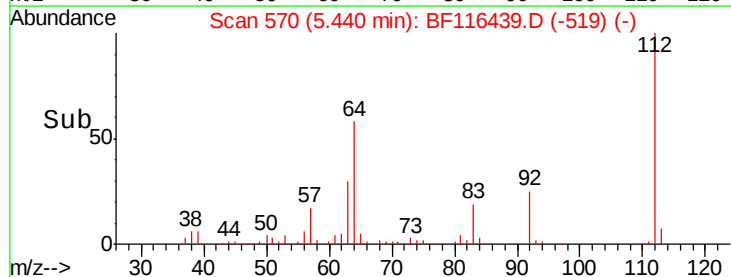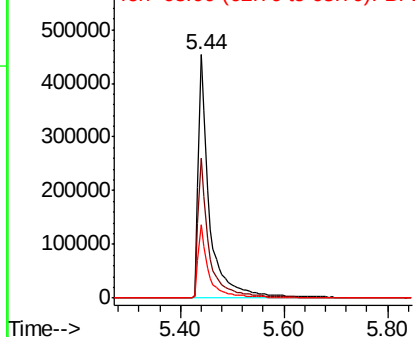



#7

Phenol-d6

Concen: 116.152 ng

RT: 6.45 min Scan# 742

Delta R.T. -0.01 min

Lab File: BF116439.D

Acq: 20 Aug 2019 19:31

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 99 Resp: 800672

Ion Ratio Lower Upper

99 100

42 16.9 13.8 20.8



71 32.8 27.3 40.9

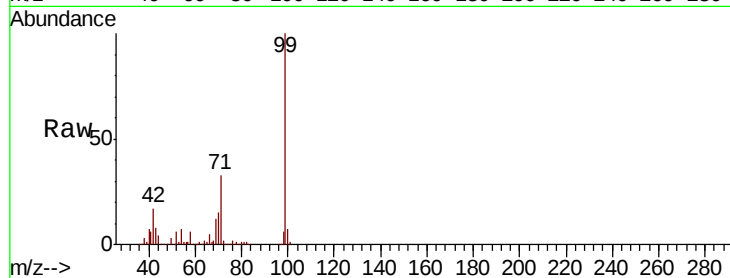

Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

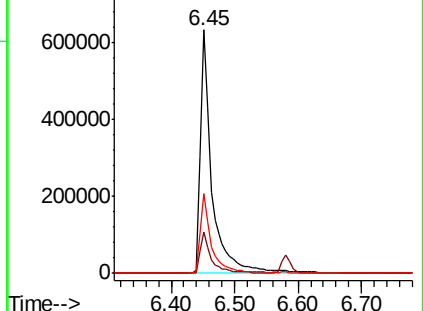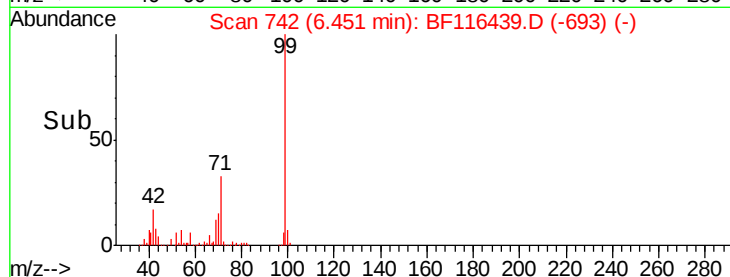

#19

n-Nitroso-di-n-propylamine

Concen: 19.267 ng

RT: 7.37 min Scan# 898

Delta R.T. 0.14 min

Lab File: BF116439.D

Acq: 20 Aug 2019 19:31

Tgt Ion: 70 Resp: 82302


Ion Ratio Lower Upper

70 100

42 42.4 40.9 61.3

101 0.0 7.9 11.9#

130 2.0 16.9 25.3#


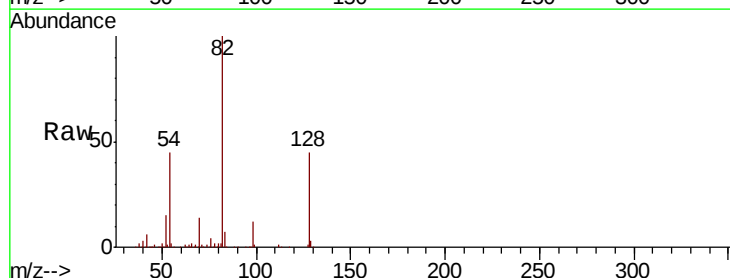


Abundance Ion 70.00 (69.70 to 70.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 101.00 (100.70 to 101.70): BF1

Ion 130.00 (129.70 to 130.70): BF1



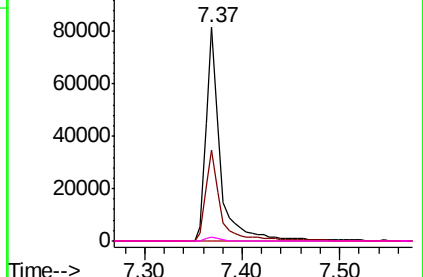
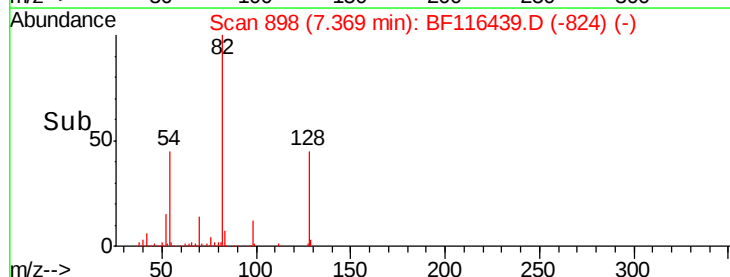




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.09 min Scan# 1020
Delta R.T. -0.01 min
Lab File: BF116439.D
Acq: 20 Aug 2019 19:31




Instrument :
BNA_F
ClientSampleId :


Tot Ion:136	Resp:	354951
Ion	Ratio	Lower Upper
136	100	
137	10.8	9.0 13.4
54	6.4	5.8 8.6
68	5.9	5.2 7.8

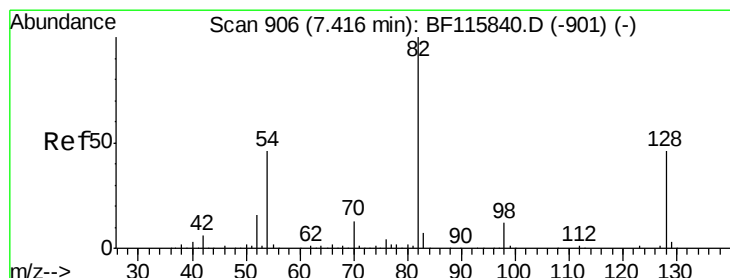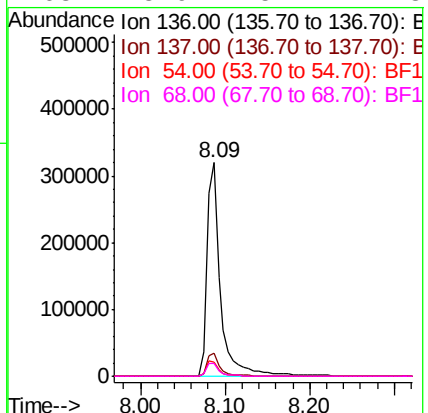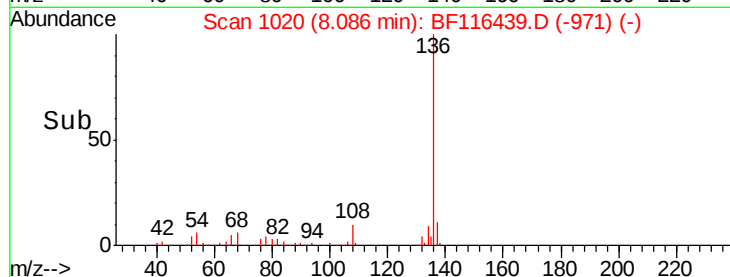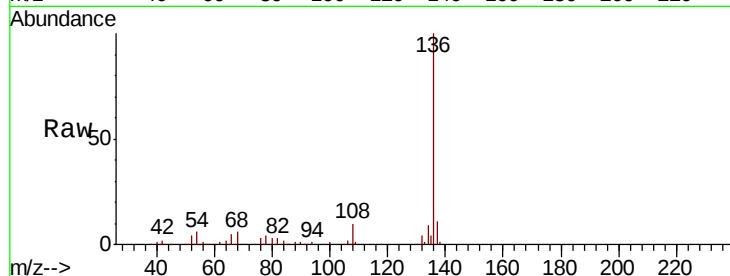

#23
Nitrobenzene-d5
Concen: 100.624 ng
RT: 7.37 min Scan# 898
Delta R.T. -0.02 min
Lab File: BF116439.D
Acq: 20 Aug 2019 19:31

Tgt Ion: 82	Resp:	618759
Ion	Ratio	Lower Upper
82	100	
128	45.2	36.5 54.7
54	45.4	36.0 54.0

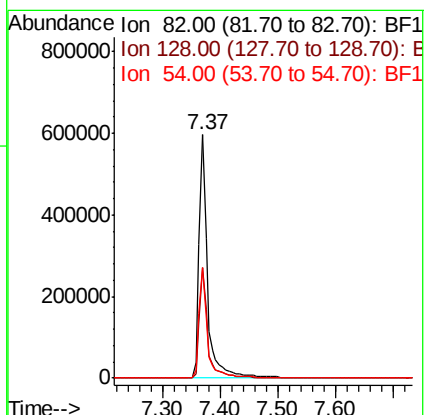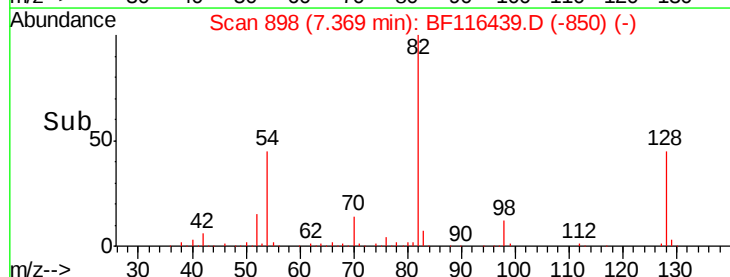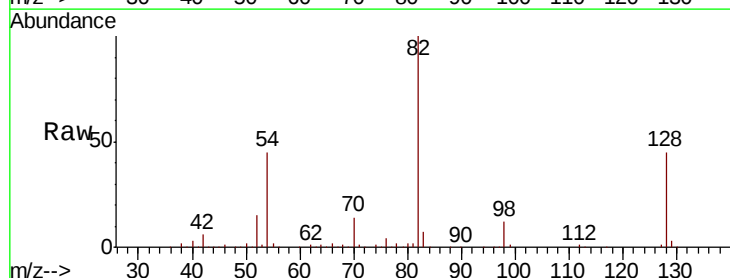

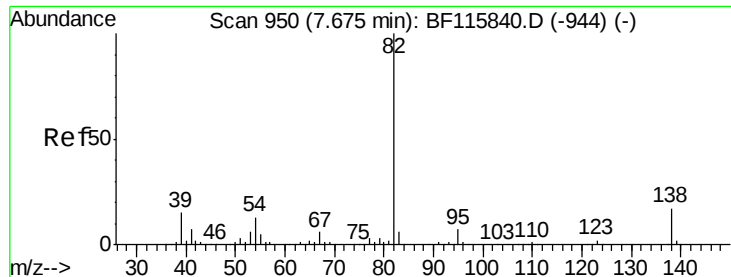

#25

Isophorone

Concen: 52.624 ng

RT: 7.37 min Scan# 898

Delta R.T. -0.27 min

Lab File: BF116439.D

Acq: 20 Aug 2019 19:31

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 82 Resp: 618759

Ion Ratio Lower Upper




82 100

95 0.0 5.4 8.0#

138 0.0 14.5 21.7#



Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 95.00 (94.70 to 95.70): BF1
Ion 138.00 (137.70 to 138.70): E

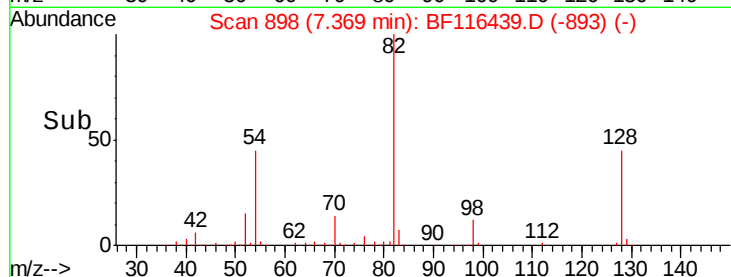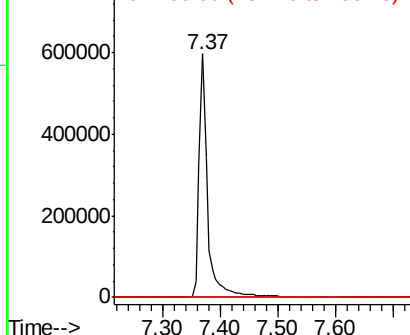

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.83 min Scan# 1317

Delta R.T. -0.02 min

Lab File: BF116439.D

Acq: 20 Aug 2019 19:31


Tgt Ion: 164 Resp: 192836

Ion Ratio Lower Upper



164 100

162 101.7 82.6 124.0

160 46.5 37.6 56.4



Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

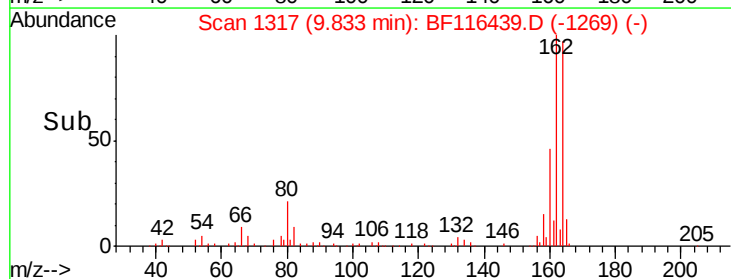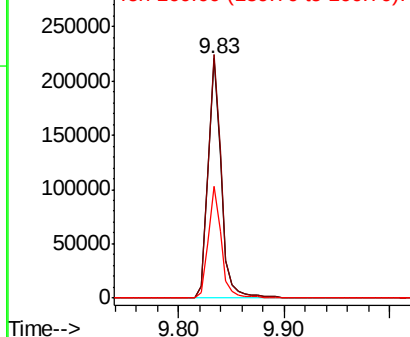




#42
 2,4,6-Tribromophenol
 Concen: 151.894 ng
 RT: 10.63 min Scan# 1452
 Delta R.T. -0.02 min
 Lab File: BF116439.D
 Acq: 20 Aug 2019 19:31

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.6	76.8	115.2
141	33.9	26.3	39.5



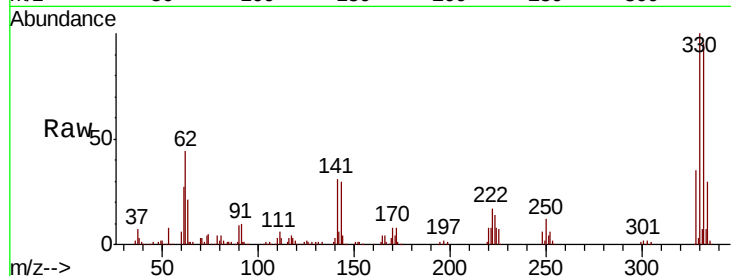


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

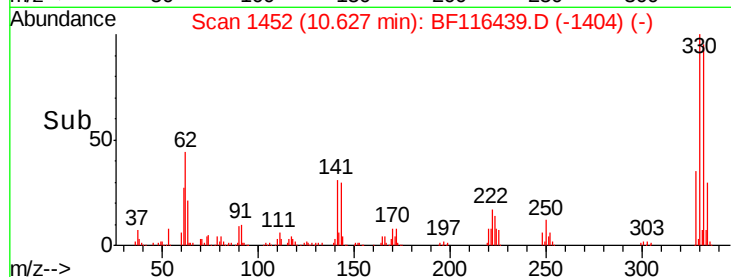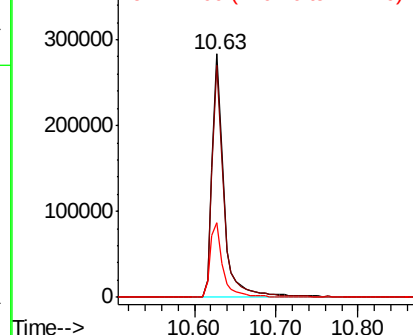

#45
 2-Fluorobiphenyl
 Concen: 106.787 ng
 RT: 9.16 min Scan# 1202
 Delta R.T. -0.01 min
 Lab File: BF116439.D
 Acq: 20 Aug 2019 19:31

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.7	29.6	44.4
170	24.8	20.1	30.1






Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

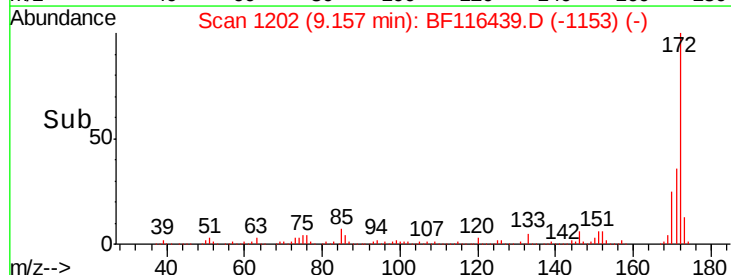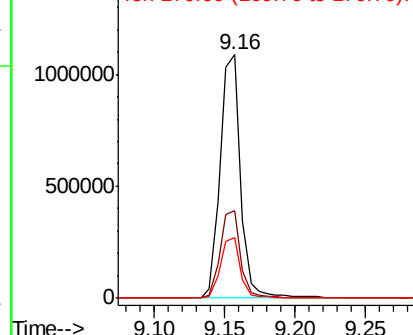

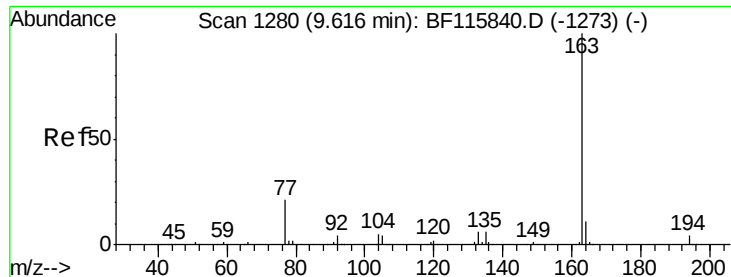

#50

Dimethylphthalate

Concen: 3.207 ng

RT: 9.56 min Scan# 1270

Delta R.T. -0.01 min

Lab File: BF116439.D

Acq: 20 Aug 2019 19:31

Instrument :

BNA_F

ClientSampleId :


Tot Ion:163 Resp: 42114

Ion Ratio Lower Upper

163 100

194 3.9 3.0 4.6




164 9.9 8.4 12.6



Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

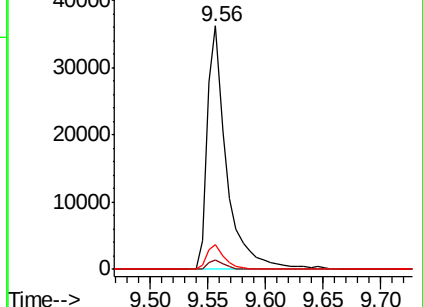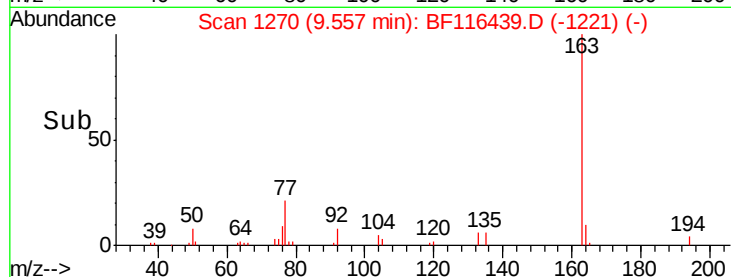

#51

2,6-Dinitrotoluene

Concen: 8.662 ng

RT: 9.83 min Scan# 1317

Delta R.T. 0.19 min

Lab File: BF116439.D

Acq: 20 Aug 2019 19:31


Tgt Ion:165 Resp: 24715

Ion Ratio Lower Upper

165 100

63 1.2 38.2 57.2#



89 1.1 42.9 64.3#




Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF1

Ion 89.00 (88.70 to 89.70): BF1

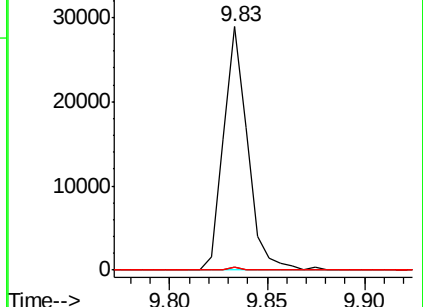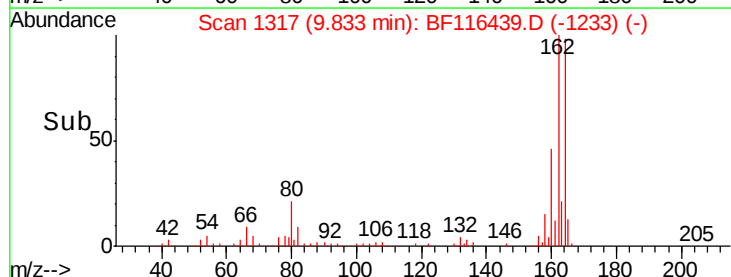


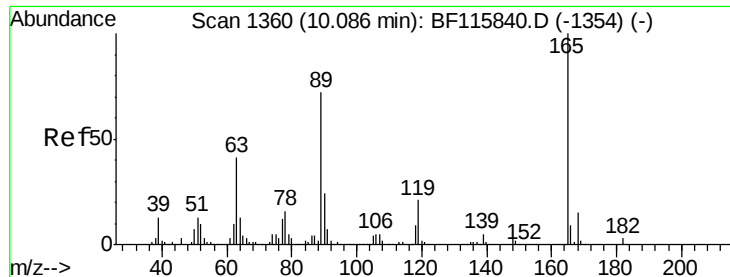

#57
 2,4-Dinitrotoluene
 Concen: 6.506 ng
 RT: 9.83 min Scan# 1317
 Delta R.T. -0.22 min
 Lab File: BF116439.D
 Acq: 20 Aug 2019 19:31

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
165	100		
63	1.2	39.6	59.4#
89	1.1	62.2	93.2#
182	0.0	2.1	3.1#



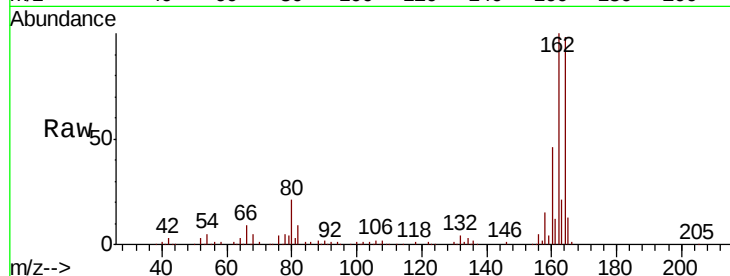


Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF1


Ion 89.00 (88.70 to 89.70): BF1

Ion 182.00 (181.70 to 182.70): E

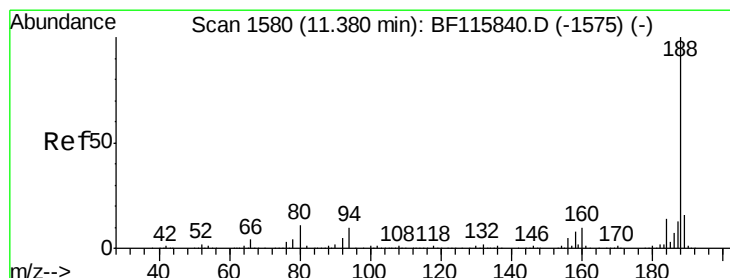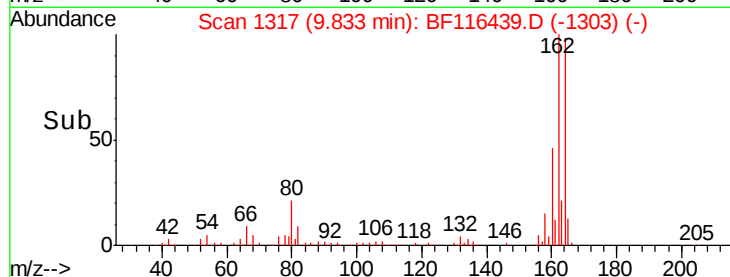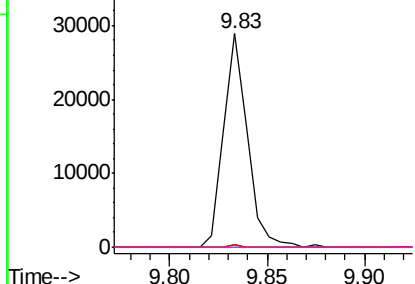

#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 11.32 min Scan# 1570
 Delta R.T. -0.02 min
 Lab File: BF116439.D
 Acq: 20 Aug 2019 19:31



Tgt Ion	Ratio	Lower	Upper
188	100		
94	9.6	8.1	12.1
80	10.2	8.7	13.1

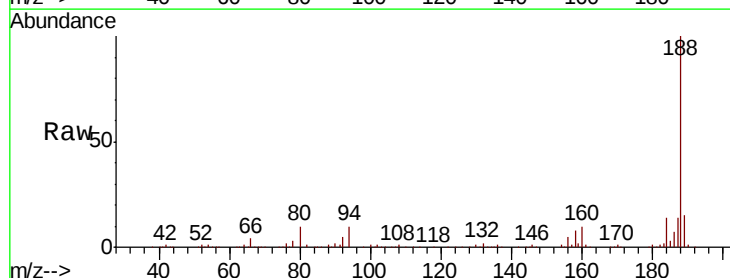


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

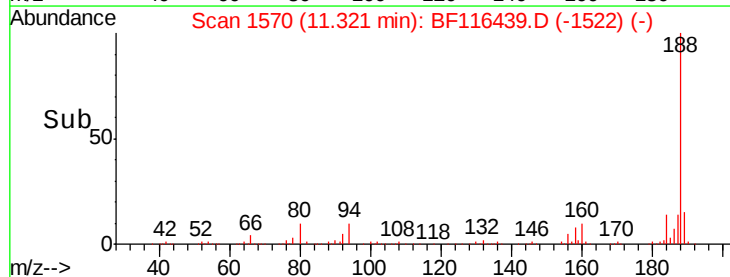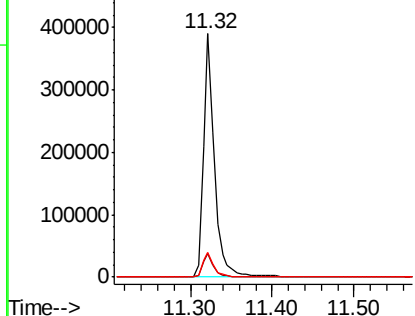


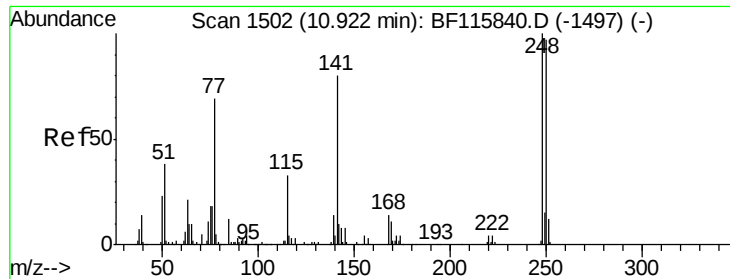




#67
 4-Bromophenyl-phenylether
 Concen: 4.382 ng
 RT: 10.63 min Scan# 1452
 Delta R.T. -0.25 min
 Lab File: BF116439.D
 Acq: 20 Aug 2019 19:31

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:248 Resp: 17250
 Ion Ratio Lower Upper
 248 100
 250 200.5 77.4 116.2#
 141 500.1 56.8 85.2#

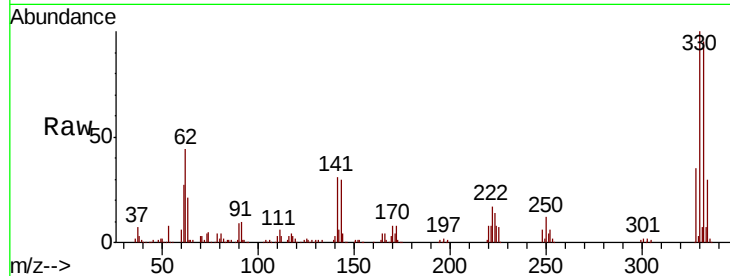


Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E

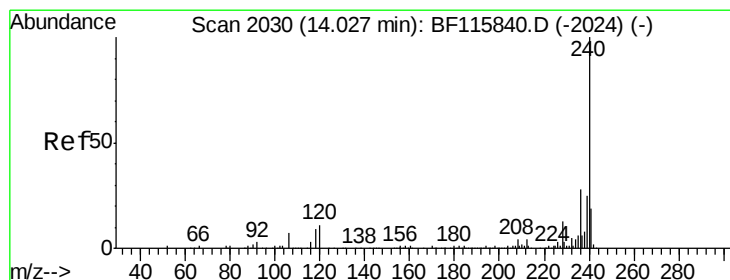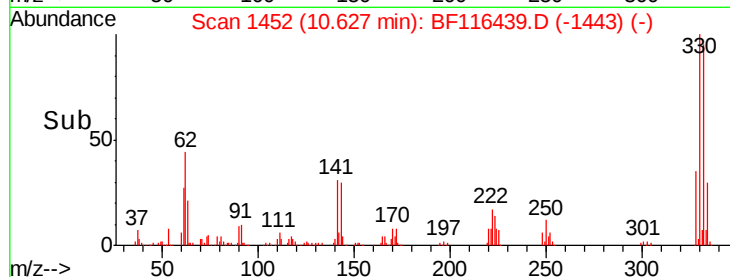
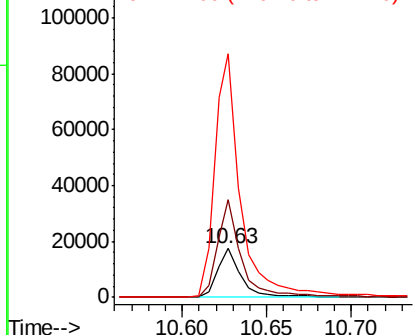



#76
 Chrysene-d12
 Concen: 20.000 ng
 RT: 13.96 min Scan# 2019
 Delta R.T. -0.02 min
 Lab File: BF116439.D
 Acq: 20 Aug 2019 19:31

Tgt Ion:240 Resp: 316651
 Ion Ratio Lower Upper
 240 100
 120 12.1 10.7 16.1
 236 27.1 22.2 33.2

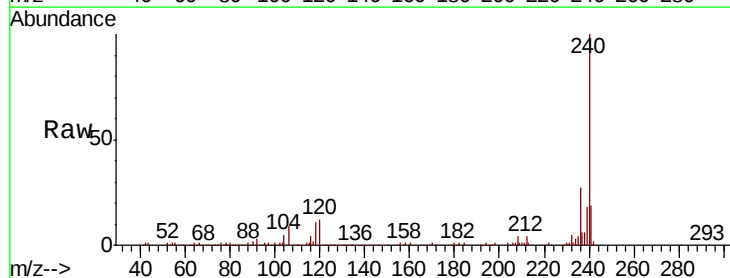

Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E

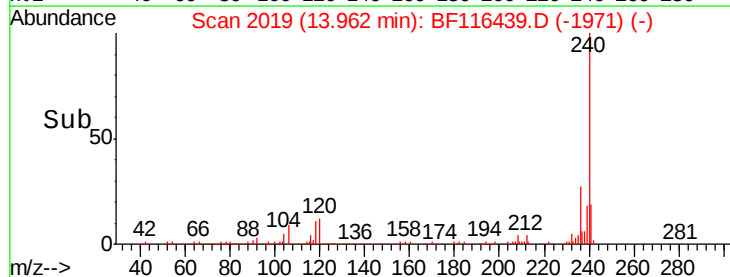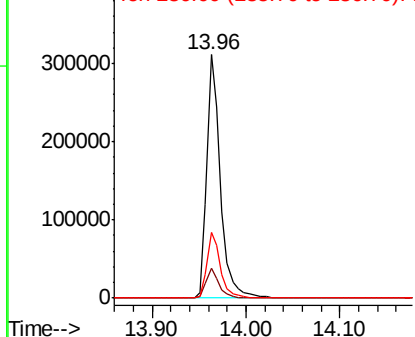

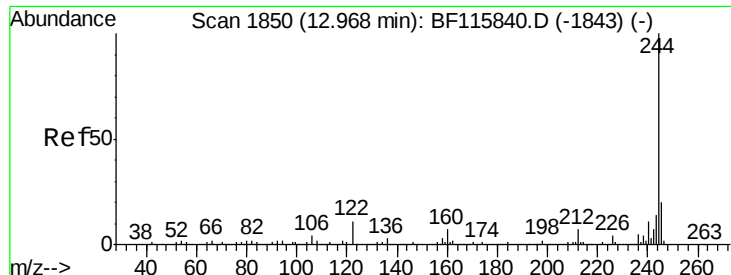

#79

Terphenyl-d14

Concen: 93.042 ng

RT: 12.90 min Scan# 1839

Delta R.T. -0.01 min

Lab File: BF116439.D

Acq: 20 Aug 2019 19:31

Instrument :

BNA_F

ClientSampleId :


Tot Ion:244 Resp: 1398171

Ion Ratio Lower Upper

244 100

212 7.0 5.8 8.8




122 10.7 9.0 13.4



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

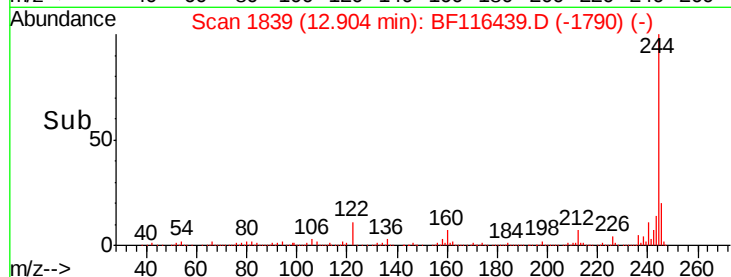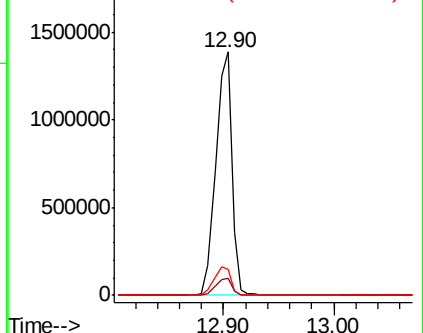

#87

Perylene-d12

Concen: 20.000 ng

RT: 15.42 min Scan# 2267

Delta R.T. -0.02 min

Lab File: BF116439.D

Acq: 20 Aug 2019 19:31


Tgt Ion:264 Resp: 337200

Ion Ratio Lower Upper

264 100

260 23.5 19.7 29.5

265 22.2 17.4 26.0



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

