

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082019\
 Data File : BF116451.D
 Acq On : 21 Aug 2019 00:54
 Operator : HP/JU
 Sample : K4403-20
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 T1-H1-H4-(0-2.5)

Quant Time: Aug 21 07:20:36 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF073019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 19 06:03:31 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.80	152	90160	20.00	ng	-0.01
21) Naphthalene-d8	8.09	136	347482	20.00	ng	-0.01
39) Acenaphthene-d10	9.83	164	187556	20.00	ng	-0.02
64) Phenanthrene-d10	11.32	188	357214	20.00	ng	-0.02
76) Chrysene-d12	13.96	240	315407	20.00	ng	-0.02
87) Perylene-d12	15.42	264	317718	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.44	112	697212	129.46	ng	0.00
7) Phenol-d6	6.45	99	830693	122.25	ng	-0.01
23) Nitrobenzene-d5	7.37	82	637000	105.82	ng	-0.02
42) 2,4,6-Tribromophenol	10.63	330	286892	157.77	ng	-0.02
45) 2-Fluorobiphenyl	9.16	172	1126700	112.52	ng	-0.01
79) Terphenyl-d14	12.90	244	1488450	99.44	ng	-0.01
Target Compounds						
50) Dimethylphthalate	9.56	163	28576	2.238	ng	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082019\
Data File : BF116451.D
Acq On : 21 Aug 2019 00:54
Operator : HP/JU
Sample : K4403-20
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
T1-H1-H4-(0-2.5)

Quant Time: Aug 21 07:20:36 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF073019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 19 06:03:31 2019
Response via : Initial Calibration

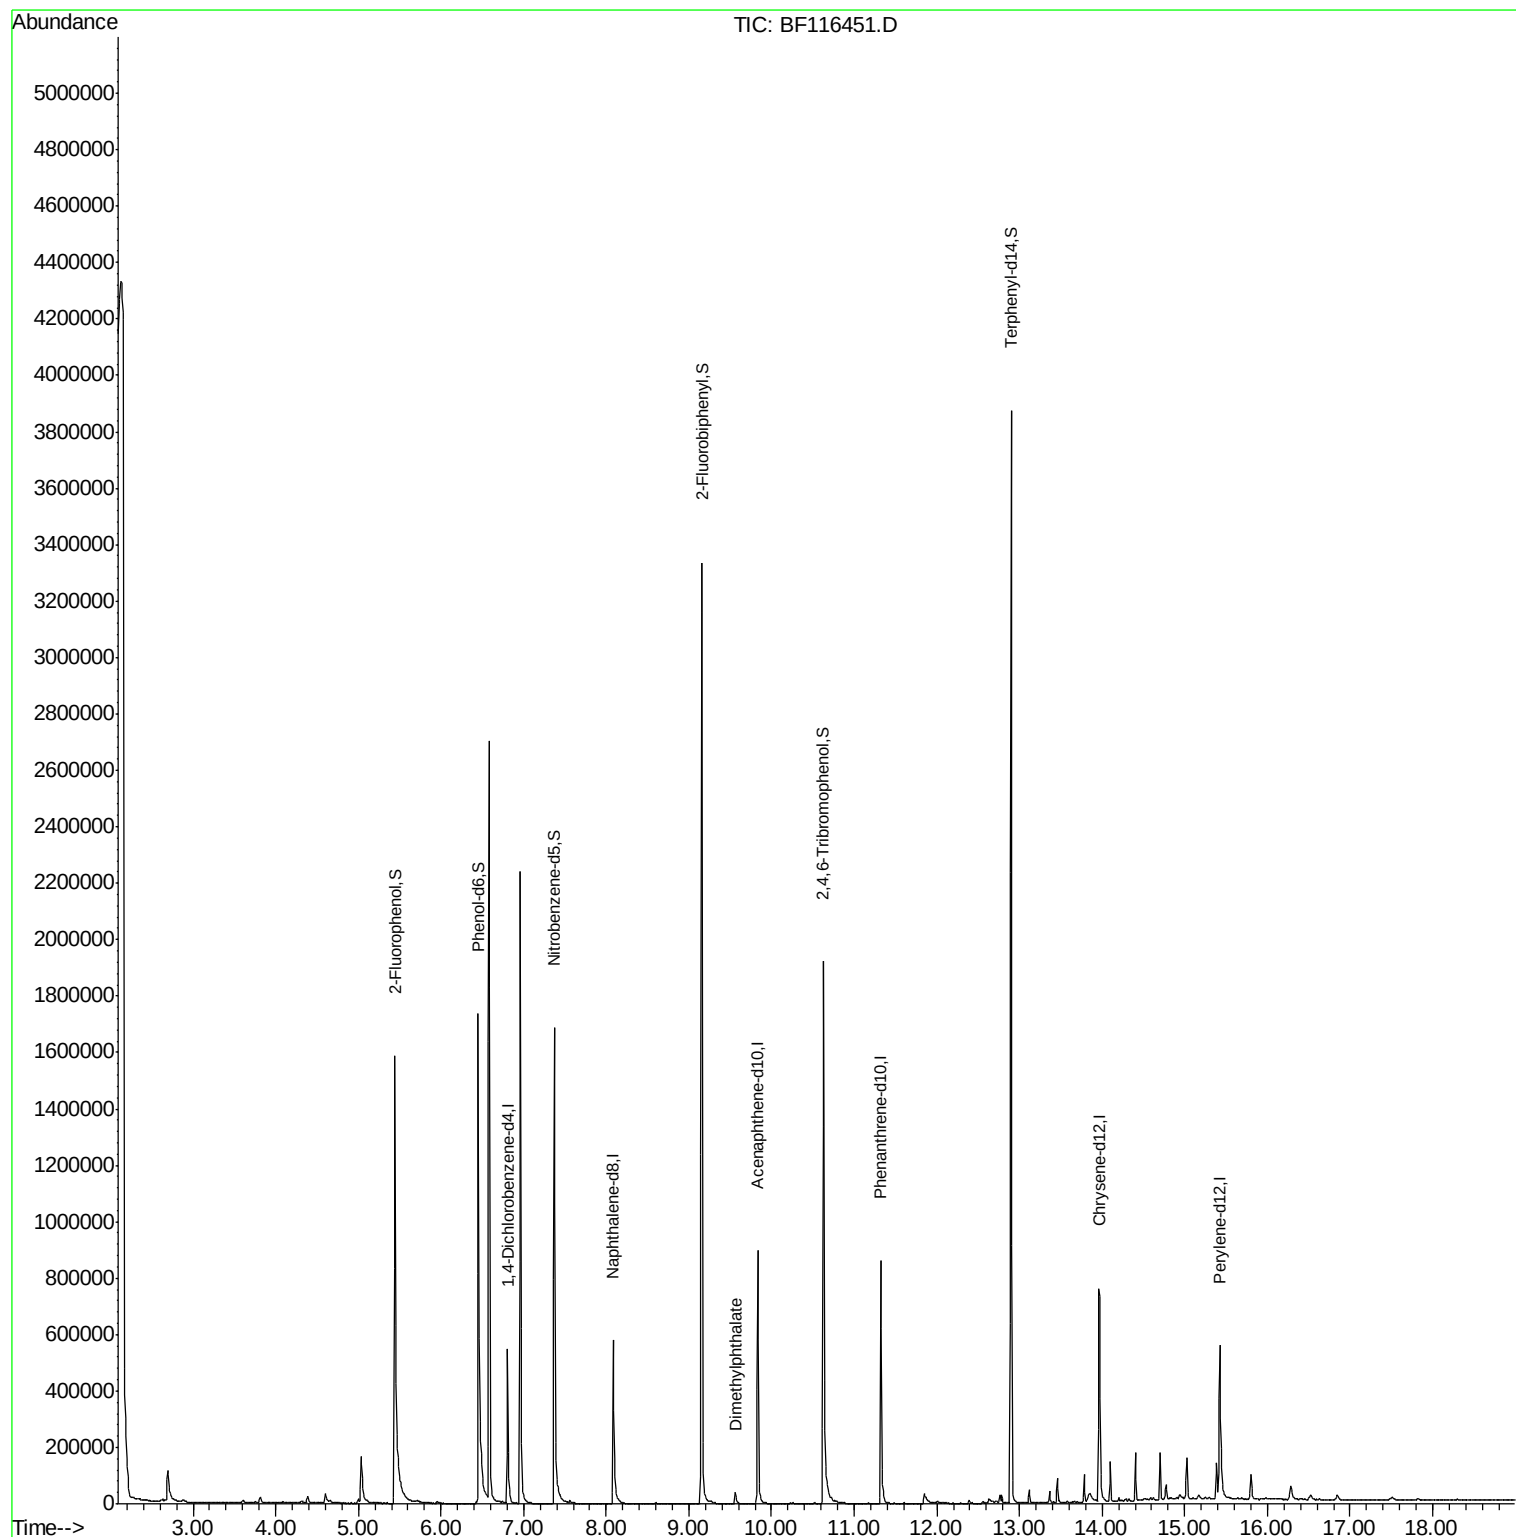

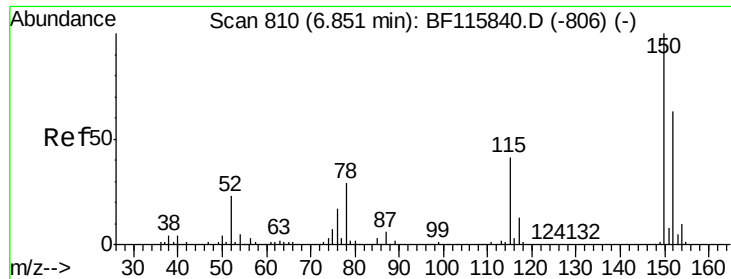


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.80 min Scan# 802
Delta R.T. -0.01 min
Lab File: BF116451.D
Acq: 21 Aug 2019 00:54

Instrument :
BNA_F
ClientSampleId :
T1-H1-H4-(0-2.5)

Tot Ion	Ratio	Lower	Upper
152	100		
150	155.3	126.2	189.2
115	61.6	49.9	74.9



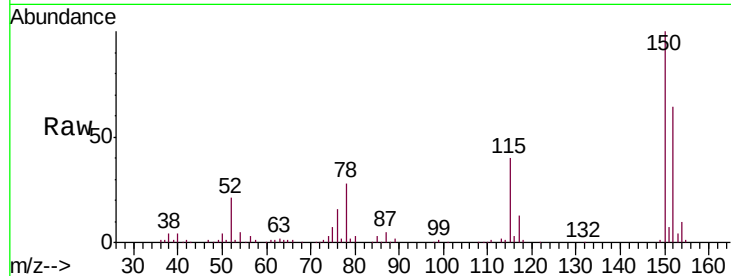


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

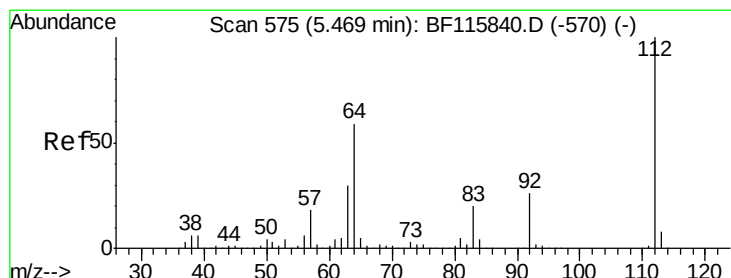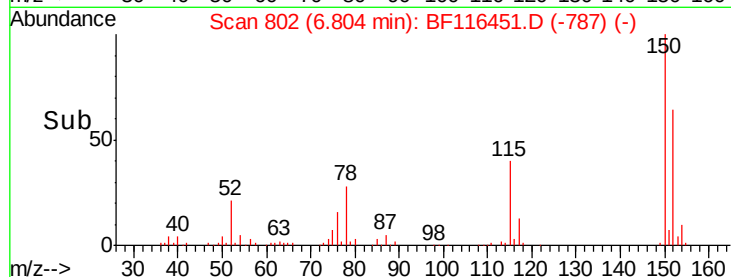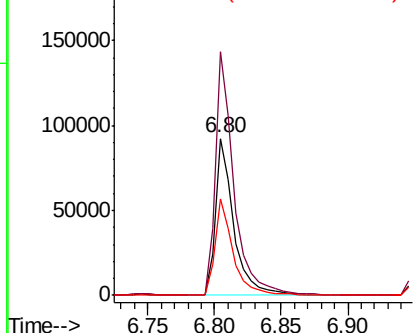

#5

2-Fluorophenol
Concen: 129.456 ng
RT: 5.44 min Scan# 570
Delta R.T. 0.00 min
Lab File: BF116451.D
Acq: 21 Aug 2019 00:54

Tgt Ion	Ratio	Lower	Upper
112	100		
64	56.4	45.4	68.2
63	29.1	23.7	35.5


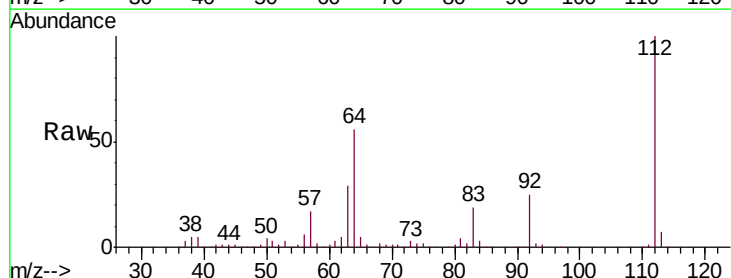



Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF1

Ion 63.00 (62.70 to 63.70): BF1

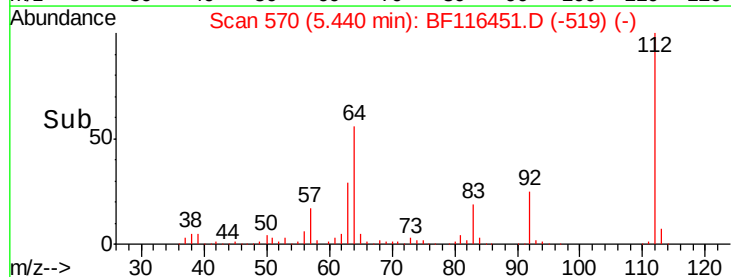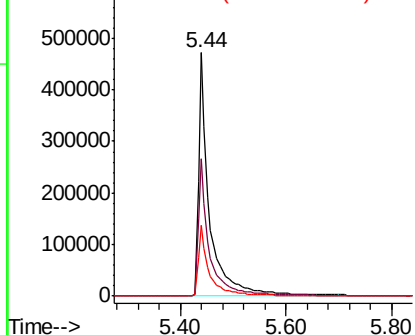



#7

Phenol-d6

Concen: 122.250 ng

RT: 6.45 min Scan# 742

Delta R.T. -0.01 min

Lab File: BF116451.D

Acq: 21 Aug 2019 00:54

Instrument :

BNA_F

ClientSampleId :

T1-H1-H4-(0-2.5)


Tot Ion: 99 Resp: 830693

Ion Ratio Lower Upper




99 100

42 16.9 13.8 20.8

71 33.4 27.3 40.9

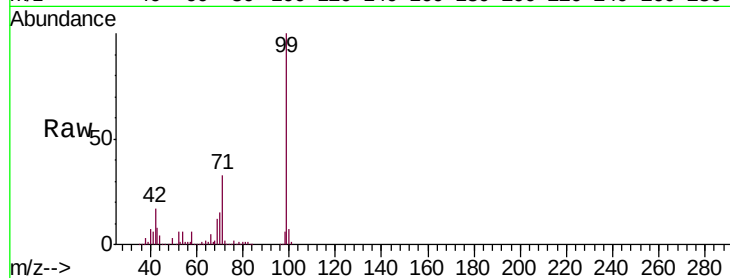

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

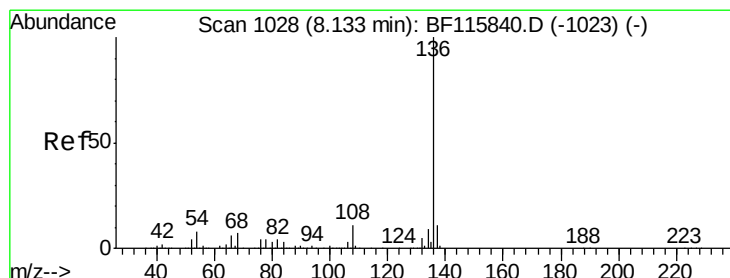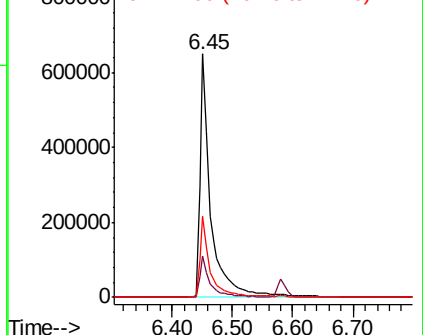

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.09 min Scan# 1020

Delta R.T. -0.01 min

Lab File: BF116451.D

Acq: 21 Aug 2019 00:54

Tgt Ion: 136 Resp: 347482


Ion Ratio Lower Upper

136 100



137 10.7 9.0 13.4


54 6.7 5.8 8.6

68 5.5 5.2 7.8

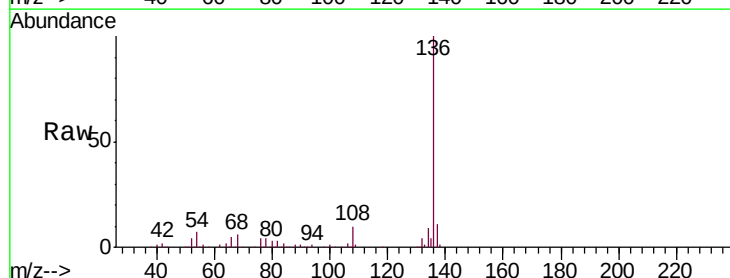

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1



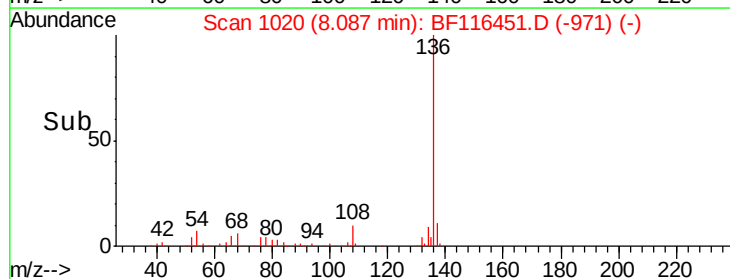
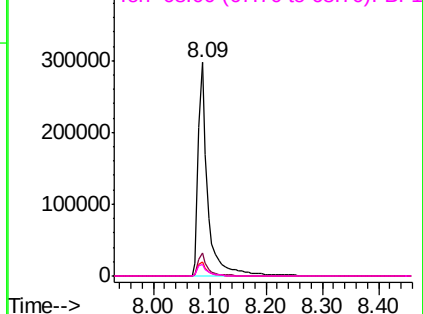




#23
 Nitrobenzene-d5
 Concen: 105.817 ng
 RT: 7.37 min Scan# 898
 Delta R.T. -0.02 min
 Lab File: BF116451.D
 Acq: 21 Aug 2019 00:54




Instrument :
 BNA_F
 ClientSampleId :
 T1-H1-H4-(0-2.5)


Tot Ion: 82 Resp: 637000
 Ion Ratio Lower Upper
 82 100
 128 44.7 36.5 54.7
 54 45.0 36.0 54.0

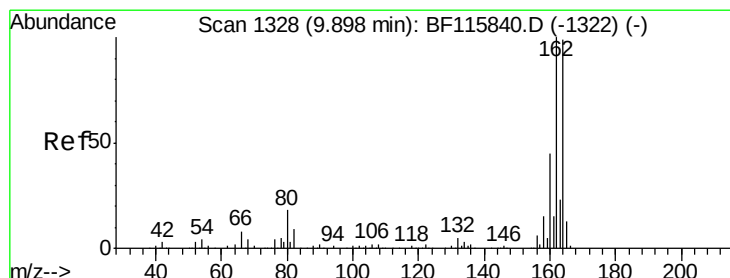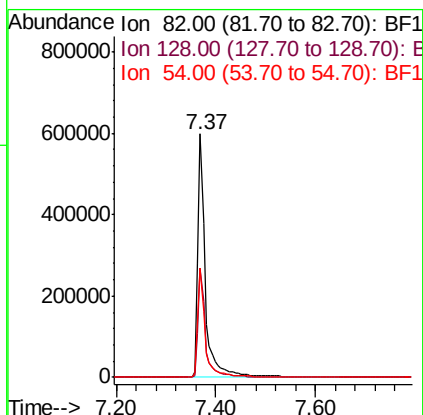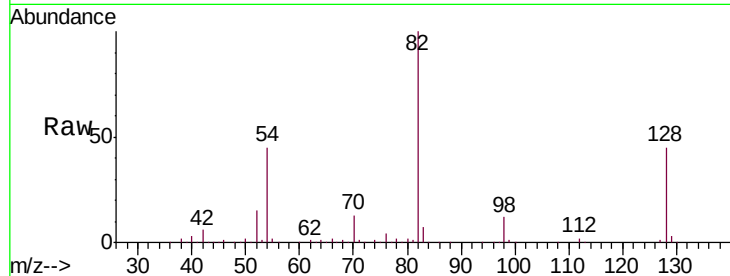

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.83 min Scan# 1317
 Delta R.T. -0.02 min
 Lab File: BF116451.D
 Acq: 21 Aug 2019 00:54

Tgt Ion:164 Resp: 187556
 Ion Ratio Lower Upper
 164 100
 162 101.4 82.6 124.0
 160 45.8 37.6 56.4

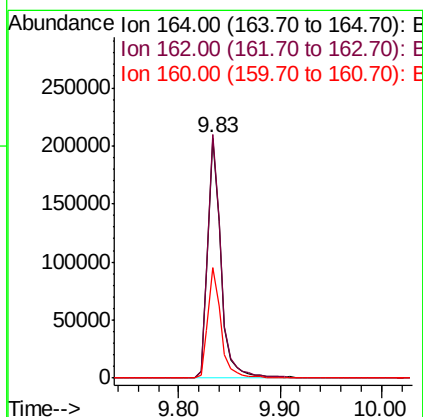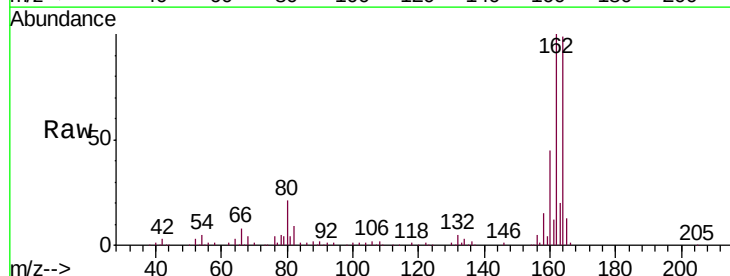



#42

2,4,6-Tribromophenol

Concen: 157.771 ng

RT: 10.63 min Scan# 1452

Delta R.T. -0.02 min

Lab File: BF116451.D

Acq: 21 Aug 2019 00:54

Instrument :

BNA_F

ClientSampleId :

T1-H1-H4-(0-2.5)


Tot Ion:330 Resp: 286892

Ion Ratio Lower Upper

330 100

332 98.1 76.8 115.2




141 34.6 26.3 39.5

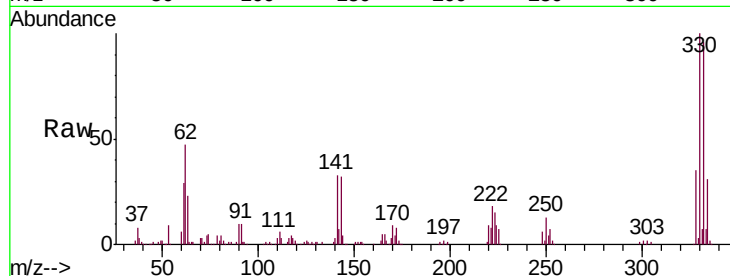

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

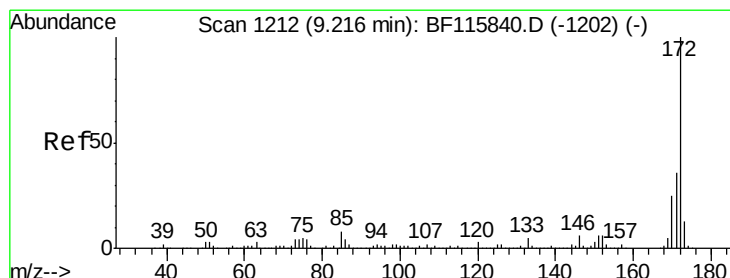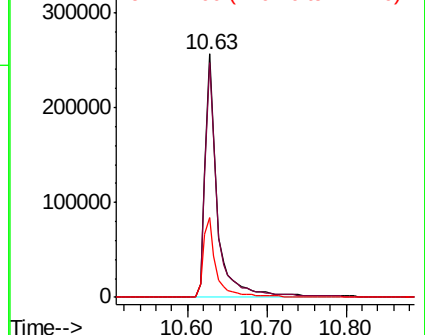

#45

2-Fluorobiphenyl

Concen: 112.521 ng

RT: 9.16 min Scan# 1202

Delta R.T. -0.01 min

Lab File: BF116451.D

Acq: 21 Aug 2019 00:54


Tgt Ion:172 Resp: 1126700

Ion Ratio Lower Upper

172 100

171 36.0 29.6 44.4



170 24.9 20.1 30.1

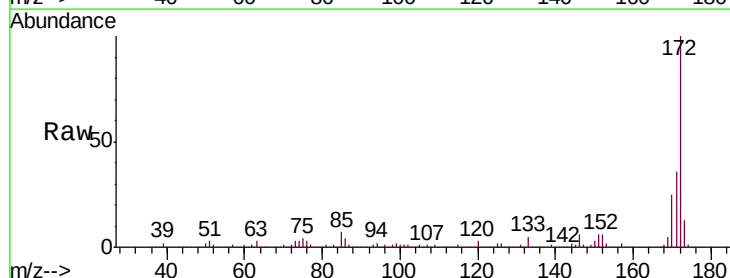


Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

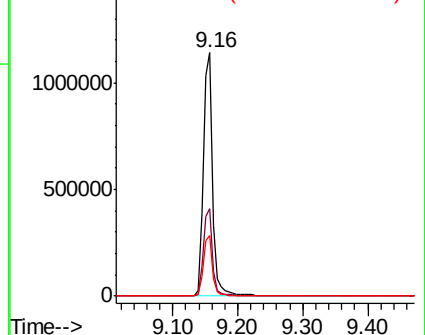

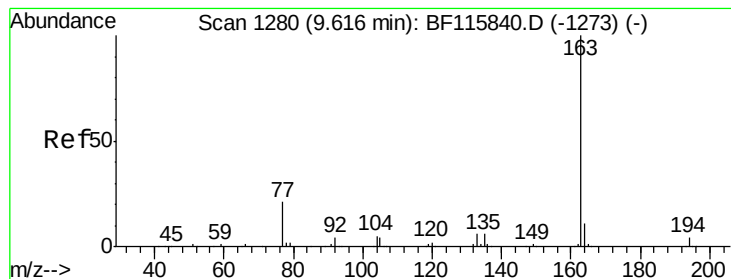

#50

Dimethylphthalate

Concen: 2.238 ng

RT: 9.56 min Scan# 1271

Delta R.T. -0.01 min

Lab File: BF116451.D

Acq: 21 Aug 2019 00:54

Instrument :

BNA_F

ClientSampleId :

T1-H1-H4-(0-2.5)


Tot Ion:163 Resp: 28576

Ion Ratio Lower Upper




163 100

194 3.6 3.0 4.6

164 10.4 8.4 12.6

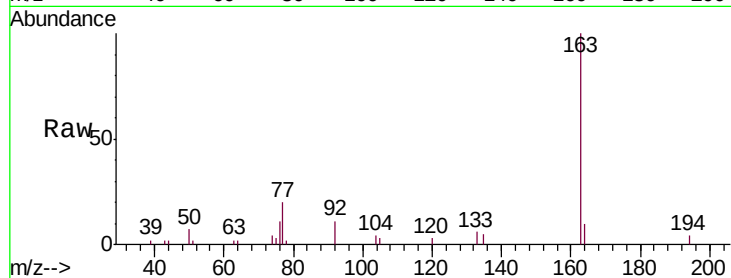

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

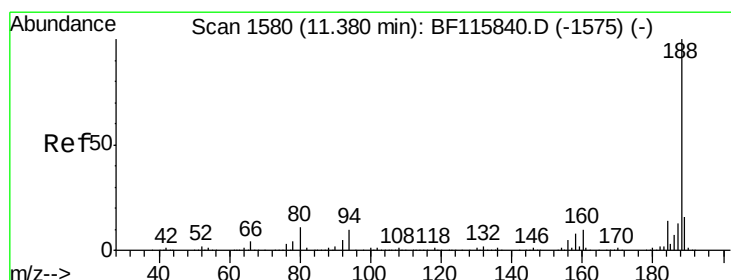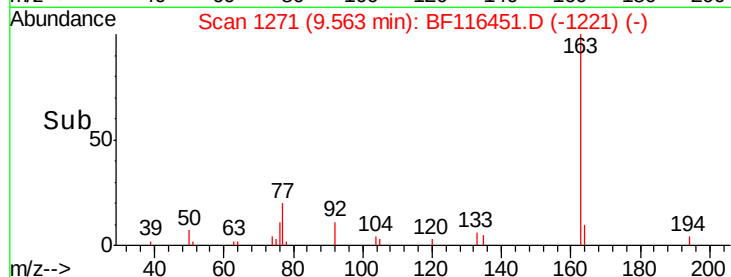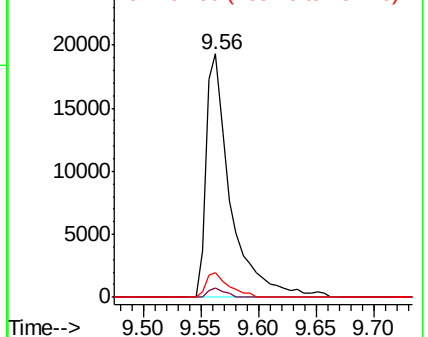

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.32 min Scan# 1570

Delta R.T. -0.02 min

Lab File: BF116451.D

Acq: 21 Aug 2019 00:54


Tgt Ion:188 Resp: 357214

Ion Ratio Lower Upper



188 100


94 10.0 8.1 12.1

80 10.8 8.7 13.1

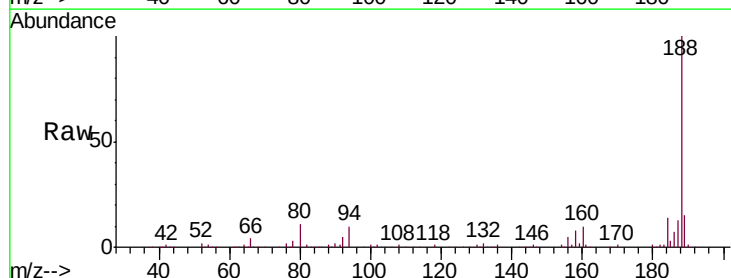

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1

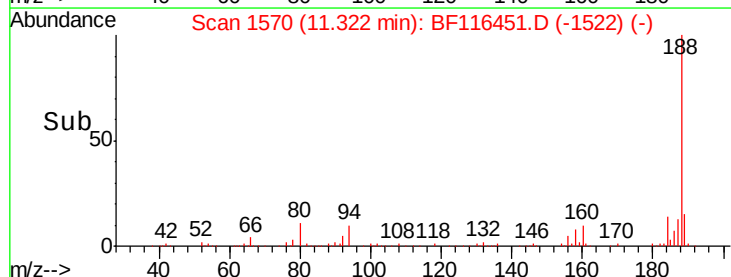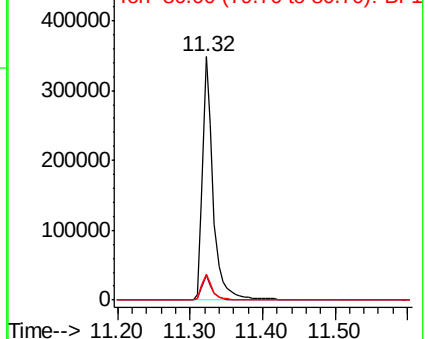



#76

Chrysene-d12

Concen: 20.000 ng

RT: 13.96 min Scan# 2019

Delta R.T. -0.02 min

Lab File: BF116451.D

Acq: 21 Aug 2019 00:54

Instrument :

BNA_F

ClientSampleId :

T1-H1-H4-(0-2.5)


Tot Ion:240 Resp: 315407

Ion Ratio Lower Upper

240 100

120 12.4 10.7 16.1




236 26.9 22.2 33.2

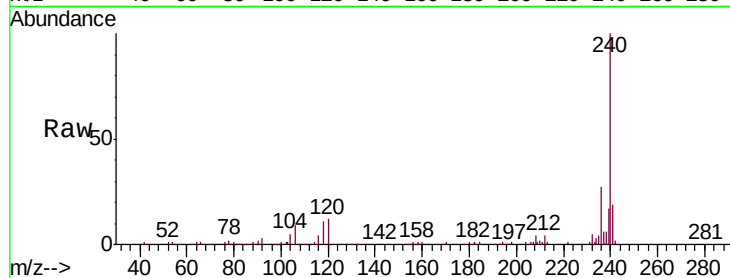

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

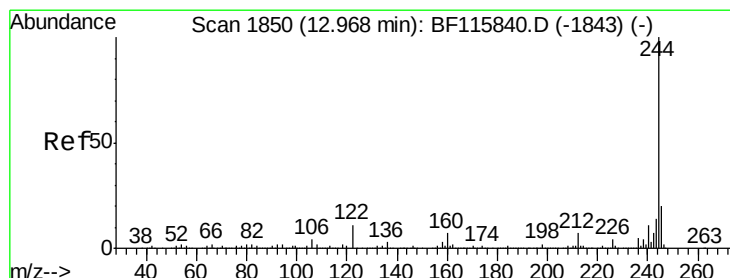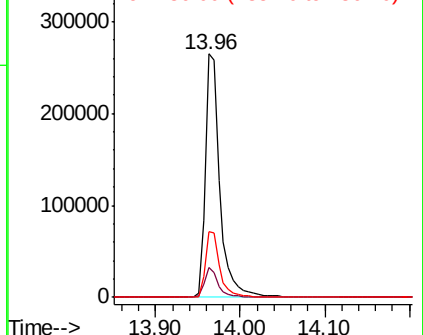

#79

Terphenyl-d14

Concen: 99.440 ng

RT: 12.90 min Scan# 1839

Delta R.T. -0.01 min

Lab File: BF116451.D

Acq: 21 Aug 2019 00:54


Tgt Ion:244 Resp: 1488450

Ion Ratio Lower Upper

244 100

212 7.2 5.8 8.8



122 10.9 9.0 13.4

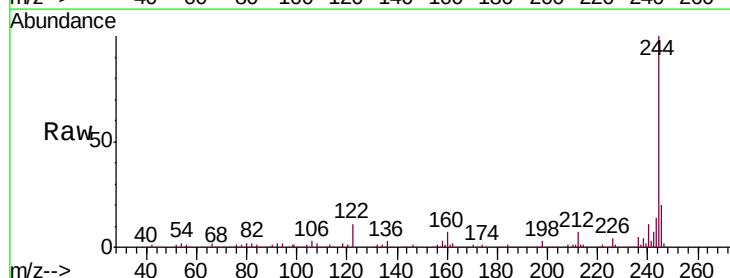


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

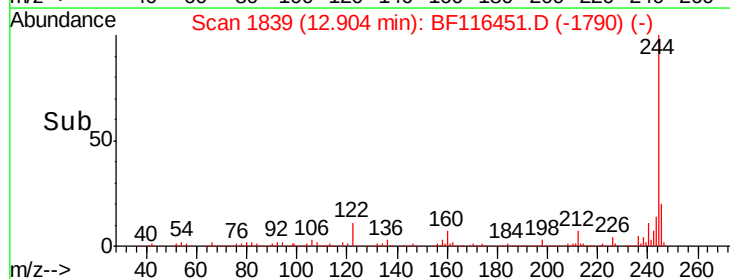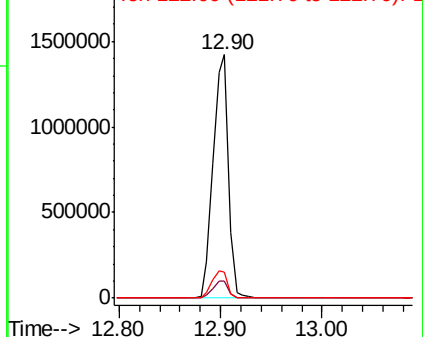


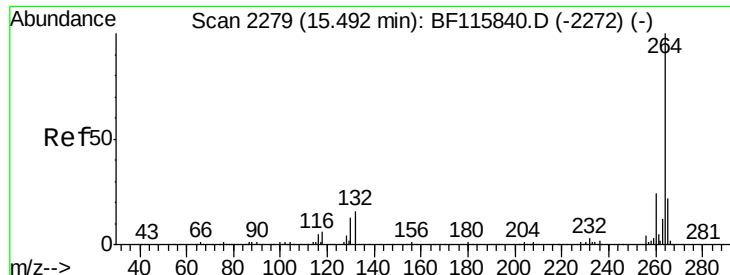

#87
Pervlene-d12
Concen: 20.000 ng
RT: 15.42 min Scan# 2267
Delta R.T. -0.02 min
Lab File: BF116451.D
Acq: 21 Aug 2019 00:54

Instrument :
BNA_F
ClientSampleId :
T1-H1-H4-(0-2.5)

Tot Ion	Ratio	Lower	Upper
264	100		
260	24.2	19.7	29.5
265	22.2	17.4	26.0

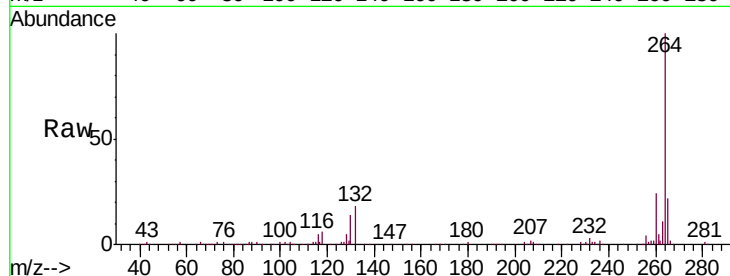

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

