

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082019\
 Data File : BF116454.D
 Acq On : 21 Aug 2019 2:15
 Operator : HP/JU
 Sample : K4354-01 10X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PX-01-081319

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF073019.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.487	575	578	602	rBV2	22201	97010	10.15%	1.483%
2	6.492	746	749	765	rBV	40443	129436	13.54%	1.979%
3	6.604	765	768	780	rVB	94500	166650	17.43%	2.548%
4	6.804	799	802	819	rBV	468395	471884	49.35%	7.215%
5	6.963	826	829	848	rVB	102573	135588	14.18%	2.073%
6	7.404	901	904	920	rBV2	28083	83136	8.70%	1.271%
7	8.086	1017	1020	1035	rBV	563482	654066	68.41%	10.001%
8	9.157	1199	1202	1213	rBV	178419	190209	19.89%	2.908%
9	9.563	1266	1271	1279	rBV	16168	22804	2.39%	0.349%
10	9.833	1314	1317	1331	rBV	902366	818490	85.61%	12.515%
11	10.639	1452	1454	1466	rBV	53721	89261	9.34%	1.365%
12	11.322	1567	1570	1581	rBV	931841	948511	99.20%	14.503%
13	11.416	1583	1586	1592	rVB	9166	13206	1.38%	0.202%
14	11.869	1660	1663	1669	rVB	12183	13104	1.37%	0.200%
15	11.945	1673	1676	1678	rBV	10494	10768	1.13%	0.165%
16	12.380	1747	1750	1752	rBV2	16140	17130	1.79%	0.262%
17	12.404	1752	1754	1757	rVB3	20898	16674	1.74%	0.255%
18	12.545	1775	1778	1791	rBV	108118	117992	12.34%	1.804%
19	12.774	1810	1817	1823	rBV	96337	128470	13.44%	1.964%
20	12.827	1823	1826	1831	rVB2	7959	11279	1.18%	0.172%
21	12.898	1834	1838	1846	rVV	294390	268795	28.11%	4.110%
22	12.992	1850	1854	1859	rVB2	8178	11617	1.22%	0.178%
23	13.104	1870	1873	1878	rVB2	12967	16481	1.72%	0.252%
24	13.210	1888	1891	1897	rVV4	8975	12863	1.35%	0.197%
25	13.745	1977	1982	1985	rVB4	13070	16248	1.70%	0.248%
26	13.786	1985	1989	1991	rBV	12414	13577	1.42%	0.208%
27	13.963	2015	2019	2035	rBV	871231	956113	100.00%	14.619%
28	14.363	2085	2087	2091	rVV	10128	10831	1.13%	0.166%
29	14.404	2091	2094	2097	rVB	21067	20726	2.17%	0.317%
30	14.698	2141	2144	2147	rBV	25764	31801	3.33%	0.486%
31	15.021	2194	2199	2209	rBV2	62939	117524	12.29%	1.797%
32	15.315	2245	2249	2253	rBV	24628	33297	3.48%	0.509%
33	15.380	2256	2260	2263	rVV2	52581	82742	8.65%	1.265%
34	15.421	2263	2267	2281	rVB	524151	747081	78.14%	11.423%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082019\
Data File : BF116454.D
Acq On : 21 Aug 2019 2:15
Operator : HP/JU
Sample : K4354-01 10X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PX-01-081319

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF073019.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	15.804	2329	2332	2336	rVB2	28260	38548	4.03%	0.589%
36	16.280	2410	2413	2420	rBV4	15417	26273	2.75%	0.402%


Sum of corrected areas: 6540185

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082019\
Data File : BF116454.D
Acq On : 21 Aug 2019 2:15
Operator : HP/JU
Sample : K4354-01 10X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PX-01-081319

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF073019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

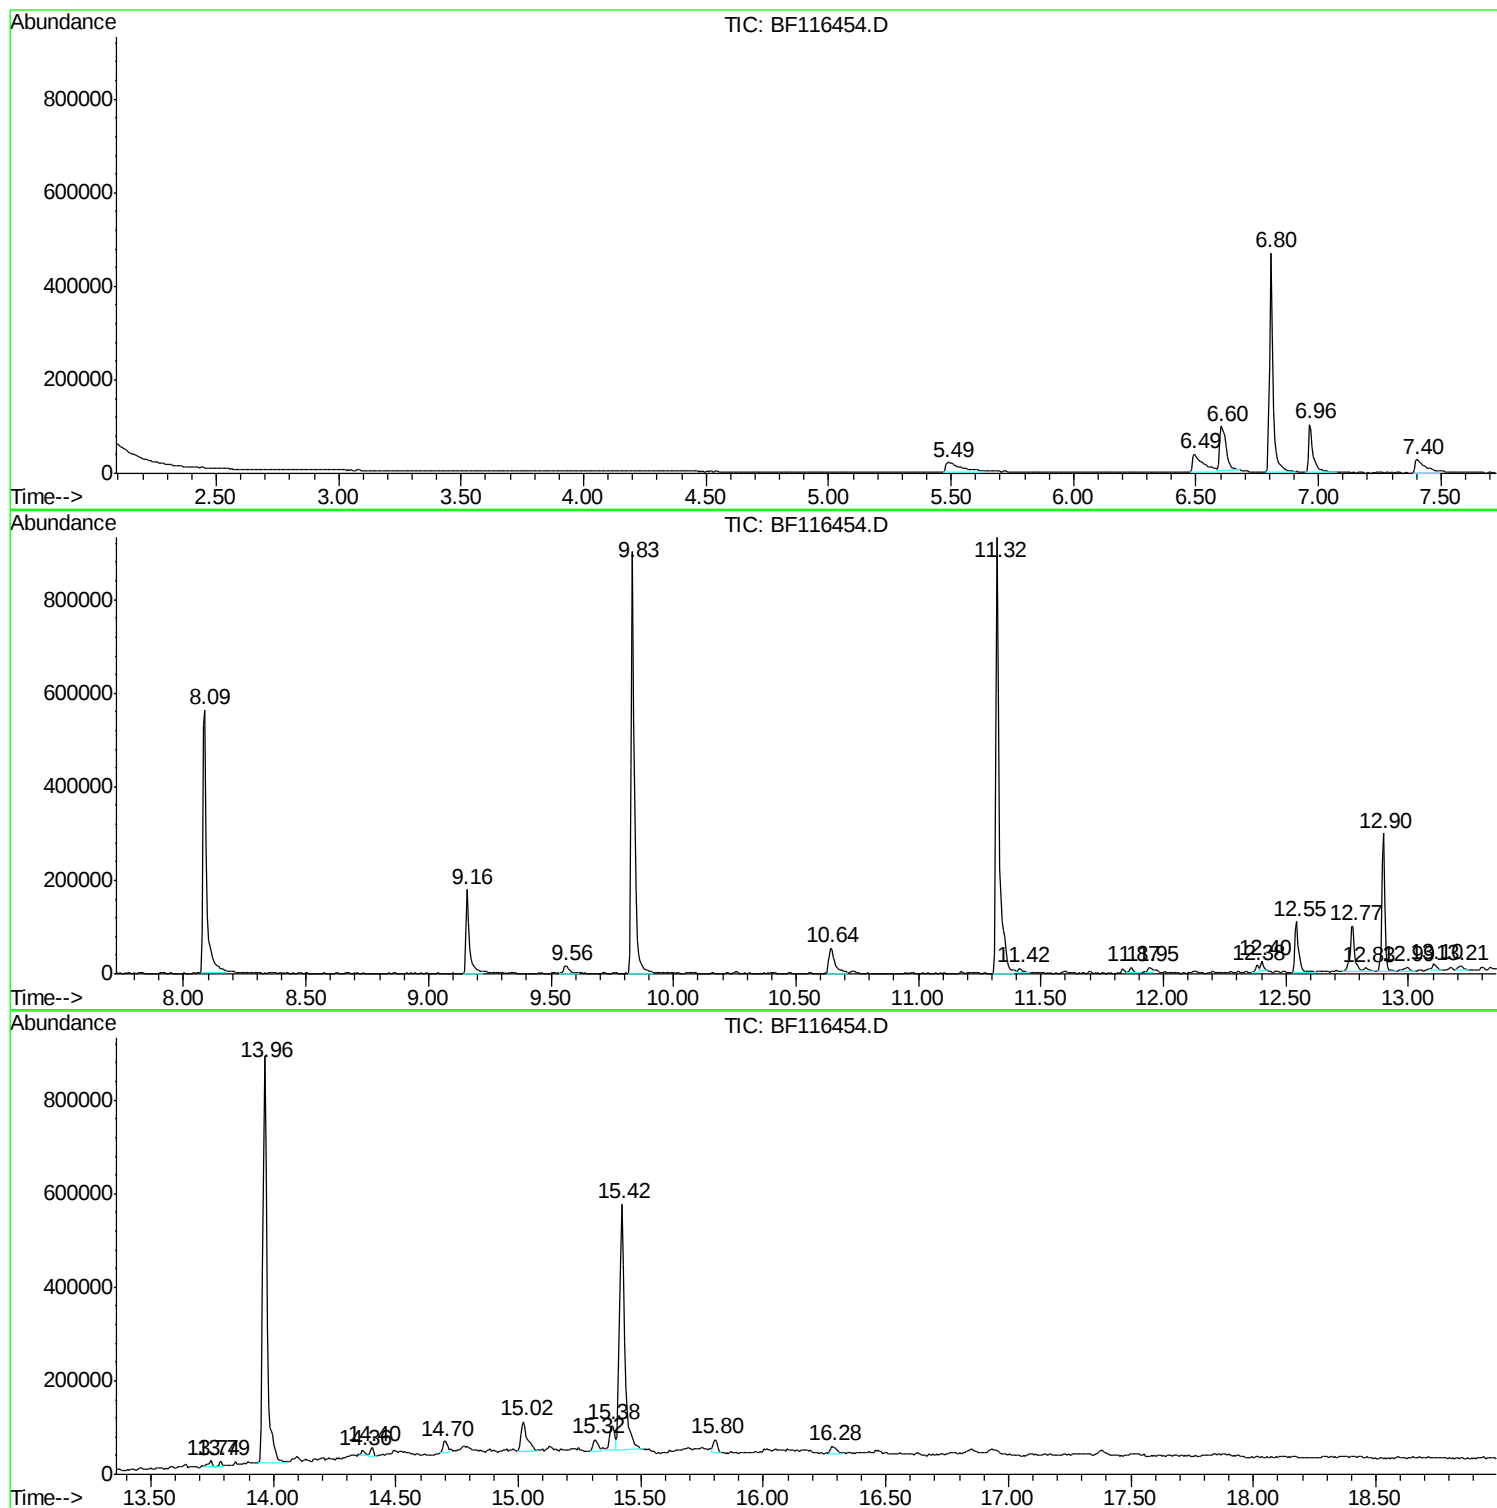

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082019\
Data File : BF116454.D
Acq On : 21 Aug 2019 2:15
Operator : HP/JU
Sample : K4354-01 10X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PX-01-081319










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF073019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.60 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.60	7.06 ng	166650	1,4-Dichlorobenzene-d4	6.80

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	22
2			5-Aminoindole	132	C8H8N2	005192-03-0	10
3			5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9
4			(5-Methyl-2-pyridyl)acetonitrile	132	C8H8N2	1000241-93-9	9
5			2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9

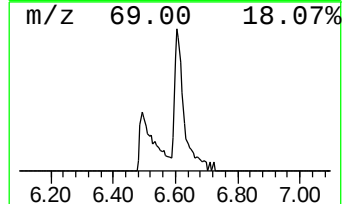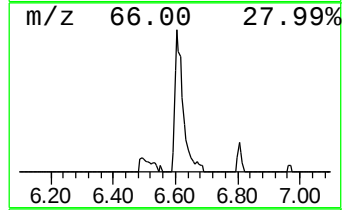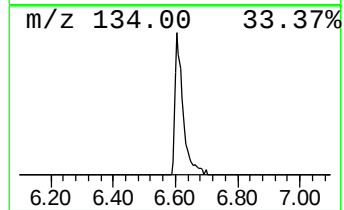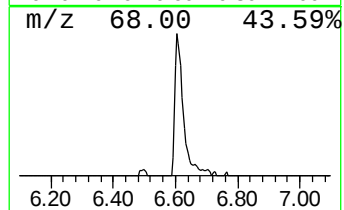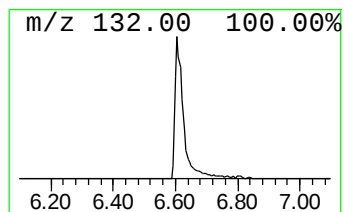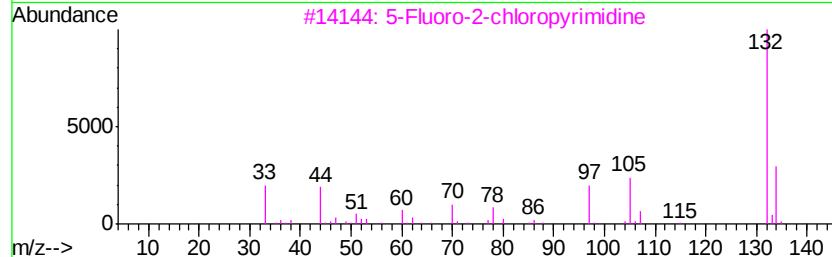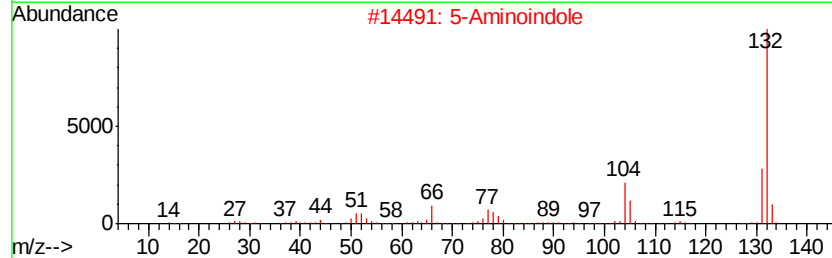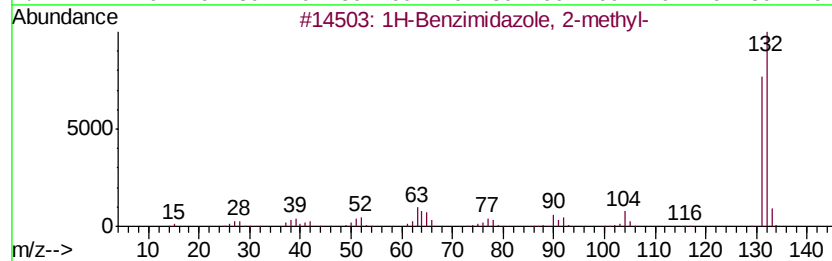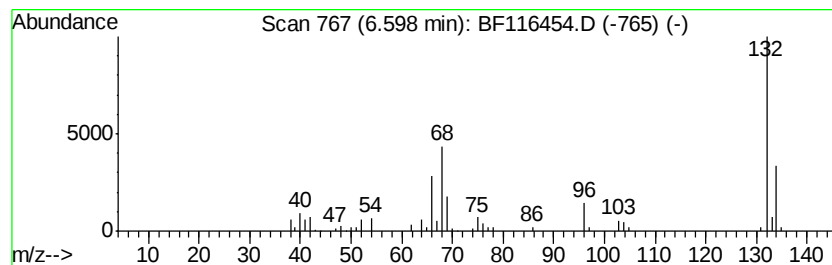

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082019\
Data File : BF116454.D
Acq On : 21 Aug 2019 2:15
Operator : HP/JU
Sample : K4354-01 10X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PX-01-081319

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF073019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.60	6.60	7.1	ng	166650	1	6.80	471884	20.0