


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082019\
 Data File : BF116419.D
 Acq On : 20 Aug 2019 8:06
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF073019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 19 06:03:31 2019

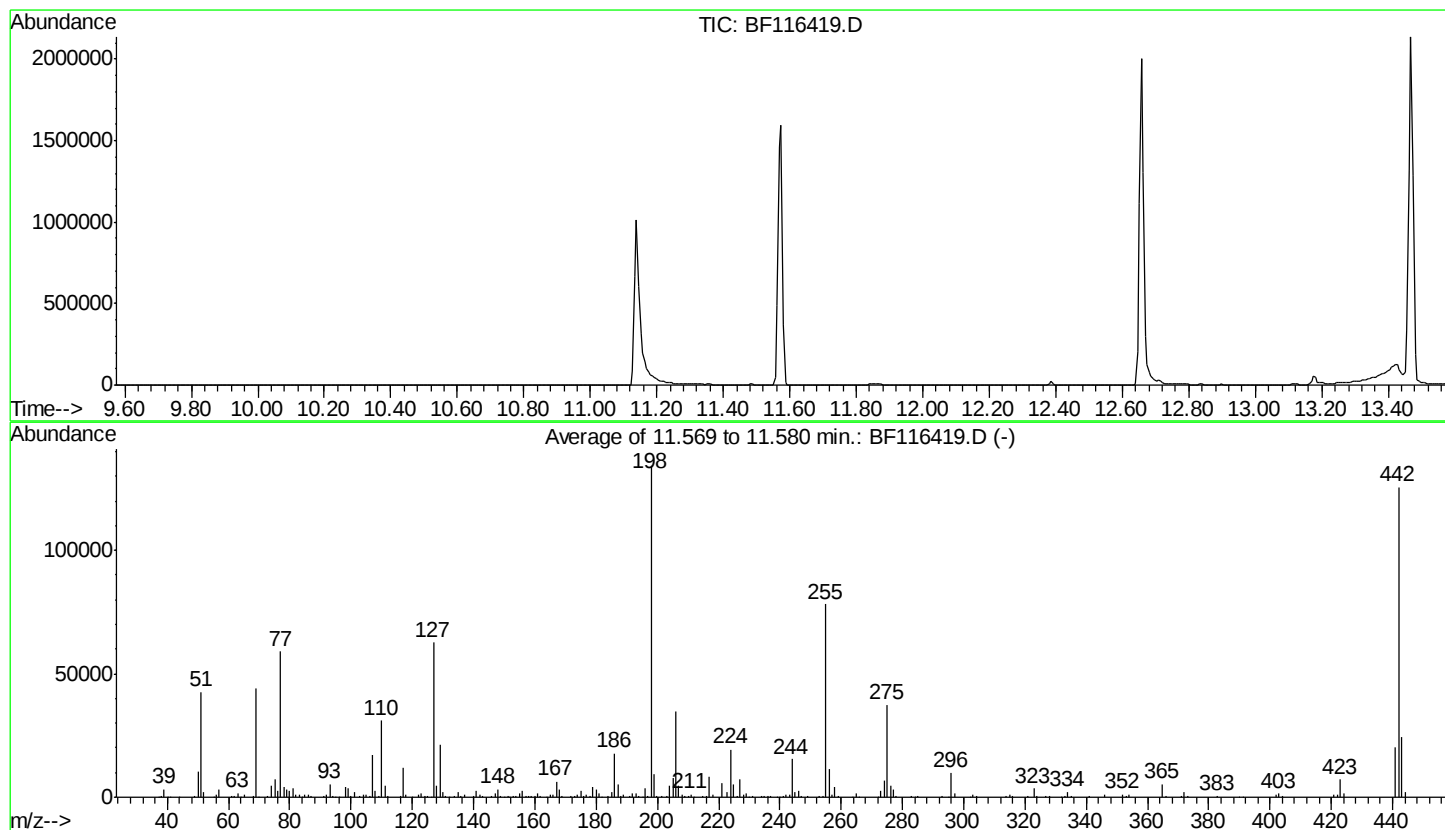

AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.7	42557	PASS
68	69	0.00	2	1.4	625	PASS
69	198	0.00	100	32.8	44039	PASS
70	69	0.00	2	0.5	226	PASS
127	198	10	80	46.5	62507	PASS
197	198	0.00	2	0.5	659	PASS
198	198	100	100	100.0	134330	PASS
199	198	5	9	6.9	9297	PASS
275	198	10	60	27.8	37338	PASS
365	198	1	100	3.9	5268	PASS
441	198	0.01	100	15.2	20391	PASS
442	198	50	100	93.6	125741	PASS
443	442	15	24	19.3	24320	PASS