
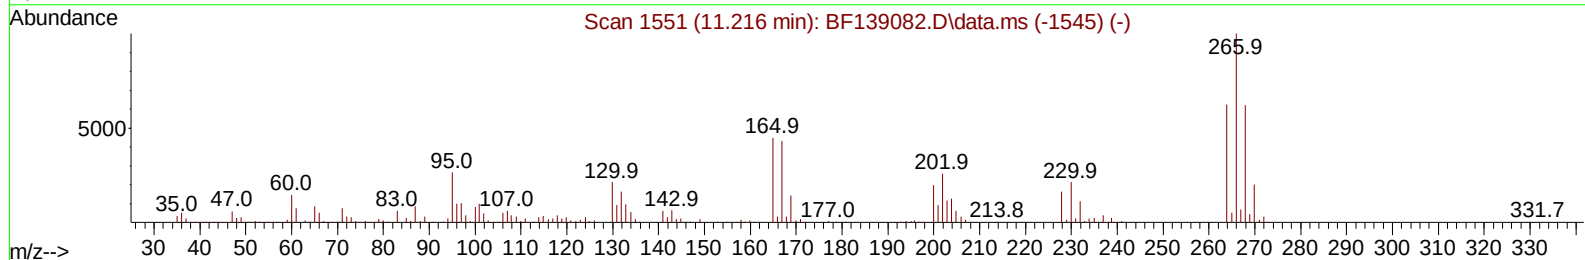
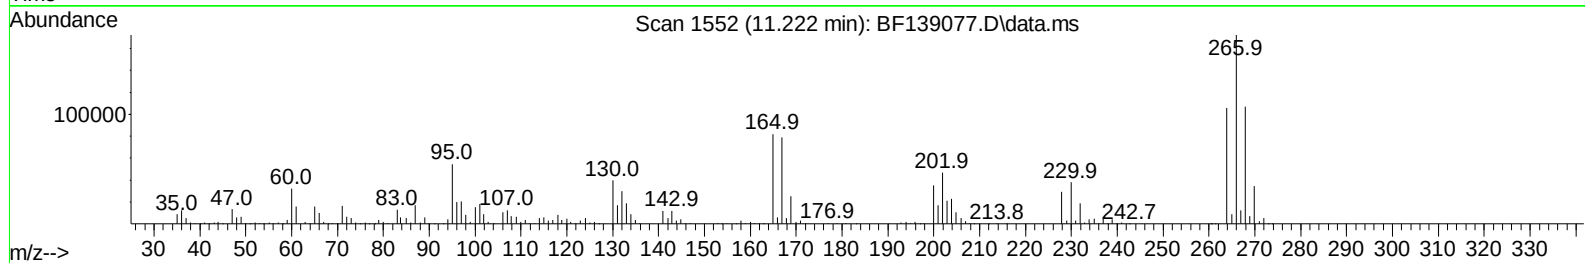


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082024\
Data File : BF139077.D
Acq On : 20 Aug 2024 16:39
Operator : RC/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 21 01:32:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 21 01:25:05 2024
Response via : Initial Calibration

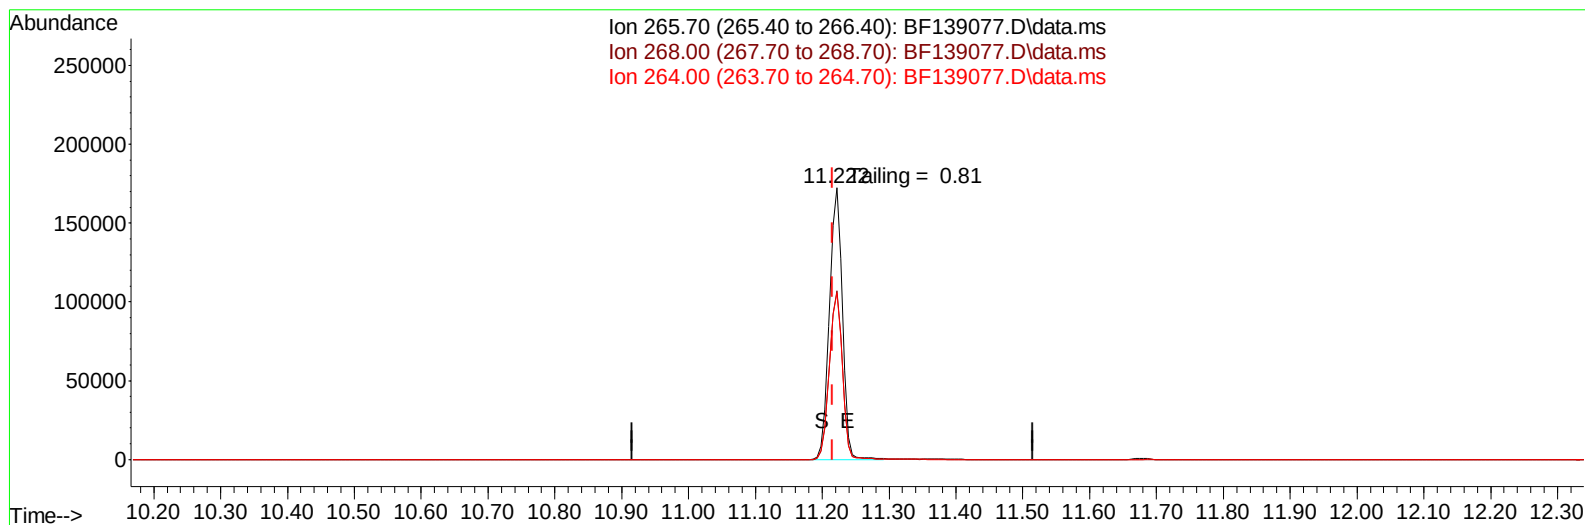

TIC: BF139077.D\data.ms




(70) Pentachlorophenol (C)

11.222min (+ 0.006) 19410.97 ng

response 232437

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.90	62.12
264.00	62.50	61.53
0.00	0.00	0.00

Quant Time: Aug 21 01:32:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 21 01:25:05 2024
Response via : Initial Calibration

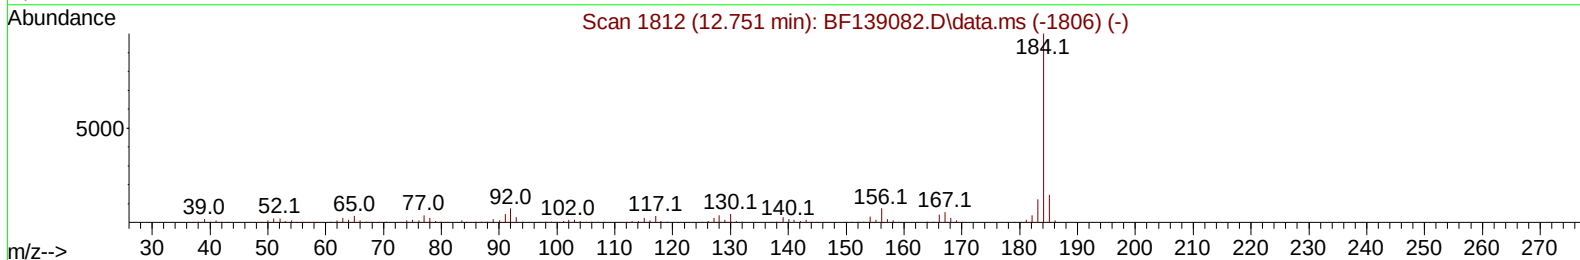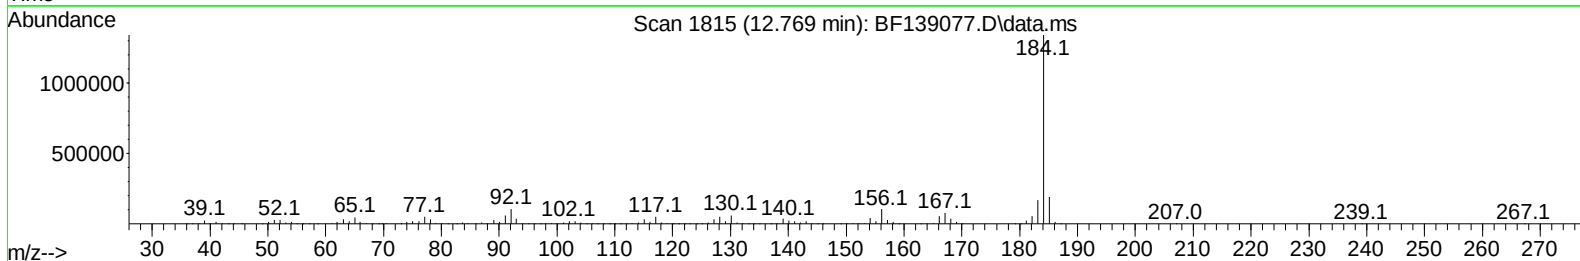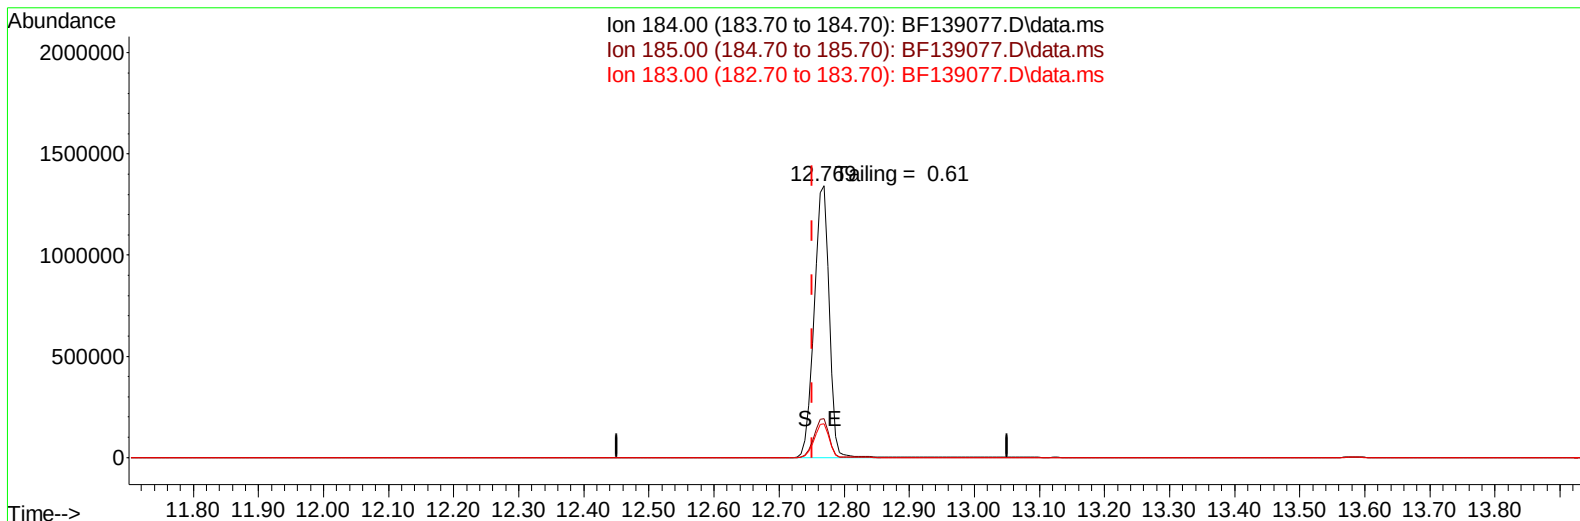

TIC: BF139077.D\data.ms

(77) Benzidine

12.769min (+ 0.018) 0.00 ng

response **2156347**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.24
183.00	12.20	12.45
0.00	0.00	0.00