

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082118\
 Data File : BF108327.D
 Acq On : 21 Aug 2018 9:57
 Operator : JU/SJ
 Sample : J4500-12
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP-6

Quant Time: Aug 21 11:40:46 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 12:24:24 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.01	152	172142	20.00	ng	0.00
21) Naphthalene-d8	8.29	136	638646	20.00	ng	-0.01
38) Acenaphthene-d10	10.05	164	328004	20.00	ng	-0.02
63) Phenanthrene-d10	11.55	188	682399	20.00	ng	-0.01
75) Chrysene-d12	14.20	240	541185	20.00	ng	-0.02
86) Perylene-d12	15.76	264	338665	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.65	112	1279636	134.58	ng	0.02
7) Phenol-d6	6.64	99	1540153	121.89	ng	0.00
23) Nitrobenzene-d5	7.57	82	1248738	109.11	ng	0.00
41) 2,4,6-Tribromophenol	10.85	330	598336	182.88	ng	-0.01
44) 2-Fluorobiphenyl	9.37	172	2196565	107.51	ng	-0.01
78) Terphenyl-d14	13.14	244	2644097	124.22	ng	0.00


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082118\
Data File : BF108327.D
Acq On : 21 Aug 2018 9:57
Operator : JU/SJ
Sample : J4500-12
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-6

Quant Time: Aug 21 11:40:46 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 08 12:24:24 2018
Response via : Initial Calibration

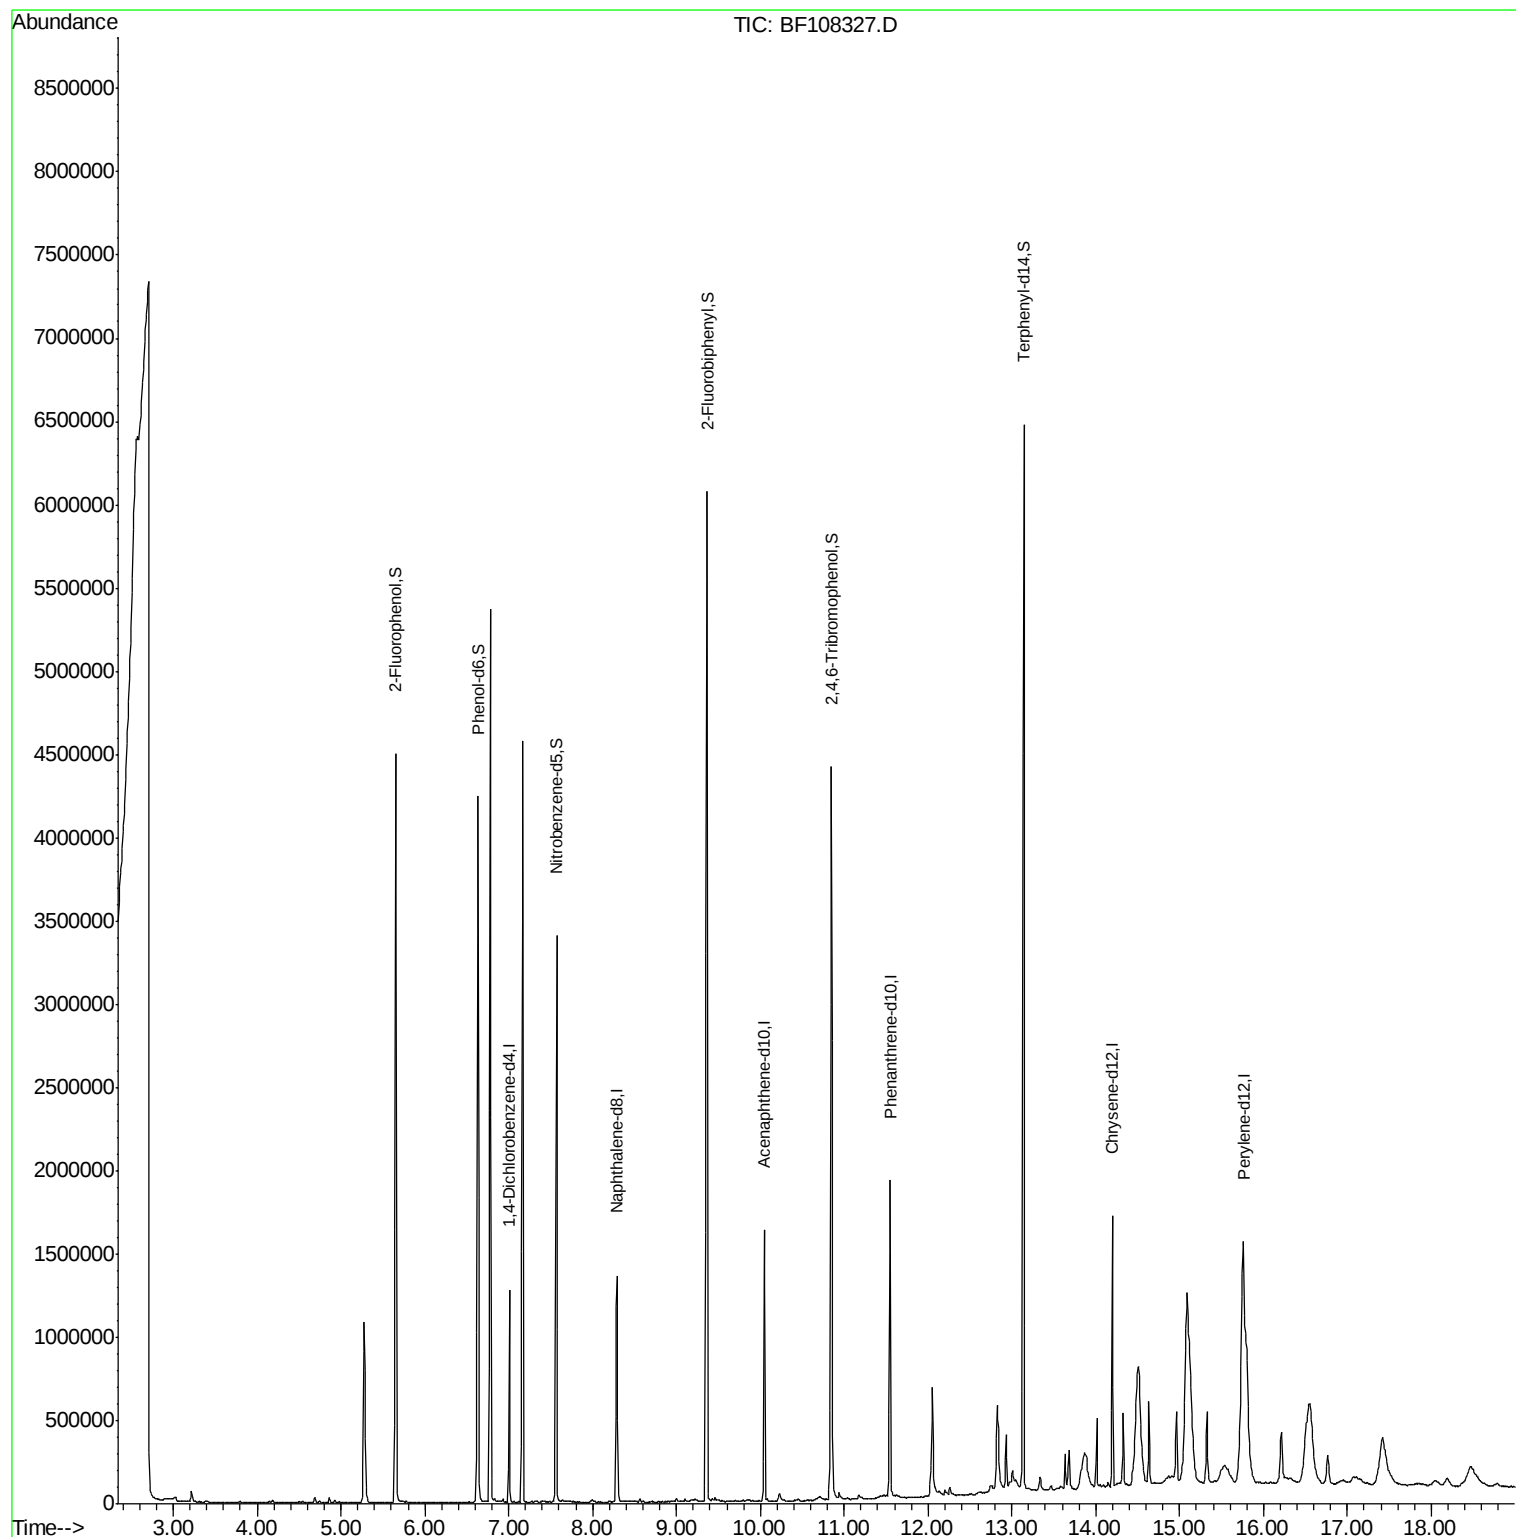




#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.01 min Scan# 794
Delta R.T. -0.01 min
Lab File: BF108327.D
Acq: 21 Aug 2018 9:57

Instrument :
BNA_F
ClientSampleId :
TP-6

Tot Ion:152 Resp: 172142
Ion Ratio Lower Upper
152 100
150 156.3 124.6 186.8
115 58.7 50.1 75.1

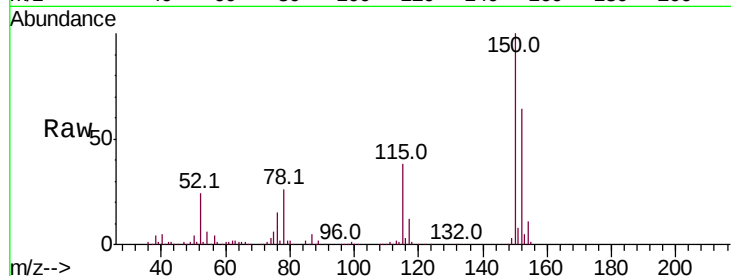


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

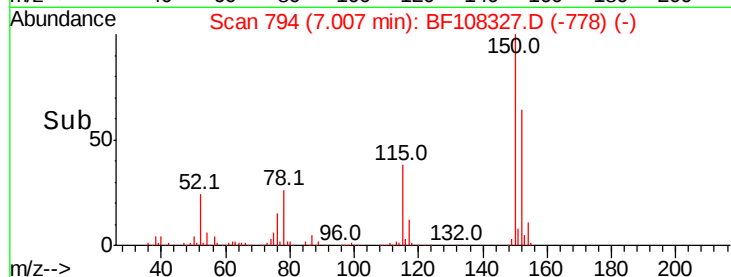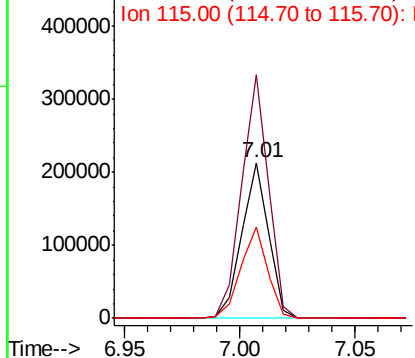



#5

2-Fluorophenol
Concen: 134.582 ng
RT: 5.65 min Scan# 564
Delta R.T. 0.02 min
Lab File: BF108327.D
Acq: 21 Aug 2018 9:57

Tgt Ion:112 Resp: 1279636
Ion Ratio Lower Upper
112 100
64 71.1 47.9 71.9
63 37.8 23.7 35.5#

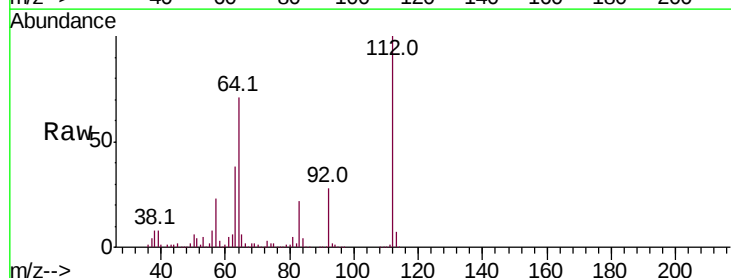

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

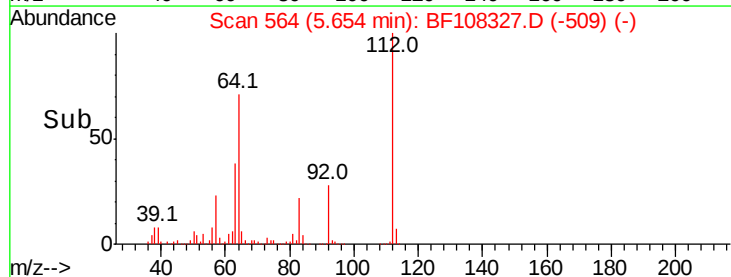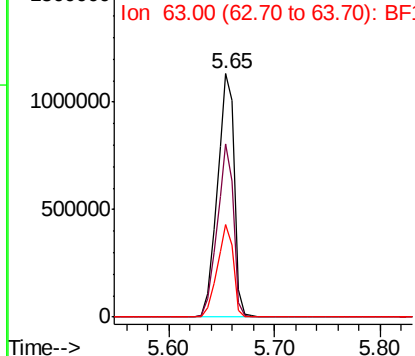



#7

Phenol-d6

Concen: 121.894 ng

RT: 6.64 min Scan# 731

Delta R.T. 0.01 min

Lab File: BF108327.D

Acq: 21 Aug 2018 9:57

Instrument :


BNA_F

ClientSampleId :




TP-6

Tot Ion: 99 Resp: 1540153

Ion	Ratio	Lower	Upper
99	100		
42	22.5	14.5	21.7#
71	37.7	25.4	38.0

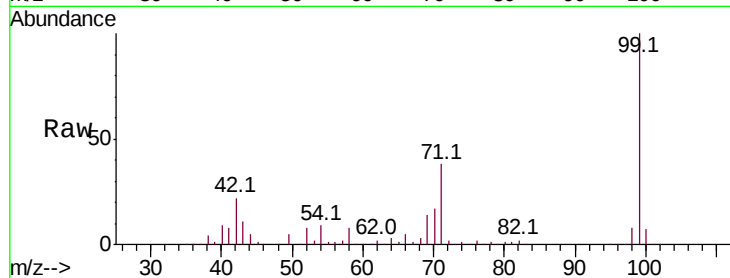

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

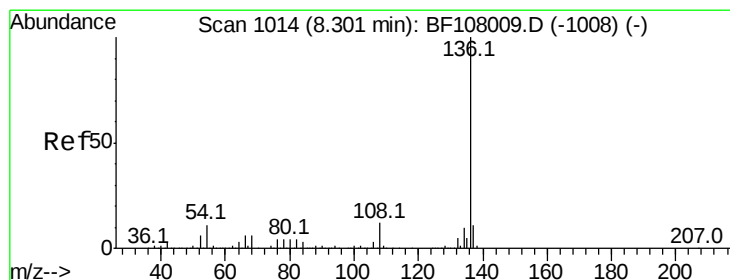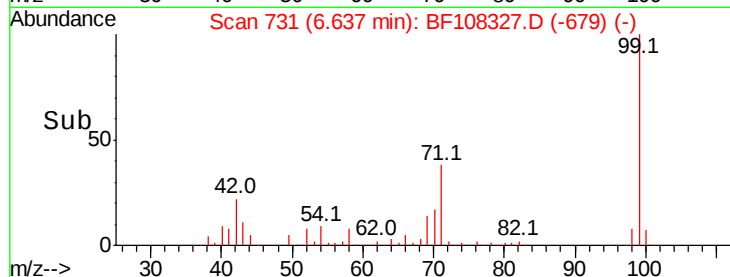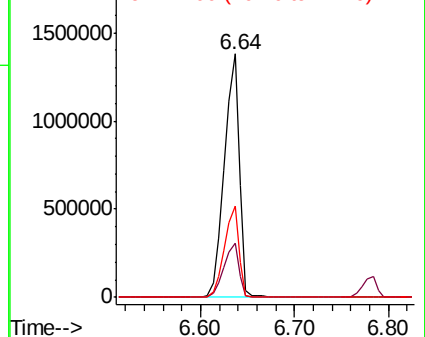

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.29 min Scan# 1012


Delta R.T. -0.01 min

Lab File: BF108327.D



Acq: 21 Aug 2018 9:57

Tgt Ion: 136 Resp: 638646

Ion	Ratio	Lower	Upper
136	100		
137	11.1	8.9	13.3
54	9.0	6.6	9.8
68	5.8	5.0	7.4

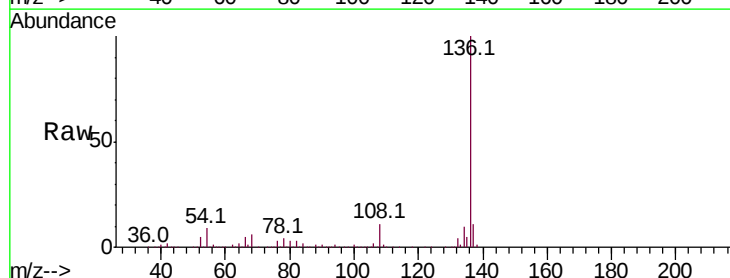

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

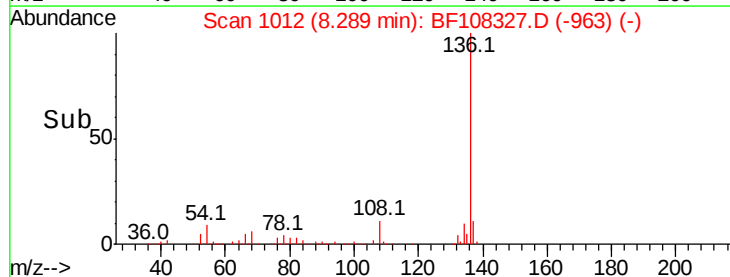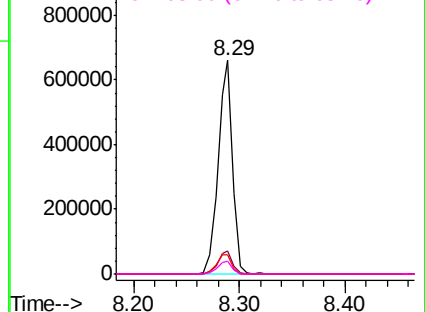



#23

Nitrobenzene-d5

Concen: 109.108 ng

RT: 7.57 min Scan# 890

Delta R.T. -0.01 min

Lab File: BF108327.D

Acq: 21 Aug 2018 9:57

Instrument :

BNA_F

ClientSampleId :

TP-6


Tot Ion: 82 Resp: 1248738

Ion Ratio Lower Upper

82 100

128 42.7 36.1 54.1




54 57.4 41.4 62.2

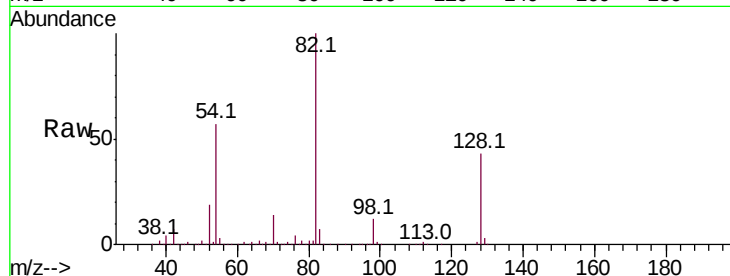

Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 128.00 (127.70 to 128.70): BF1

Ion 54.00 (53.70 to 54.70): BF1

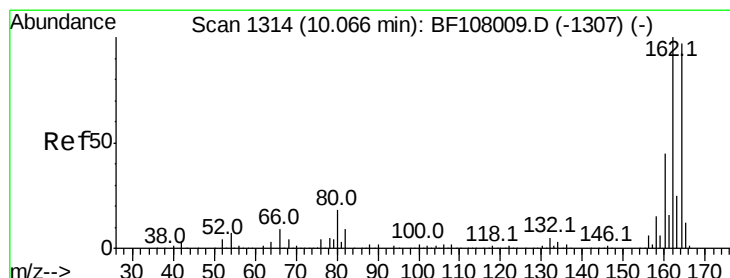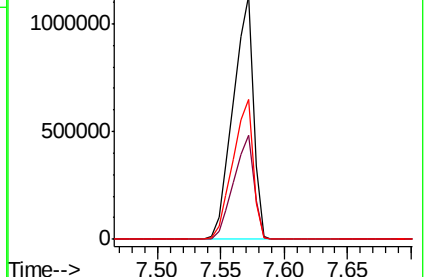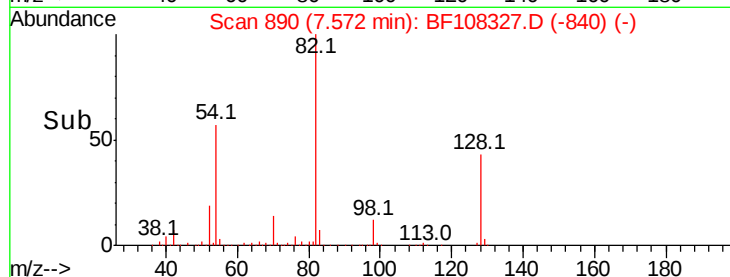

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 10.05 min Scan# 1311

Delta R.T. -0.02 min

Lab File: BF108327.D

Acq: 21 Aug 2018 9:57


Tgt Ion:164 Resp: 328004

Ion Ratio Lower Upper

164 100

162 103.7 86.1 129.1



160 46.4 38.3 57.5

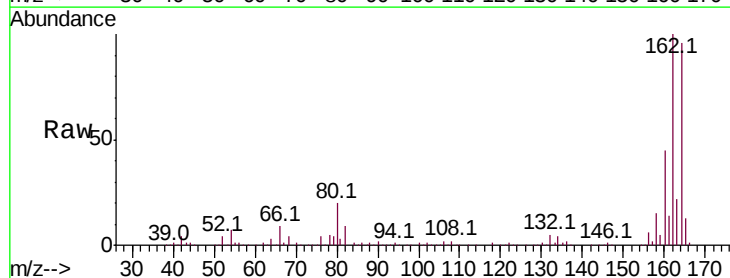

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

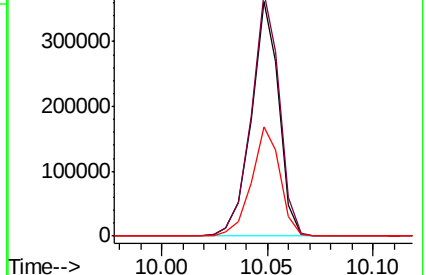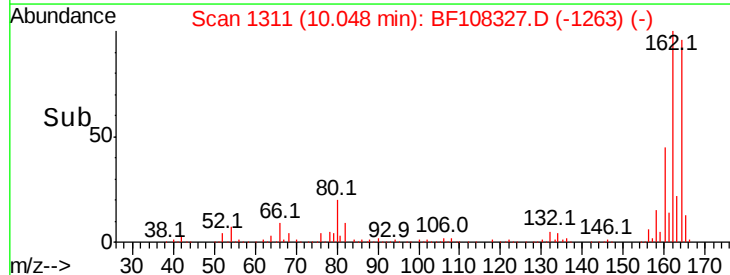






#41
 2,4,6-Tribromophenol
 Concen: 182.879 ng
 RT: 10.85 min Scan# 1447
 Delta R.T. -0.01 min
 Lab File: BF108327.D
 Acq: 21 Aug 2018 9:57

Instrument :
 BNA_F
 ClientSampleId :
 TP-6

Tot Ion:330 Resp: 598336
 Ion Ratio Lower Upper
 330 100
 332 97.6 77.0 115.6
 141 31.6 29.9 44.9

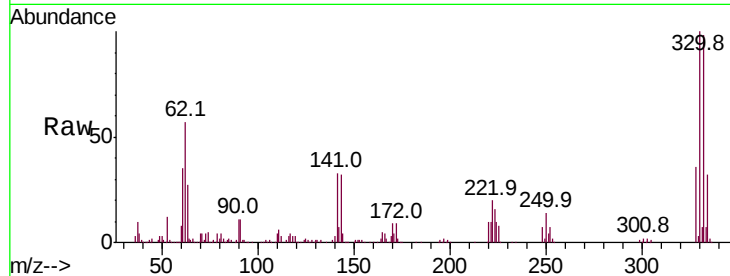


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

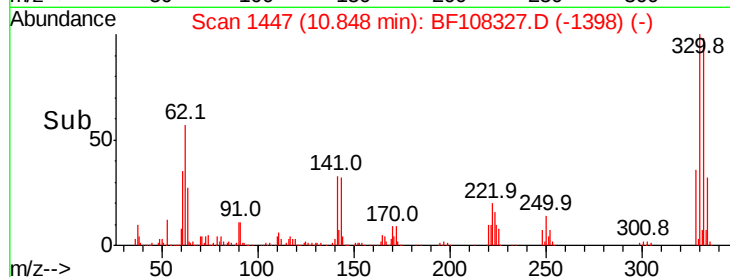
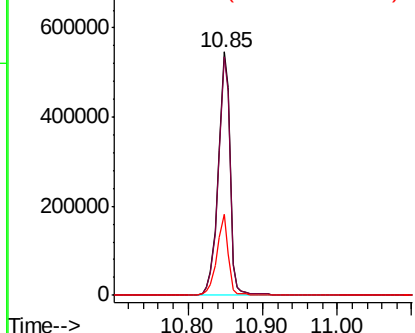


#44
 2-Fluorobiphenyl
 Concen: 107.514 ng
 RT: 9.37 min Scan# 1195
 Delta R.T. -0.01 min
 Lab File: BF108327.D
 Acq: 21 Aug 2018 9:57

Tgt Ion:172 Resp: 2196565
 Ion Ratio Lower Upper
 172 100
 171 37.8 29.7 44.5
 170 25.6 19.6 29.4

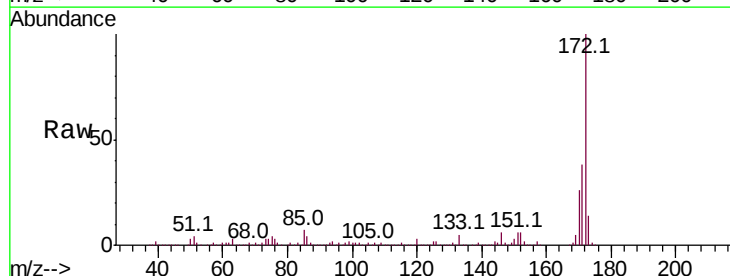

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

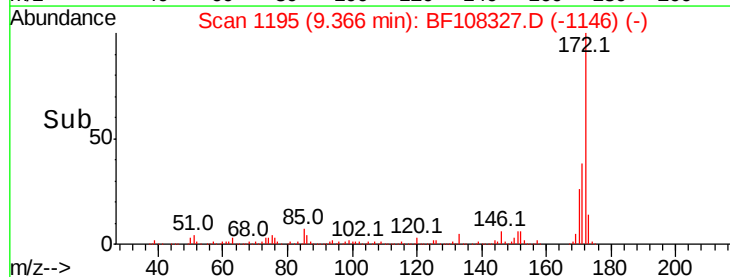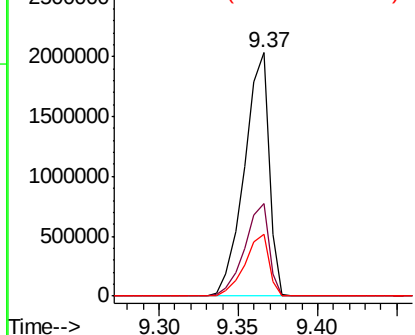







#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.55 min Scan# 1566
Delta R.T. -0.01 min
Lab File: BF108327.D
Acq: 21 Aug 2018 9:57

Instrument :
BNA_F
ClientSampled :
TP-6

Tot Ion	Ratio	Lower	Upper
188	100		
94	8.2	8.5	12.7#
80	8.9	9.2	13.8#

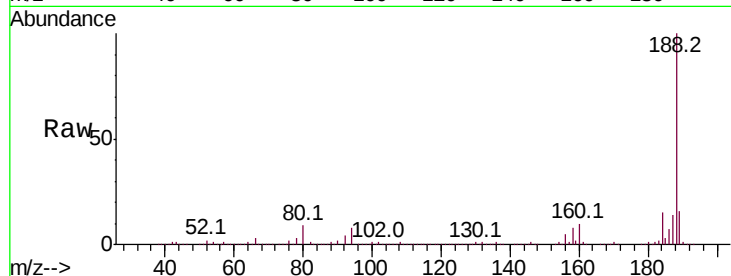


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1

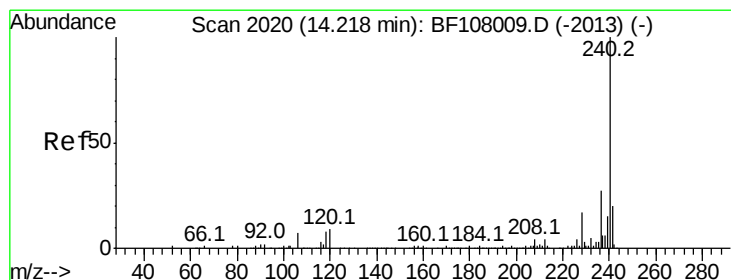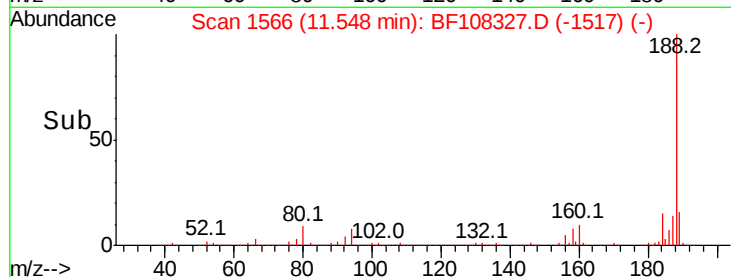
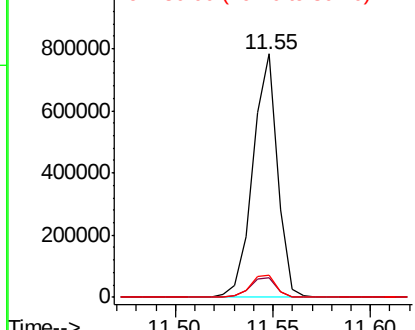



#75
Chrysene-d12
Concen: 20.000 ng
RT: 14.20 min Scan# 2017
Delta R.T. -0.02 min
Lab File: BF108327.D
Acq: 21 Aug 2018 9:57

Tgt Ion	Ratio	Lower	Upper
240	100		
120	8.9	9.5	14.3#
236	26.3	20.7	31.1

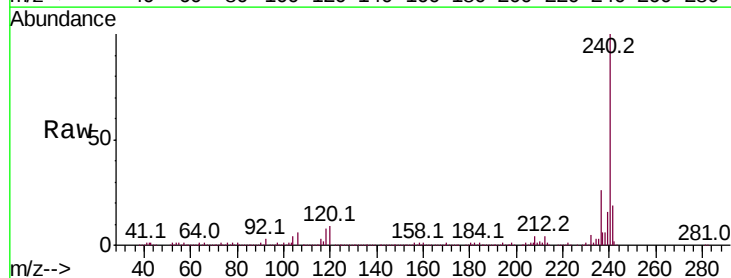

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

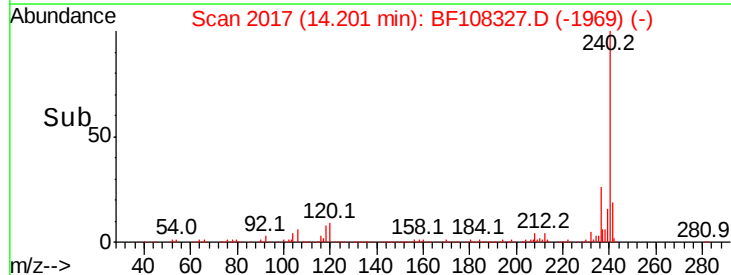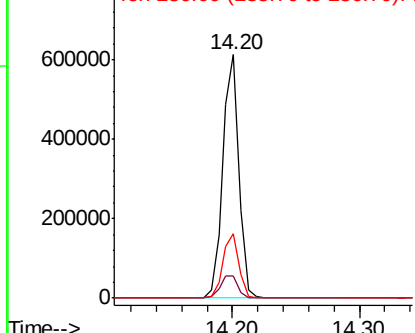

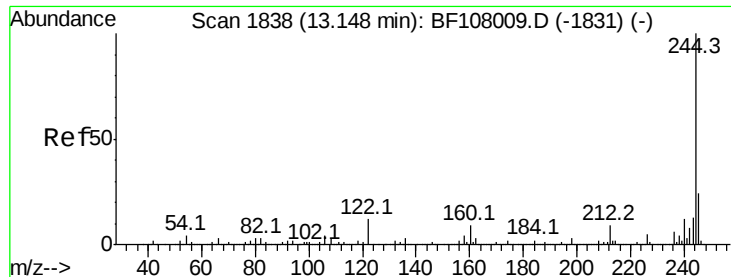

#78

Terphenyl-d14

Concen: 124.224 ng

RT: 13.14 min Scan# 1837

Delta R.T. -0.01 min

Lab File: BF108327.D

Acq: 21 Aug 2018 9:57

Instrument :

BNA_F

ClientSampleId :

TP-6


Tot Ion:244 Resp: 2644097

Ion Ratio Lower Upper

244 100

212 7.9 5.4 8.0




122 10.2 11.0 16.4#

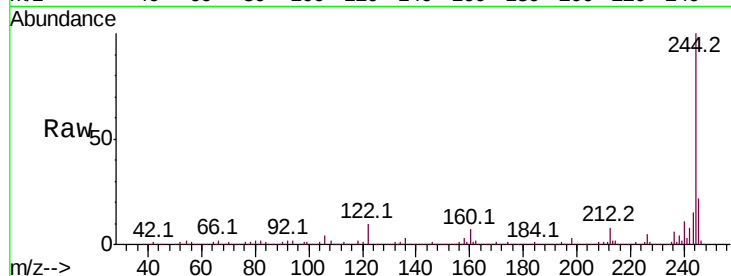

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

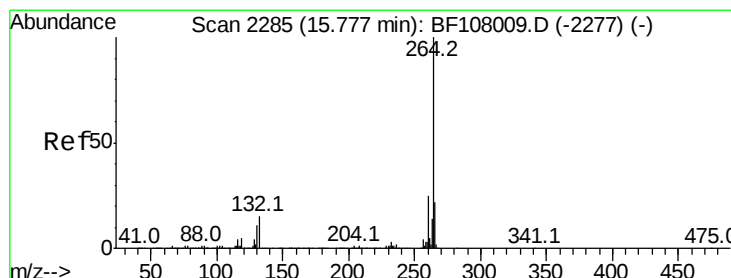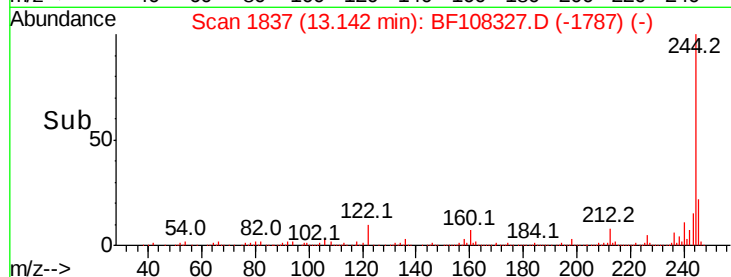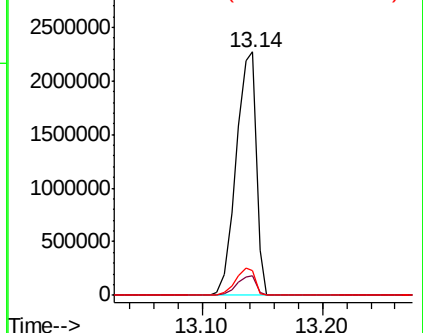

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.76 min Scan# 2282

Delta R.T. -0.02 min

Lab File: BF108327.D

Acq: 21 Aug 2018 9:57


Tgt Ion:264 Resp: 338665

Ion Ratio Lower Upper

264 100

260 23.9 19.2 28.8

265 21.1 17.5 26.3

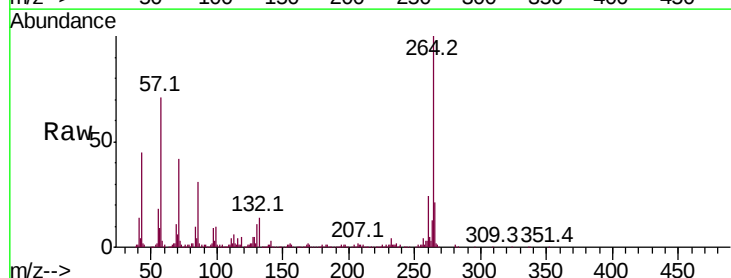

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

