

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082118\
 Data File : BF108358.D
 Acq On : 22 Aug 2018 00:47
 Operator : JU/SJ
 Sample : J4271-13 10X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 HR-06-082018-C

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.619	554	558	567	rBV	351219	313602	23.56%	2.645%
2	6.613	723	727	732	rBV	407983	347699	26.12%	2.933%
3	6.766	750	753	760	rVB	391881	351978	26.45%	2.969%
4	7.001	789	793	797	rBV	1096198	1028857	77.30%	8.679%
5	7.160	816	820	823	rBV	320131	269326	20.24%	2.272%
6	7.560	884	888	896	rVB	244600	228350	17.16%	1.926%
7	8.289	1007	1012	1015	rBV	1565965	1280041	96.18%	10.798%
8	8.331	1017	1019	1022	rVV	26154	25136	1.89%	0.212%
9	8.366	1022	1025	1030	rVB7	9830	15470	1.16%	0.130%
10	8.566	1056	1059	1063	rVB4	15971	16463	1.24%	0.139%
11	8.689	1077	1080	1083	rVB	22562	15633	1.17%	0.132%
12	8.860	1104	1109	1114	rBV2	22627	24696	1.86%	0.208%
13	9.289	1179	1182	1185	rVB	20643	15999	1.20%	0.135%
14	9.360	1190	1194	1201	rBV	460144	397198	29.84%	3.351%
15	9.425	1202	1205	1211	rBV	28904	26941	2.02%	0.227%
16	9.748	1255	1260	1268	rVB	58203	65491	4.92%	0.552%
17	9.907	1284	1287	1291	rBV	18680	17487	1.31%	0.148%
18	9.954	1292	1295	1300	rVB	22377	19361	1.45%	0.163%
19	10.048	1307	1311	1315	rBV2	1516487	1330943	100.00%	11.227%
20	10.083	1315	1317	1325	rVB	18852	20043	1.51%	0.169%
21	10.601	1402	1405	1411	rVB	22974	24521	1.84%	0.207%
22	10.836	1442	1445	1453	rBV	182800	179351	13.48%	1.513%
23	10.942	1458	1463	1469	rBV5	14851	27042	2.03%	0.228%
24	11.148	1491	1498	1501	rBV6	12118	15352	1.15%	0.130%
25	11.542	1562	1565	1568	rBV	1228892	1159922	87.15%	9.784%
26	11.566	1568	1569	1573	rVV	208315	137130	10.30%	1.157%
27	11.619	1575	1578	1583	rVB	56151	46921	3.53%	0.396%
28	12.048	1647	1651	1653	rBV	27677	25562	1.92%	0.216%
29	12.071	1653	1655	1661	rVB2	38181	36043	2.71%	0.304%
30	12.160	1666	1670	1673	rBV2	49882	58483	4.39%	0.493%
31	12.342	1697	1701	1703	rBV	21585	21384	1.61%	0.180%
32	12.595	1741	1744	1748	rBV2	24103	37313	2.80%	0.315%
33	12.689	1756	1760	1763	rBV	21097	25057	1.88%	0.211%
34	12.760	1768	1772	1776	rBV	372366	353643	26.57%	2.983%

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082118\
Data File : BF108358.D
Acq On : 22 Aug 2018 00:47
Operator : JU/SJ
Sample : J4271-13 10X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
HR-06-082018-C

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	12.901	1791	1796	1797	rBV5	12825	17155	1.29%	0.145%
36	12.995	1809	1812	1817	rVB	343894	302084	22.70%	2.548%
37	13.042	1817	1820	1823	rVB2	20681	18552	1.39%	0.156%
38	13.124	1830	1834	1837	rBV	340902	292430	21.97%	2.467%
39	13.201	1844	1847	1848	rBV2	27283	23320	1.75%	0.197%
40	13.318	1864	1867	1872	rVB2	54159	58113	4.37%	0.490%
41	13.366	1872	1875	1877	rBV	21188	24197	1.82%	0.204%
42	13.389	1877	1879	1881	rVB	42072	31647	2.38%	0.267%
43	13.424	1881	1885	1888	rBV2	40733	49976	3.75%	0.422%
44	13.518	1899	1901	1904	rBV2	17682	18231	1.37%	0.154%
45	13.554	1904	1907	1909	rBV2	22717	23786	1.79%	0.201%
46	13.807	1946	1950	1952	rBV2	42421	48441	3.64%	0.409%
47	13.830	1952	1954	1959	rVB	25874	31966	2.40%	0.270%
48	13.948	1970	1974	1976	rBV3	38417	48876	3.67%	0.412%
49	13.971	1976	1978	1980	rVV	34256	34945	2.63%	0.295%
50	14.007	1980	1984	1987	rVV2	37400	58100	4.37%	0.490%
51	14.036	1987	1989	1993	rVB	30666	33807	2.54%	0.285%
52	14.195	2011	2016	2019	rBV2	1159802	1248850	93.83%	10.535%
53	14.218	2019	2020	2026	rVB	193380	171714	12.90%	1.448%
54	14.301	2032	2034	2036	rBV	33937	32523	2.44%	0.274%
55	14.612	2084	2087	2089	rBV3	42830	46868	3.52%	0.395%
56	15.283	2198	2201	2205	rBV	108530	172725	12.98%	1.457%
57	15.618	2255	2258	2264	rVB	65253	84398	6.34%	0.712%
58	15.683	2265	2269	2273	rBV	113531	142620	10.72%	1.203%
59	15.754	2275	2281	2285	rBV	629680	881040	66.20%	7.432%


Sum of corrected areas: 11854802

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082118\
Data File : BF108358.D
Acq On : 22 Aug 2018 00:47
Operator : JU/SJ
Sample : J4271-13 10X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
HR-06-082018-C

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

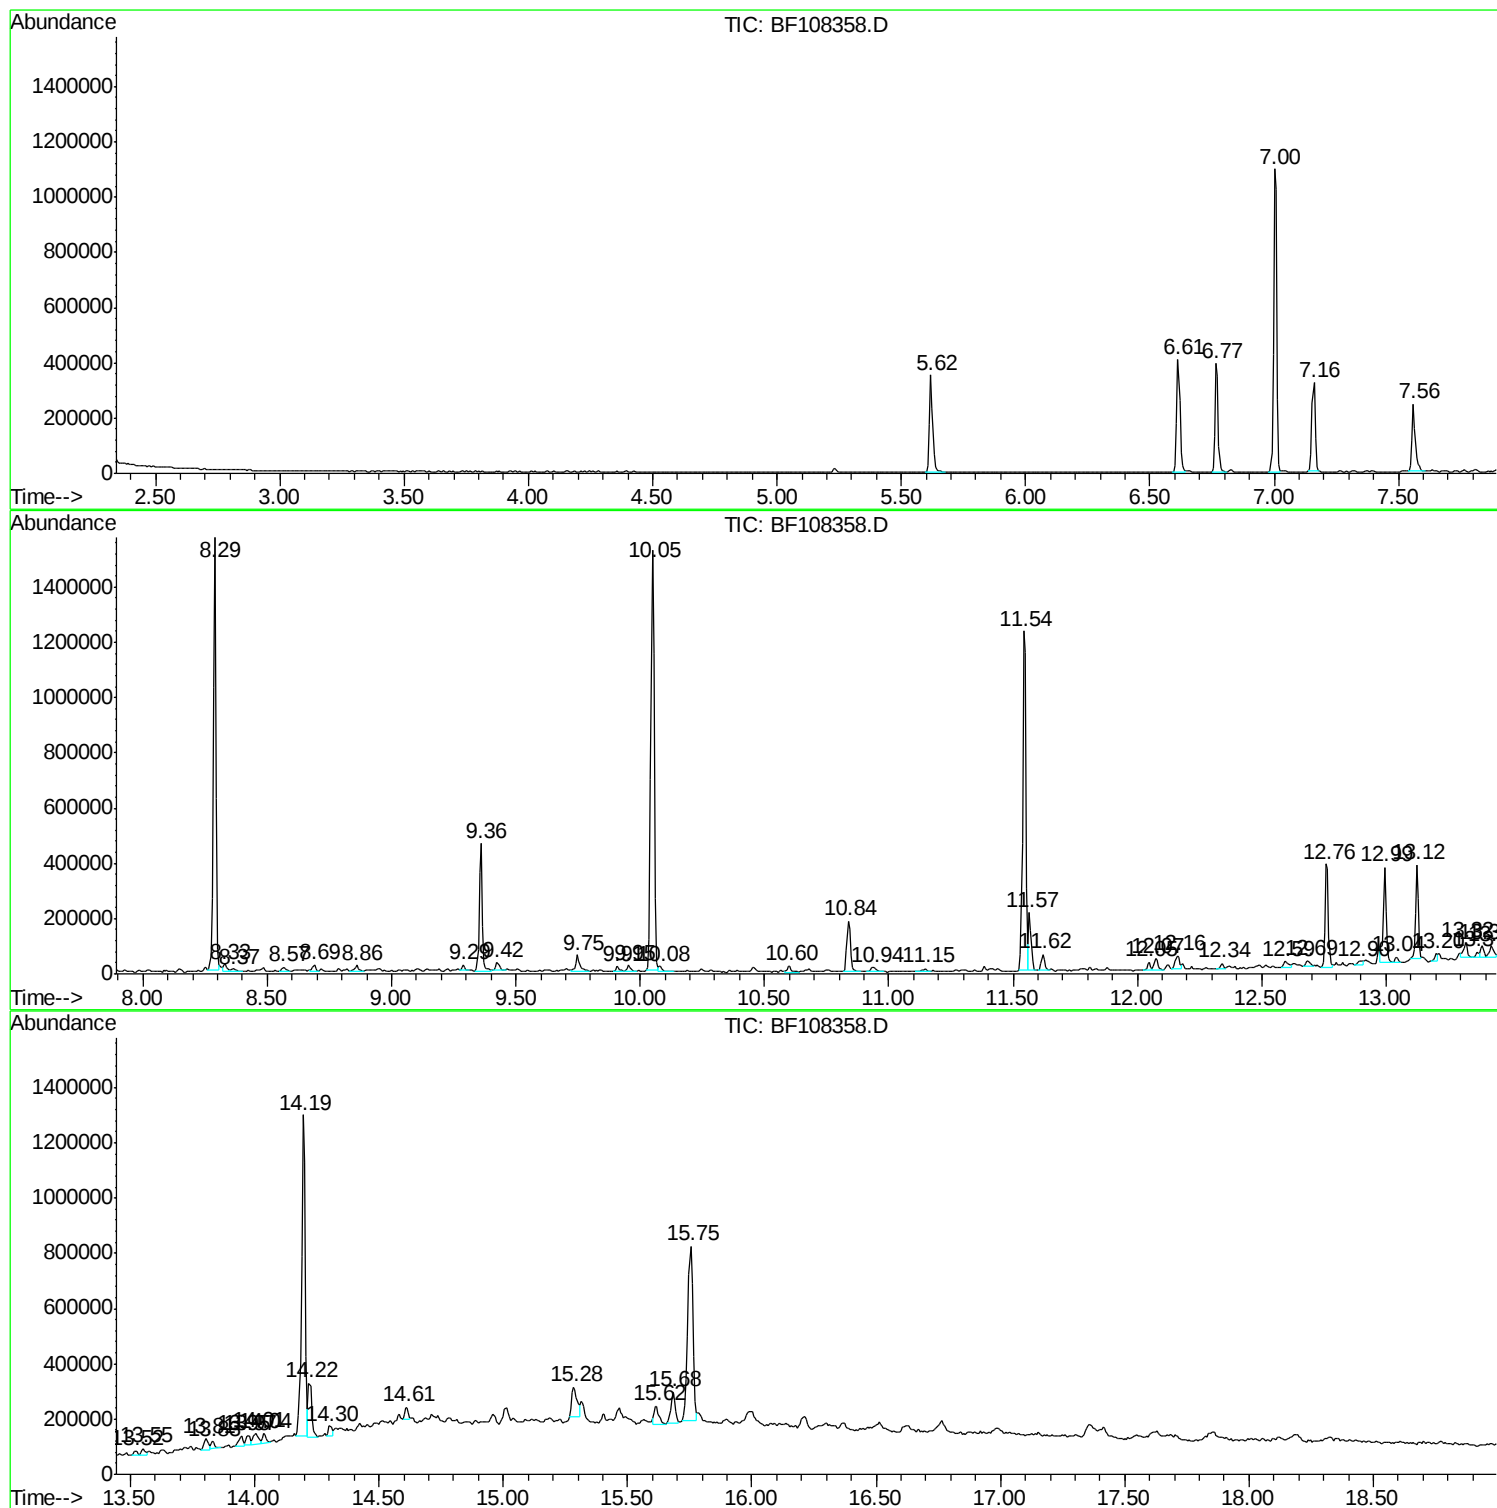

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082118\
Data File : BF108358.D
Acq On : 22 Aug 2018 00:47
Operator : JU/SJ
Sample : J4271-13 10X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
HR-06-082018-C










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.77 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.77	6.84 ng	351978	1,4-Dichlorobenzene-d4	7.00

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2			5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
3			5-Aminoindole	132	C8H8N2	005192-03-0	10
4			(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	9
5			Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9

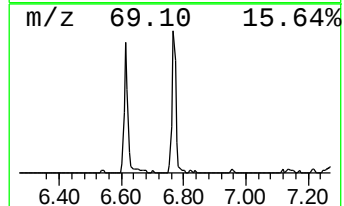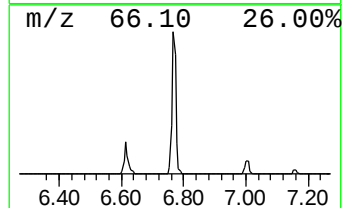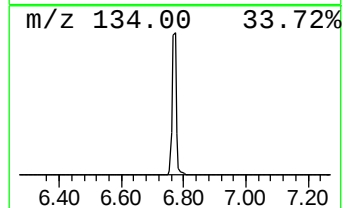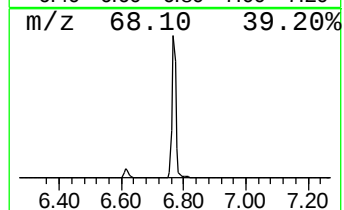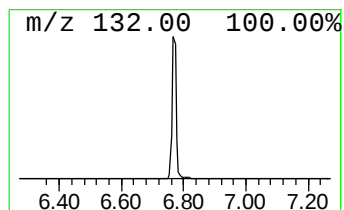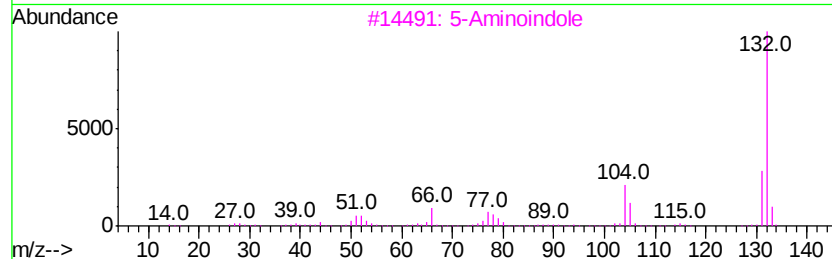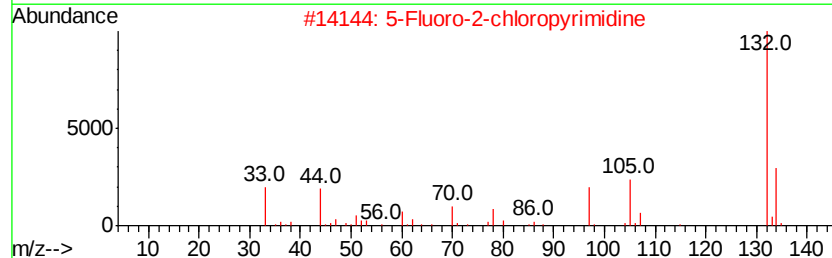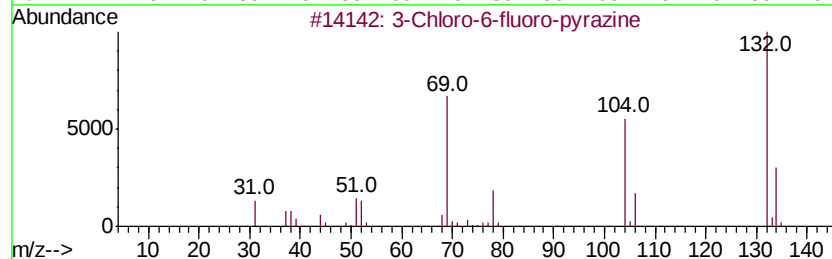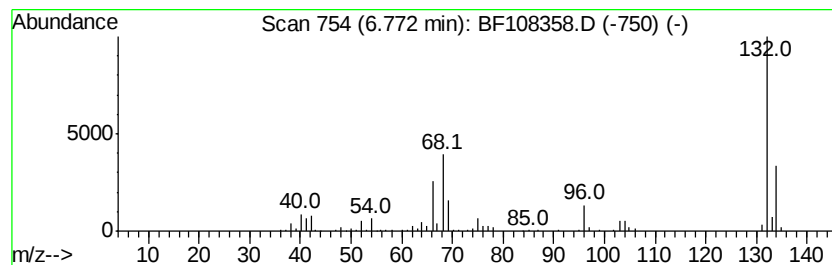

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082118\
Data File : BF108358.D
Acq On : 22 Aug 2018 00:47
Operator : JU/SJ
Sample : J4271-13 10X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
HR-06-082018-C

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.77	6.77	6.8	ng	351978	1	7.00	1028860	20.0